

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071618\
 Data File : PS001078.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jul 2018 06:42
 Operator : UA
 Sample : J3831-02
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 17 08:31:21 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 09 02:00:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.627	11.043	23304778	17951154	112.954	82.421 #
Target Compounds							
2) T	3,5-DICHL...	0.000	9.281	0	25639560	N.D.	87.164 #
6) T	MCP	12.320	0.000	3336418	0	6.074	N.D. #
7) T	MCPA	12.603	0.000	5248918	0	5.751	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071618\
Data File : PS001078.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jul 2018 06:42
Operator : UA
Sample : J3831-02
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 17 08:31:21 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
Quant Title : 8080.M
QLast Update : Mon Jul 09 02:00:25 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

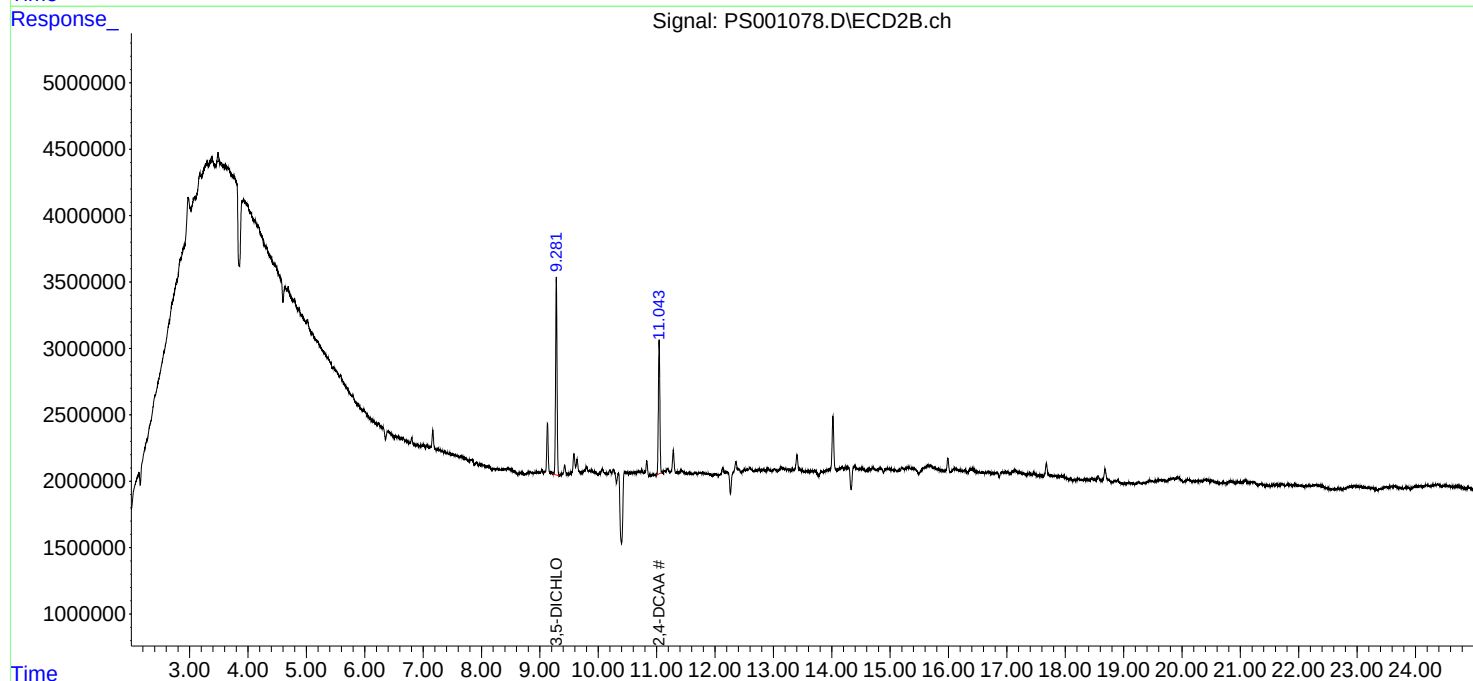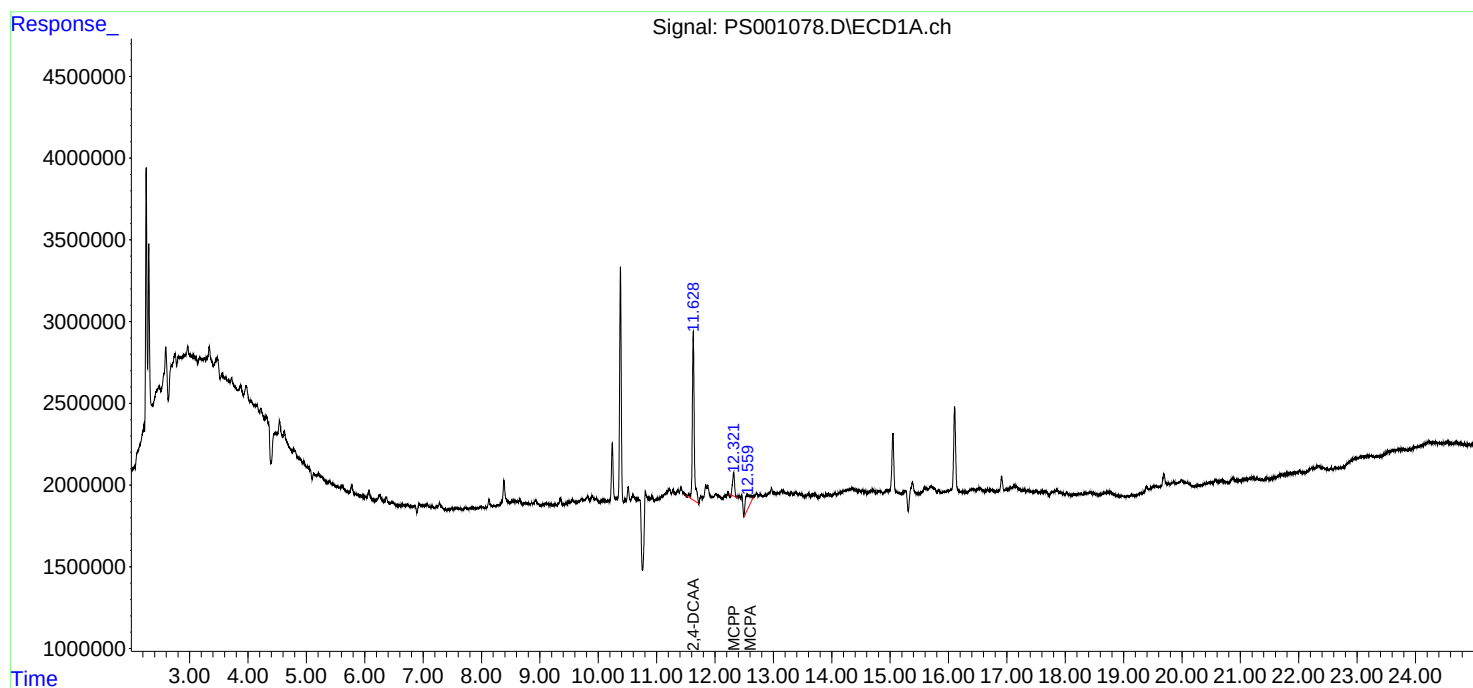


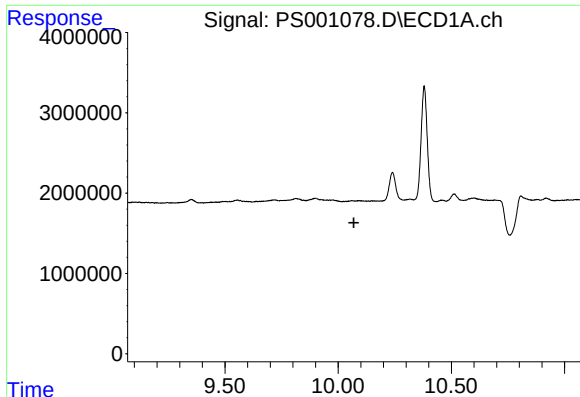

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 10.070 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

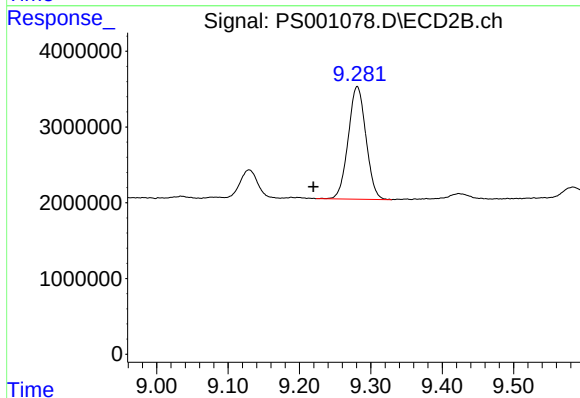


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.281 min
Delta R.T.: 0.062 min
Response: 25639560
Conc: 87.16 ng/ml

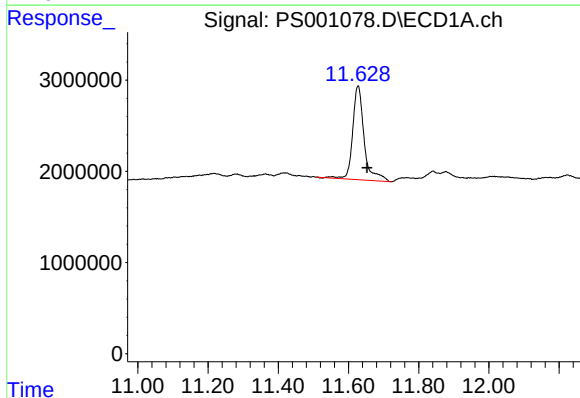


#4 2,4-DCAA

R.T.: 11.627 min
Delta R.T.: -0.026 min
Response: 23304778
Conc: 112.95 ng/ml

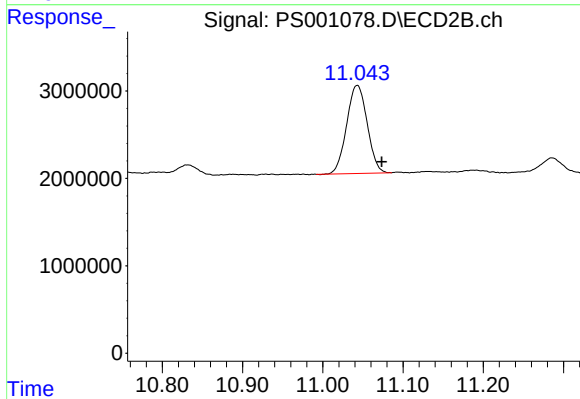

#4 2,4-DCAA


R.T.: 11.043 min
Delta R.T.: -0.031 min
Response: 17951154
Conc: 82.42 ng/ml

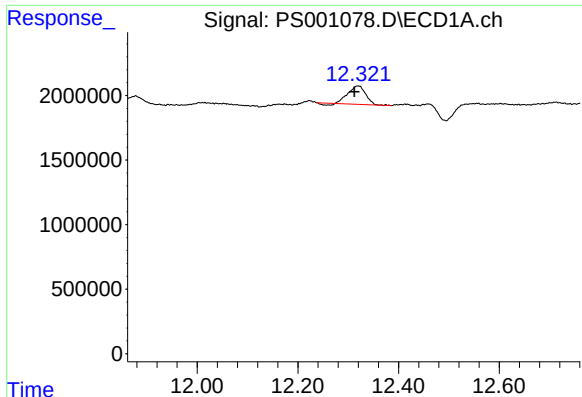

#6 MCPP


R.T.: 12.320 min
Delta R.T.: 0.008 min
Response: 3336418
Conc: 6.07 ug/ml

Instrument :
ECD_S
ClientSampleId :

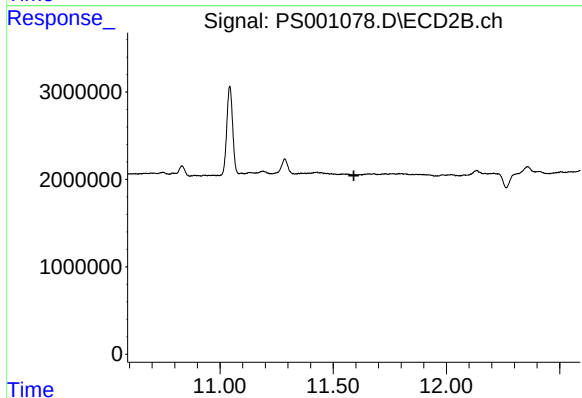


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 11.591 min
Response: 0
Conc: N.D.

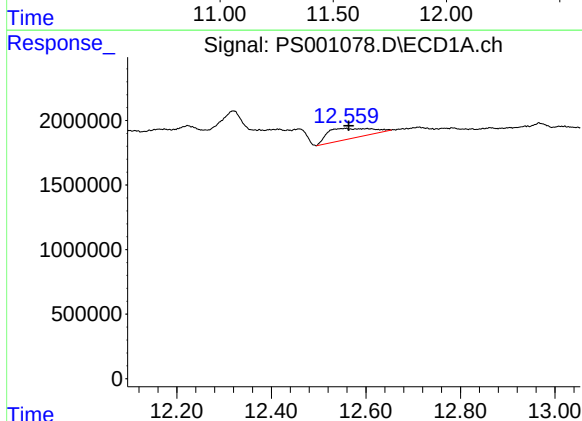

#7 MCPA

R.T.: 12.603 min
Delta R.T.: 0.039 min
Response: 5248918
Conc: 5.75 ug/ml

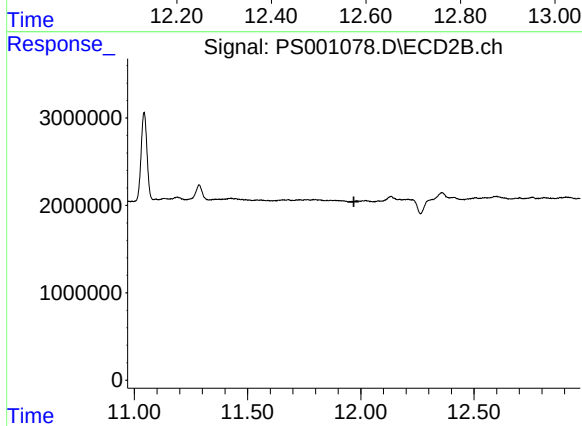

#7 MCPA

R.T.: 0.000 min
Exp R.T. : 11.969 min
Response: 0
Conc: N.D.