

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071618\
 Data File : PS001079.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jul 2018 07:13
 Operator : UA
 Sample : J3959-02
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 17 08:31:39 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 09 02:00:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.664	11.079	85796341	74601820	415.841	342.529
Target Compounds							
1) T	Dalapon	3.006	2.443	3162351	1636900	11.777	6.075 #
2) T	3,5-DICHL...	0.000	9.165	0	20447589	N.D.	69.513 #
5) T	DICAMBA	0.000	11.324	0	7663888	N.D.	9.764 #
6) T	MCP	12.358	0.000	11034785	0	20.089	N.D. #
7) T	MCPA	12.497	0.000	4126300	0	4.521	N.D. #
8) T	DICHLORPROP	0.000	12.450	0	2918588	N.D.	14.450 #
9) T	2,4-D	0.000	12.948	0	5019873	N.D.	18.125 #
11) T	2,4,5-TP ...	0.000	14.057	0	6891589	N.D.	5.492 #
15) T	Picloram	0.000	16.971	0	12297572	N.D.	8.076 #
16) T	DCPA	17.705	16.971	15193815	12297572	10.437	7.153 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071618\
Data File : PS001079.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jul 2018 07:13
Operator : UA
Sample : J3959-02
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 17 08:31:39 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
Quant Title : 8080.M
QLast Update : Mon Jul 09 02:00:25 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

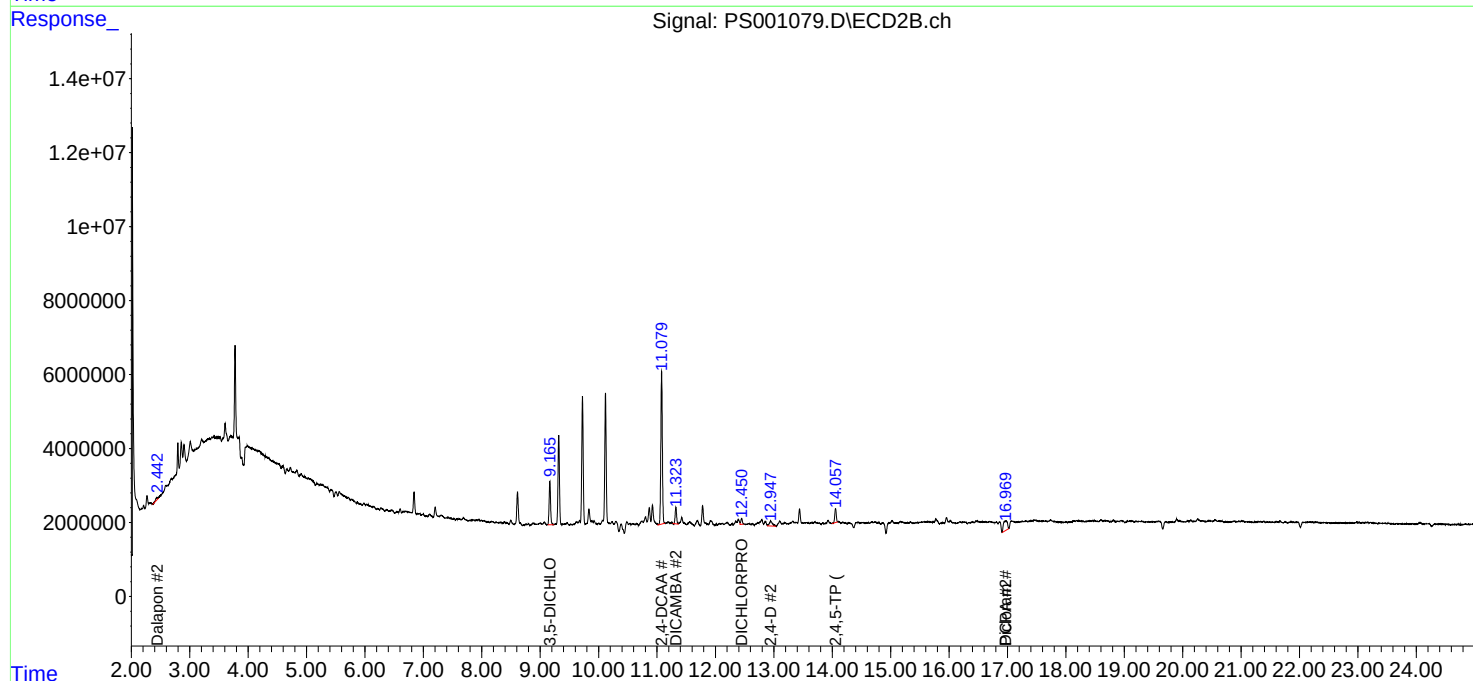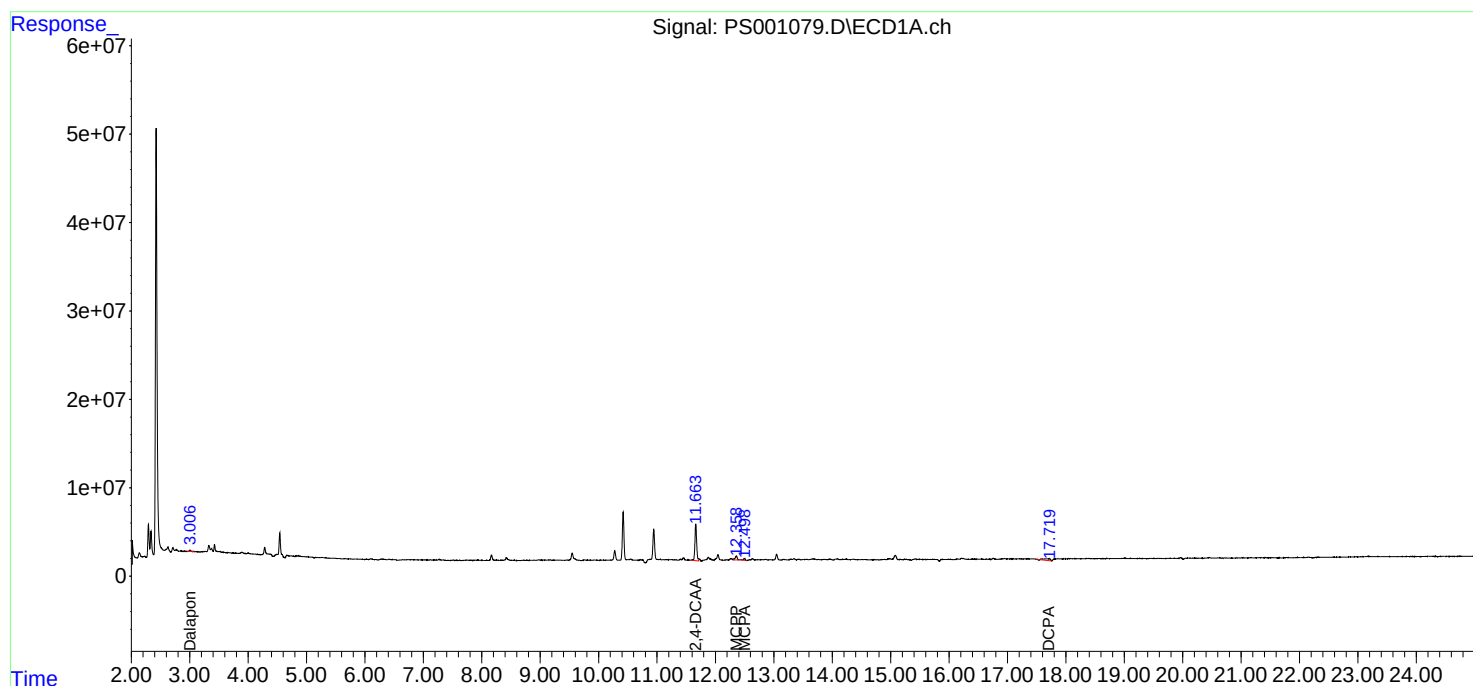


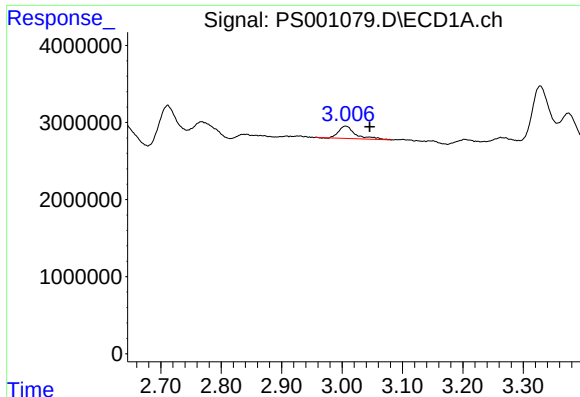

#1 Dalapon


R.T.: 3.006 min
Delta R.T.: -0.040 min
Response: 3162351
Conc: 11.78 ng/ml

Instrument :
ECD_S
ClientSampleId :

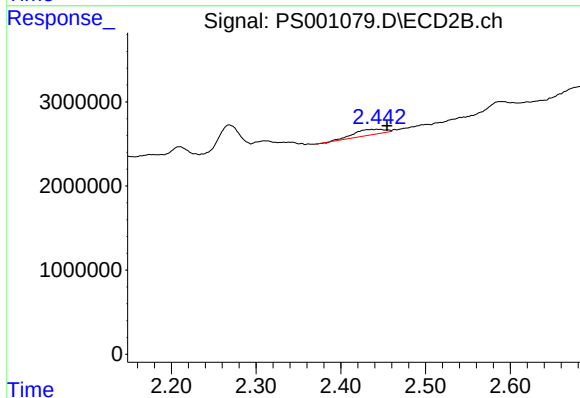


#1 Dalapon

R.T.: 2.443 min
Delta R.T.: -0.012 min
Response: 1636900
Conc: 6.08 ng/ml

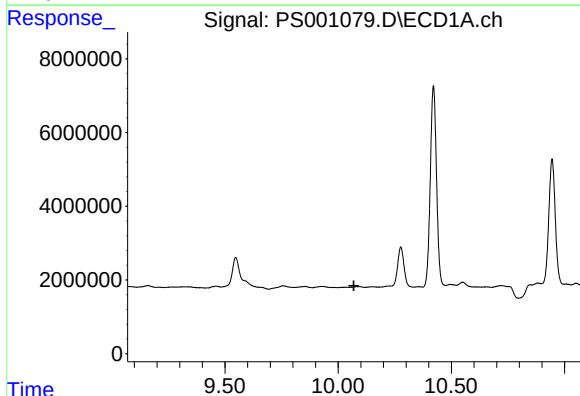


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 10.070 min
Response: 0
Conc: N.D.

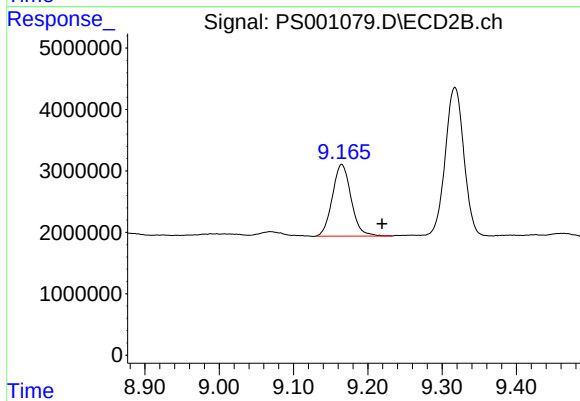

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.165 min
Delta R.T.: -0.055 min
Response: 20447589
Conc: 69.51 ng/ml

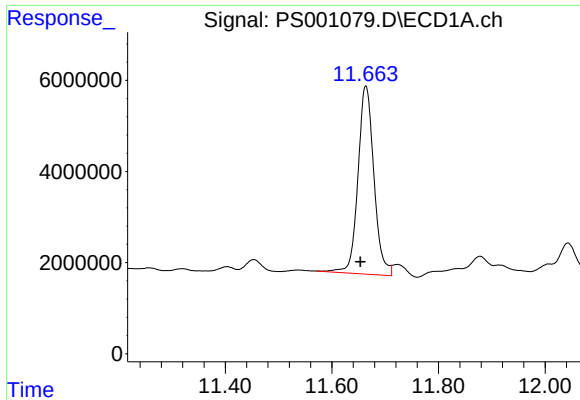

#4 2,4-DCAA


R.T.: 11.664 min
Delta R.T.: 0.010 min
Response: 85796341
Conc: 415.84 ng/ml

Instrument :
ECD_S
ClientSampleId :

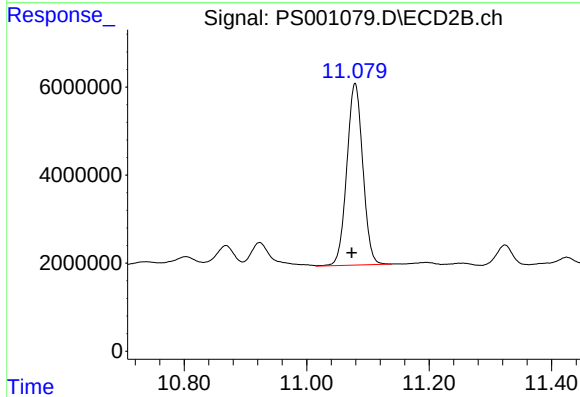


#4 2,4-DCAA

R.T.: 11.079 min
Delta R.T.: 0.005 min
Response: 74601820
Conc: 342.53 ng/ml

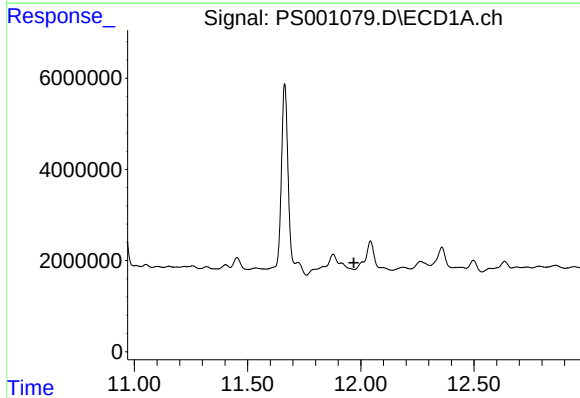


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.970 min
Response: 0
Conc: N.D.

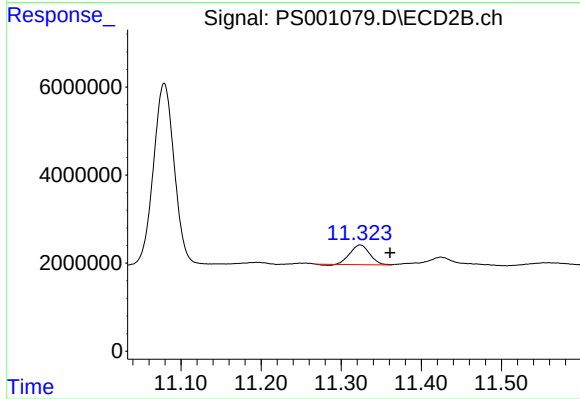

#5 DICAMBA


R.T.: 11.324 min
Delta R.T.: -0.037 min
Response: 7663888
Conc: 9.76 ng/ml

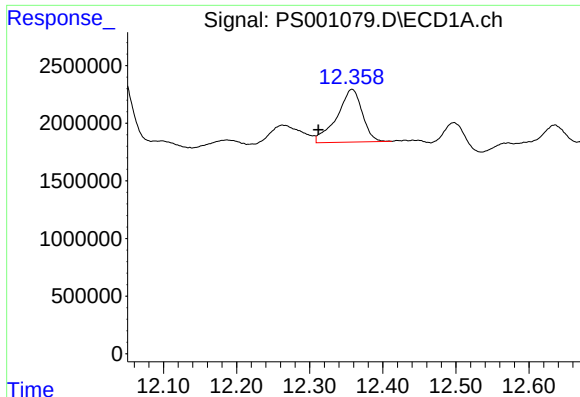

#6 MCPP


R.T.: 12.358 min
Delta R.T.: 0.046 min
Response: 11034785
Conc: 20.09 ug/ml

Instrument :
ECD_S
ClientSampleId :

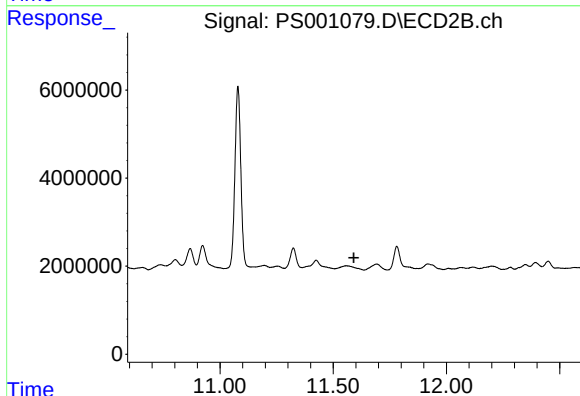


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 11.591 min
Response: 0
Conc: N.D.

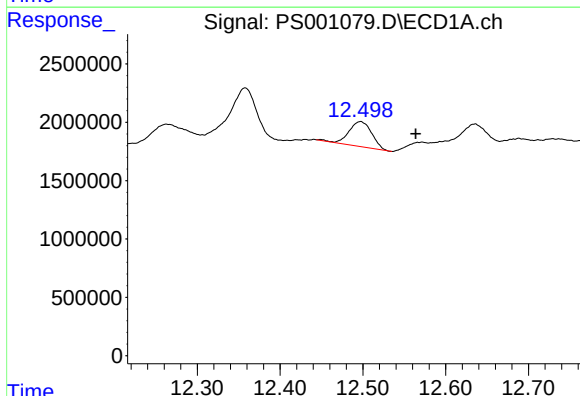


#7 MCPA

R.T.: 12.497 min
Delta R.T.: -0.067 min
Response: 4126300
Conc: 4.52 ug/ml

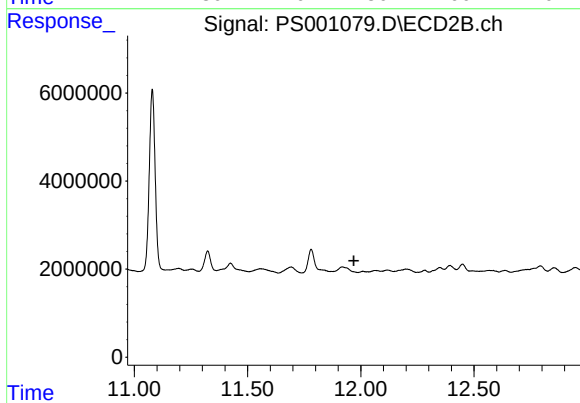

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 11.969 min
Response: 0
Conc: N.D.

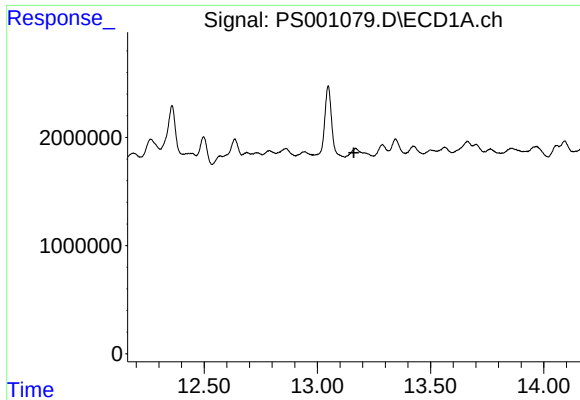

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 13.161 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

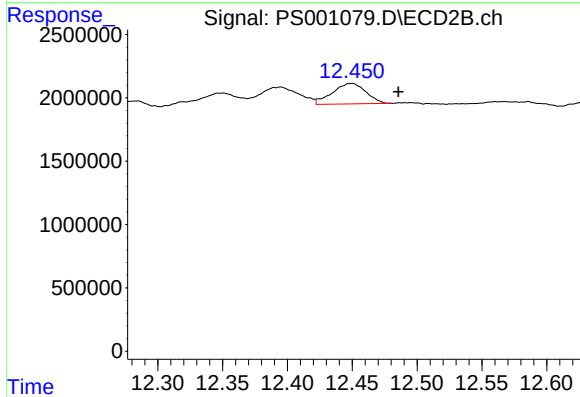


#8 DICHLORPROP

R.T.: 12.450 min
Delta R.T.: -0.036 min
Response: 2918588
Conc: 14.45 ng/ml

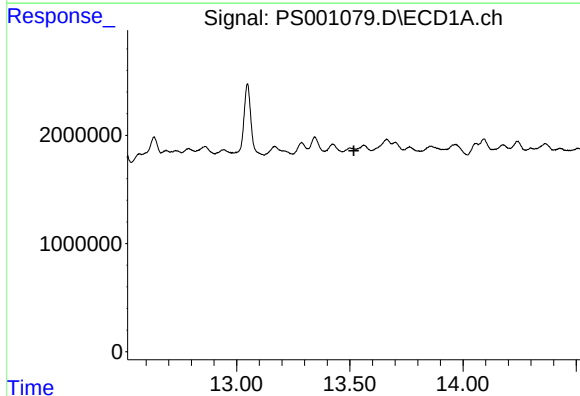


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 13.518 min
Response: 0
Conc: N.D.

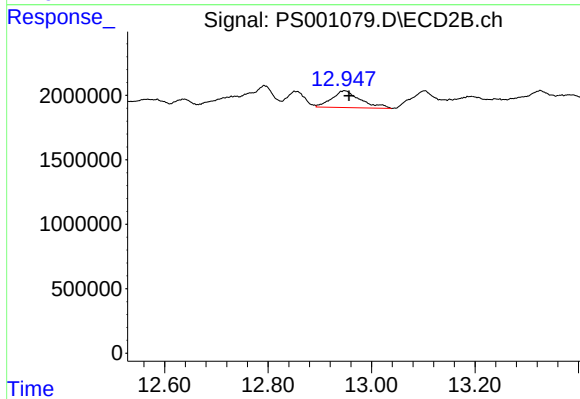

#9 2,4-D


R.T.: 12.948 min
Delta R.T.: -0.009 min
Response: 5019873
Conc: 18.12 ng/ml

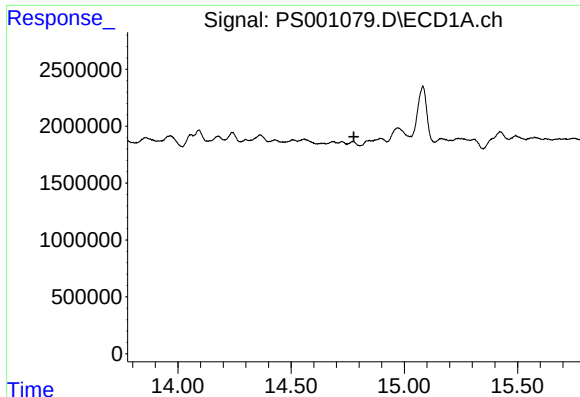

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.777 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

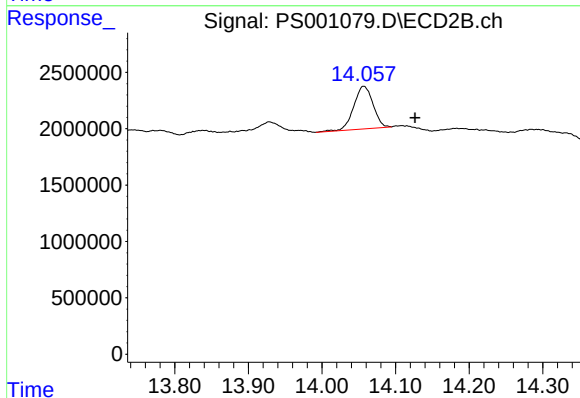


#11 2,4,5-TP (SILVEX)

R.T.: 14.057 min
Delta R.T.: -0.070 min
Response: 6891589
Conc: 5.49 ng/ml

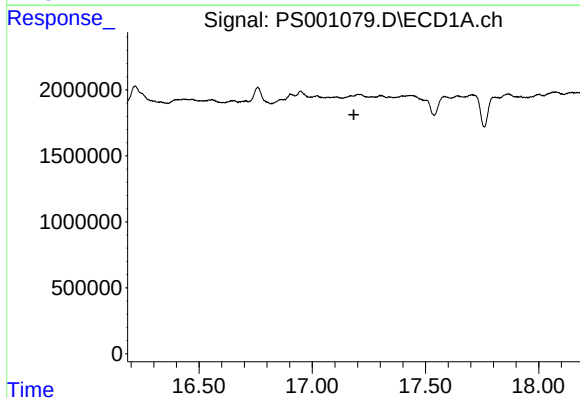


#15 Picloram

R.T.: 0.000 min
Exp R.T.: 17.184 min
Response: 0
Conc: N.D.

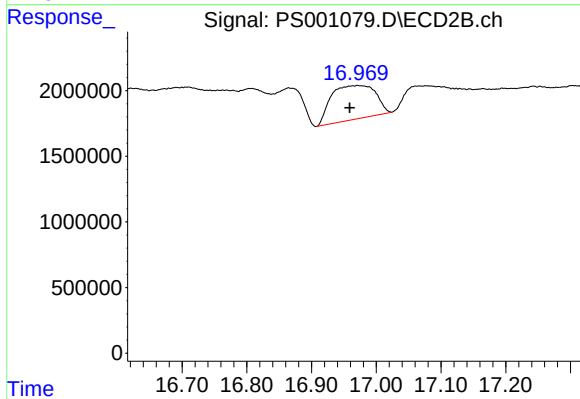

#15 Picloram


R.T.: 16.971 min
Delta R.T.: 0.012 min
Response: 12297572
Conc: 8.08 ng/ml

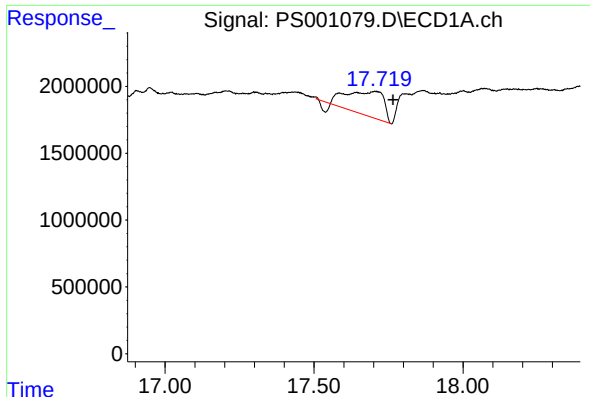

#16 DCPA

R.T.: 17.705 min
Delta R.T.: -0.061 min
Response: 15193815
Conc: 10.44 ng/ml

Instrument :
ECD_S
ClientSampleId :

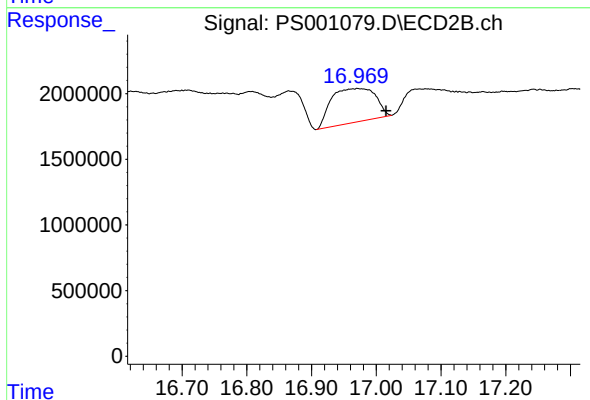

#16 DCPA

R.T.: 16.971 min
Delta R.T.: -0.044 min
Response: 12297572
Conc: 7.15 ng/ml