

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071619\
 Data File : PS005500.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Jul 2019 11:17
 Operator : SM\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 17 00:40:52 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 20 11:04:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
2) T	3,5-DICHL...	4.949	0.000	401.9E6	0	199.983	N.D. #
5) T	DICAMBA	0.000	5.448	0	265.7E6	N.D.	70.982
6) T	MCCP	0.000	5.448	0	265.7E6	N.D.	95.391
9) T	2,4-D	6.623	0.000	383.2E6	0	246.501	N.D. #
12) T	2,4,5-T	7.589	7.402	50453474	43925602	6.269	8.611 #
15) T	Picloram	9.121	9.109	125.8E6	144.0E6	10.943	19.084 #
16) T	DCPA	9.583	9.109	13382167	144.0E6	1.342	21.155 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071619\
Data File : PS005500.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Jul 2019 11:17
Operator : SM\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 17 00:40:52 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
Quant Title : 8080.M
QLast Update : Thu Jun 20 11:04:04 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

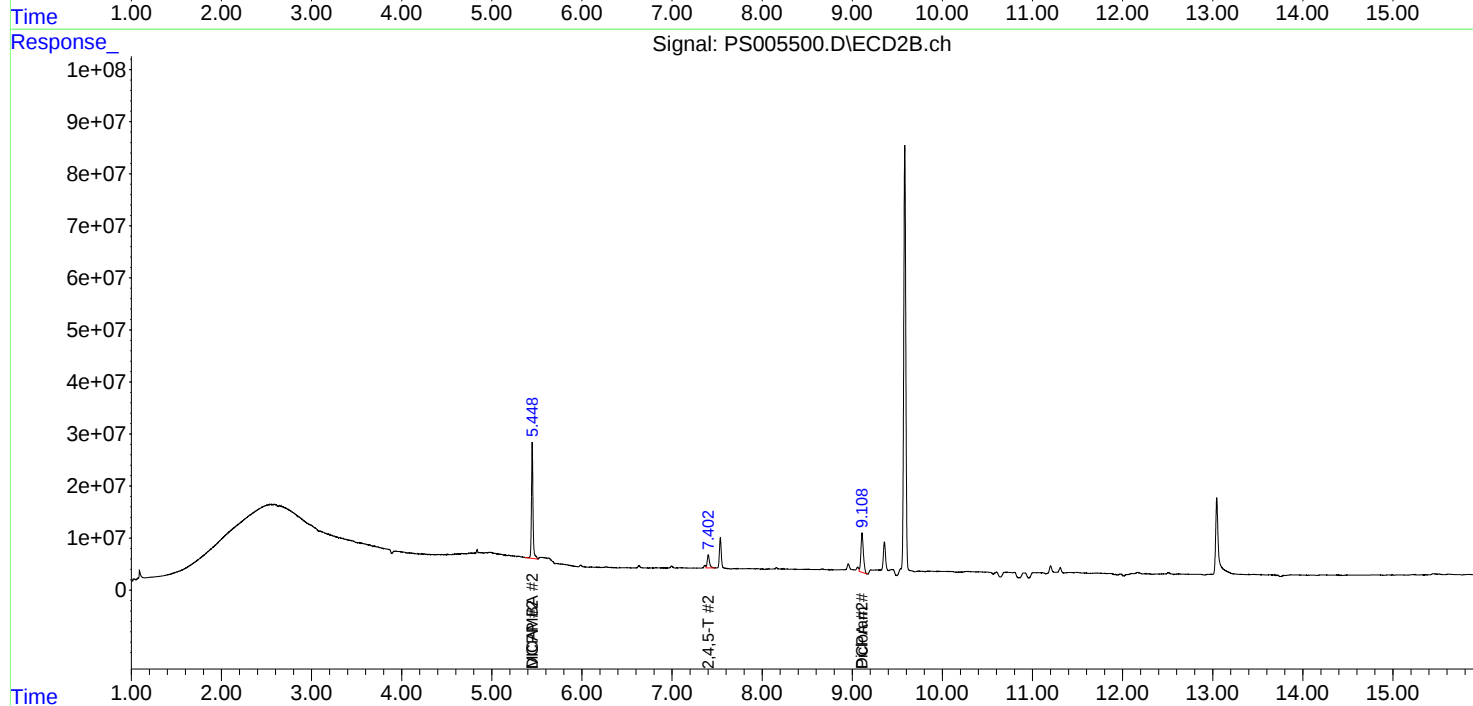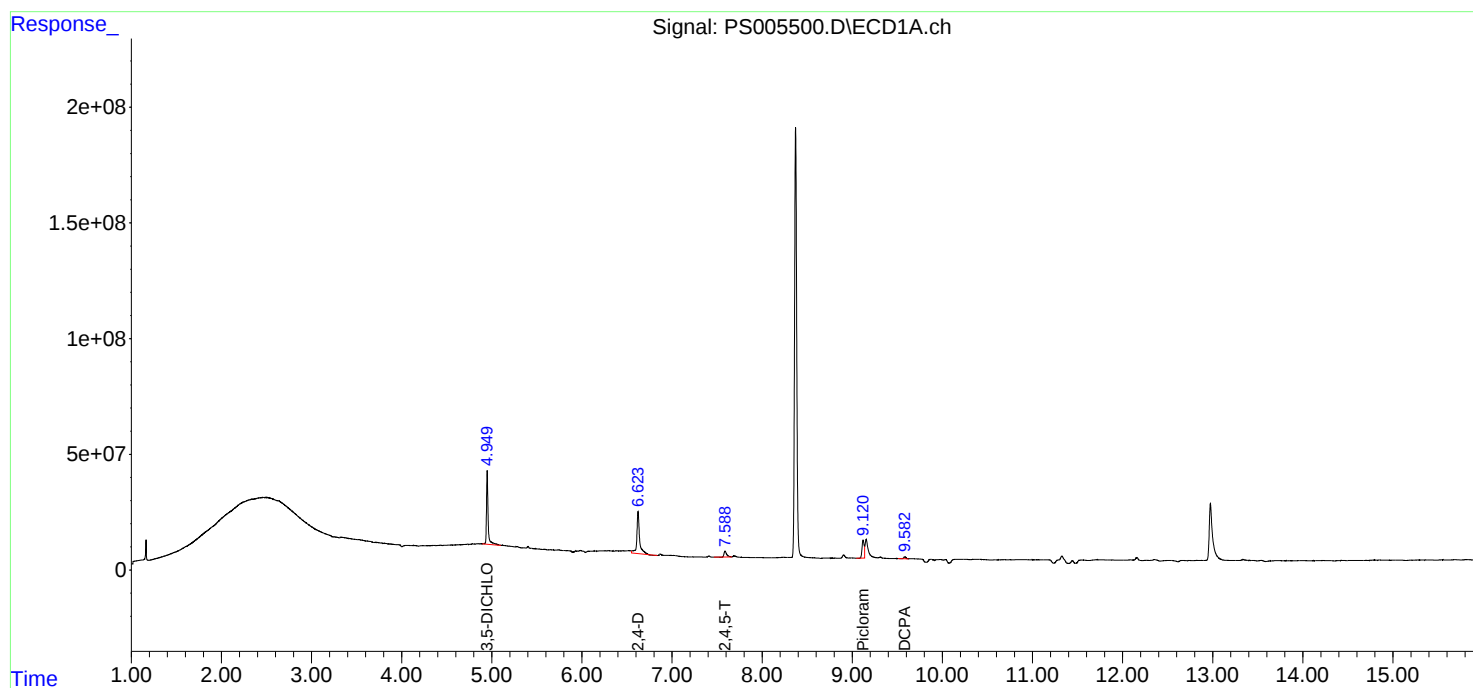


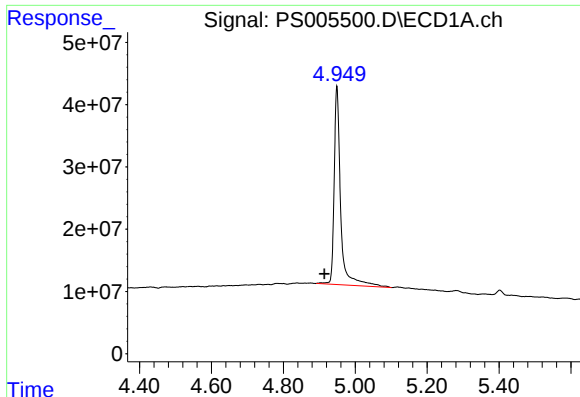

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.949 min
Delta R.T.: 0.035 min
Response: 401909570
Conc: 199.98 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

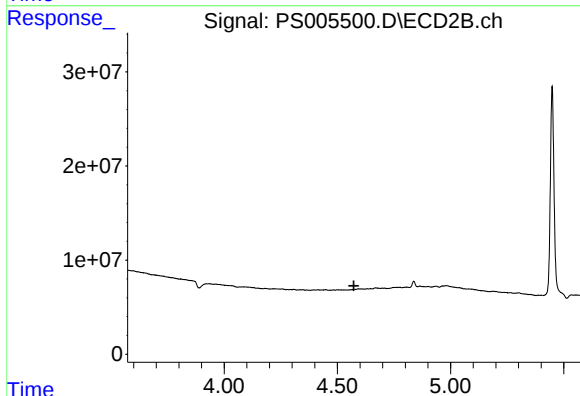


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.573 min
Response: 0
Conc: N.D.

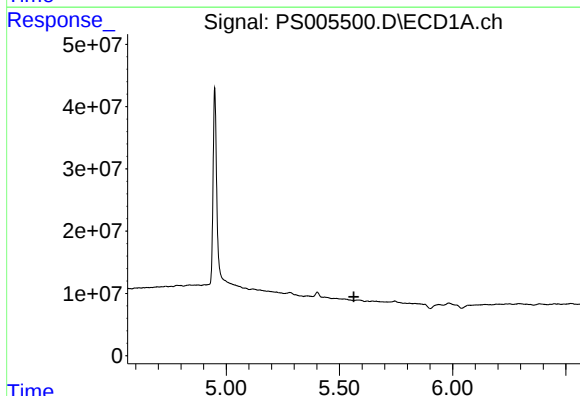


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 5.564 min
Response: 0
Conc: N.D.

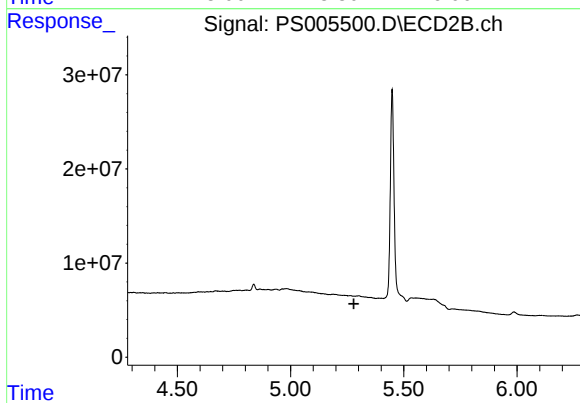

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 5.280 min
Response: 0
Conc: N.D.

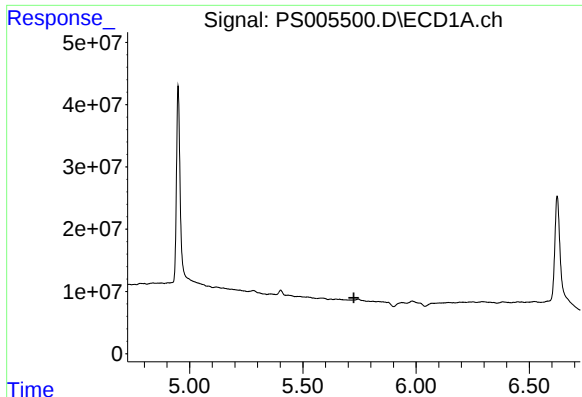

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.725 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

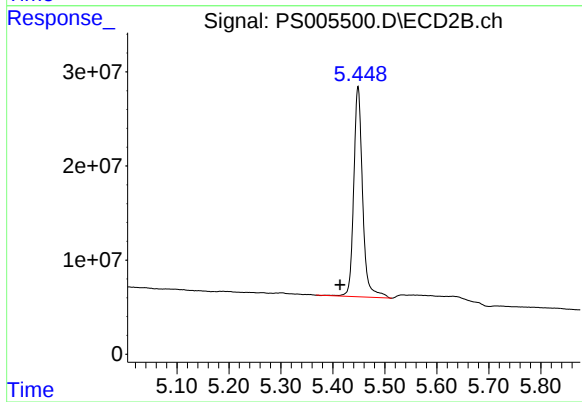


#5 DICAMBA

R.T.: 5.448 min
Delta R.T.: 0.034 min
Response: 265708695
Conc: 70.98 ng/ml

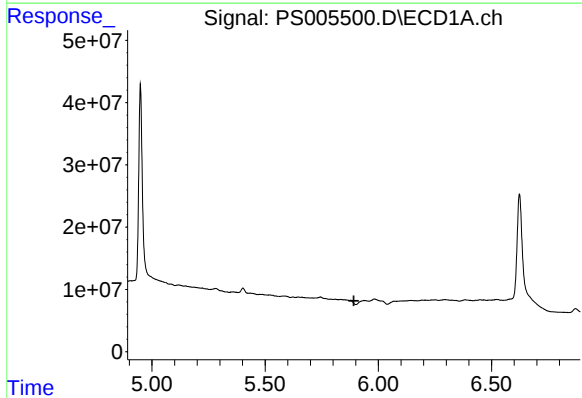


#6 MCPP

R.T.: 0.000 min
Exp R.T.: 5.892 min
Response: 0
Conc: N.D.

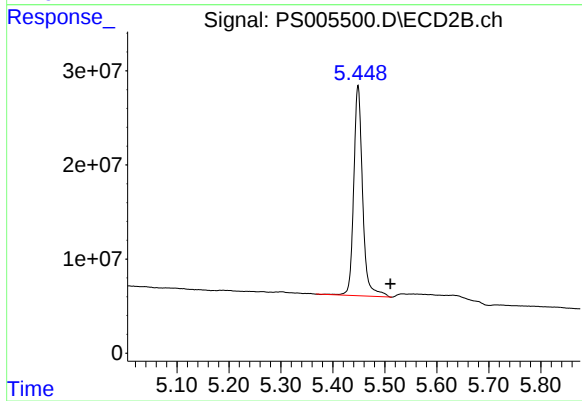

#6 MCPP


R.T.: 5.448 min
Delta R.T.: -0.062 min
Response: 265708695
Conc: 95.39 ug/ml

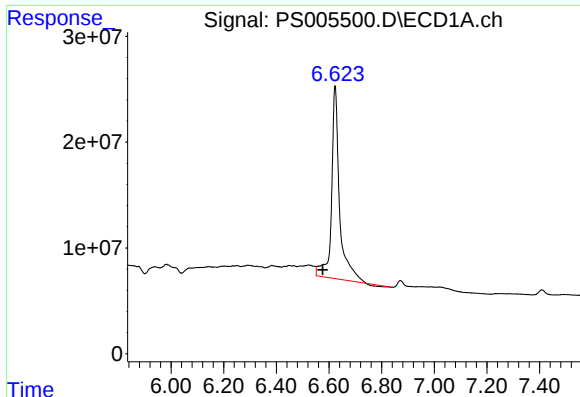

#9 2,4-D


R.T.: 6.623 min
Delta R.T.: 0.047 min
Response: 383209852
Conc: 246.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

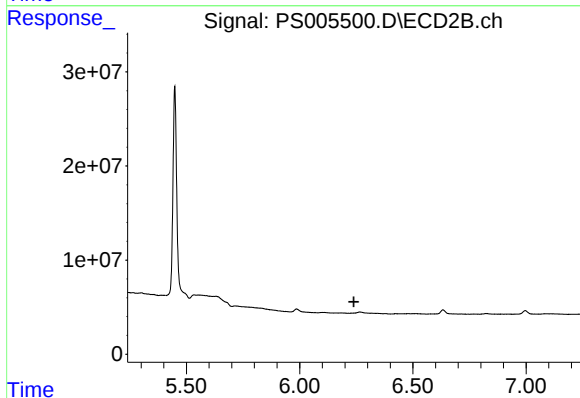


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.240 min
Response: 0
Conc: N.D.

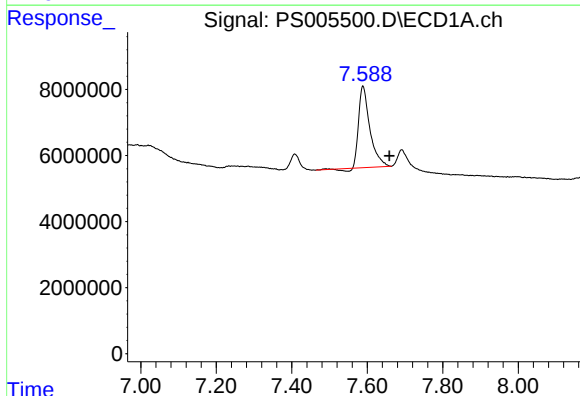


#12 2,4,5-T

R.T.: 7.589 min
Delta R.T.: -0.070 min
Response: 50453474
Conc: 6.27 ng/ml

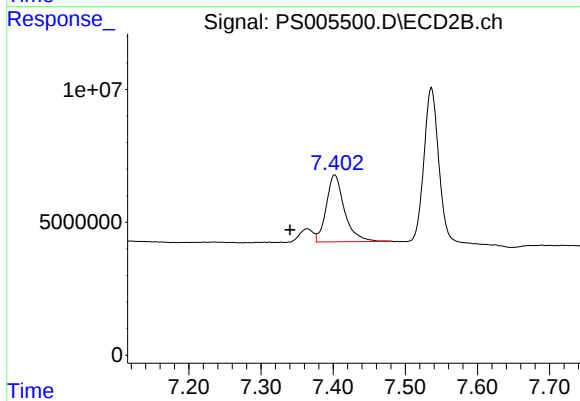

#12 2,4,5-T


R.T.: 7.402 min
Delta R.T.: 0.062 min
Response: 43925602
Conc: 8.61 ng/ml

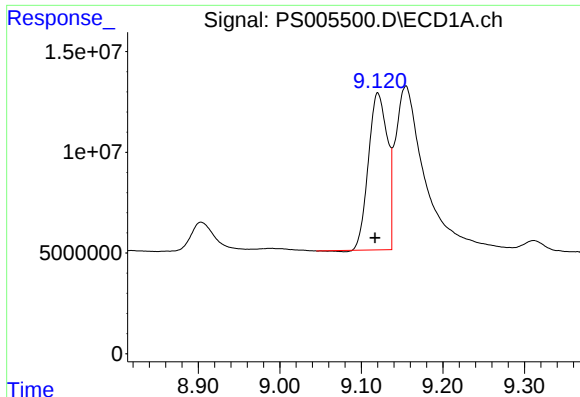

#15 Picloram


R.T.: 9.121 min
Delta R.T.: 0.004 min
Response: 125751362
Conc: 10.94 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

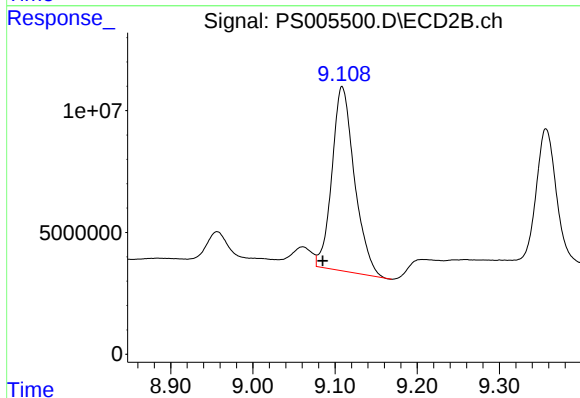


#15 Picloram

R.T.: 9.109 min
Delta R.T.: 0.024 min
Response: 144013676
Conc: 19.08 ng/ml

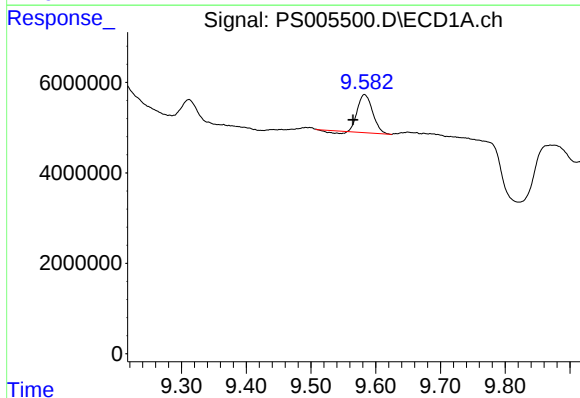

#16 DCPA

R.T.: 9.583 min
Delta R.T.: 0.018 min
Response: 13382167
Conc: 1.34 ng/ml

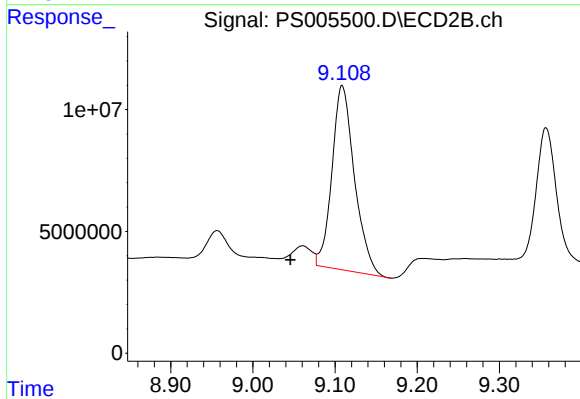

#16 DCPA

R.T.: 9.109 min
Delta R.T.: 0.063 min
Response: 144013676
Conc: 21.16 ng/ml