

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071620\
 Data File : PS011246.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Jul 2020 16:29
 Operator : DD\AJ
 Sample : L3302-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 16 17:04:00 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071320.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 13 16:10:29 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.226	6.918	238.2E6	142.4E6	245.460	252.991
Target Compounds							
1) T	Dalapon	2.994	2.583	40633137	98088820	33.766	127.774 #
2) T	3,5-DICHL...	0.000	6.098	0	48868282	N.D.	58.187
6) T	MCPD	7.583	0.000	6653073	0	2.197	N.D. #
7) T	MCPA	7.775	7.380	21340949	41193957	5.004	14.292 #
8) T	DICHLORPROP	0.000	7.650	0	5935996	N.D.	9.862
9) T	2,4-D	0.000	7.984	0	8254506	N.D.	11.011
10) T	Pentachlo...	8.649	8.434	17880002	22762288	1.353	3.266 #
11) T	2,4,5-TP ...	9.239	8.840	7811148	-3357791	1.475	N.D. #
12) T	2,4,5-T	9.505	9.167	5822015	12305745	1.154	4.057 #
13) T	2,4-DB	9.990	9.705	7167319	36145921	11.120	84.552 #
14) T	DINOSEB	11.164	10.032	64906228	47697164	16.838	22.237 #
15) T	Picloram	10.989	11.024	132.7E6	10848649	21.031	2.481 #
16) T	DCPA	11.470	0.000	19586415	0	3.040	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071620\
Data File : PS011246.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Jul 2020 16:29
Operator : DD\AJ
Sample : L3302-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 16 17:04:00 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071320.M
Quant Title : 8080.M
QLast Update : Mon Jul 13 16:10:29 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

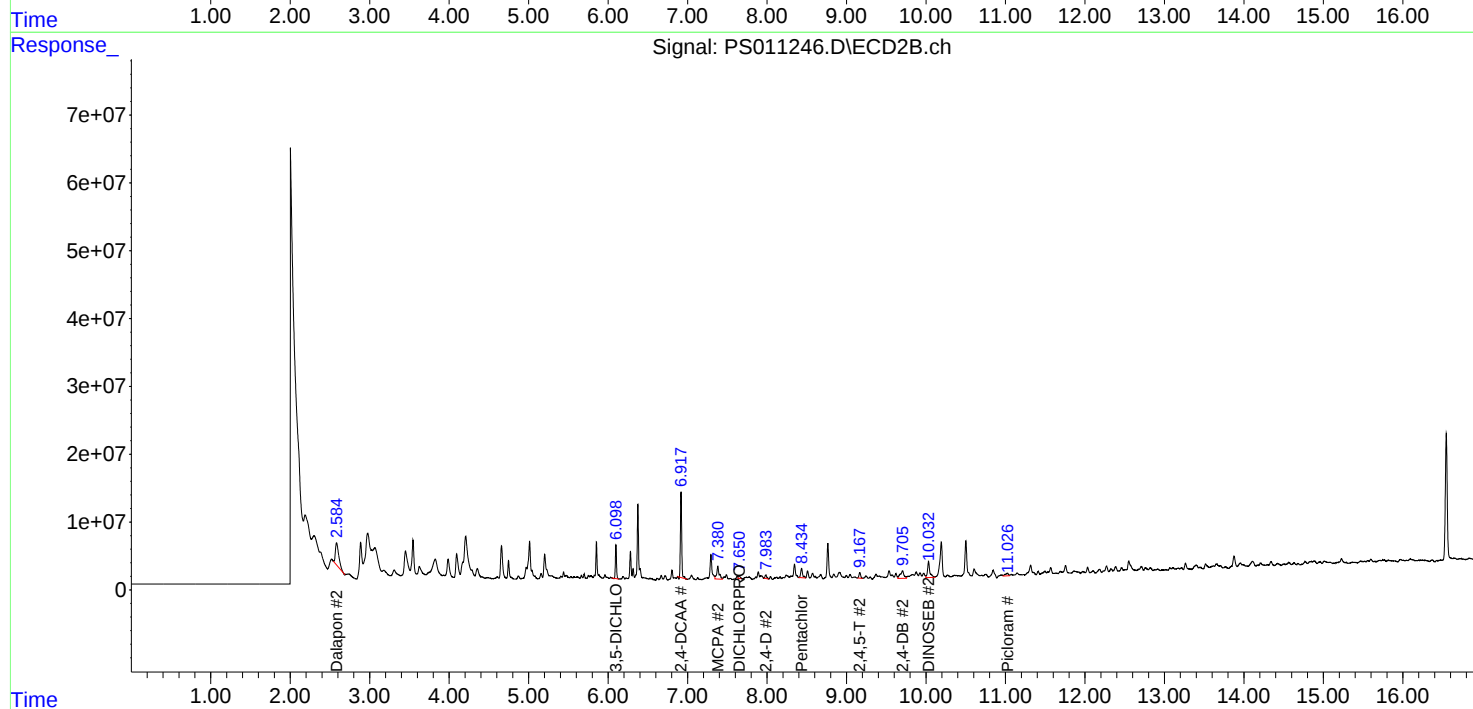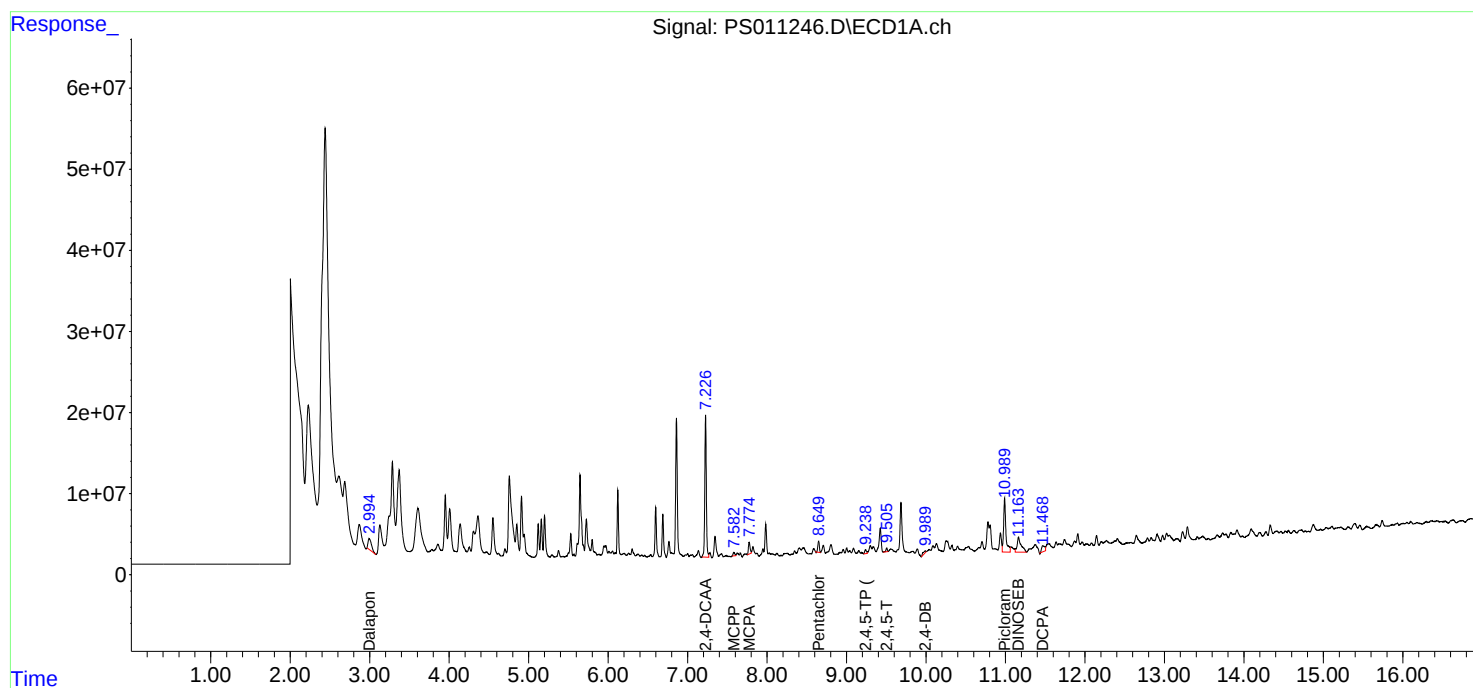


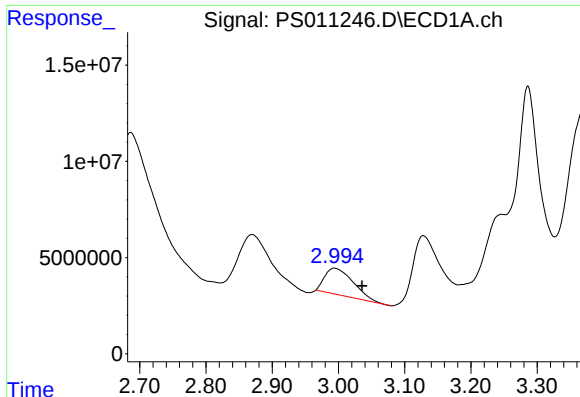

#1 Dalapon


R.T.: 2.994 min
Delta R.T.: -0.042 min
Response: 40633137
Conc: 33.77 ng/ml

Instrument :
ECD_S
ClientSampleId :

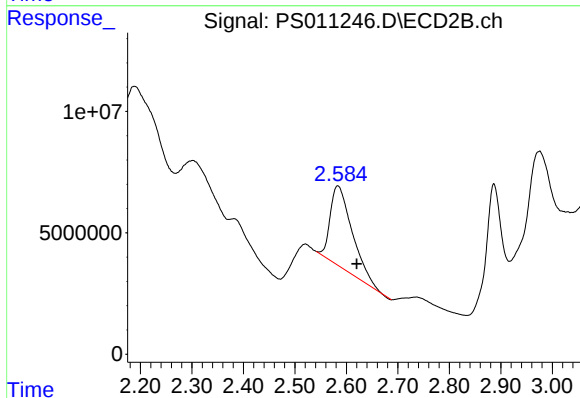


#1 Dalapon

R.T.: 2.583 min
Delta R.T.: -0.037 min
Response: 98088820
Conc: 127.77 ng/ml

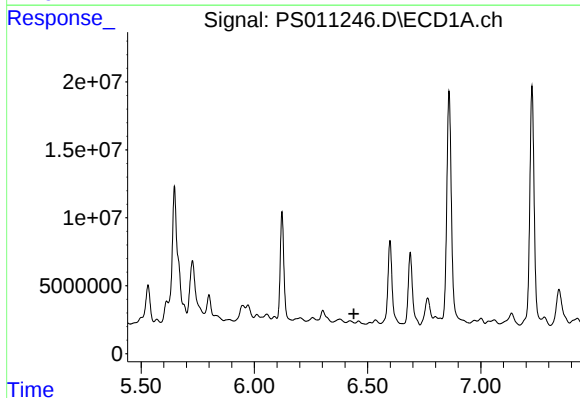


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.439 min
Response: 0
Conc: N.D.

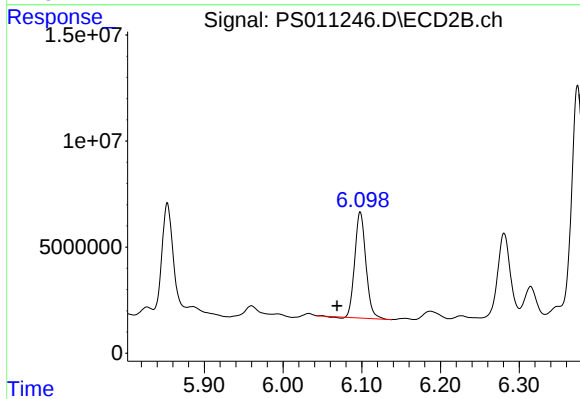

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.098 min
Delta R.T.: 0.030 min
Response: 48868282
Conc: 58.19 ng/ml

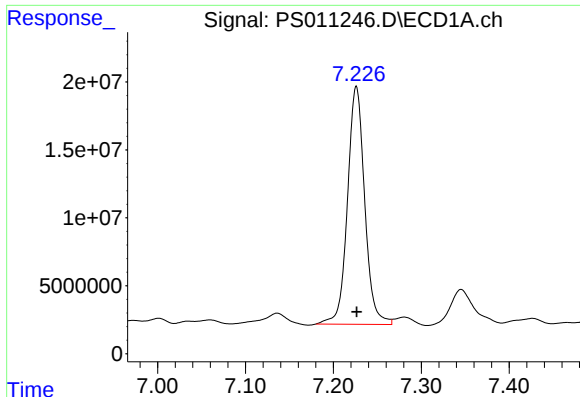

#4 2,4-DCAA


R.T.: 7.226 min
Delta R.T.: 0.000 min
Response: 238178994
Conc: 245.46 ng/ml

Instrument :
ECD_S
ClientSampleId :

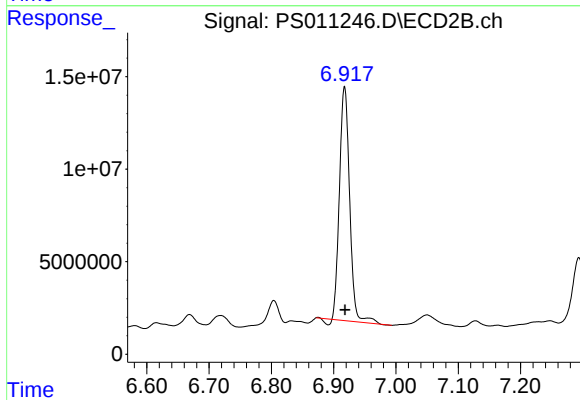


#4 2,4-DCAA

R.T.: 6.918 min
Delta R.T.: 0.000 min
Response: 142439827
Conc: 252.99 ng/ml

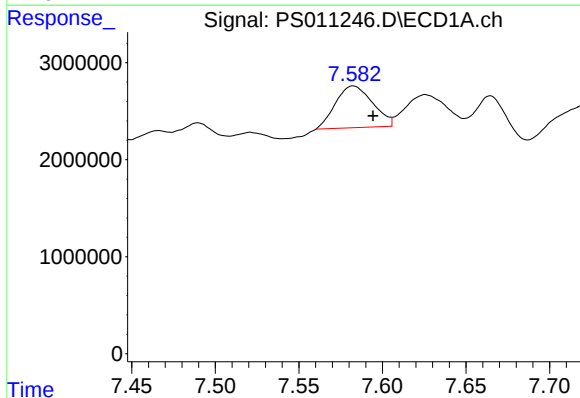


#6 MCP

R.T.: 7.583 min
Delta R.T.: -0.012 min
Response: 6653073
Conc: 2.20 ug/ml

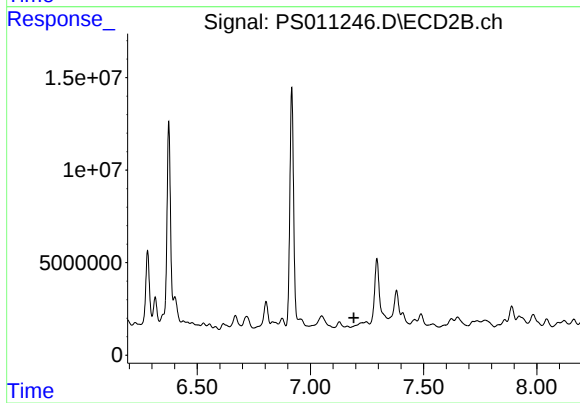

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.192 min
Response: 0
Conc: N.D.

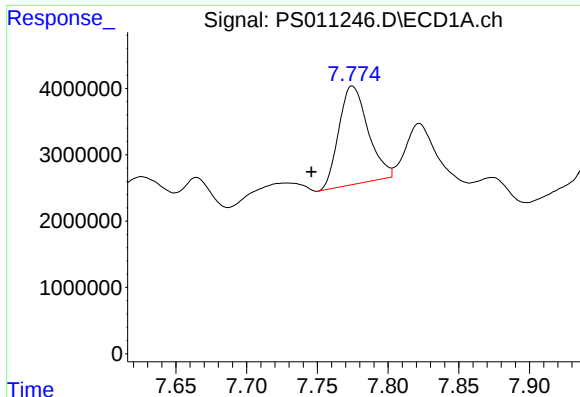

#7 MCPA


R.T.: 7.775 min
Delta R.T.: 0.029 min
Response: 21340949
Conc: 5.00 ug/ml

Instrument :
ECD_S
ClientSampleId :

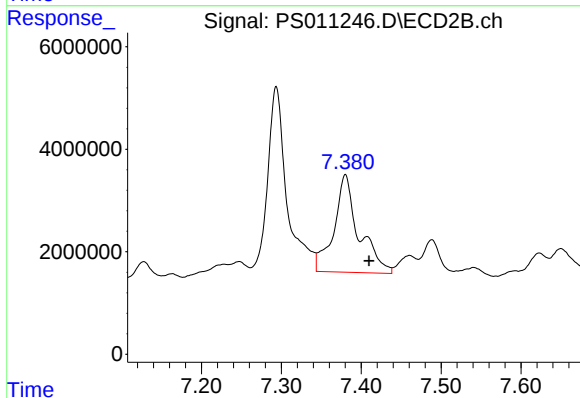


#7 MCPA

R.T.: 7.380 min
Delta R.T.: -0.030 min
Response: 41193957
Conc: 14.29 ug/ml

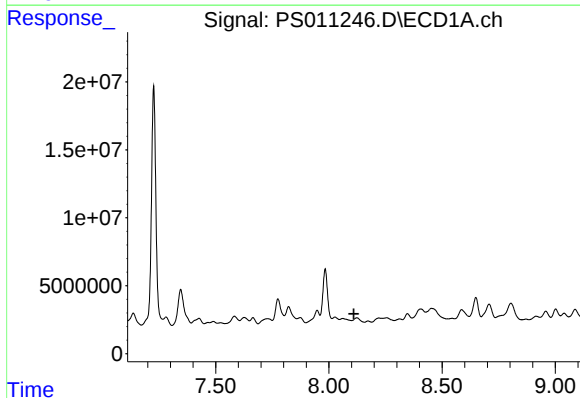


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.110 min
Response: 0
Conc: N.D.

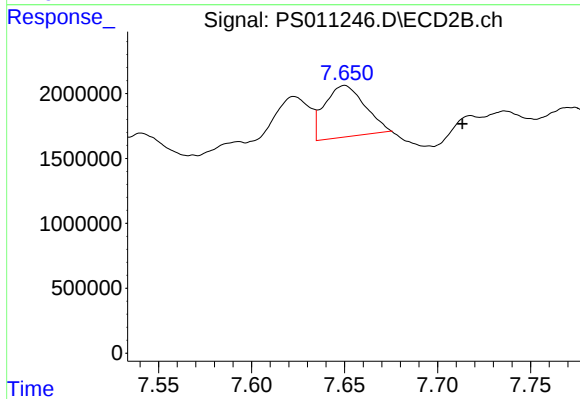

#8 DICHLORPROP


R.T.: 7.650 min
Delta R.T.: -0.063 min
Response: 5935996
Conc: 9.86 ng/ml

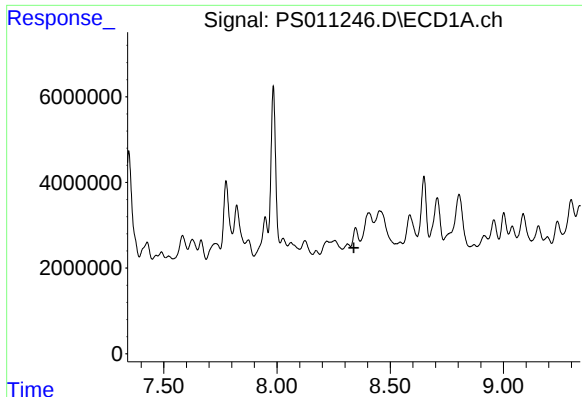

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.339 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

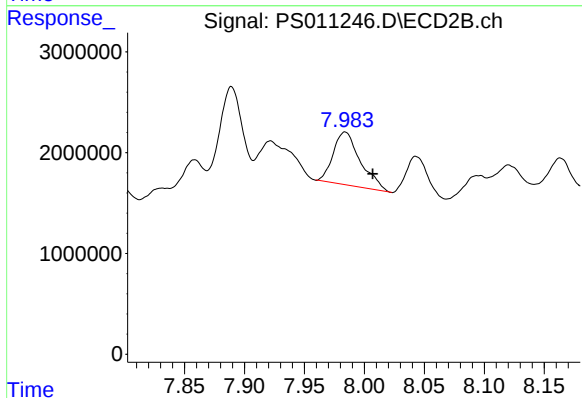


#9 2,4-D

R.T.: 7.984 min
Delta R.T.: -0.023 min
Response: 8254506
Conc: 11.01 ng/ml

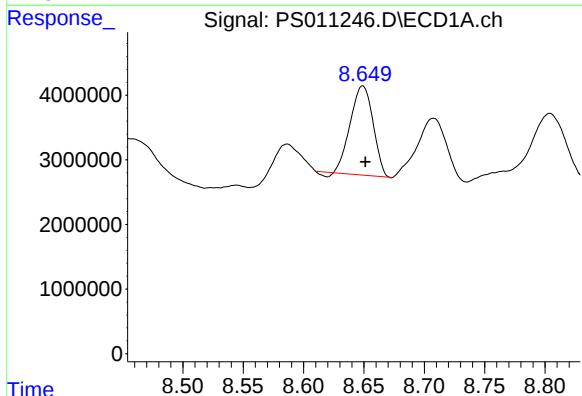


#10 Pentachlorophenol

R.T.: 8.649 min
Delta R.T.: -0.002 min
Response: 17880002
Conc: 1.35 ng/ml

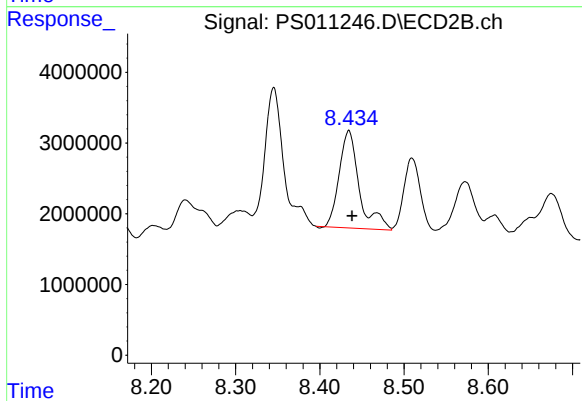

#10 Pentachlorophenol


R.T.: 8.434 min
Delta R.T.: -0.004 min
Response: 22762288
Conc: 3.27 ng/ml

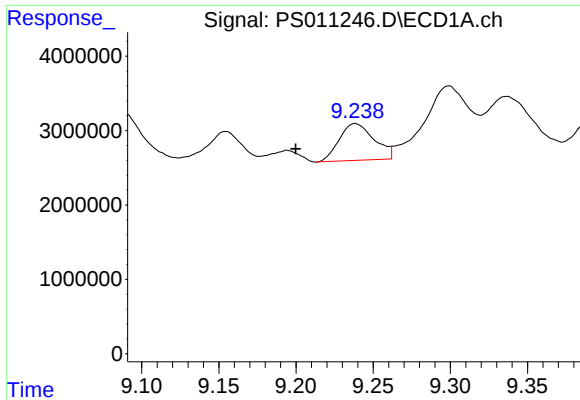

#11 2,4,5-TP (SILVEX)


R.T.: 9.239 min
Delta R.T.: 0.039 min
Response: 7811148
Conc: 1.47 ng/ml

Instrument :
ECD_S
ClientSampleId :

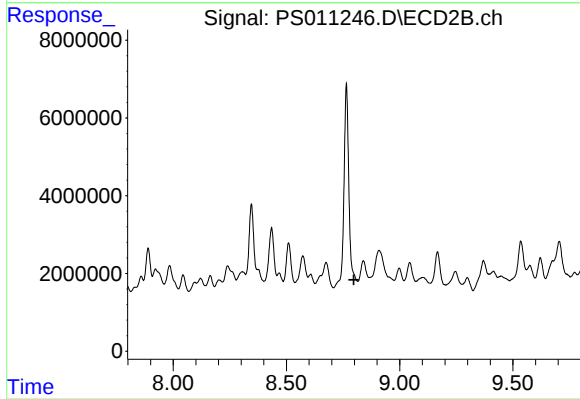


#11 2,4,5-TP (SILVEX)

R.T.: 8.840 min
Delta R.T.: 0.042 min
Response: -3357791
Conc: N.D.

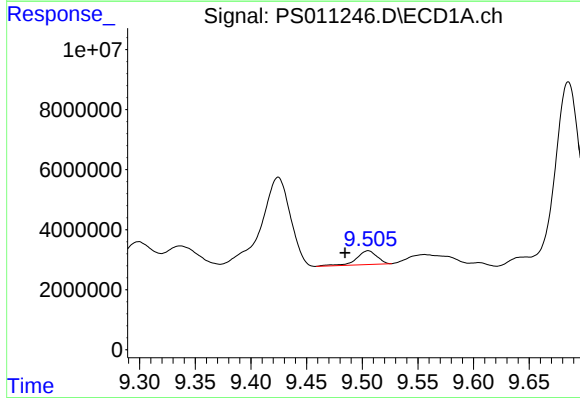


#12 2,4,5-T

R.T.: 9.505 min
Delta R.T.: 0.021 min
Response: 5822015
Conc: 1.15 ng/ml

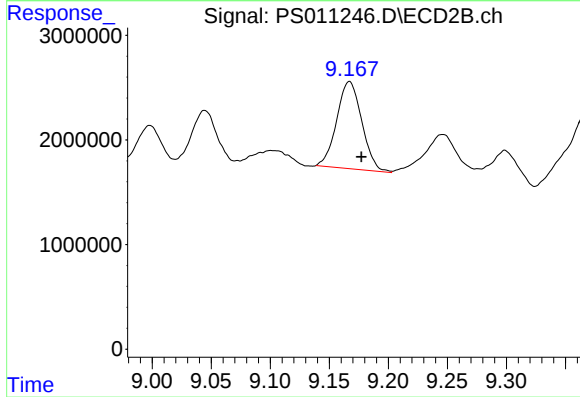

#12 2,4,5-T


R.T.: 9.167 min
Delta R.T.: -0.010 min
Response: 12305745
Conc: 4.06 ng/ml

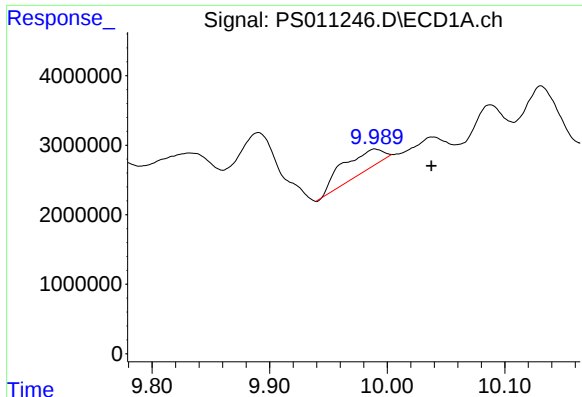

#13 2,4-DB


R.T.: 9.990 min
Delta R.T.: -0.048 min
Response: 7167319
Conc: 11.12 ng/ml

Instrument :
ECD_S
ClientSampleId :

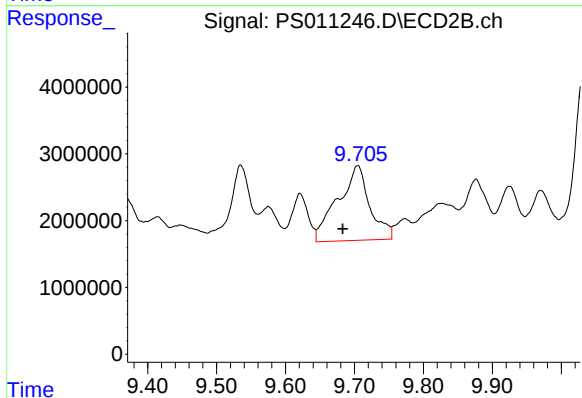


#13 2,4-DB

R.T.: 9.705 min
Delta R.T.: 0.022 min
Response: 36145921
Conc: 84.55 ng/ml

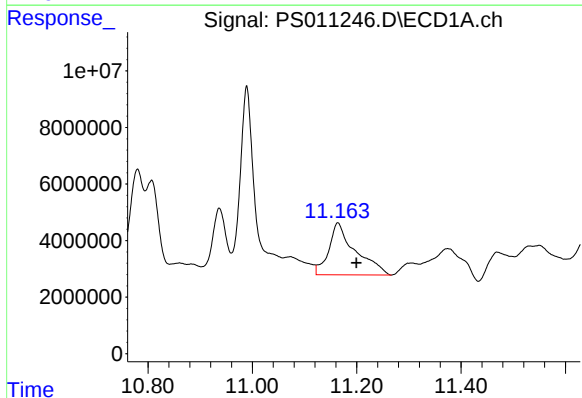


#14 DINOSEB

R.T.: 11.164 min
Delta R.T.: -0.035 min
Response: 64906228
Conc: 16.84 ng/ml

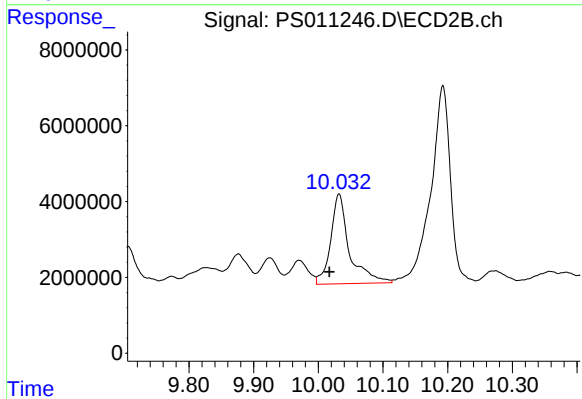

#14 DINOSEB


R.T.: 10.032 min
Delta R.T.: 0.015 min
Response: 47697164
Conc: 22.24 ng/ml

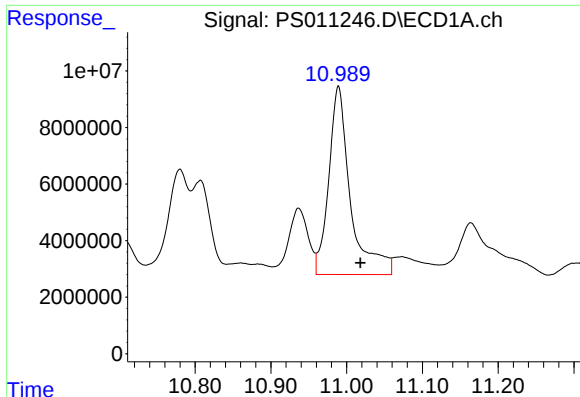

#15 Picloram


R.T.: 10.989 min
Delta R.T.: -0.029 min
Response: 132705730
Conc: 21.03 ng/ml

Instrument :
ECD_S
ClientSampleId :

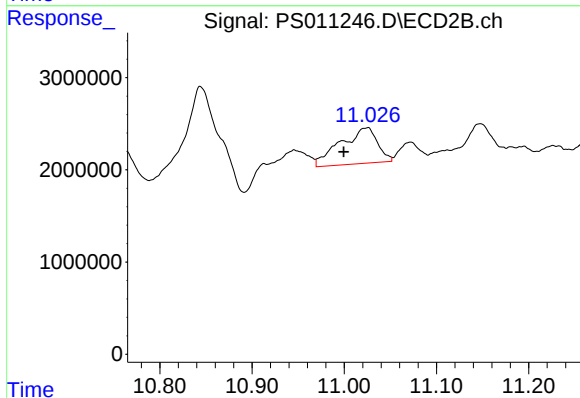


#15 Picloram

R.T.: 11.024 min
Delta R.T.: 0.024 min
Response: 10848649
Conc: 2.48 ng/ml

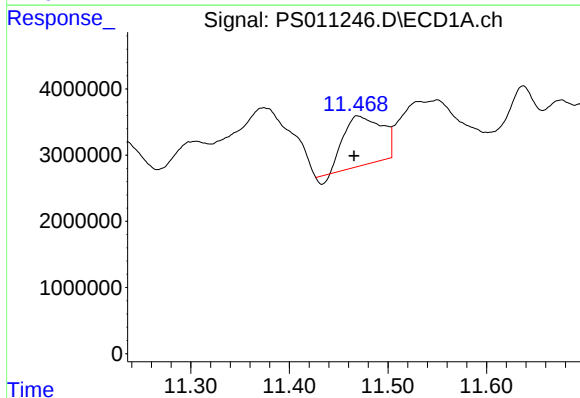

#16 DCPA

R.T.: 11.470 min
Delta R.T.: 0.005 min
Response: 19586415
Conc: 3.04 ng/ml

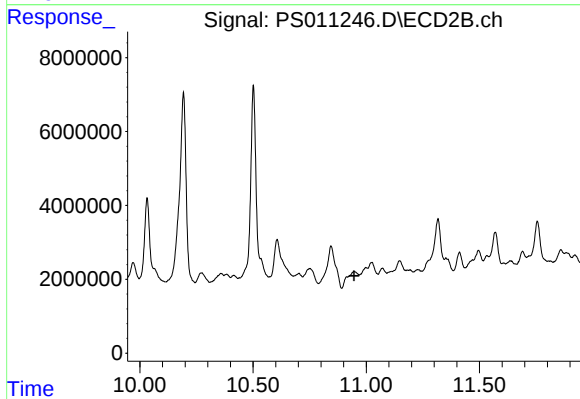

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 10.946 min
Response: 0
Conc: N.D.