

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071620\
 Data File : PS011256.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Jul 2020 20:18
 Operator : DD\AJ
 Sample : PB130250BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 17 02:18:29 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071320.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 13 16:10:29 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.225	6.916	599.5E6	386.6E6	617.776	686.655
Target Compounds							
1) T	Dalapon	2.994	2.584	62458879	246.7E6	51.903	321.409 #
2) T	3,5-DICHL...	0.000	6.098	0	56965971	N.D.	67.829
3) T	4-Nitroph...	7.000	0.000	10784948	0	24.464	N.D. #
6) T	MCP	7.580	0.000	7150378	0	2.361	N.D. #
7) T	MCPA	7.773	7.380	22800767	24219003	5.346	8.403 #
9) T	2,4-D	0.000	7.982	0	10739425	N.D.	14.326
10) T	Pentachlo...	8.704	0.000	23283250	0	1.761	N.D. #
12) T	2,4,5-T	9.504	0.000	12612294	0	2.500	N.D. #
13) T	2,4-DB	9.991	0.000	18874033	0	29.283	N.D. #
14) T	DINOSEB	11.161	10.032	60100160	16737249	15.592	7.803 #
15) T	Picloram	10.988	0.000	301.1E6	0	47.711	N.D. #
16) T	DCPA	11.532	0.000	18916479	0	2.936	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071620\
Data File : PS011256.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Jul 2020 20:18
Operator : DD\AJ
Sample : PB130250BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 17 02:18:29 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071320.M
Quant Title : 8080.M
QLast Update : Mon Jul 13 16:10:29 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

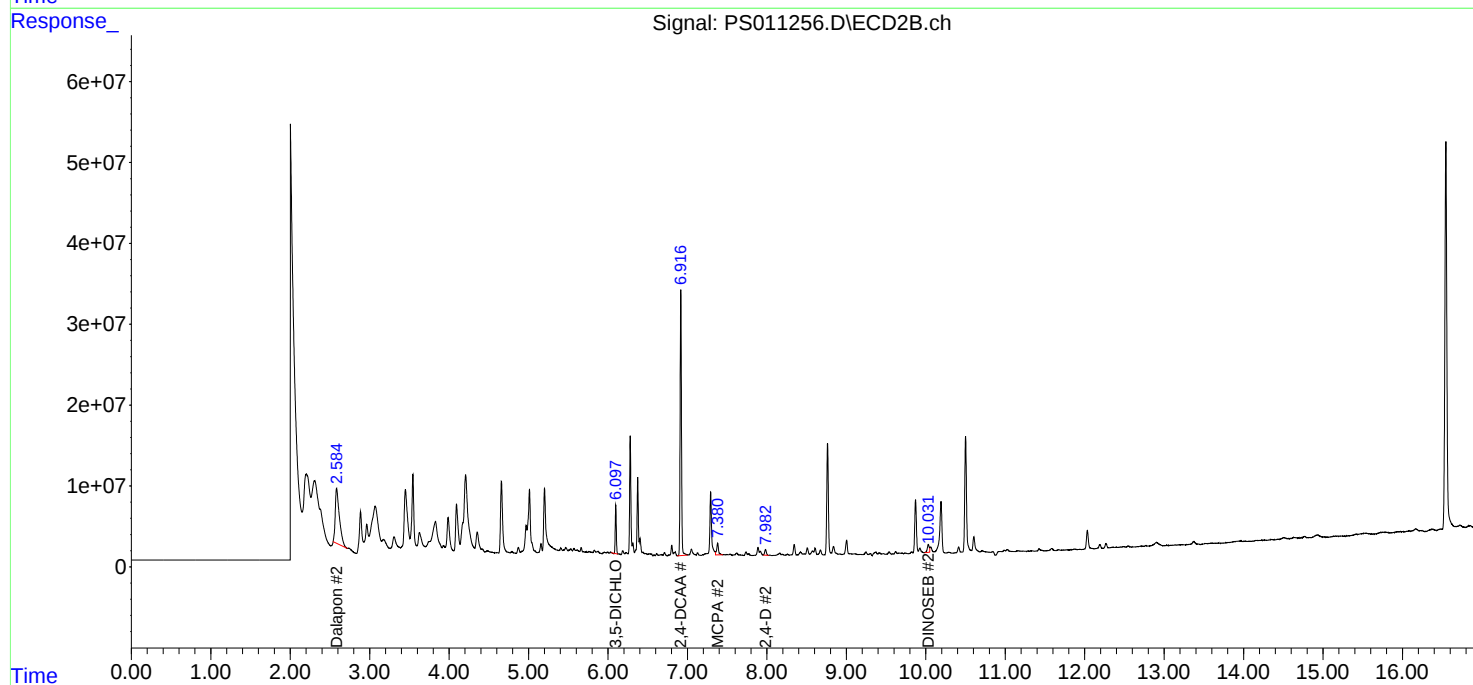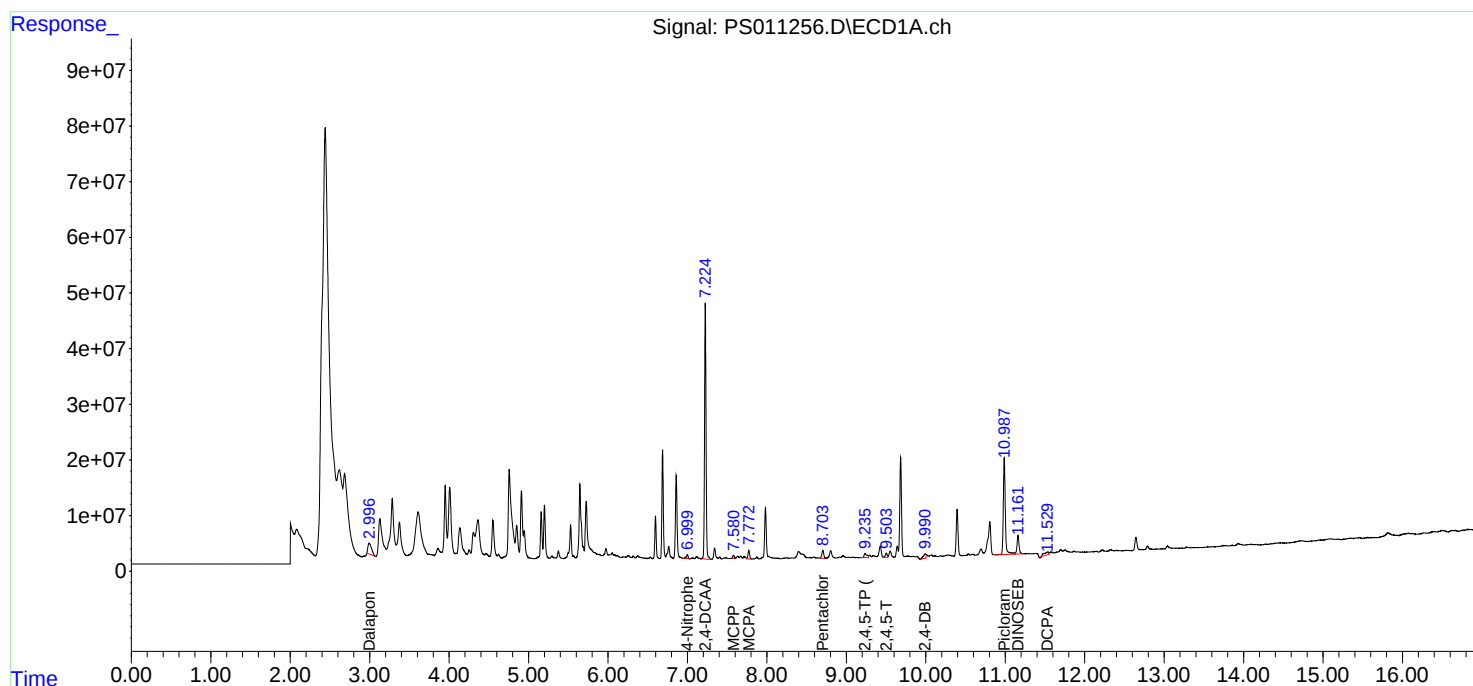


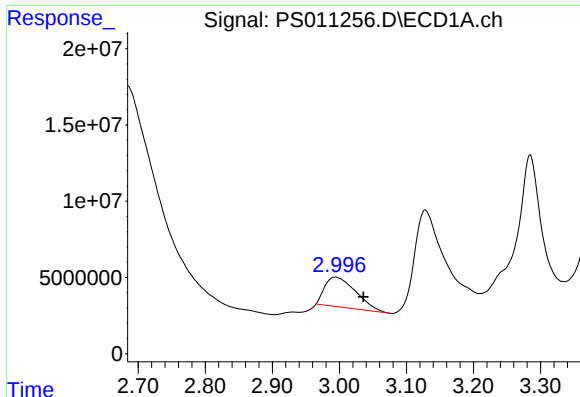

#1 Dalapon


R.T.: 2.994 min
Delta R.T.: -0.042 min
Response: 62458879
Conc: 51.90 ng/ml

Instrument :
ECD_S
ClientSampleId :

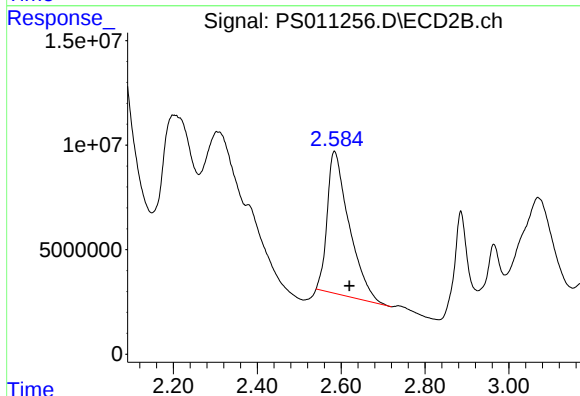


#1 Dalapon

R.T.: 2.584 min
Delta R.T.: -0.036 min
Response: 246736408
Conc: 321.41 ng/ml

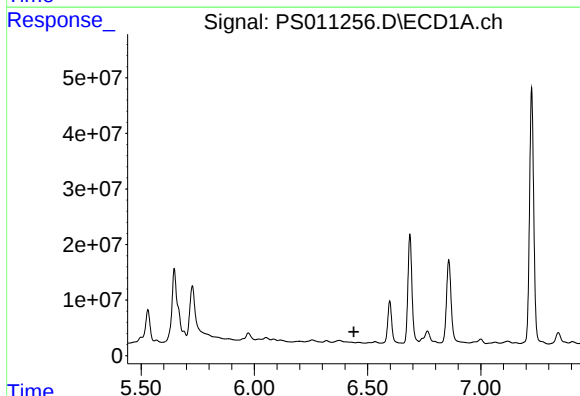


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.439 min
Response: 0
Conc: N.D.

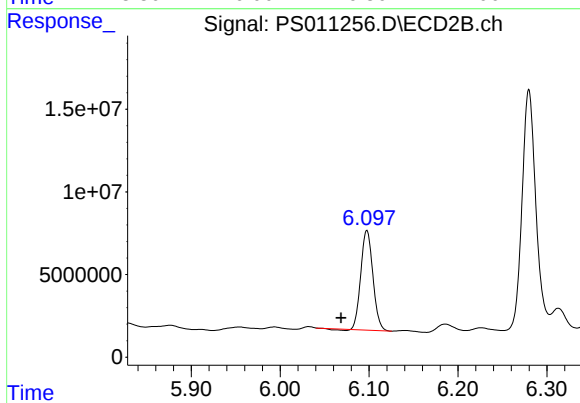

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.098 min
Delta R.T.: 0.029 min
Response: 56965971
Conc: 67.83 ng/ml

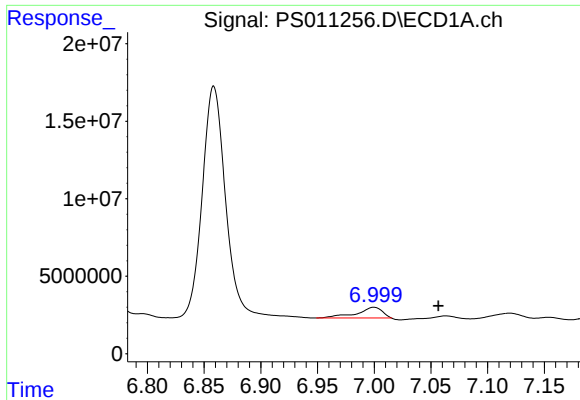

#3 4-Nitrophenol


R.T.: 7.000 min
Delta R.T.: -0.057 min
Response: 10784948
Conc: 24.46 ng/ml

Instrument :
ECD_S
ClientSampleId :

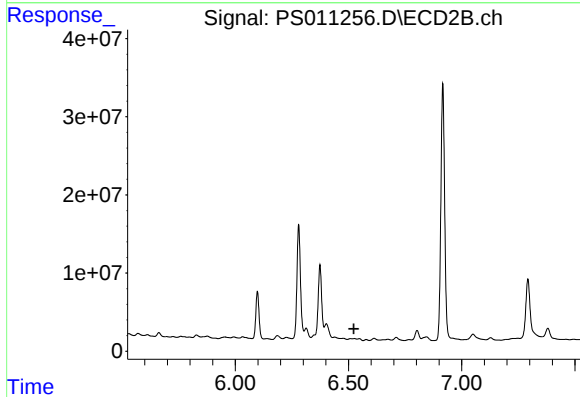


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.524 min
Response: 0
Conc: N.D.

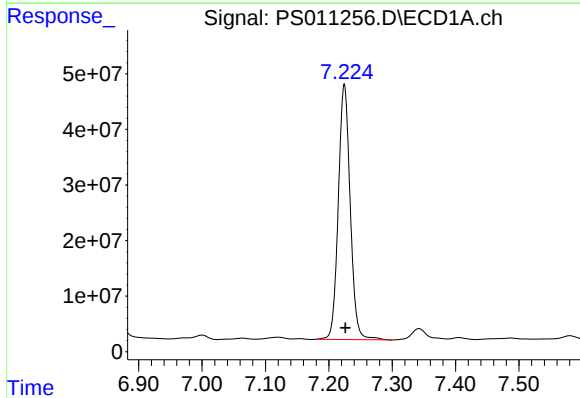


#4 2,4-DCAA

R.T.: 7.225 min
Delta R.T.: -0.002 min
Response: 599451467
Conc: 617.78 ng/ml

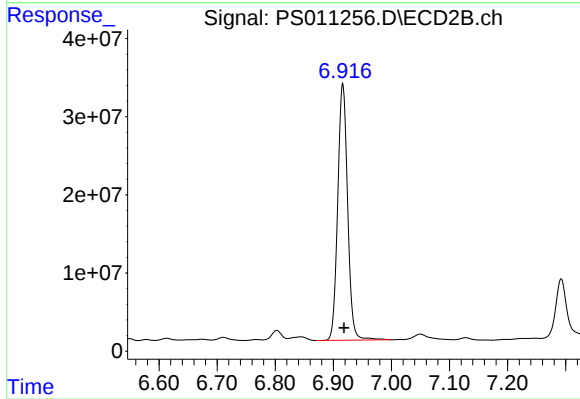

#4 2,4-DCAA


R.T.: 6.916 min
Delta R.T.: -0.002 min
Response: 386601943
Conc: 686.65 ng/ml

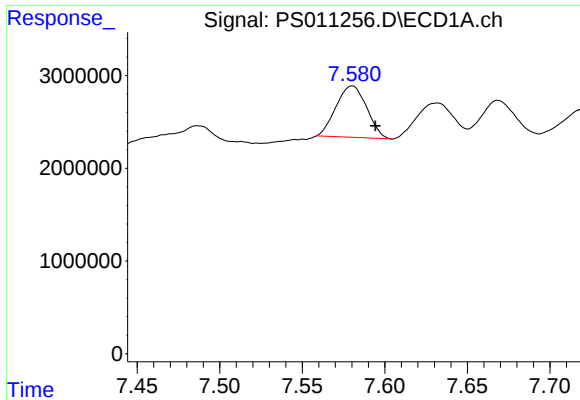

#6 MCPP


R.T.: 7.580 min
Delta R.T.: -0.014 min
Response: 7150378
Conc: 2.36 ug/ml

Instrument :
ECD_S
ClientSampleId :

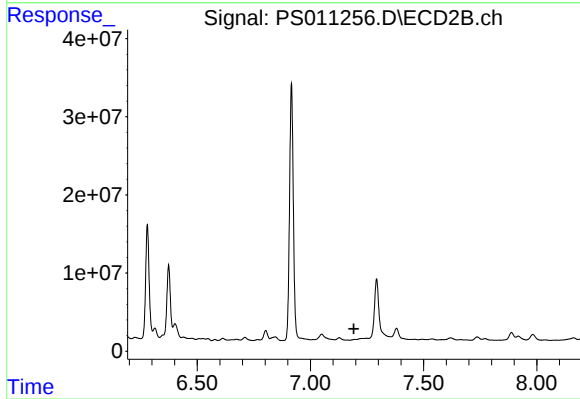


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 7.192 min
Response: 0
Conc: N.D.

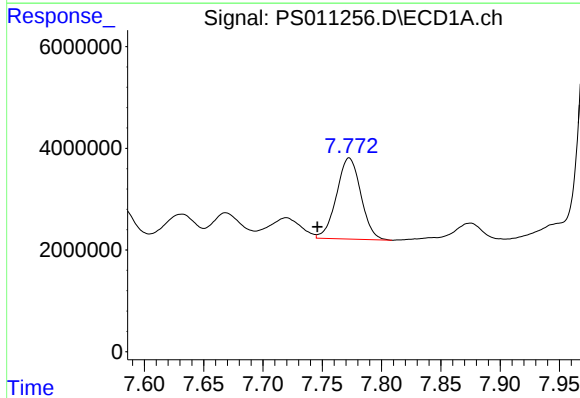


#7 MCPA

R.T.: 7.773 min
Delta R.T.: 0.027 min
Response: 22800767
Conc: 5.35 ug/ml

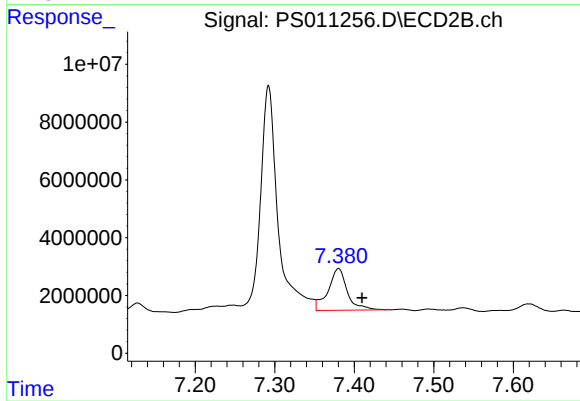

#7 MCPA


R.T.: 7.380 min
Delta R.T.: -0.030 min
Response: 24219003
Conc: 8.40 ug/ml

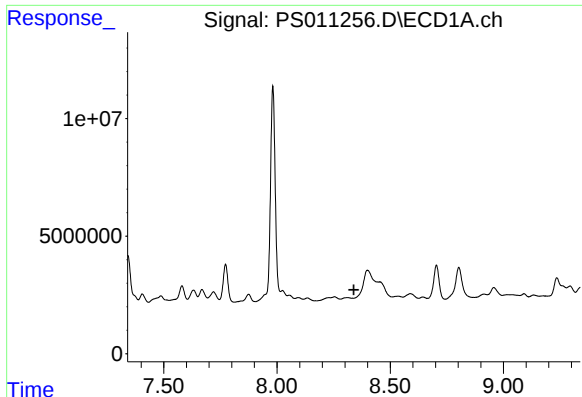

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.339 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

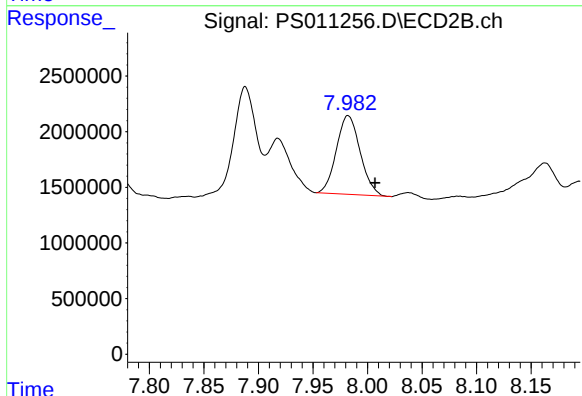


#9 2,4-D

R.T.: 7.982 min
Delta R.T.: -0.025 min
Response: 10739425
Conc: 14.33 ng/ml

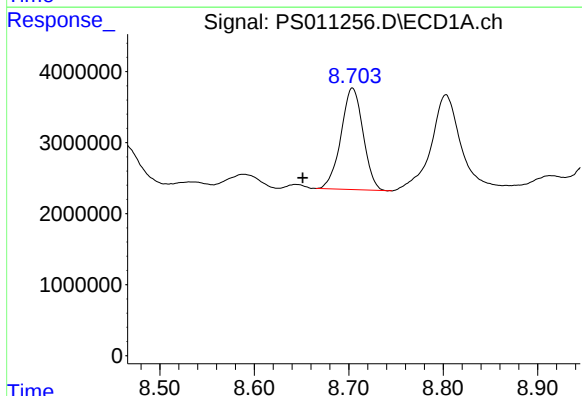


#10 Pentachlorophenol

R.T.: 8.704 min
Delta R.T.: 0.053 min
Response: 23283250
Conc: 1.76 ng/ml

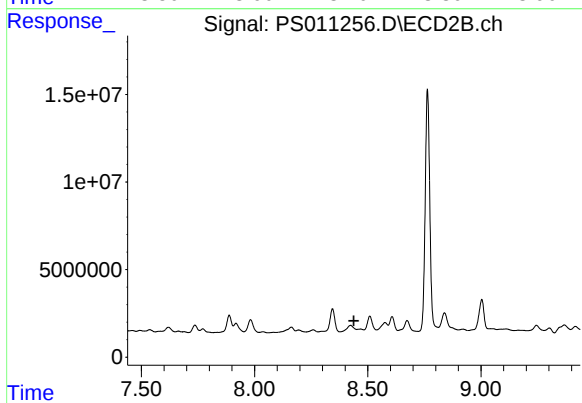

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 8.438 min
Response: 0
Conc: N.D.

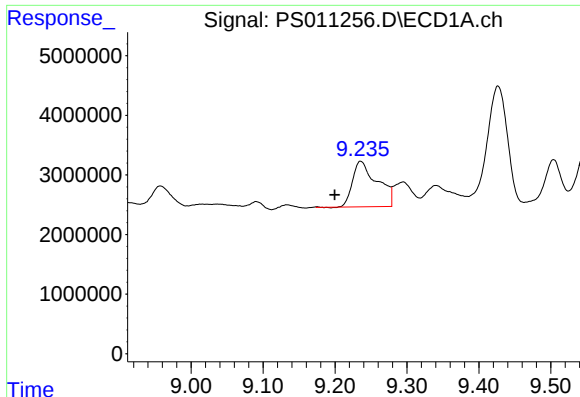

#11 2,4,5-TP (SILVEX)


R.T.: 9.236 min
Delta R.T.: 0.036 min
Response: 18134768
Conc: 3.42 ng/ml

Instrument :
ECD_S
ClientSampleId :

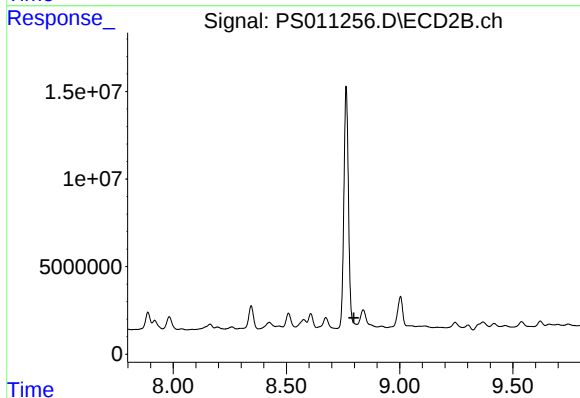


#11 2,4,5-TP (SILVEX)

R.T.: 8.839 min
Delta R.T.: 0.041 min
Response: -26786894
Conc: N.D.

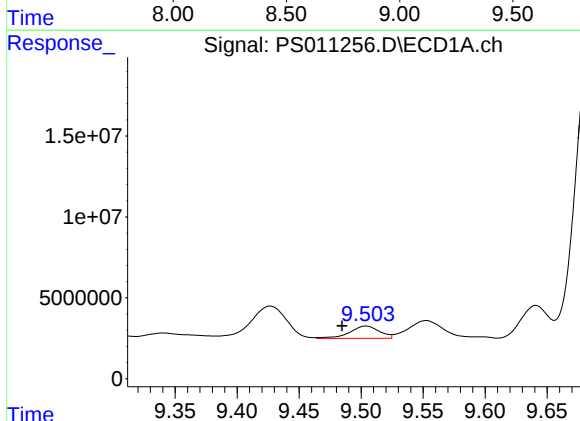


#12 2,4,5-T

R.T.: 9.504 min
Delta R.T.: 0.019 min
Response: 12612294
Conc: 2.50 ng/ml

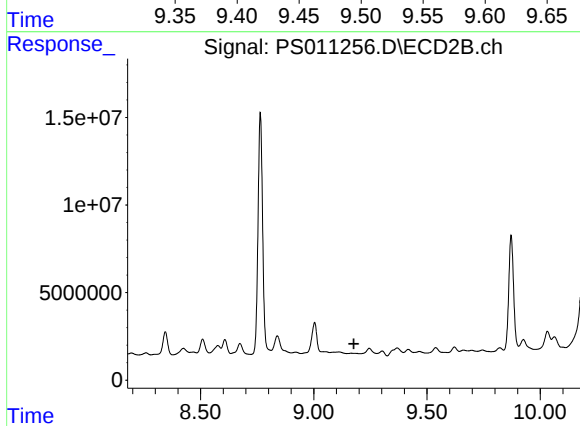

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.177 min
Response: 0
Conc: N.D.

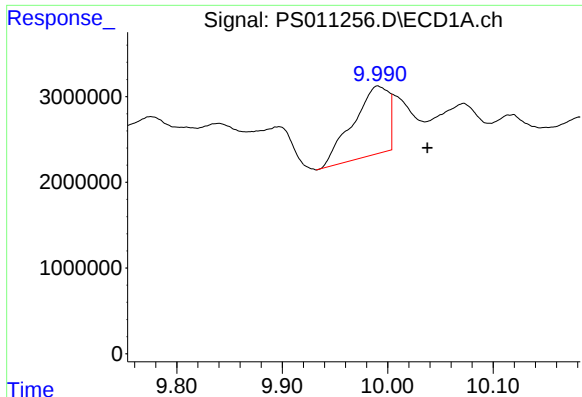

#13 2,4-DB


R.T.: 9.991 min
Delta R.T.: -0.047 min
Response: 18874033
Conc: 29.28 ng/ml

Instrument :
ECD_S
ClientSampleId :

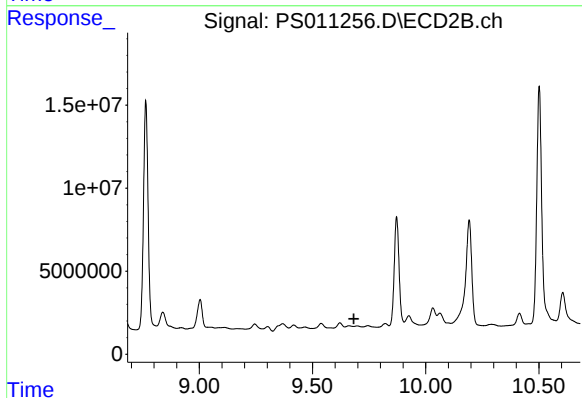


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.683 min
Response: 0
Conc: N.D.

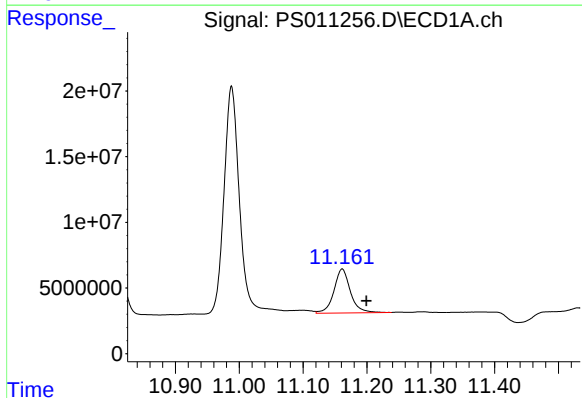


#14 DINOSEB

R.T.: 11.161 min
Delta R.T.: -0.038 min
Response: 60100160
Conc: 15.59 ng/ml

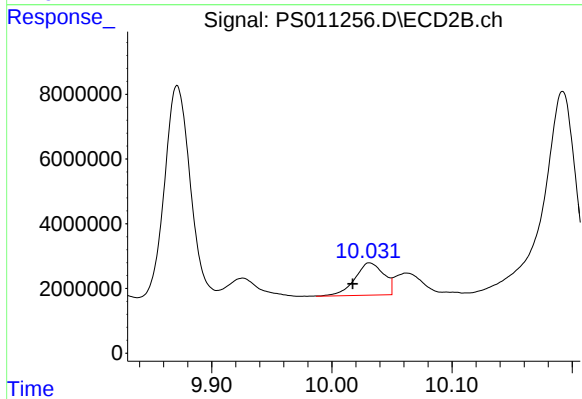

#14 DINOSEB


R.T.: 10.032 min
Delta R.T.: 0.015 min
Response: 16737249
Conc: 7.80 ng/ml

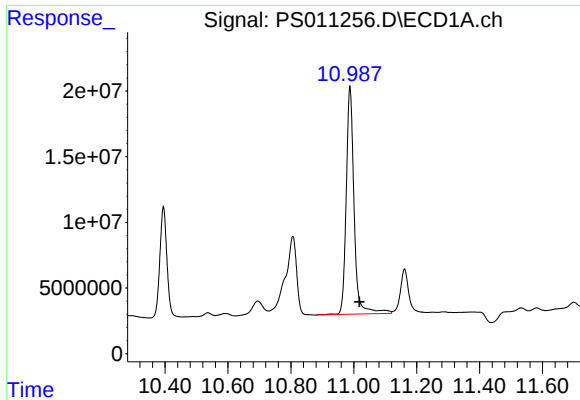

#15 Picloram


R.T.: 10.988 min
Delta R.T.: -0.030 min
Response: 301052493
Conc: 47.71 ng/ml

Instrument :
ECD_S
ClientSampleId :

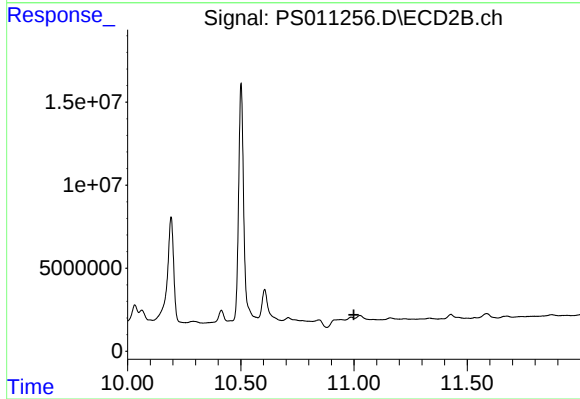


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 10.999 min
Response: 0
Conc: N.D.

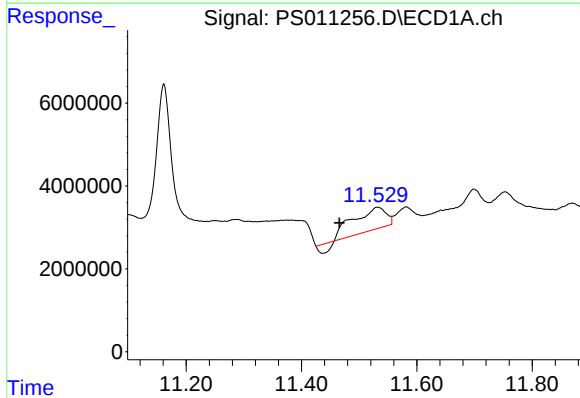

#16 DCPA

R.T.: 11.532 min
Delta R.T.: 0.066 min
Response: 18916479
Conc: 2.94 ng/ml

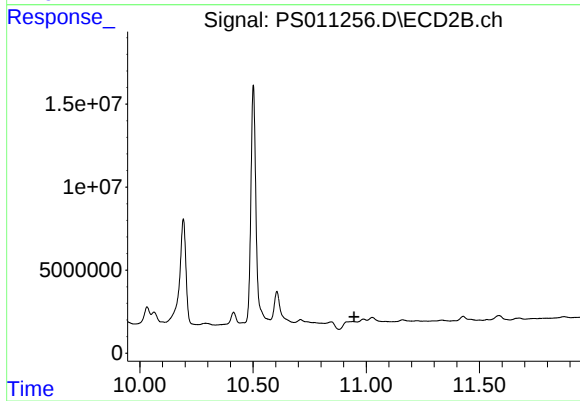

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 10.946 min
Response: 0
Conc: N.D.