

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071718\
 Data File : PS001092.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jul 2018 16:17
 Operator : UA
 Sample : J3545-04RE
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 17 17:10:22 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 09 02:00:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
4) S	2,4-DCAA	11.632	11.047	36552984	31332453	177.166	143.861
Target Compounds							
2) T	3,5-DICHL...	0.000	9.285	0	28266315	N.D.	96.094 #
5) T	DICAMBA	12.017	0.000	1805618	0	2.293	N.D. #
6) T	MCP	12.317	0.000	11806554	0	21.494	N.D. #
15) T	Picloram	17.166	16.986	12891232	11780703	7.118	7.737
16) T	DCPA	0.000	16.986	0	11780703	N.D.	6.853 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071718\
Data File : PS001092.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jul 2018 16:17
Operator : UA
Sample : J3545-04RE
Misc :
ALS Vial : 10 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 17 17:10:22 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
Quant Title : 8080.M
QLast Update : Mon Jul 09 02:00:25 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

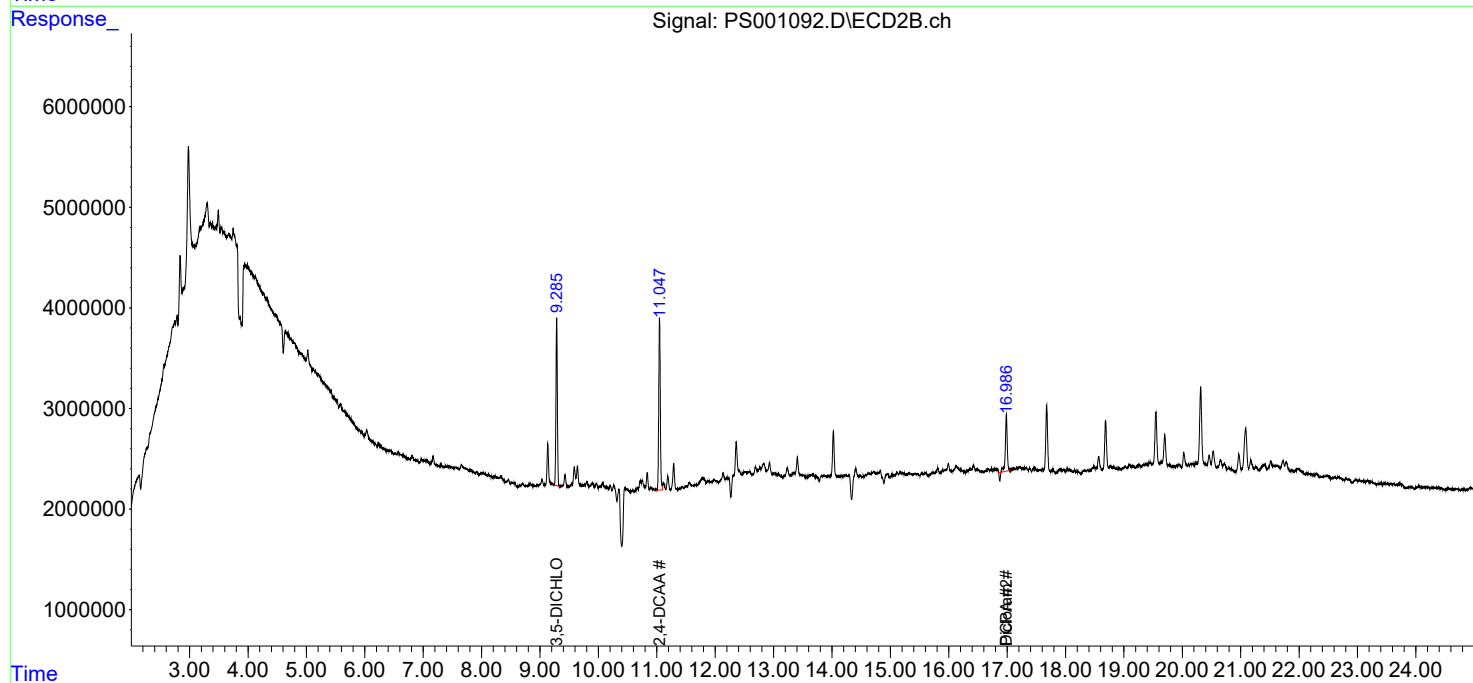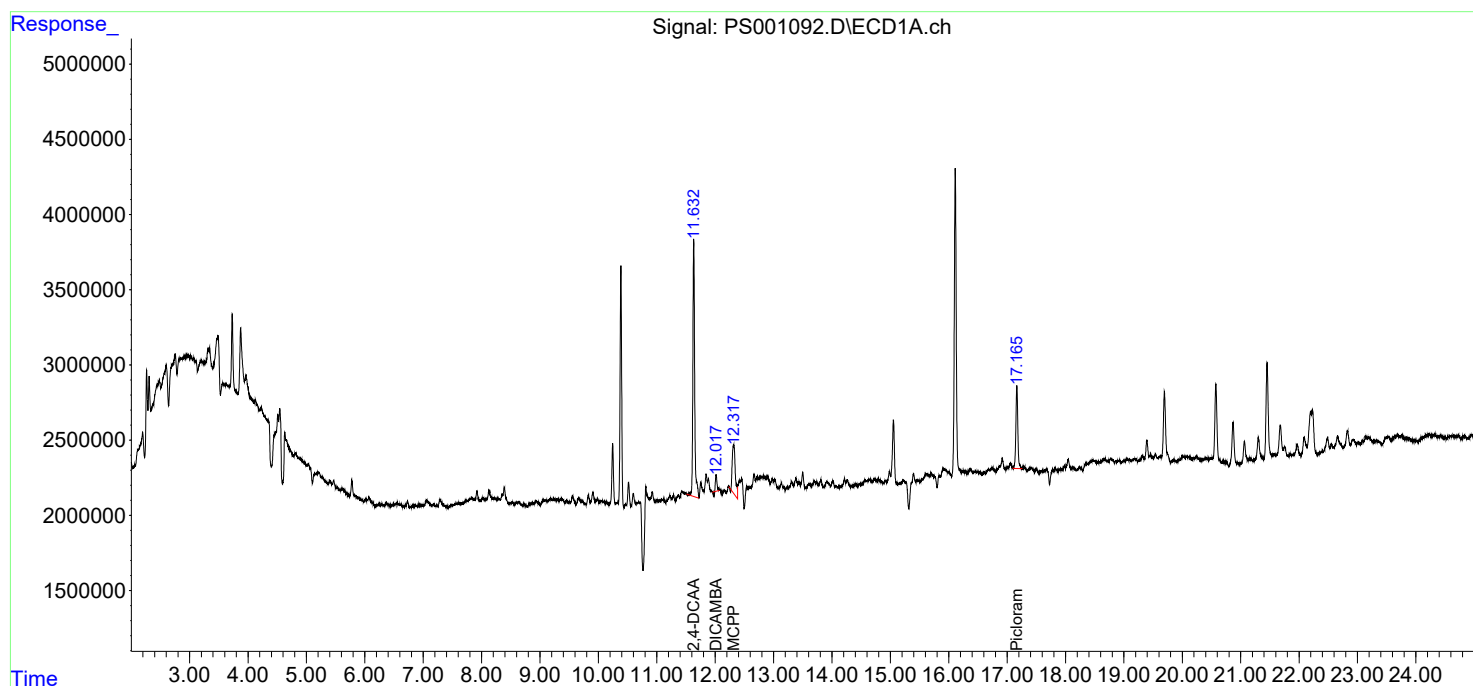

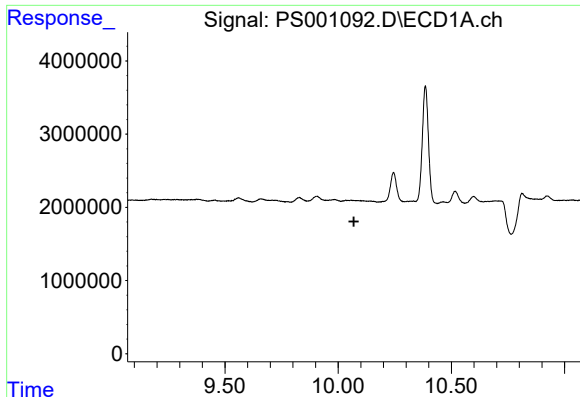


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 10.070 min
Response: 0
Conc: N.D.

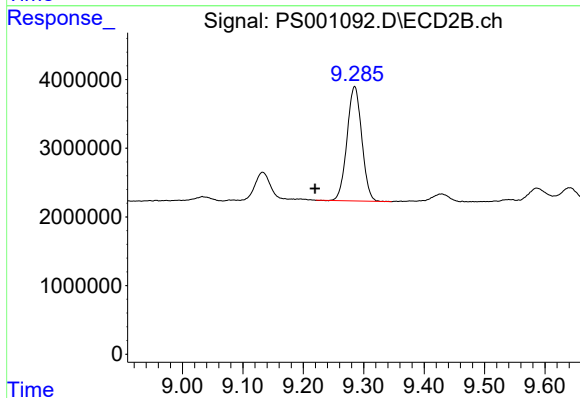


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.285 min
Delta R.T.: 0.066 min
Response: 28266315
Conc: 96.09 ng/ml

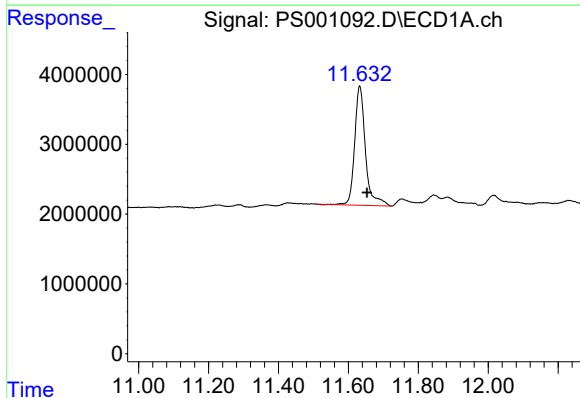


#4 2,4-DCAA

R.T.: 11.632 min
Delta R.T.: -0.021 min
Response: 36552984
Conc: 177.17 ng/ml

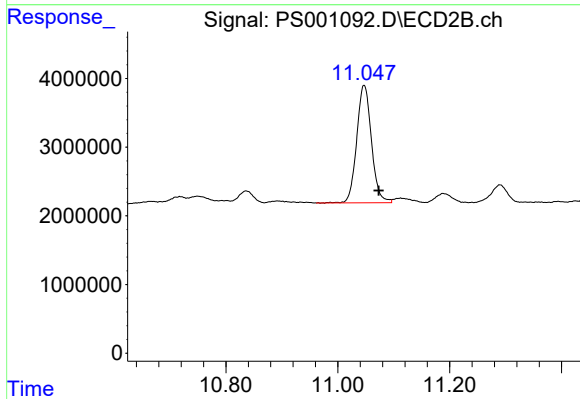


#4 2,4-DCAA

R.T.: 11.047 min
Delta R.T.: -0.027 min
Response: 31332453
Conc: 143.86 ng/ml

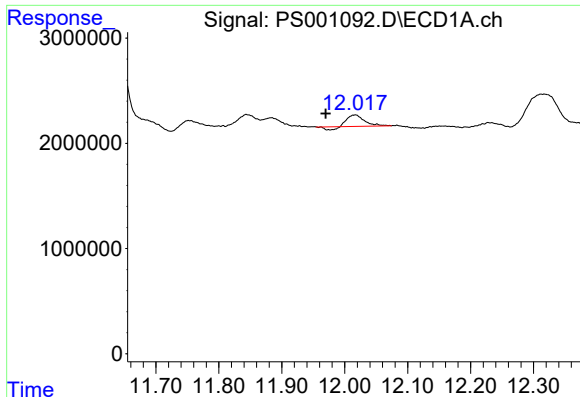


#5 DICAMBA

R.T.: 12.017 min
Delta R.T.: 0.047 min
Response: 1805618
Conc: 2.29 ng/ml

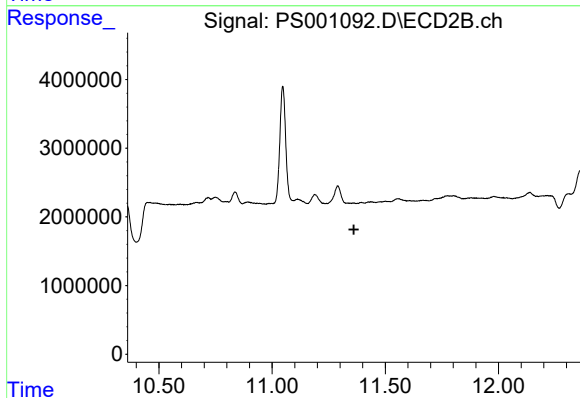


#5 DICAMBA

R.T.: 0.000 min
Exp R.T.: 11.361 min
Response: 0
Conc: N.D.

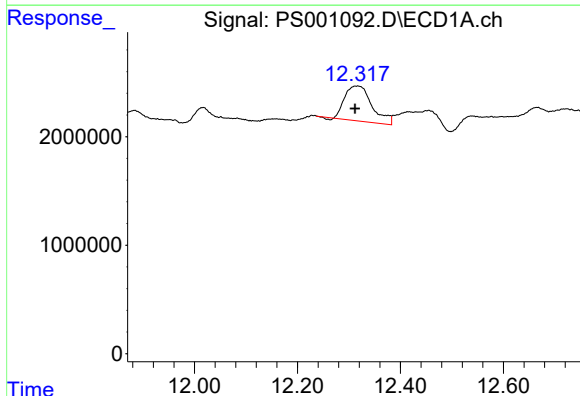


#6 MCP

R.T.: 12.317 min
Delta R.T.: 0.005 min
Response: 11806554
Conc: 21.49 ug/ml

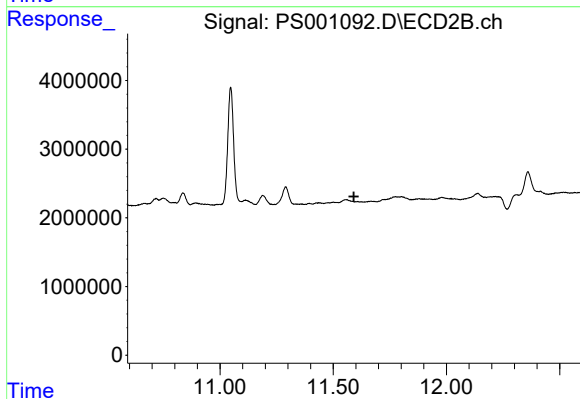


#6 MCP

R.T.: 0.000 min
Exp R.T.: 11.591 min
Response: 0
Conc: N.D.

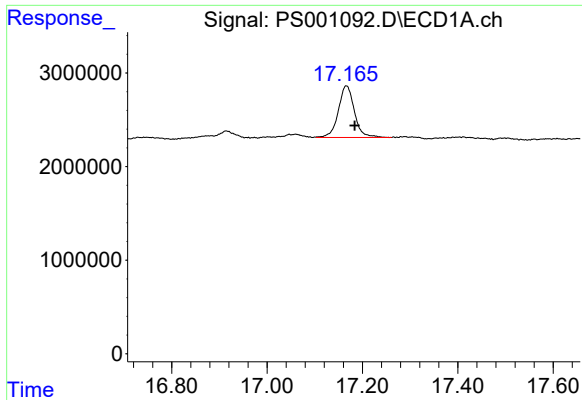


#15 Picloram

R.T.: 17.166 min
Delta R.T.: -0.017 min
Response: 12891232
Conc: 7.12 ng/ml

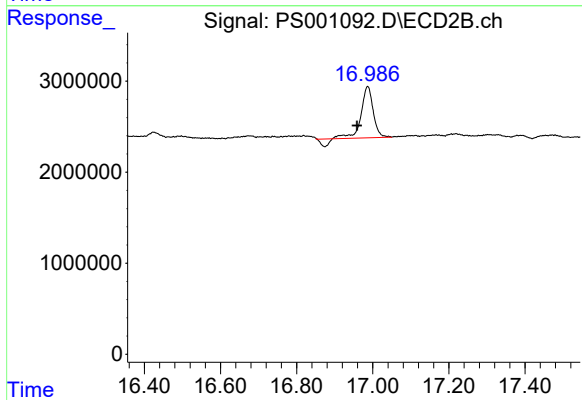


#15 Picloram

R.T.: 16.986 min
Delta R.T.: 0.027 min
Response: 11780703
Conc: 7.74 ng/ml

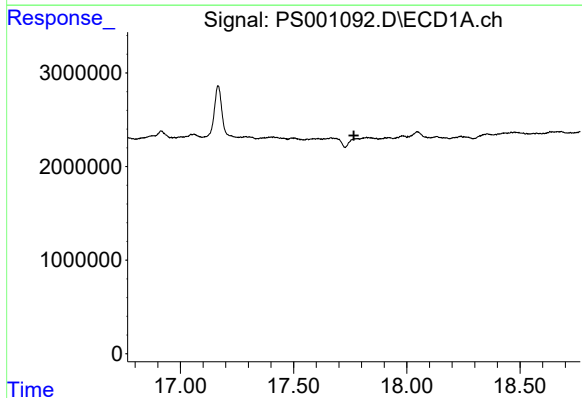

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.766 min
Response: 0
Conc: N.D.

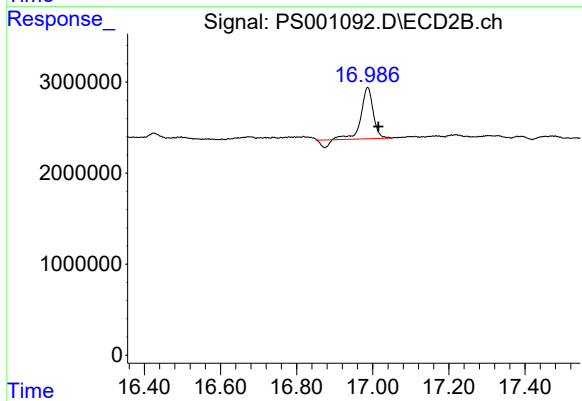

#16 DCPA

R.T.: 16.986 min
Delta R.T.: -0.029 min
Response: 11780703
Conc: 6.85 ng/ml