

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071718\
 Data File : PS001093.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jul 2018 16:48
 Operator : UA
 Sample : J3966-03RE
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 17 18:55:49 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 09 02:00:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
4) S	2,4-DCAA	11.640	11.056	33581555	27081740	162.764	124.344
Target Compounds							
5) T	DICAMBA	0.000	11.300	0	3434692	N.D.	4.376 #
6) T	MCPD	12.314	0.000	7133084	0	12.986	N.D. #
7) T	MCPA	12.596	0.000	1038228	0	1.138	N.D. #
10) T	Pentachlo...	13.898	13.495	2232202	2258928	0.735	0.720
15) T	Picloram	0.000	16.992	0	3827963	N.D.	2.514 #
16) T	DCPA	0.000	16.992	0	3827963	N.D.	2.227 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071718\
Data File : PS001093.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jul 2018 16:48
Operator : UA
Sample : J3966-03RE
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 17 18:55:49 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
Quant Title : 8080.M
QLast Update : Mon Jul 09 02:00:25 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

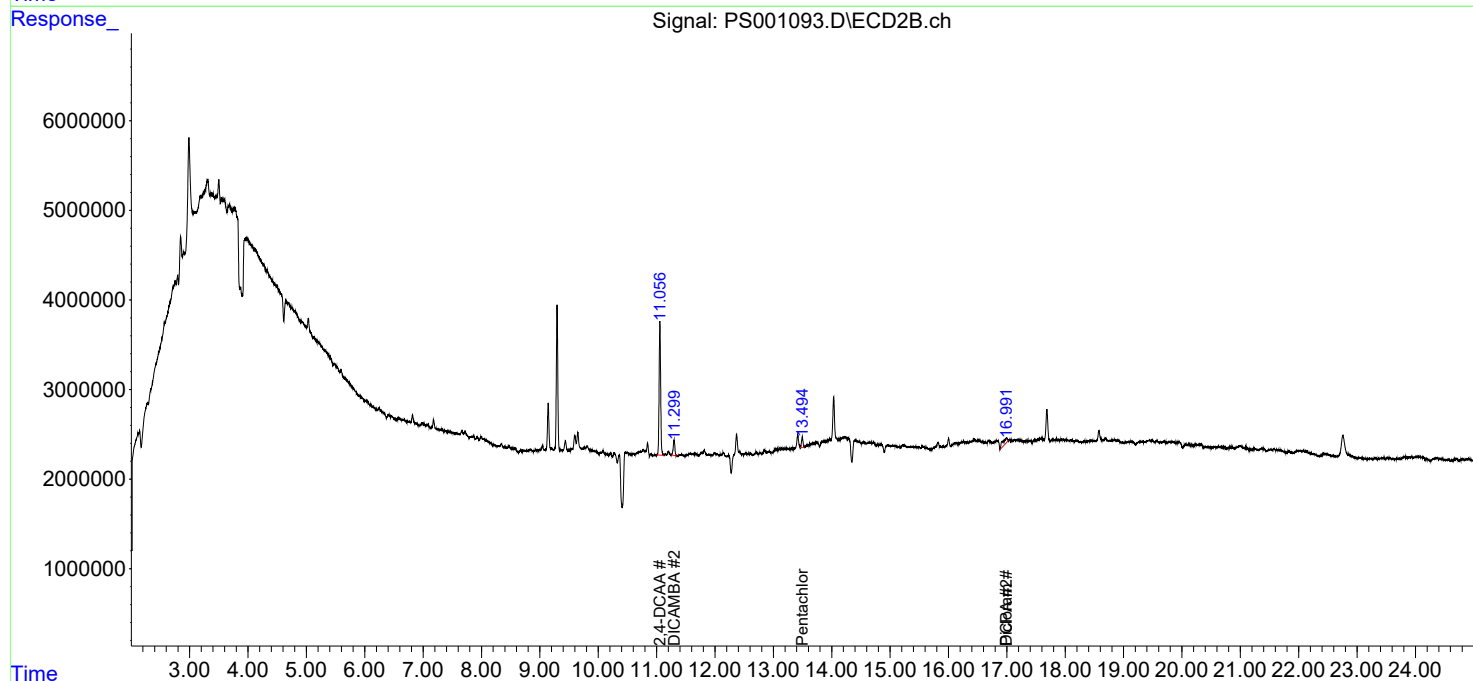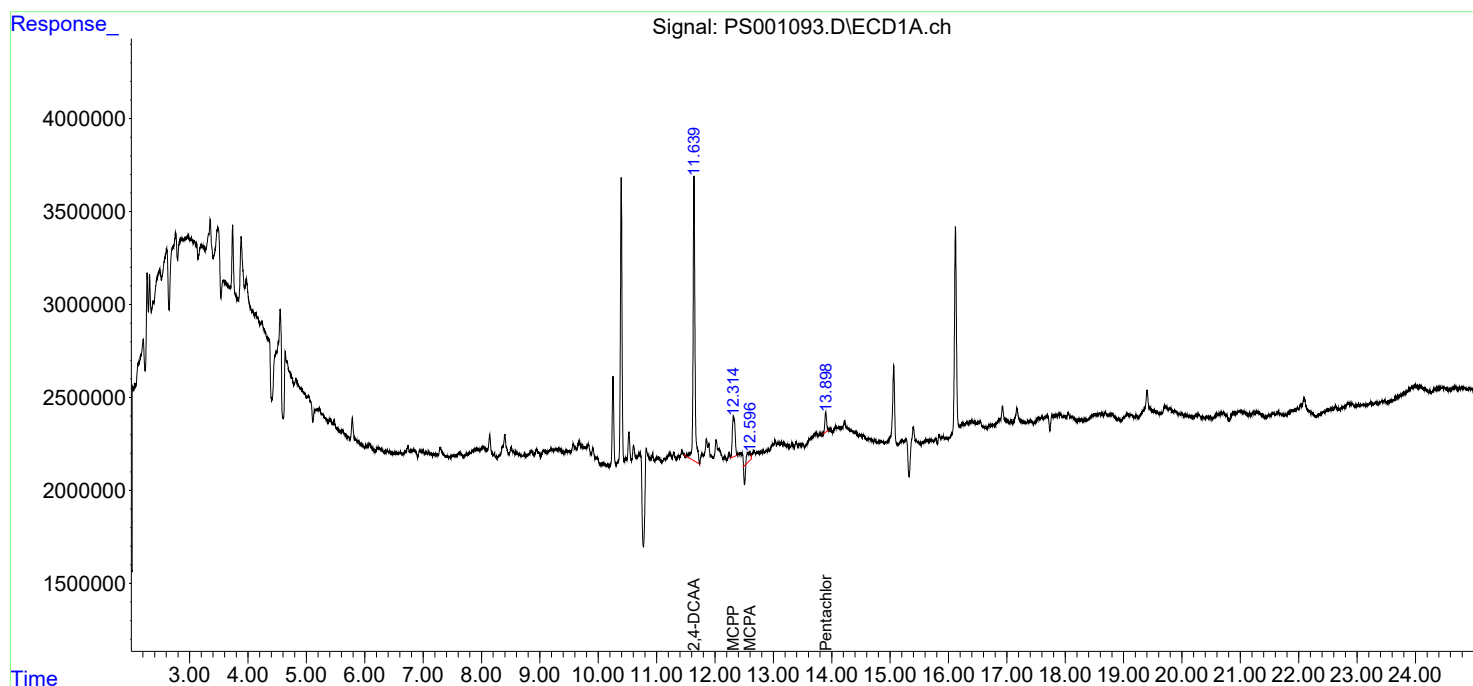

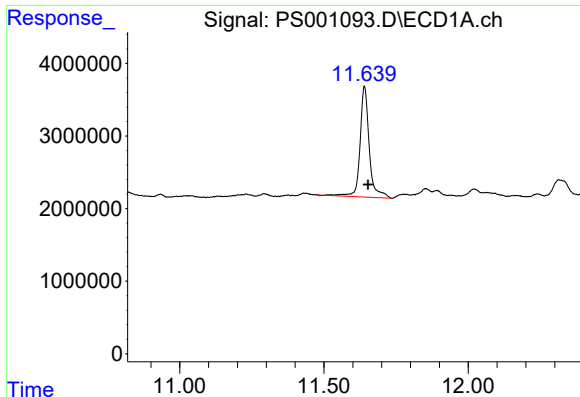


#4 2,4-DCAA

R.T.: 11.640 min
Delta R.T.: -0.013 min
Response: 33581555
Conc: 162.76 ng/ml

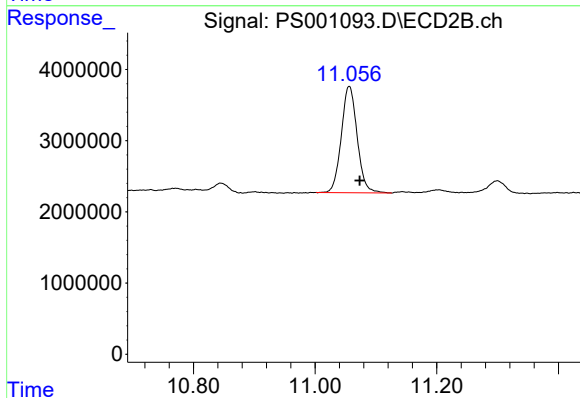


#4 2,4-DCAA

R.T.: 11.056 min
Delta R.T.: -0.017 min
Response: 27081740
Conc: 124.34 ng/ml

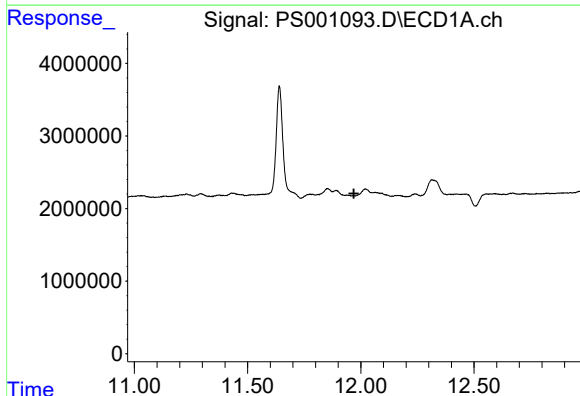


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.970 min
Response: 0
Conc: N.D.

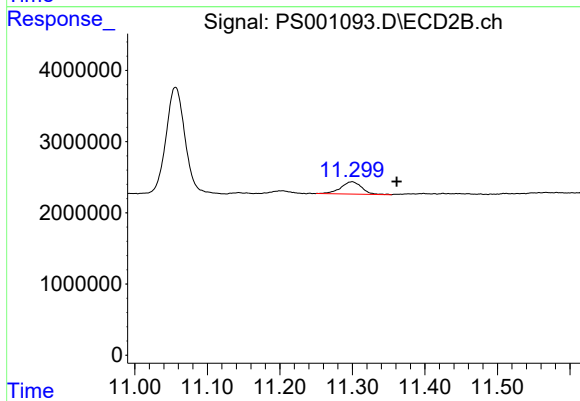


#5 DICAMBA

R.T.: 11.300 min
Delta R.T.: -0.061 min
Response: 3434692
Conc: 4.38 ng/ml

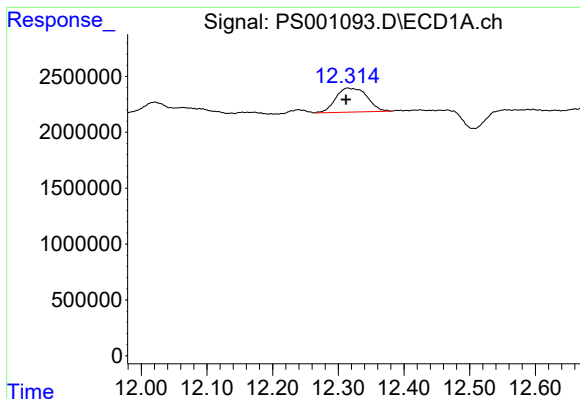


#6 MCPP

R.T.: 12.314 min
Delta R.T.: 0.002 min
Response: 7133084
Conc: 12.99 ug/ml

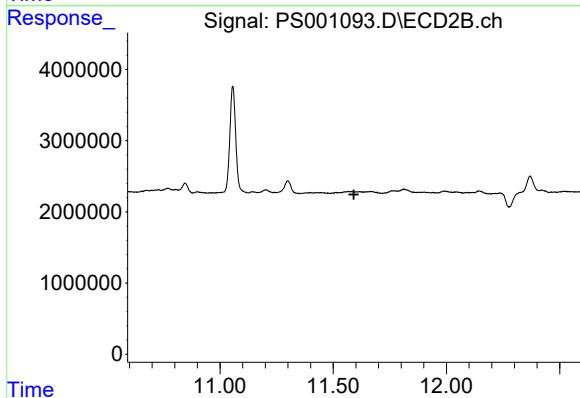


#6 MCPP

R.T.: 0.000 min
Exp R.T.: 11.591 min
Response: 0
Conc: N.D.

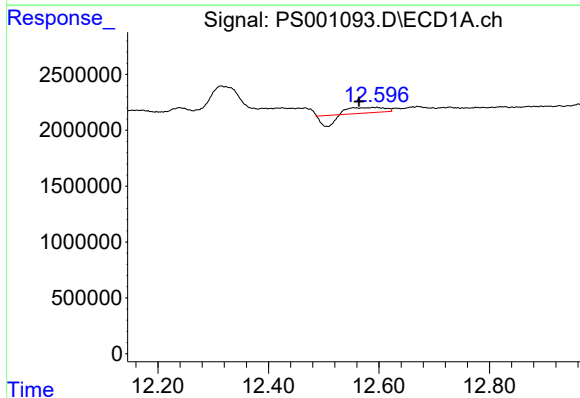


#7 MCPA

R.T.: 12.596 min
Delta R.T.: 0.032 min
Response: 1038228
Conc: 1.14 ug/ml

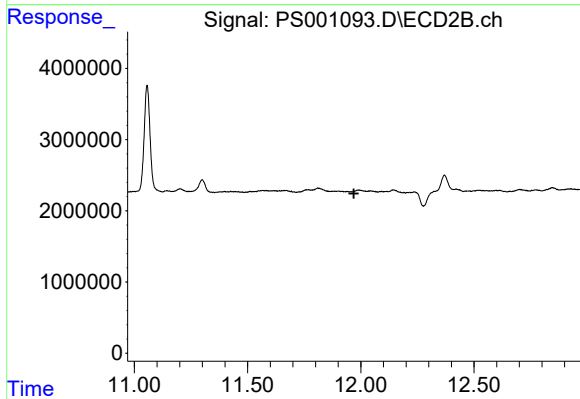


#7 MCPA

R.T.: 0.000 min
Exp R.T.: 11.969 min
Response: 0
Conc: N.D.

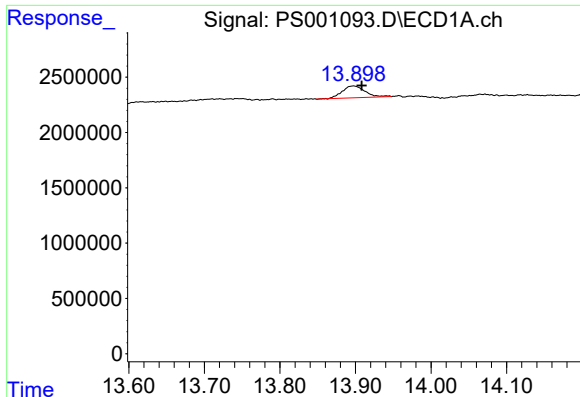


#10 Pentachlorophenol

R.T.: 13.898 min
Delta R.T.: -0.011 min
Response: 2232202
Conc: 0.73 ng/ml

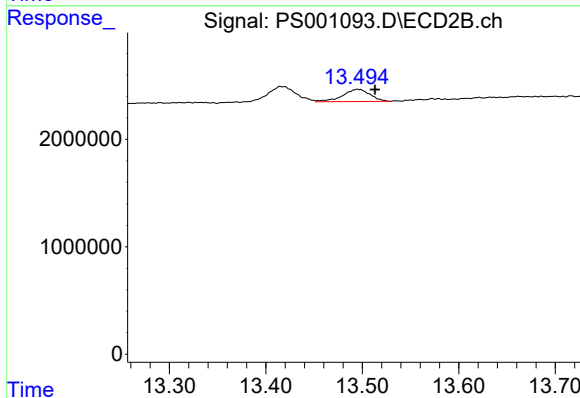


#10 Pentachlorophenol

R.T.: 13.495 min
Delta R.T.: -0.018 min
Response: 2258928
Conc: 0.72 ng/ml

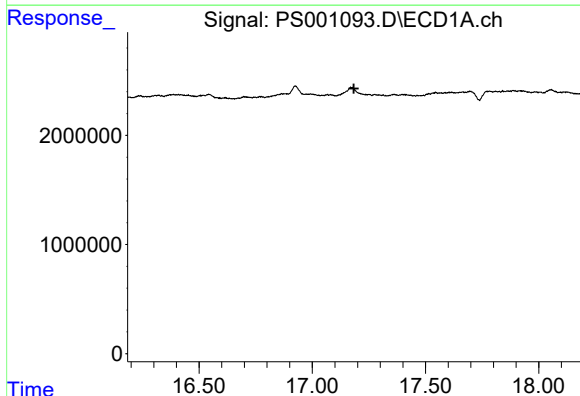


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 17.184 min
Response: 0
Conc: N.D.

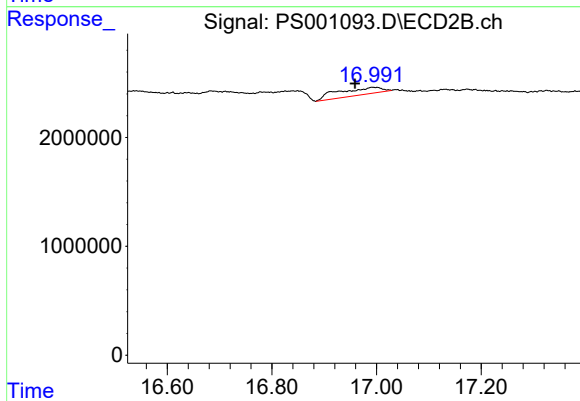


#15 Picloram

R.T.: 16.992 min
Delta R.T.: 0.033 min
Response: 3827963
Conc: 2.51 ng/ml

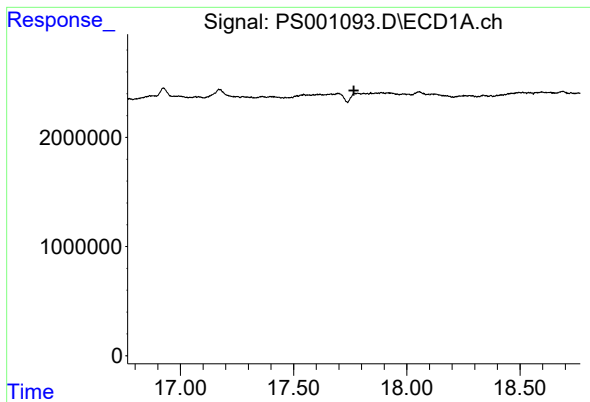

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.766 min
Response: 0
Conc: N.D.

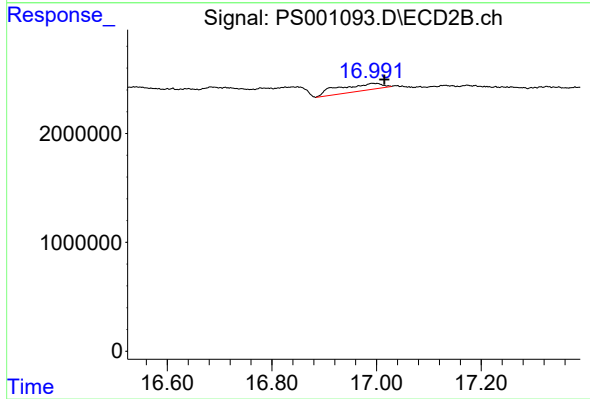

#16 DCPA

R.T.: 16.992 min
Delta R.T.: -0.023 min
Response: 3827963
Conc: 2.23 ng/ml