

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071718\
 Data File : PS001099.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jul 2018 20:51
 Operator : UA
 Sample : PB111179TB
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 18 00:49:43 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 09 02:00:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
4) S	2,4-DCAA	11.665	11.079	41409470	34510332	200.705	158.452
Target Compounds							
1) T	Dalapon	3.005	0.000	5031627	0	18.739	N.D. #
2) T	3,5-DICHL...	0.000	9.165	0	11580630	N.D.	39.369 #
5) T	DICAMBA	11.917	11.323	3161881	7075229	4.016	9.014 #
6) T	MCP	12.360	0.000	7433066	0	13.532	N.D. #
8) T	DICHLORPROP	0.000	12.450	0	1244756	N.D.	6.163 #
11) T	2,4,5-TP ...	0.000	14.058	0	10539620	N.D.	8.399 #
15) T	Picloram	0.000	17.017	0	5102863	N.D.	3.351 #
16) T	DCPA	0.000	17.017	0	5102863	N.D.	2.968 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071718\
Data File : PS001099.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jul 2018 20:51
Operator : UA
Sample : PB111179TB
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 18 00:49:43 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
Quant Title : 8080.M
QLast Update : Mon Jul 09 02:00:25 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

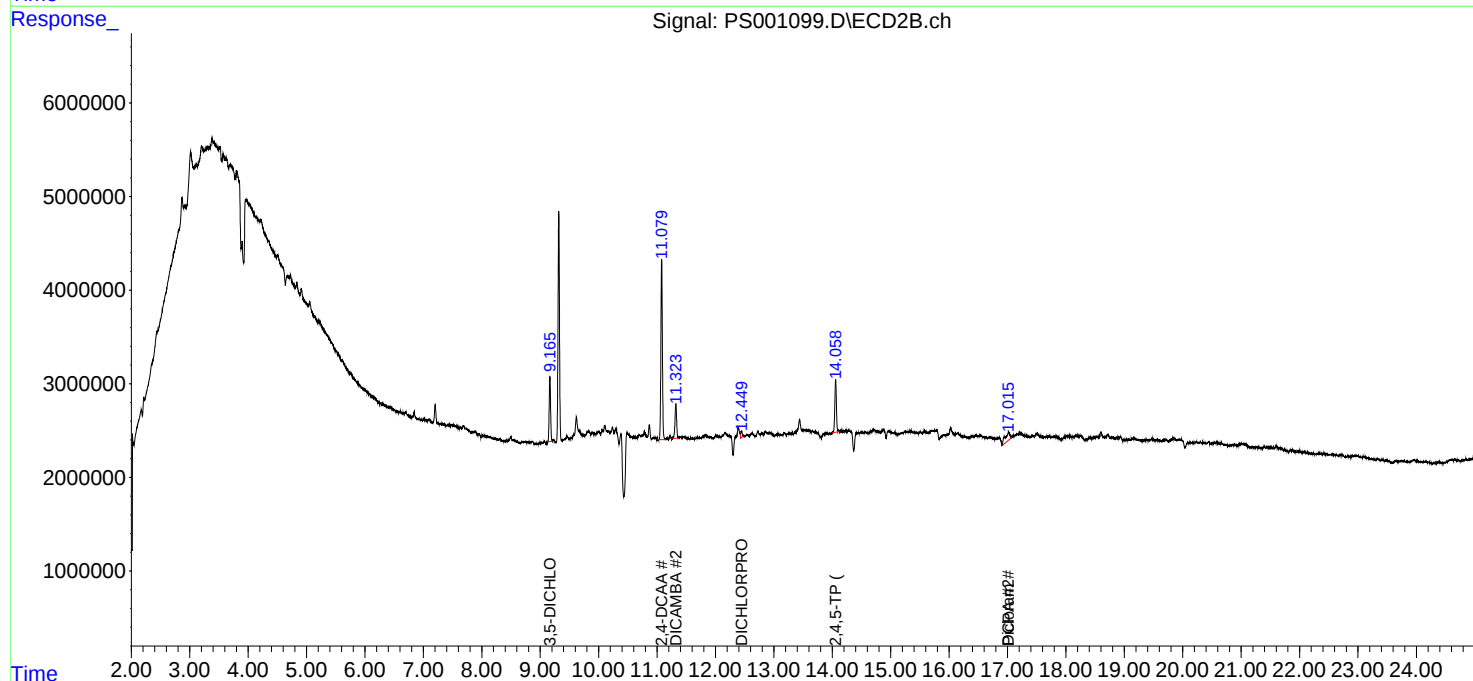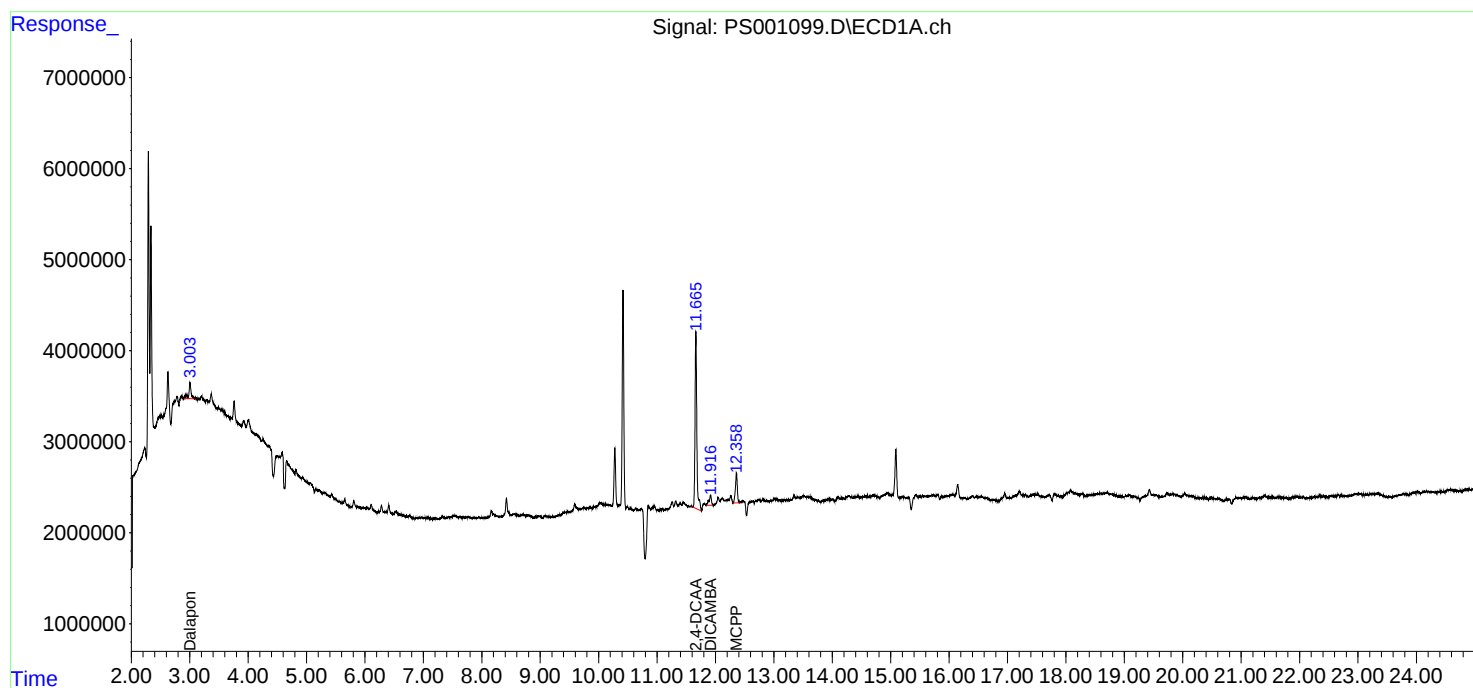

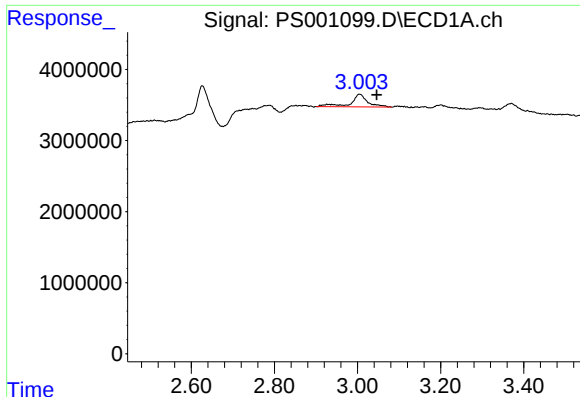


#1 Dalapon

R.T.: 3.005 min
Delta R.T.: -0.041 min
Response: 5031627
Conc: 18.74 ng/ml

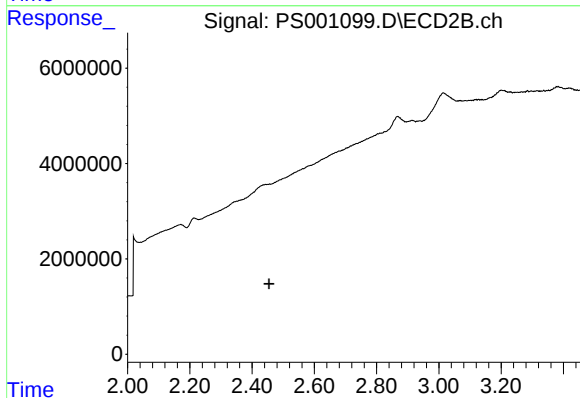


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.455 min
Response: 0
Conc: N.D.

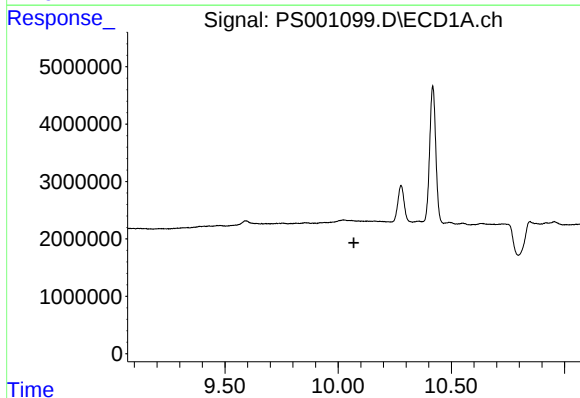


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 10.070 min
Response: 0
Conc: N.D.

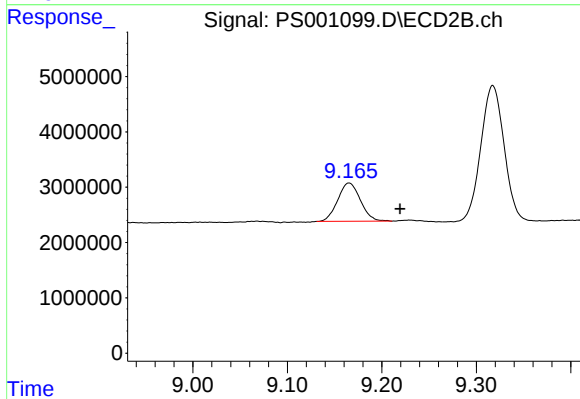


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.165 min
Delta R.T.: -0.054 min
Response: 11580630
Conc: 39.37 ng/ml

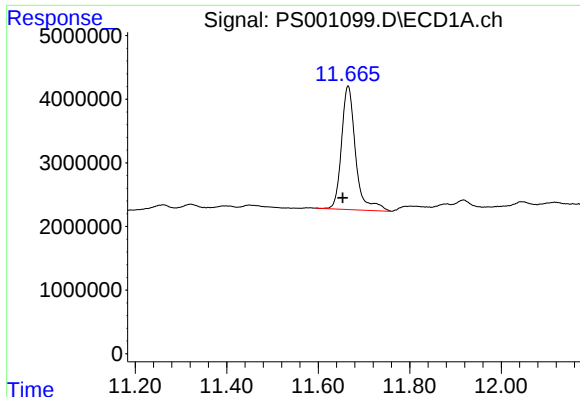


#4 2,4-DCAA

R.T.: 11.665 min
Delta R.T.: 0.012 min
Response: 41409470
Conc: 200.71 ng/ml

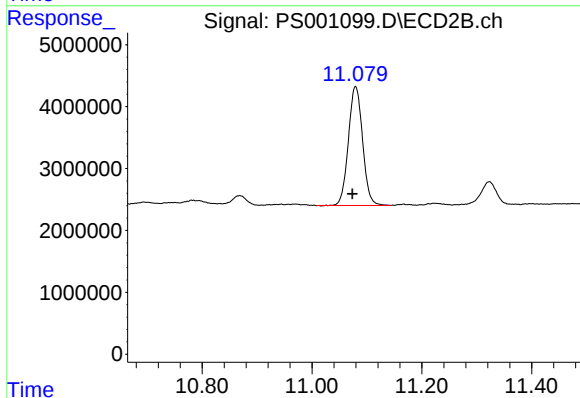


#4 2,4-DCAA

R.T.: 11.079 min
Delta R.T.: 0.006 min
Response: 34510332
Conc: 158.45 ng/ml

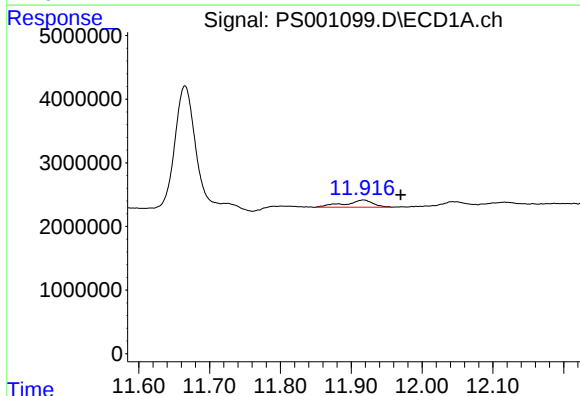


#5 DICAMBA

R.T.: 11.917 min
Delta R.T.: -0.053 min
Response: 3161881
Conc: 4.02 ng/ml

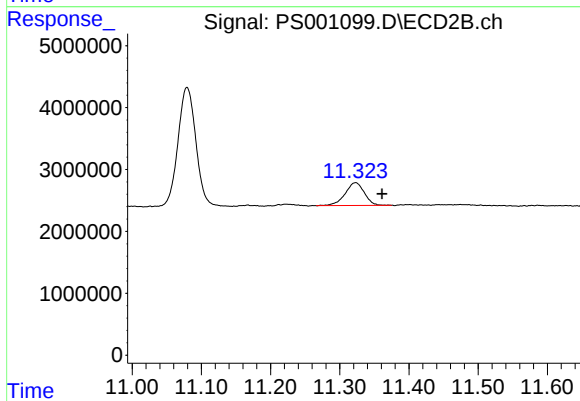


#5 DICAMBA

R.T.: 11.323 min
Delta R.T.: -0.038 min
Response: 7075229
Conc: 9.01 ng/ml

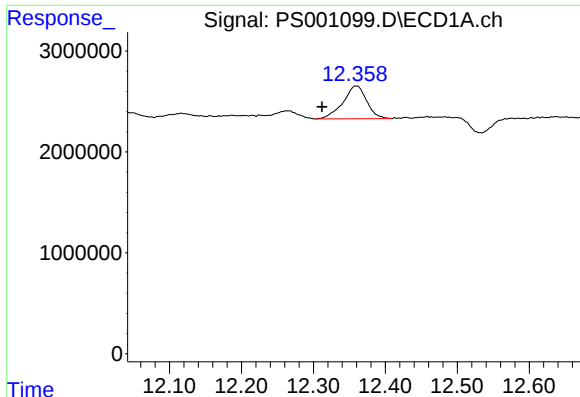


#6 MCP

R.T.: 12.360 min
Delta R.T.: 0.048 min
Response: 7433066
Conc: 13.53 ug/ml

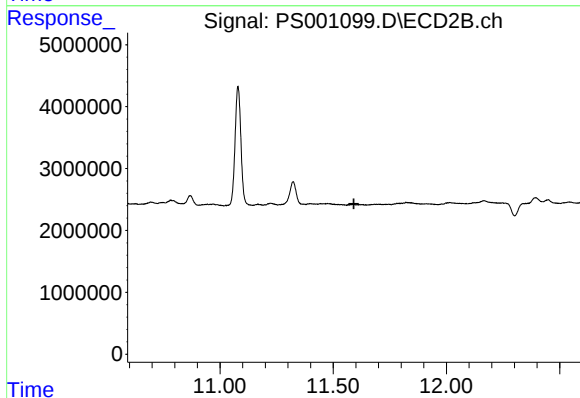


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.591 min
Response: 0
Conc: N.D.

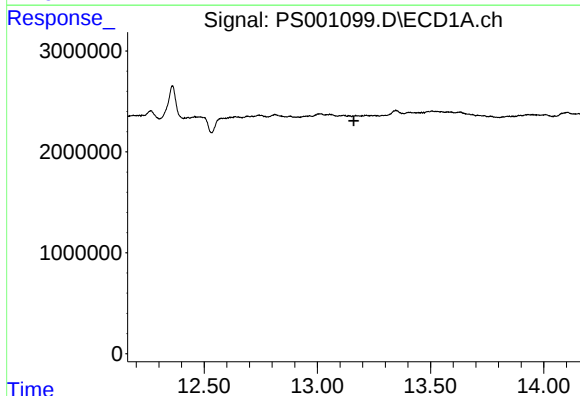


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 13.161 min
Response: 0
Conc: N.D.

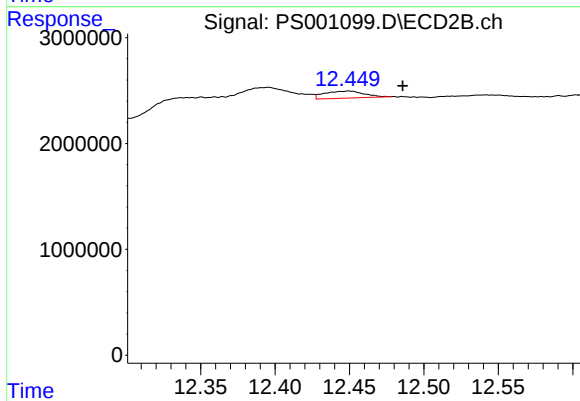


#8 DICHLORPROP

R.T.: 12.450 min
Delta R.T.: -0.036 min
Response: 1244756
Conc: 6.16 ng/ml

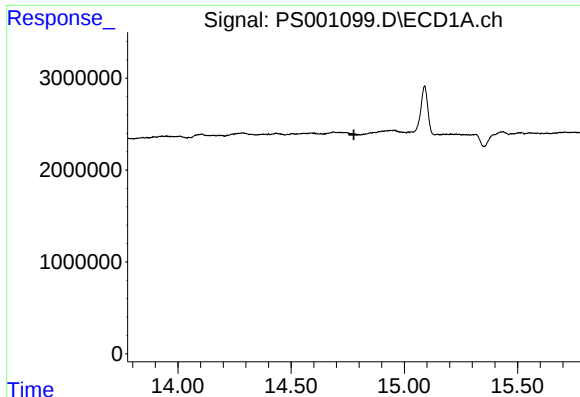


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 14.777 min
Response: 0
Conc: N.D.

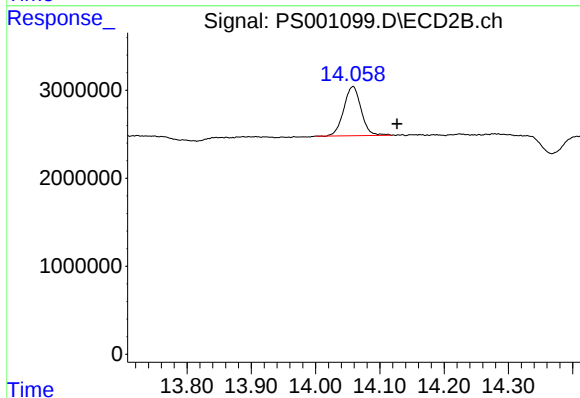


#11 2,4,5-TP (SILVEX)

R.T.: 14.058 min
Delta R.T.: -0.068 min
Response: 10539620
Conc: 8.40 ng/ml

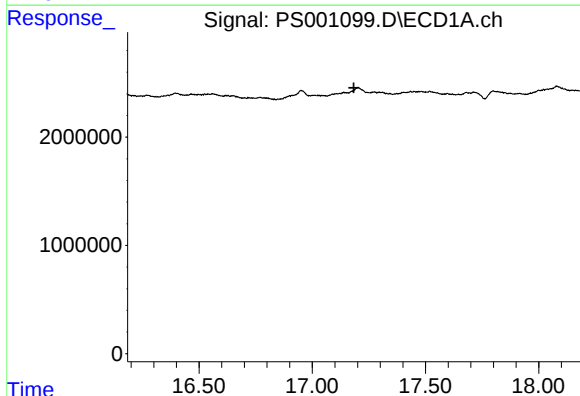


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 17.184 min
Response: 0
Conc: N.D.

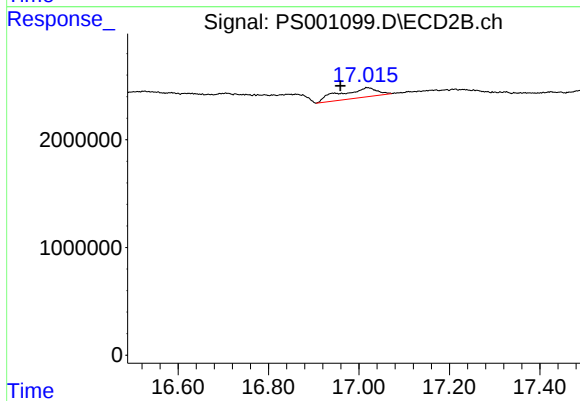


#15 Picloram

R.T.: 17.017 min
Delta R.T.: 0.058 min
Response: 5102863
Conc: 3.35 ng/ml

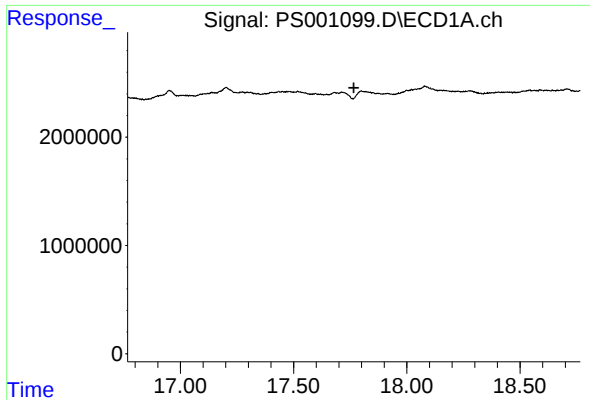

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.766 min
Response: 0
Conc: N.D.

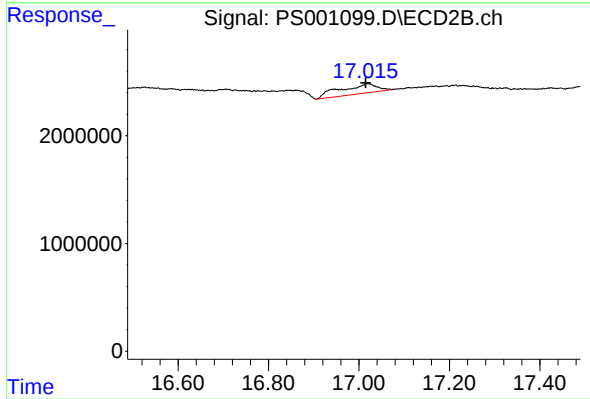

#16 DCPA

R.T.: 17.017 min
Delta R.T.: 0.002 min
Response: 5102863
Conc: 2.97 ng/ml