

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071718\
 Data File : PS001100.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jul 2018 21:22
 Operator : UA
 Sample : J3996-06
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 18 00:50:05 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 09 02:00:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
4) S	2,4-DCAA	11.646	11.062	33857327	28622861	164.101	131.420
Target Compounds							
5) T	DICAMBA	0.000	11.305	0	7016281	N.D.	8.939 #
6) T	MCP	12.342	0.000	7261197	0	13.219	N.D. #
8) T	DICHLORPROP	0.000	12.426	0	1755013	N.D.	8.689 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071718\
Data File : PS001100.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jul 2018 21:22
Operator : UA
Sample : J3996-06
Misc :
ALS Vial : 16 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 18 00:50:05 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
Quant Title : 8080.M
QLast Update : Mon Jul 09 02:00:25 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

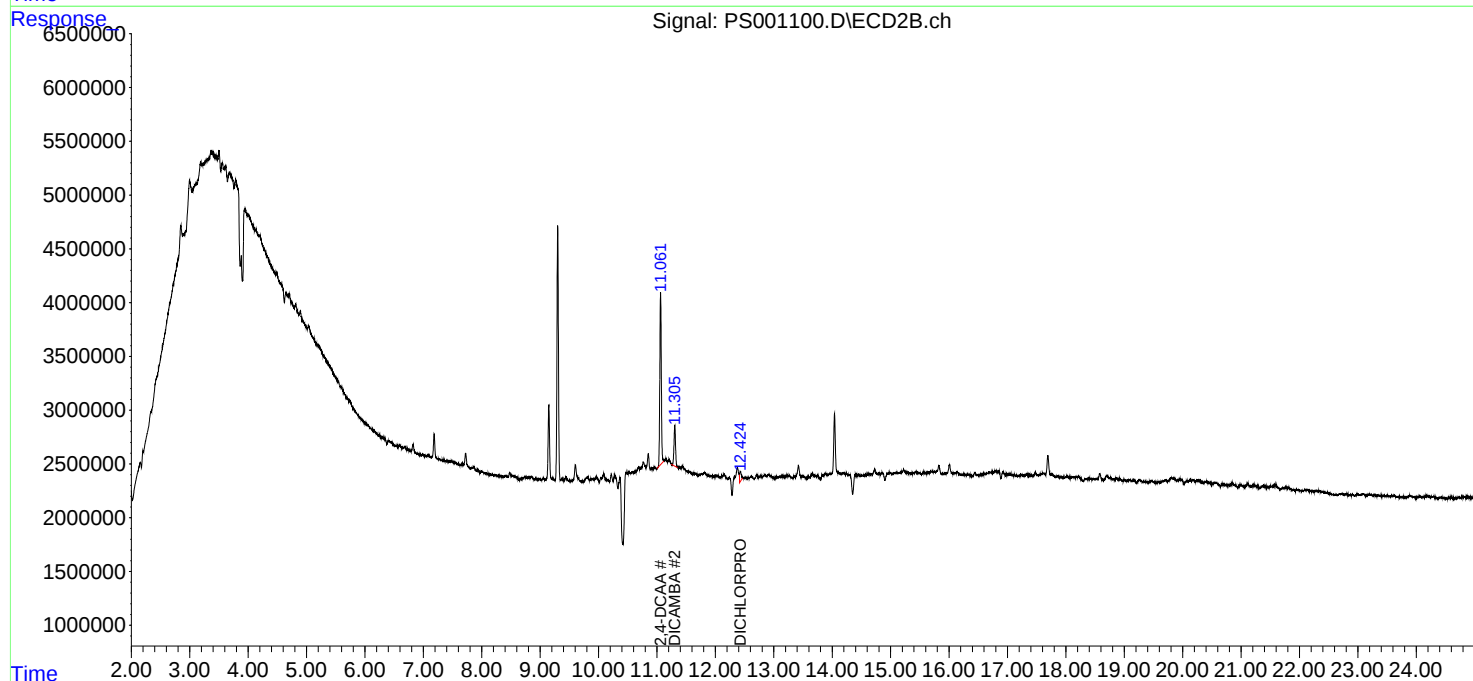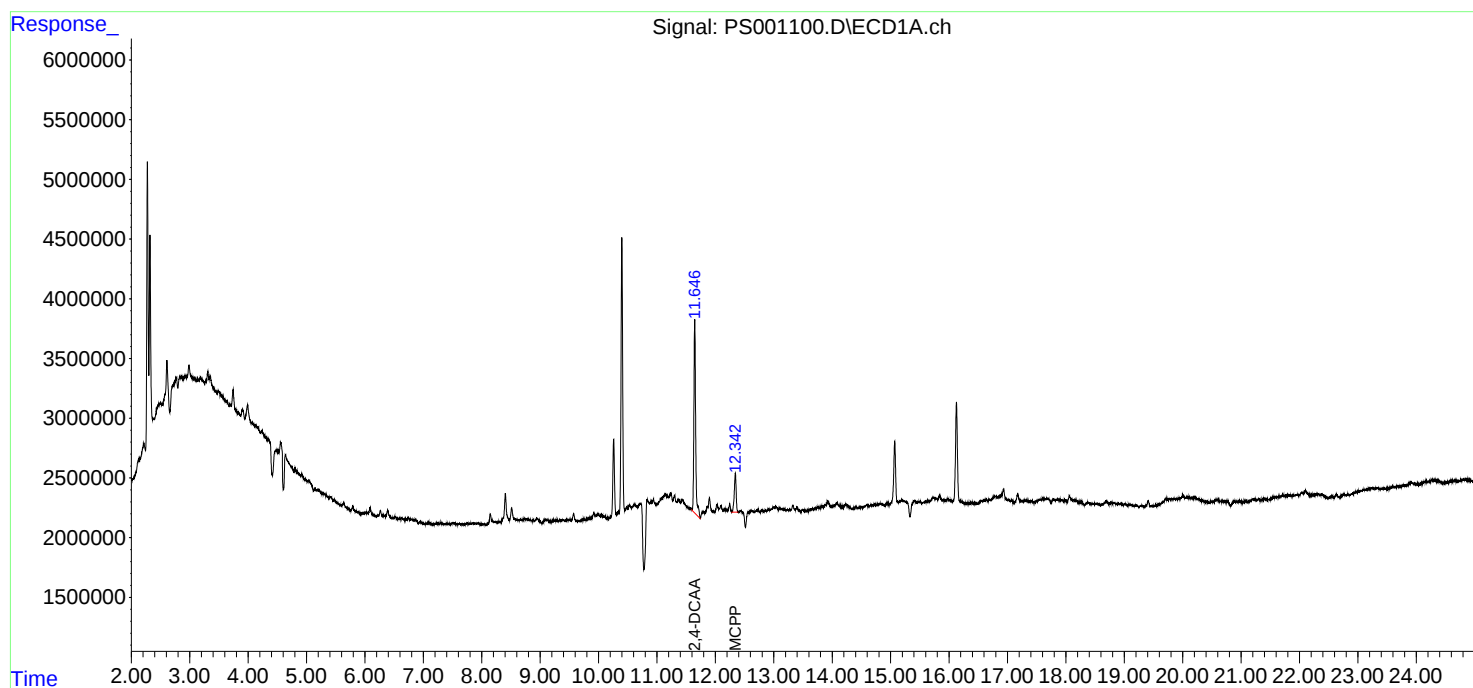

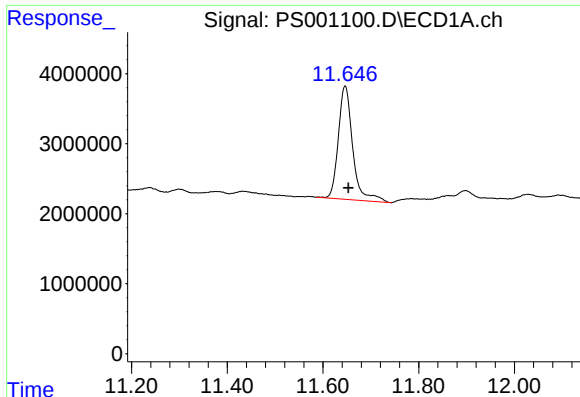


#4 2,4-DCAA

R.T.: 11.646 min
Delta R.T.: -0.007 min
Response: 33857327
Conc: 164.10 ng/ml

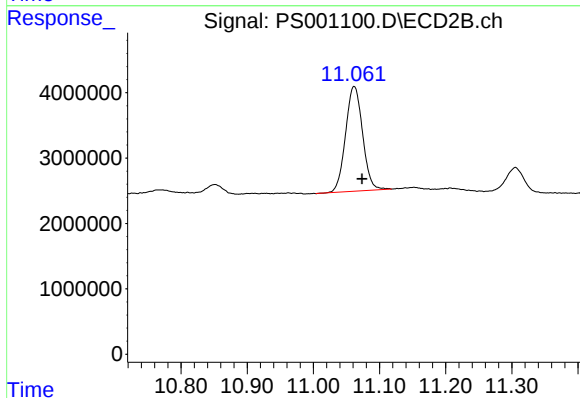


#4 2,4-DCAA

R.T.: 11.062 min
Delta R.T.: -0.012 min
Response: 28622861
Conc: 131.42 ng/ml

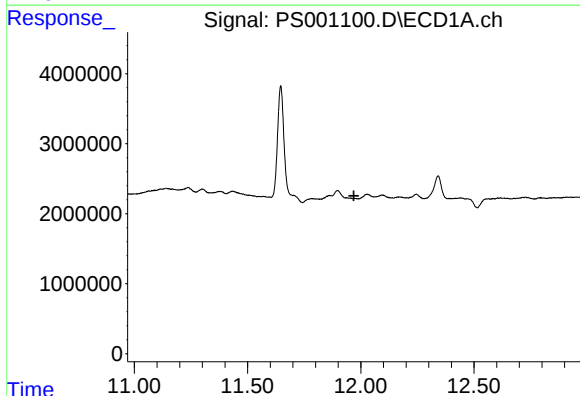


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.970 min
Response: 0
Conc: N.D.

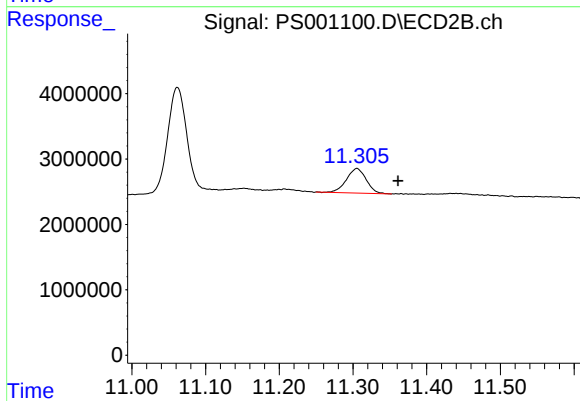


#5 DICAMBA

R.T.: 11.305 min
Delta R.T.: -0.056 min
Response: 7016281
Conc: 8.94 ng/ml

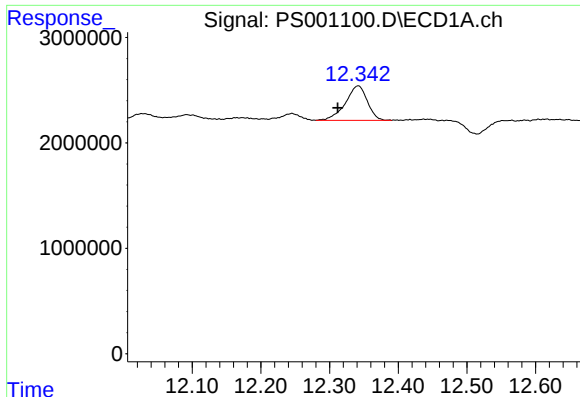


#6 MCP

R.T.: 12.342 min
Delta R.T.: 0.030 min
Response: 7261197
Conc: 13.22 ug/ml

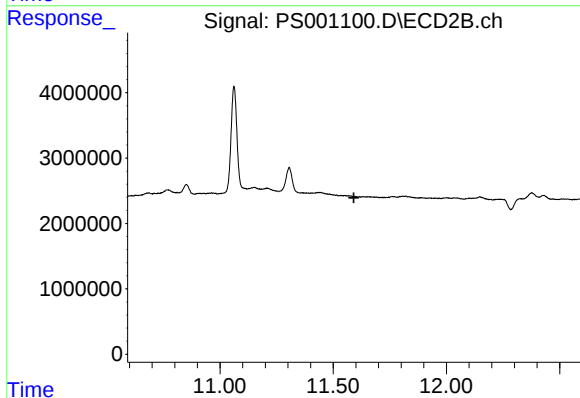


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.591 min
Response: 0
Conc: N.D.

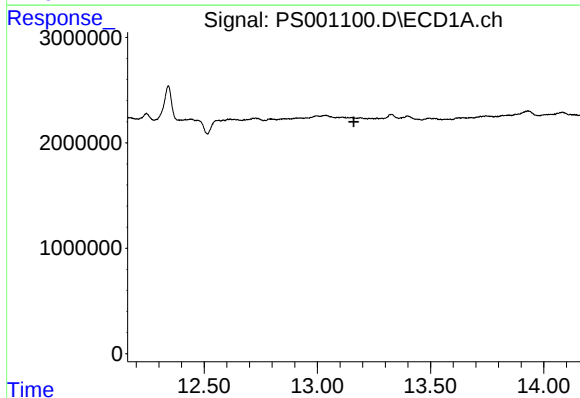

#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 13.161 min
Response: 0
Conc: N.D.

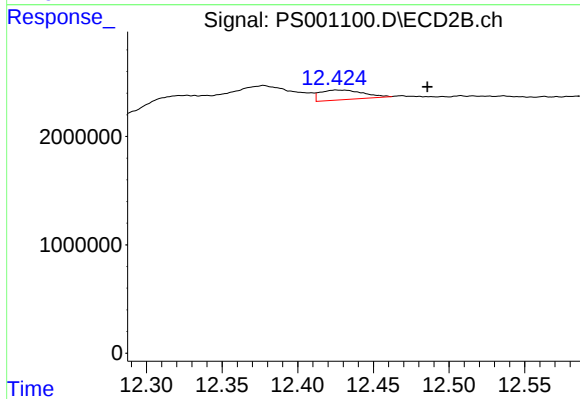

#8 DICHLORPROP

R.T.: 12.426 min
Delta R.T.: -0.060 min
Response: 1755013
Conc: 8.69 ng/ml