

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071718\
 Data File : PS001104.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jul 2018 23:26
 Operator : UA
 Sample : J3829-04
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 18 00:51:30 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 09 02:00:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
4) S	2,4-DCAA	11.627	11.043	33043954	26977989	160.159	123.868
Target Compounds							
1) T	Dalapon	0.000	2.410	0	670443	N.D.	2.488 #
2) T	3,5-DICHL...	0.000	9.281	0	41836576	N.D.	142.227 #
6) T	MCP	12.322	0.000	5468220	0	9.955	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071718\
Data File : PS001104.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jul 2018 23:26
Operator : UA
Sample : J3829-04
Misc :
ALS Vial : 20 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 18 00:51:30 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
Quant Title : 8080.M
QLast Update : Mon Jul 09 02:00:25 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

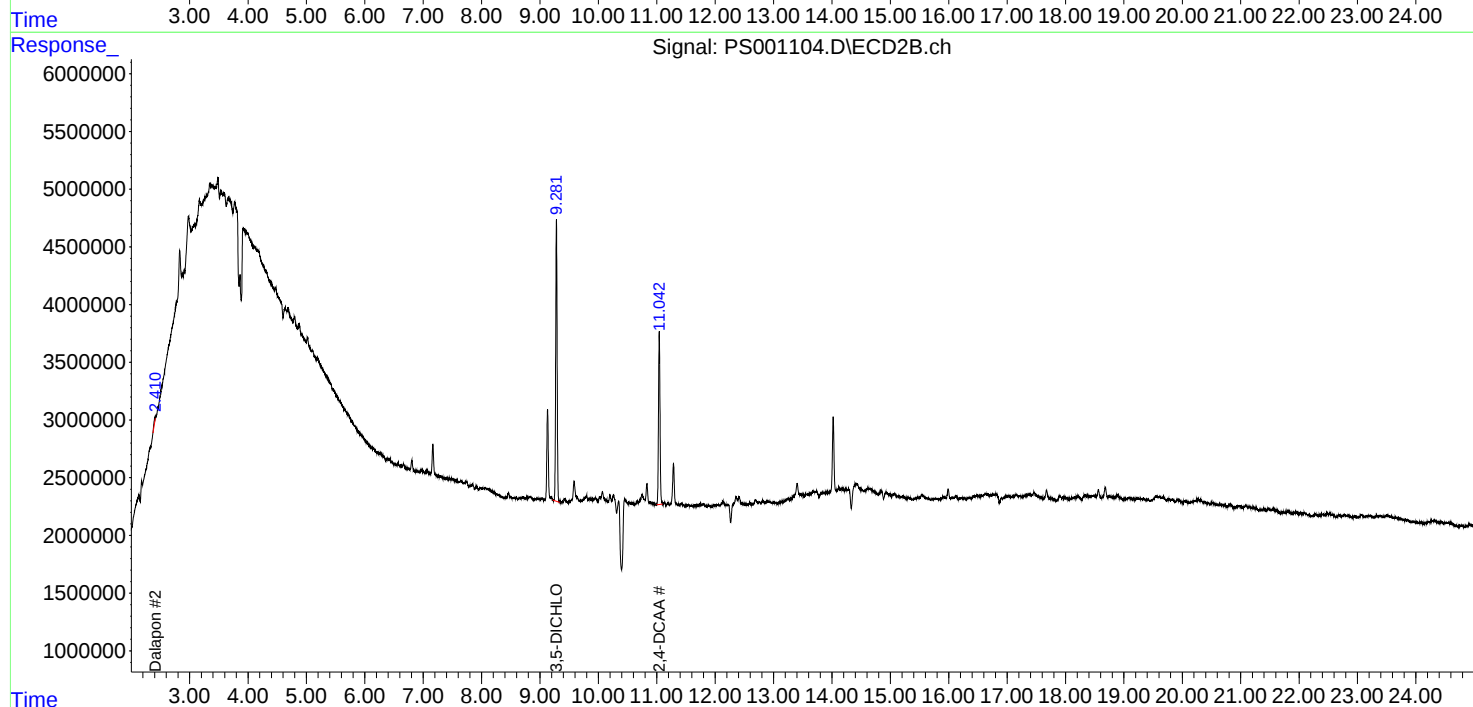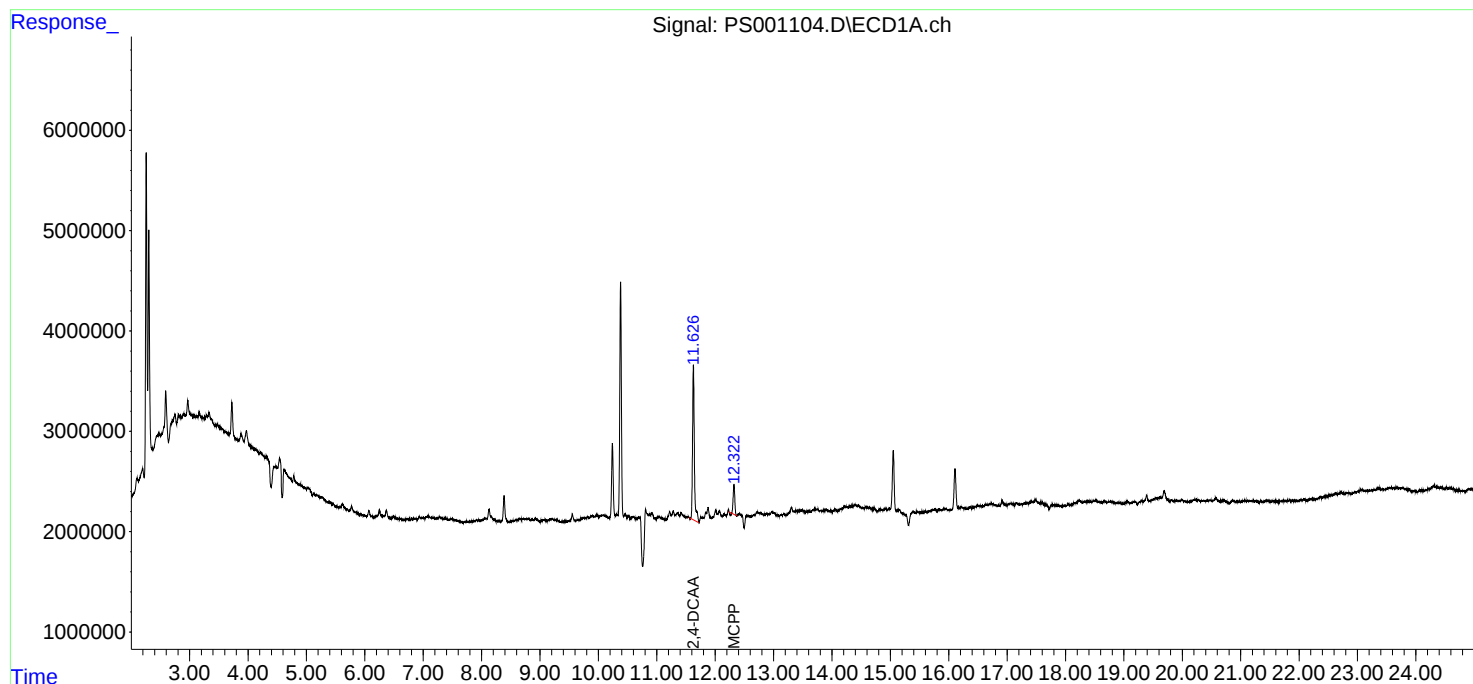

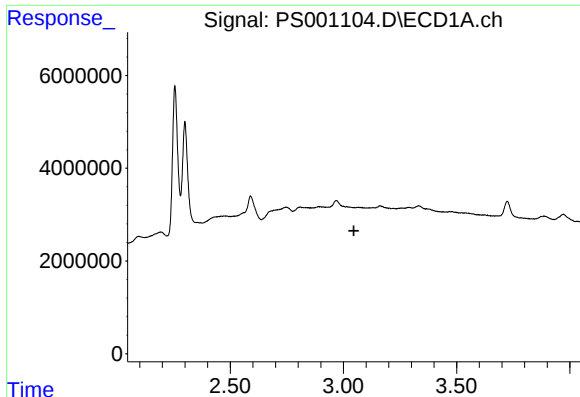


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 3.046 min
Response: 0
Conc: N.D.

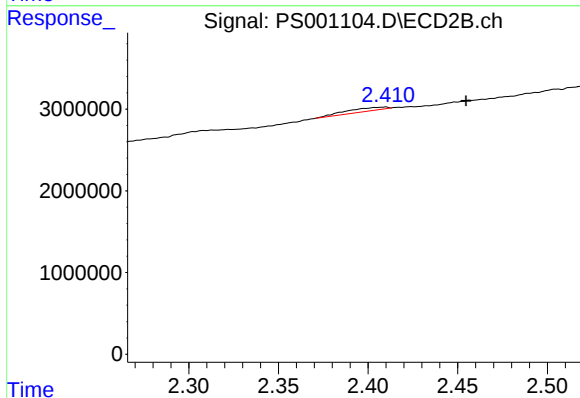


#1 Dalapon

R.T.: 2.410 min
Delta R.T.: -0.045 min
Response: 670443
Conc: 2.49 ng/ml

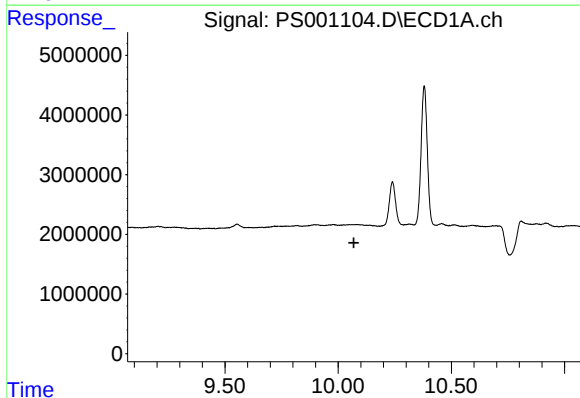


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 10.070 min
Response: 0
Conc: N.D.

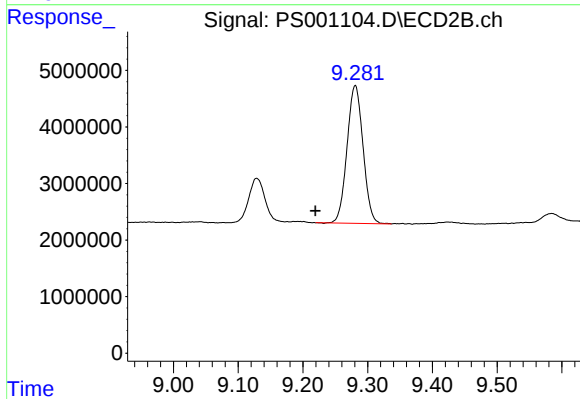


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.281 min
Delta R.T.: 0.062 min
Response: 41836576
Conc: 142.23 ng/ml

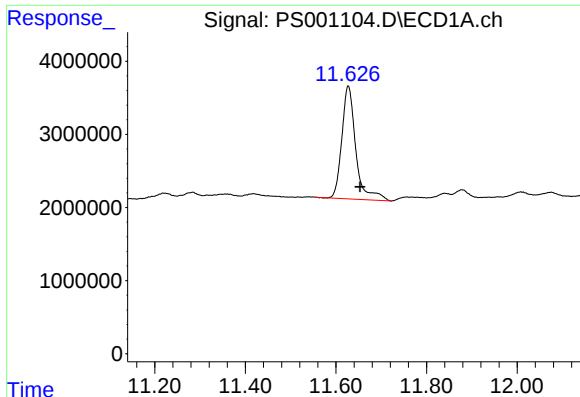


#4 2,4-DCAA

R.T.: 11.627 min
Delta R.T.: -0.026 min
Response: 33043954
Conc: 160.16 ng/ml

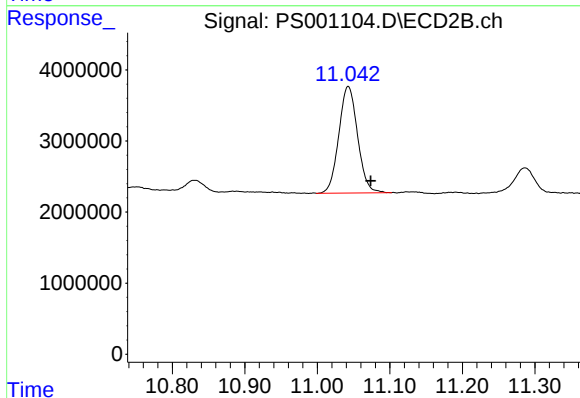


#4 2,4-DCAA

R.T.: 11.043 min
Delta R.T.: -0.031 min
Response: 26977989
Conc: 123.87 ng/ml

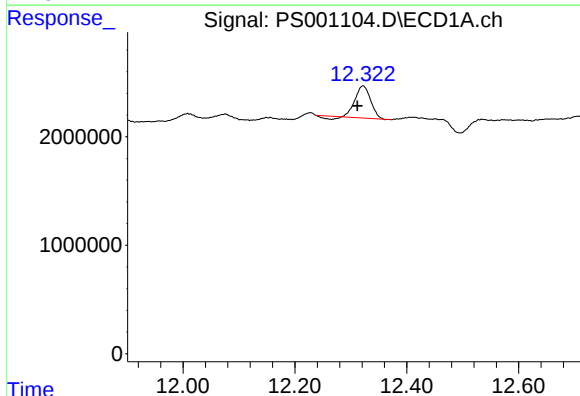

#6 MCP

R.T.: 12.322 min
Delta R.T.: 0.010 min
Response: 5468220
Conc: 9.95 ug/ml

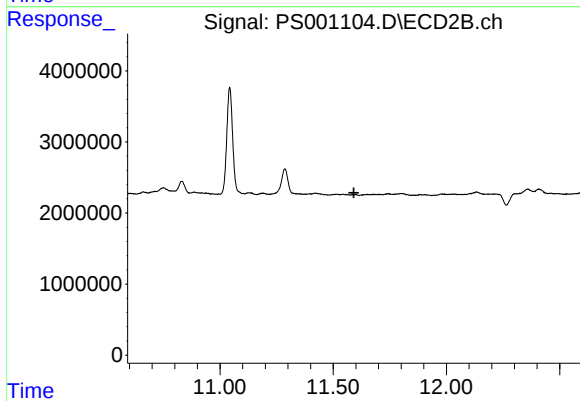

#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.591 min
Response: 0
Conc: N.D.