

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071718\
 Data File : PS001109.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jul 2018 02:01
 Operator : UA
 Sample : J3997-04
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 18 03:25:09 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 09 02:00:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
4) S	2,4-DCAA	11.665	11.080	38623597	31651479	187.202	145.326
Target Compounds							
1) T	Dalapon	3.006	2.440	4986515	1331727	18.571	4.943 #
2) T	3,5-DICHL...	0.000	9.167	0	9165165	N.D.	31.158 #
5) T	DICAMBA	0.000	11.323	0	6338662	N.D.	8.075 #
6) T	MCP	12.359	0.000	6931259	0	12.618	N.D. #
8) T	DICHLORPROP	0.000	12.446	0	1272612	N.D.	6.301 #
11) T	2,4,5-TP ...	0.000	14.058	0	10127571	N.D.	8.070 #
15) T	Picloram	17.199	17.019	3304486	4101078	1.825	2.693 #
16) T	DCPA	0.000	17.019	0	4101078	N.D.	2.386 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071718\
Data File : PS001109.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jul 2018 02:01
Operator : UA
Sample : J3997-04
Misc :
ALS Vial : 23 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 18 03:25:09 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
Quant Title : 8080.M
QLast Update : Mon Jul 09 02:00:25 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

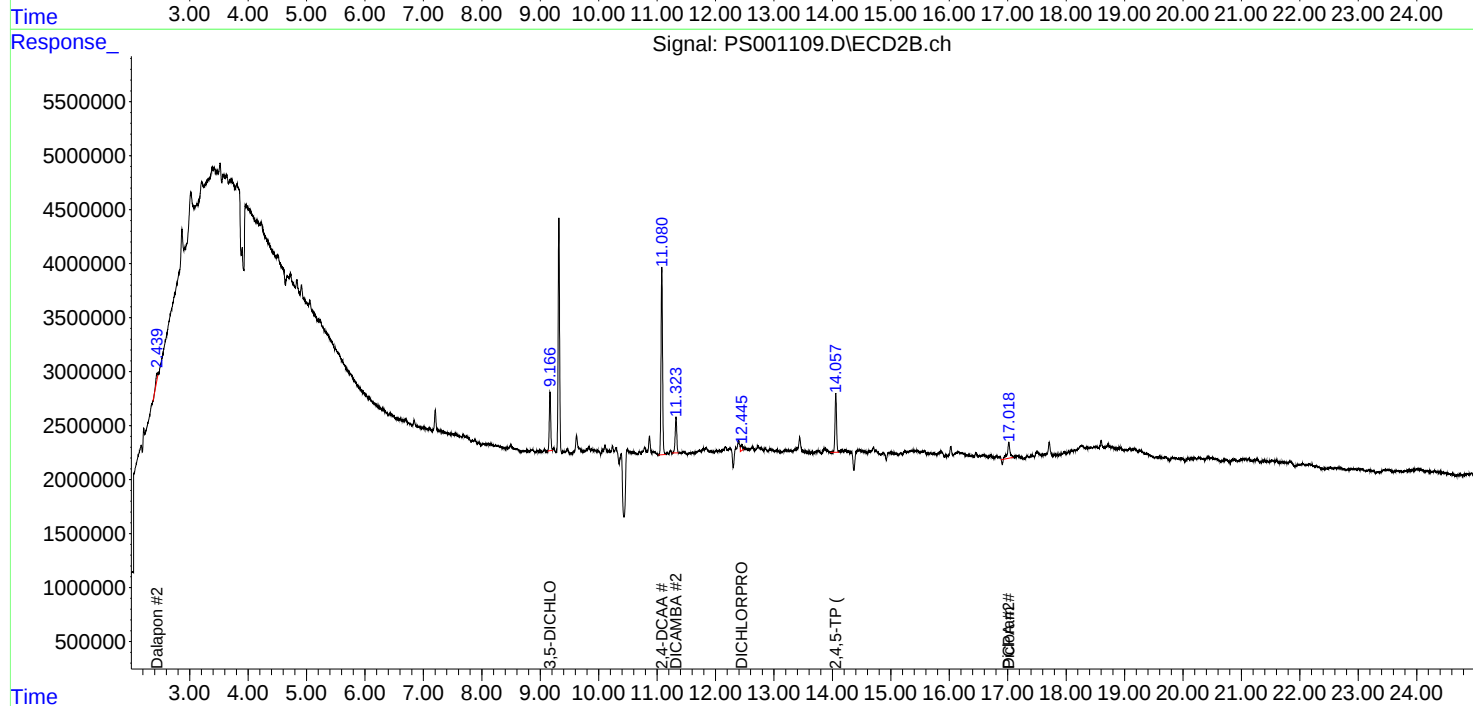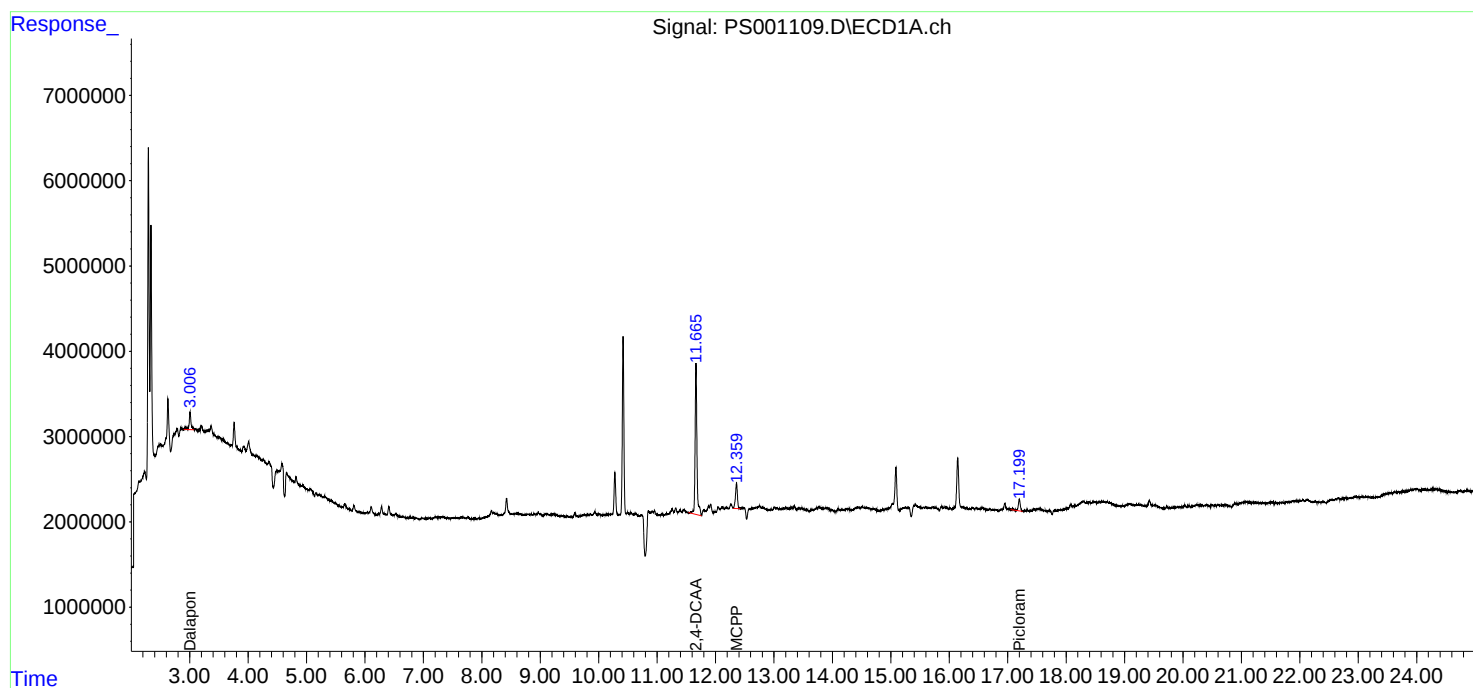

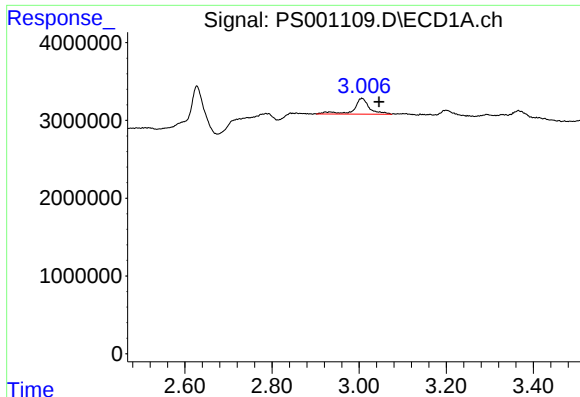


#1 Dalapon

R.T.: 3.006 min
Delta R.T.: -0.040 min
Response: 4986515
Conc: 18.57 ng/ml

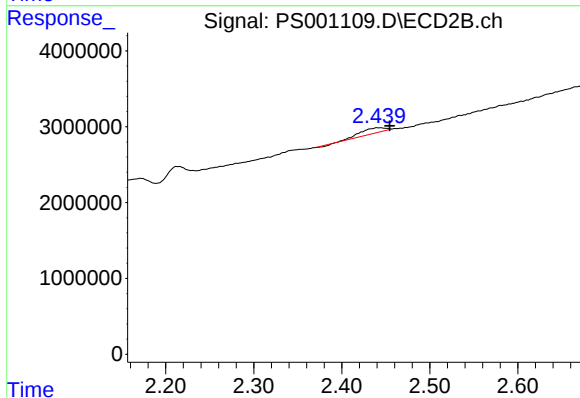


#1 Dalapon

R.T.: 2.440 min
Delta R.T.: -0.015 min
Response: 1331727
Conc: 4.94 ng/ml

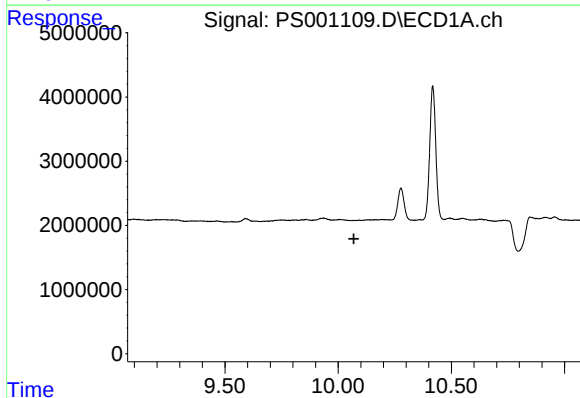


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 10.070 min
Response: 0
Conc: N.D.

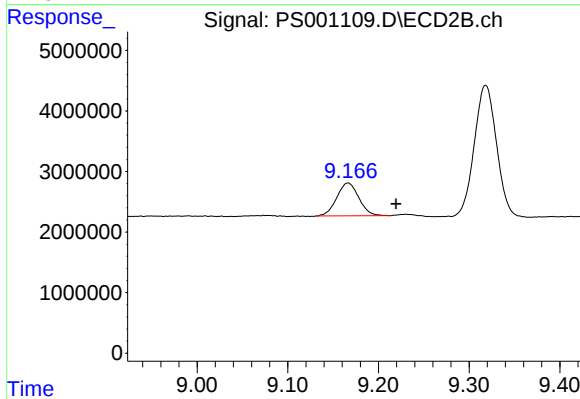


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.167 min
Delta R.T.: -0.053 min
Response: 9165165
Conc: 31.16 ng/ml

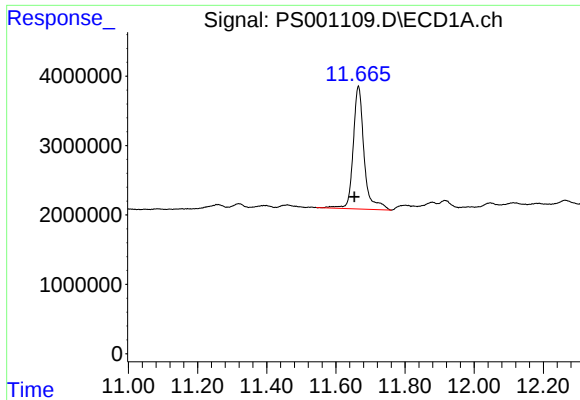


#4 2,4-DCAA

R.T.: 11.665 min
Delta R.T.: 0.012 min
Response: 38623597
Conc: 187.20 ng/ml

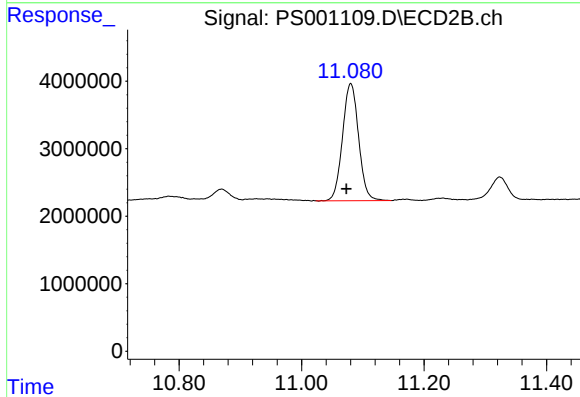


#4 2,4-DCAA

R.T.: 11.080 min
Delta R.T.: 0.007 min
Response: 31651479
Conc: 145.33 ng/ml

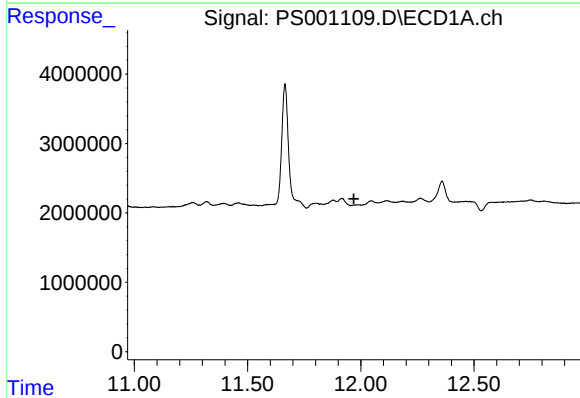


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.970 min
Response: 0
Conc: N.D.

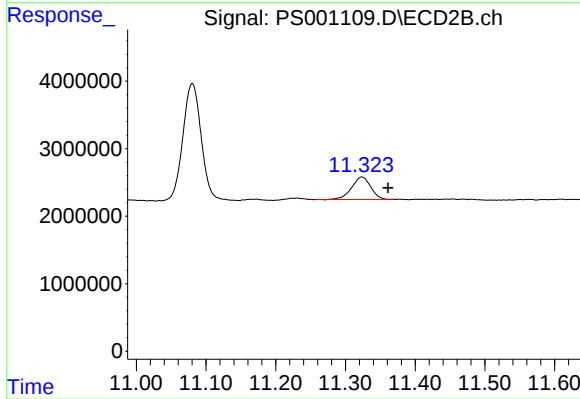


#5 DICAMBA

R.T.: 11.323 min
Delta R.T.: -0.038 min
Response: 6338662
Conc: 8.08 ng/ml

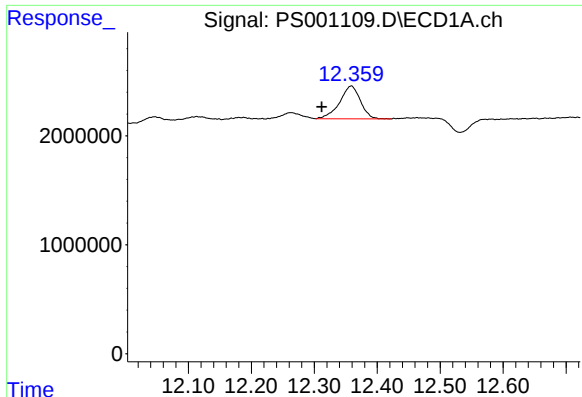


#6 MCP

R.T.: 12.359 min
Delta R.T.: 0.046 min
Response: 6931259
Conc: 12.62 ug/ml

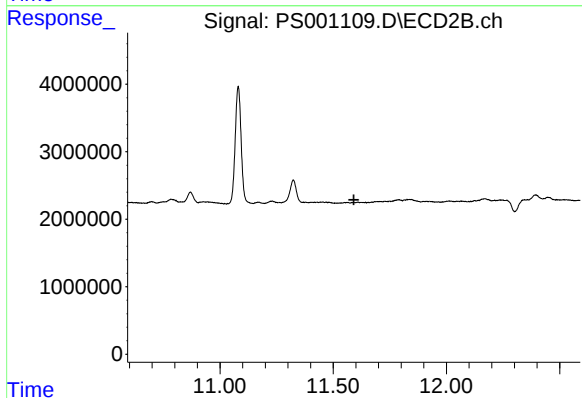


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.591 min
Response: 0
Conc: N.D.

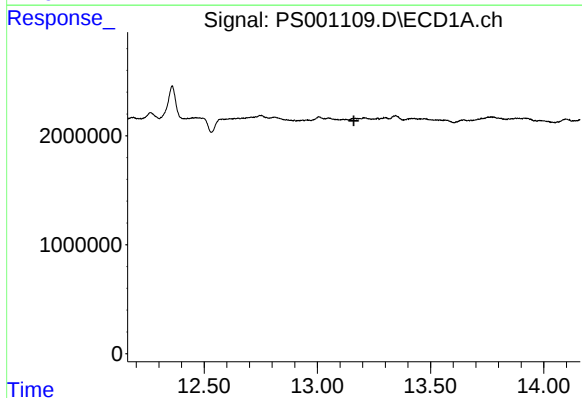


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 13.161 min
Response: 0
Conc: N.D.

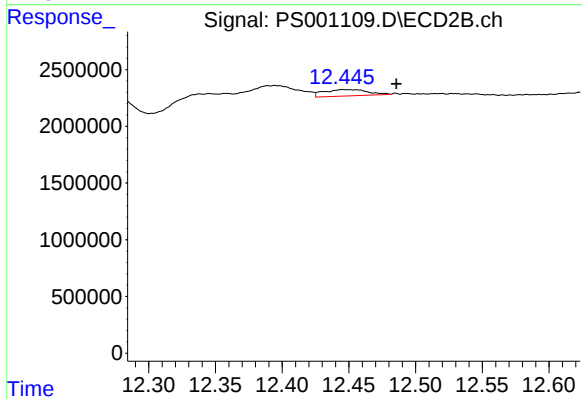


#8 DICHLORPROP

R.T.: 12.446 min
Delta R.T.: -0.040 min
Response: 1272612
Conc: 6.30 ng/ml

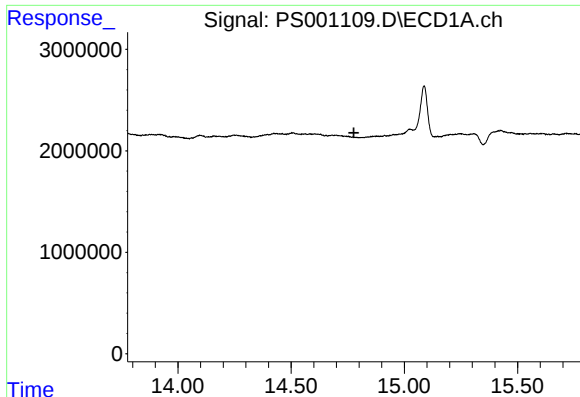


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 14.777 min
Response: 0
Conc: N.D.

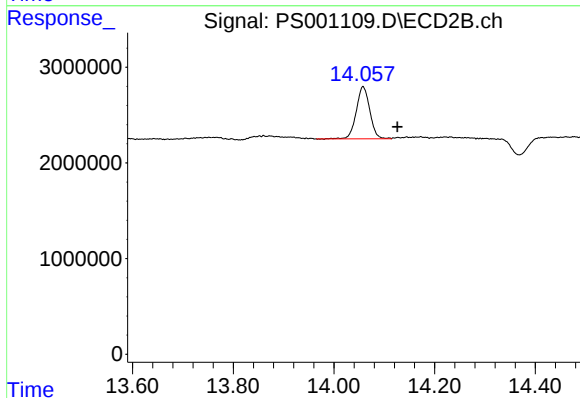


#11 2,4,5-TP (SILVEX)

R.T.: 14.058 min
Delta R.T.: -0.069 min
Response: 10127571
Conc: 8.07 ng/ml

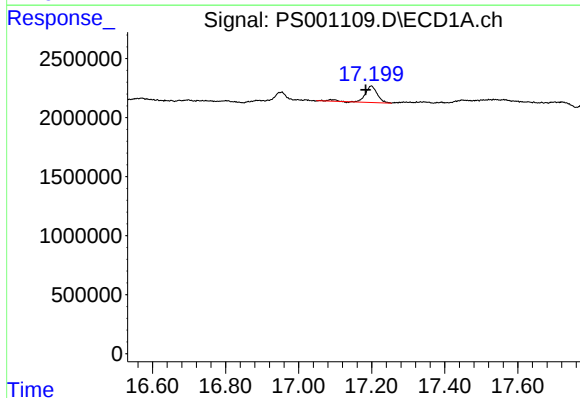


#15 Picloram

R.T.: 17.199 min
Delta R.T.: 0.015 min
Response: 3304486
Conc: 1.82 ng/ml

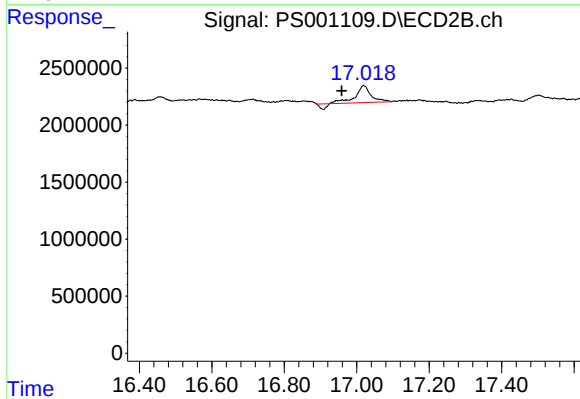


#15 Picloram

R.T.: 17.019 min
Delta R.T.: 0.060 min
Response: 4101078
Conc: 2.69 ng/ml

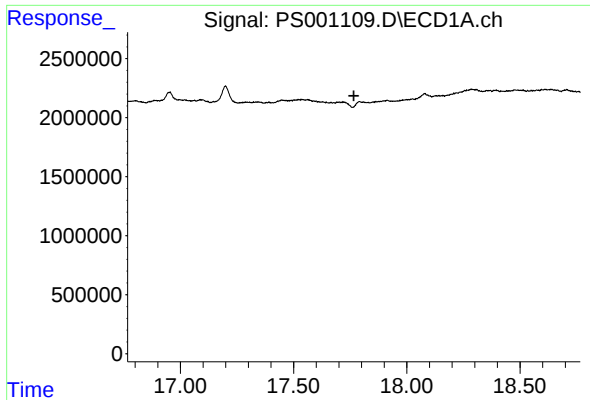

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.766 min
Response: 0
Conc: N.D.

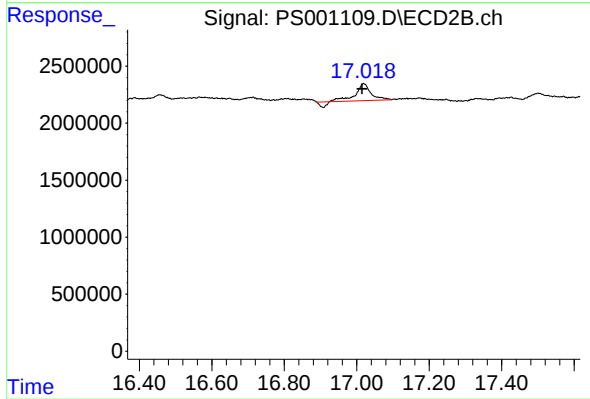

#16 DCPA

R.T.: 17.019 min
Delta R.T.: 0.004 min
Response: 4101078
Conc: 2.39 ng/ml