

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071718\
 Data File : PS001112.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jul 2018 03:34
 Operator : UA
 Sample : J3997-16
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 18 05:33:19 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 09 02:00:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
4) S	2,4-DCAA	11.662	11.077	37570005	31401623	182.096	144.178
Target Compounds							
2) T	3,5-DICHL...	0.000	9.164	0	10101540	N.D.	34.341 #
5) T	DICAMBA	11.911	11.320	2899162	7498925	3.682	9.553 #
6) T	MCP	12.356	0.000	7646394	0	13.920	N.D. #
8) T	DICHLORPROP	0.000	12.445	0	1285342	N.D.	6.364 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071718\
Data File : PS001112.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jul 2018 03:34
Operator : UA
Sample : J3997-16
Misc :
ALS Vial : 26 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 18 05:33:19 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
Quant Title : 8080.M
QLast Update : Mon Jul 09 02:00:25 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

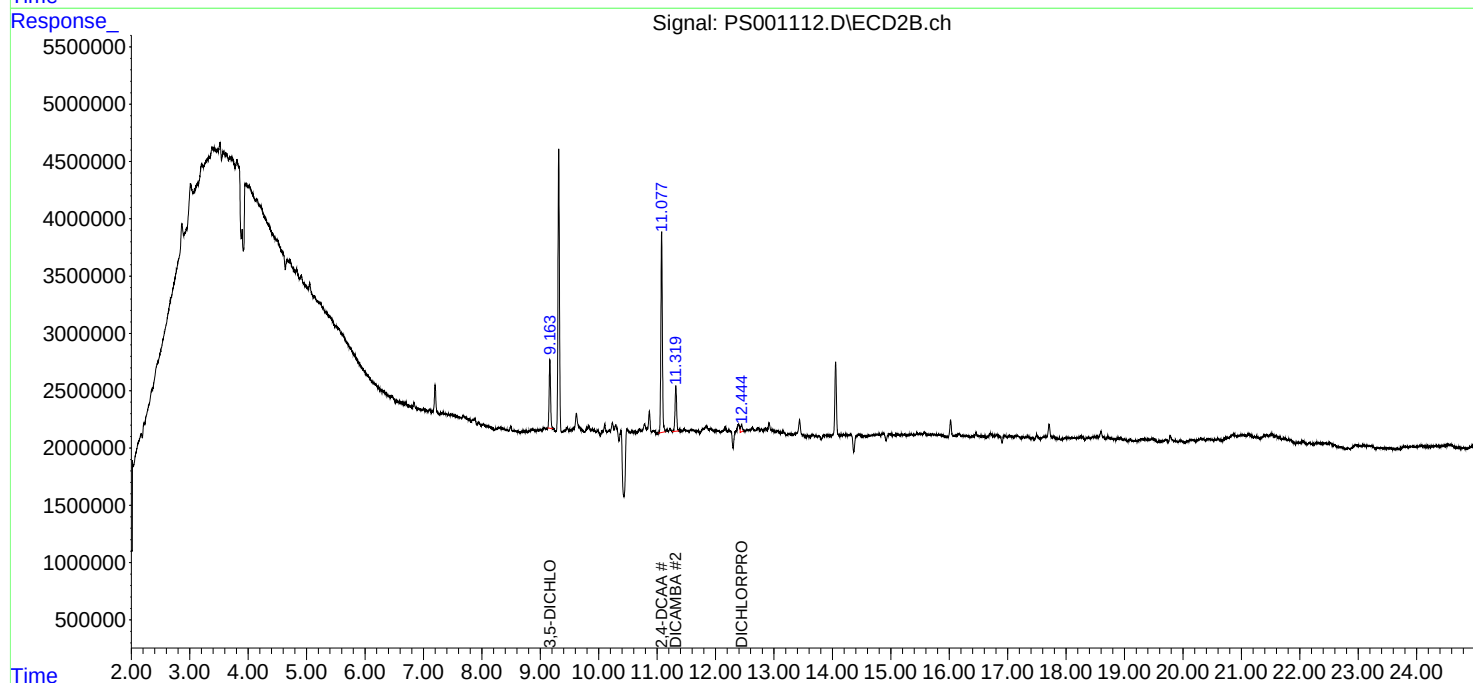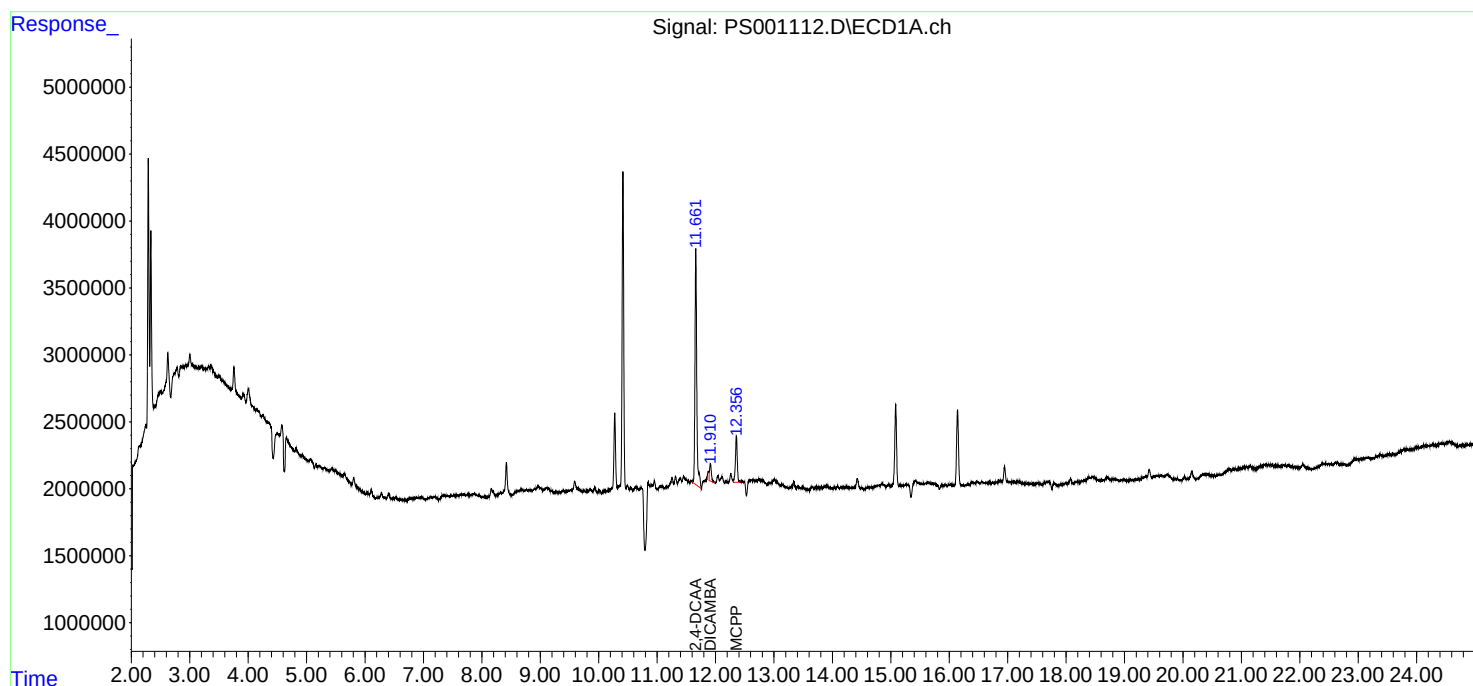

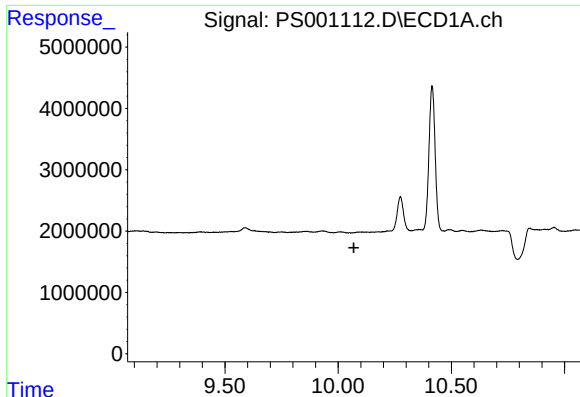


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 10.070 min
Response: 0
Conc: N.D.

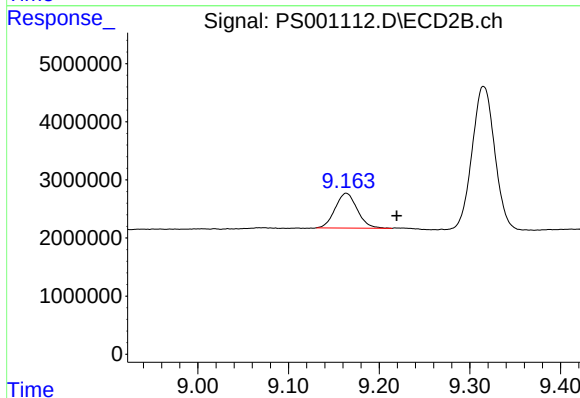


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.164 min
Delta R.T.: -0.056 min
Response: 10101540
Conc: 34.34 ng/ml

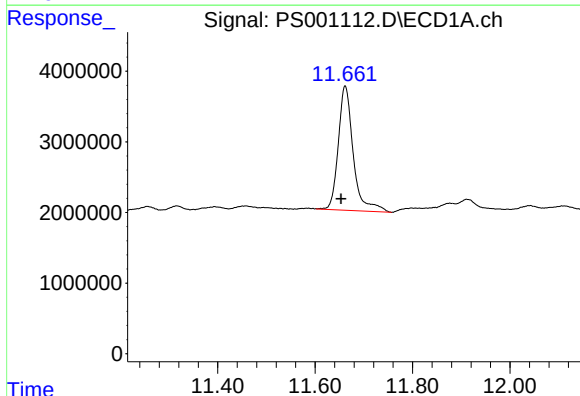


#4 2,4-DCAA

R.T.: 11.662 min
Delta R.T.: 0.008 min
Response: 37570005
Conc: 182.10 ng/ml

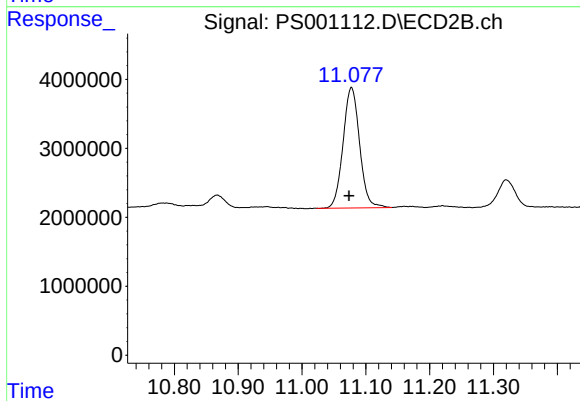


#4 2,4-DCAA

R.T.: 11.077 min
Delta R.T.: 0.004 min
Response: 31401623
Conc: 144.18 ng/ml

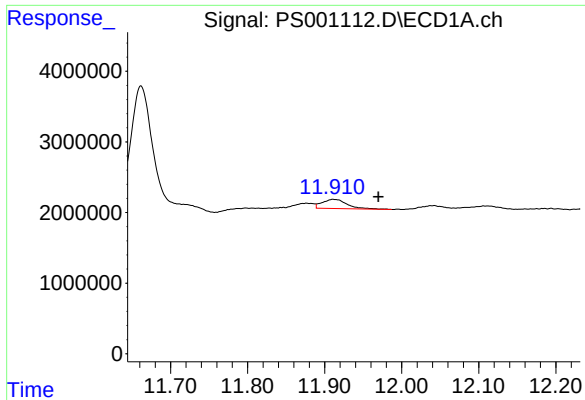


#5 DICAMBA

R.T.: 11.911 min
Delta R.T.: -0.059 min
Response: 2899162
Conc: 3.68 ng/ml

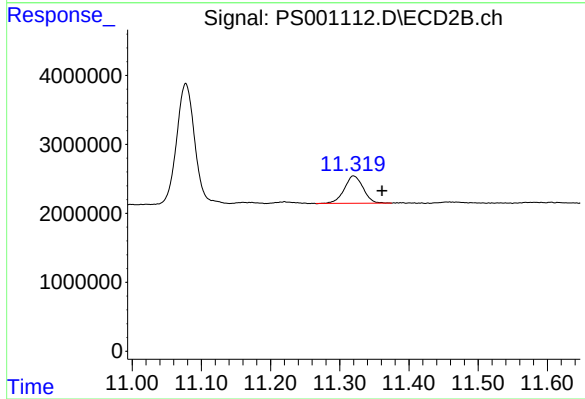


#5 DICAMBA

R.T.: 11.320 min
Delta R.T.: -0.041 min
Response: 7498925
Conc: 9.55 ng/ml

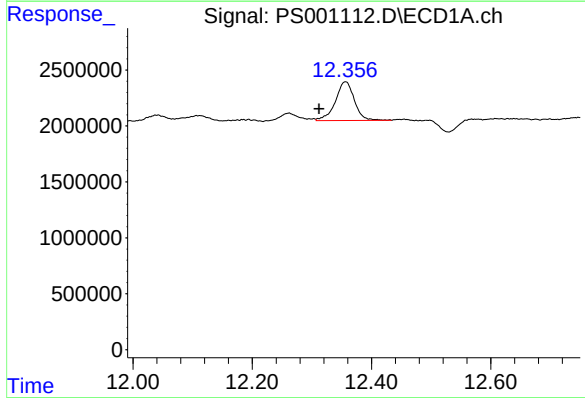


#6 MCP

R.T.: 12.356 min
Delta R.T.: 0.044 min
Response: 7646394
Conc: 13.92 ug/ml

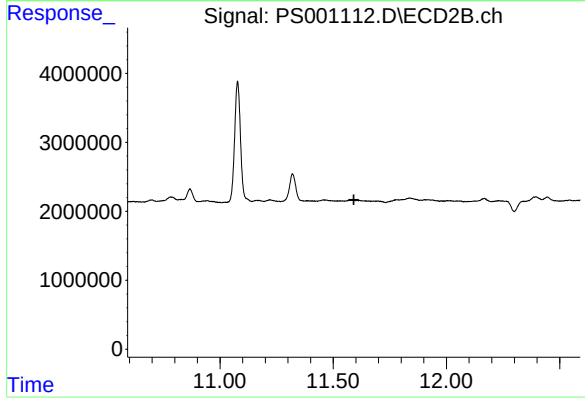


#6 MCP

R.T.: 0.000 min
Exp R.T.: 11.591 min
Response: 0
Conc: N.D.

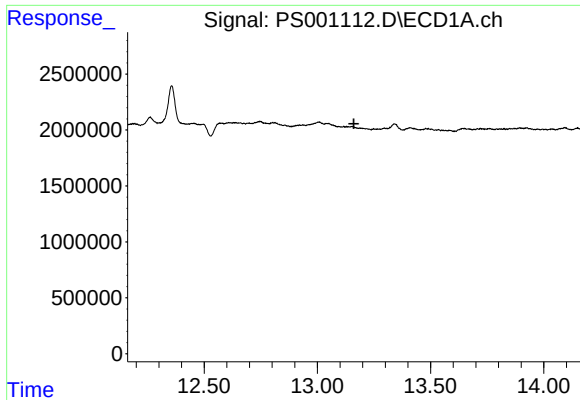

#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 13.161 min
Response: 0
Conc: N.D.

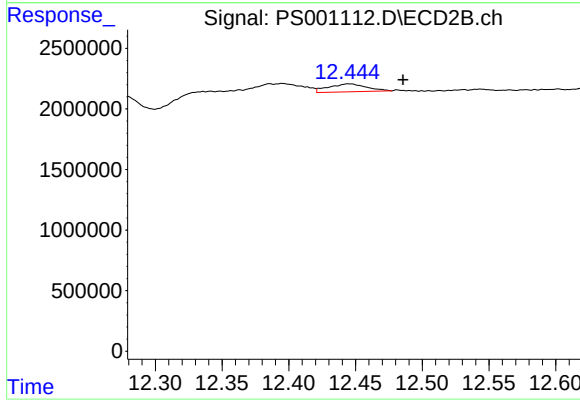

#8 DICHLORPROP

R.T.: 12.445 min
Delta R.T.: -0.041 min
Response: 1285342
Conc: 6.36 ng/ml