

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071724\
 Data File : PS027186.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jul 2024 13:50
 Operator : AR\AJ
 Sample : P3247-12
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 WC-CTW2-BL-03

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 18 03:16:34 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071224.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 27 04:33:52 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.203	7.755	670.6E6	532.1E6	265.202	229.491
Target Compounds							
1) T	Dalapon	2.579f	2.671f	445.5E6	579.5E6	133.999	139.638
2) T	3,5-DICHL...	6.414f	6.673f	-913476	2489349	N.D.	<MDL
3) T	4-Nitroph...	6.993	0.000	22458305	0	14.009	N.D. #
5) T	DICAMBA	0.000	7.942	0	8739742	N.D.	<MDL
6) T	MCPD	7.553	8.048	7756509	2130577	1.010	<MDL #
7) T	MCPA	7.683f	8.273	133.7E6	-28501702	13.116	N.D. #
8) T	DICHLORPROP	8.048f	0.000	11068986	0	4.125	N.D. #
9) T	2,4-D	0.000	8.993	0	2963875	N.D.	1.028
10) T	Pentachlo...	8.566f	9.526	28788313	975104	<MDL	<MDL #
11) T	2,4,5-TP ...	9.180	9.848f	4295738	140.9E6	<MDL	8.837 #
12) T	2,4,5-T	9.475	10.283f	4815707	52558660	<MDL	3.289 #
13) T	2,4-DB	10.045	10.922f	46623254	10356074	21.576	5.124 #
14) T	DINOSEB	11.250	11.270	8895095	17836352	<MDL	1.597 #
15) T	Picloram	11.036	12.357	64056915	6447193	3.289	<MDL #
16) T	DCPA	11.502f	12.304	85277609	16037700	4.750	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071724\
Data File : PS027186.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jul 2024 13:50
Operator : AR\AJ
Sample : P3247-12
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
WC-CTW2-BL-03

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 18 03:16:34 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071224.M
Quant Title : 8080.M
QLast Update : Thu Jun 27 04:33:52 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

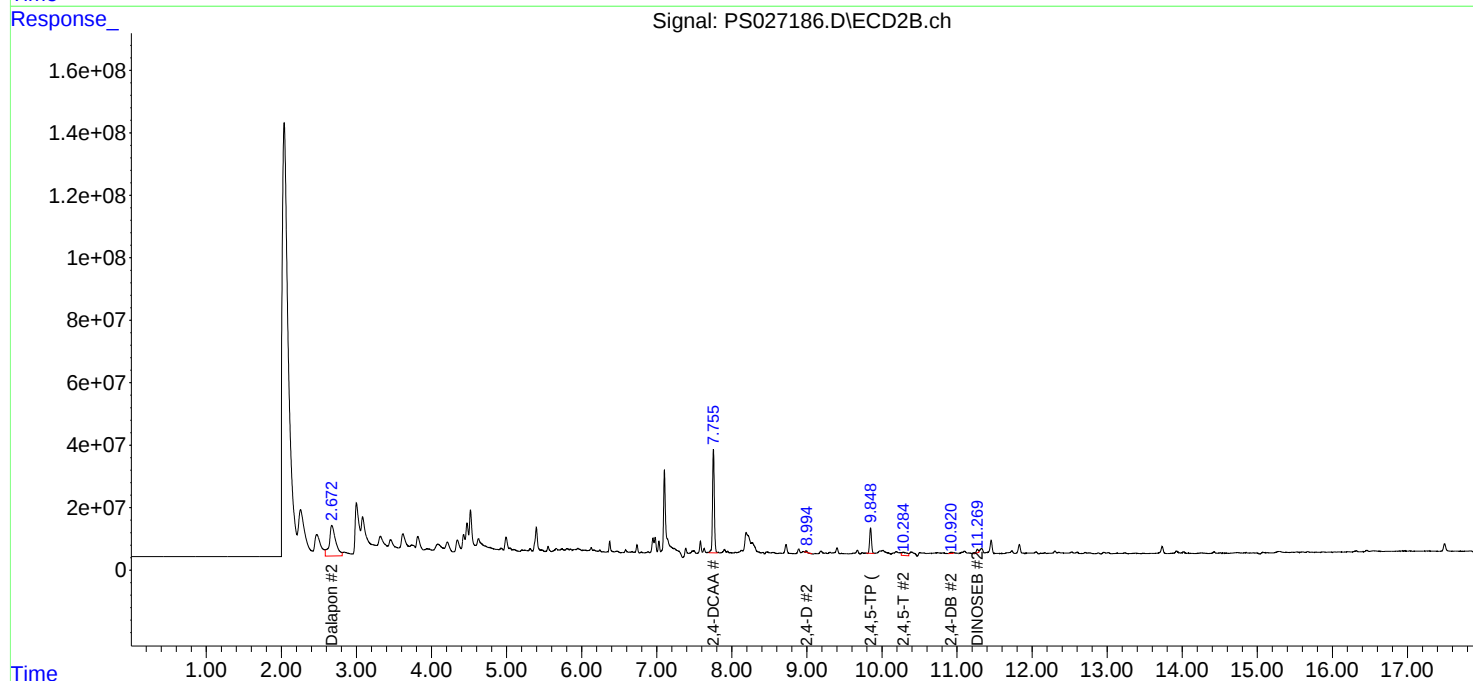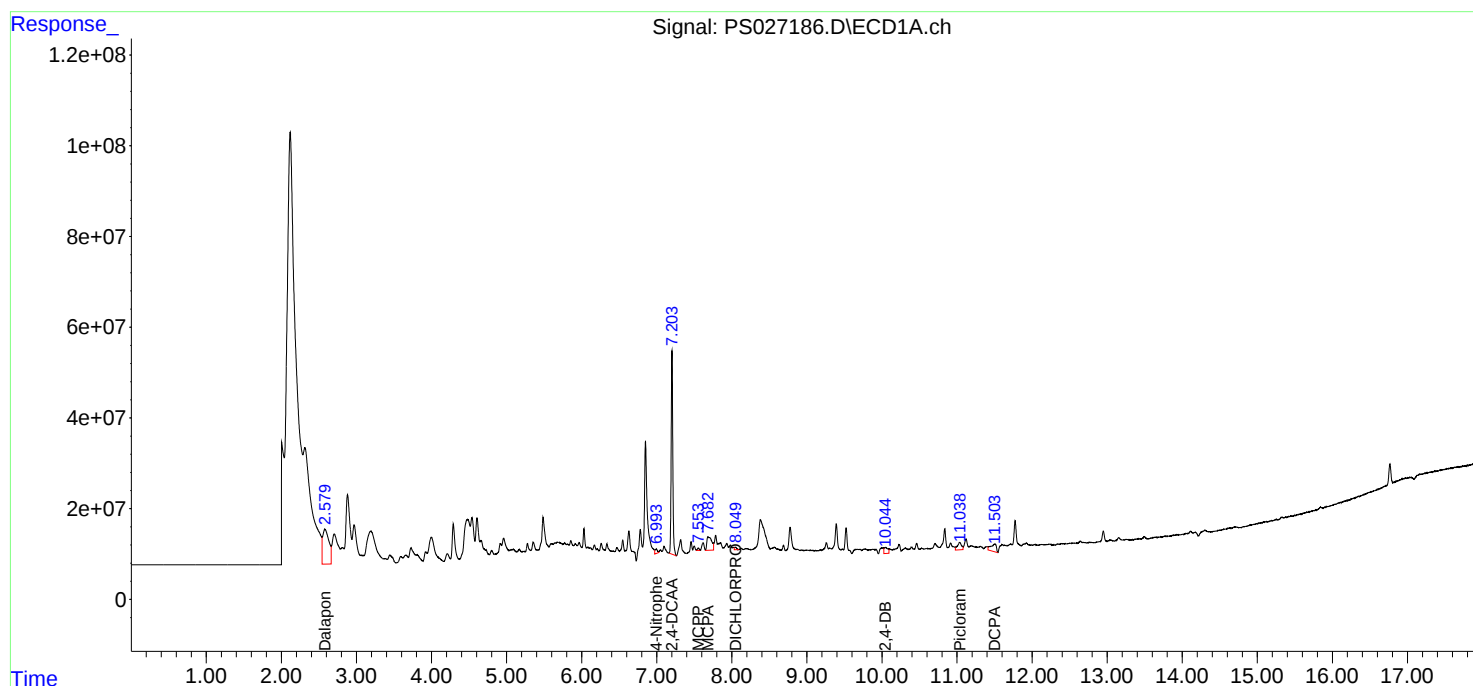


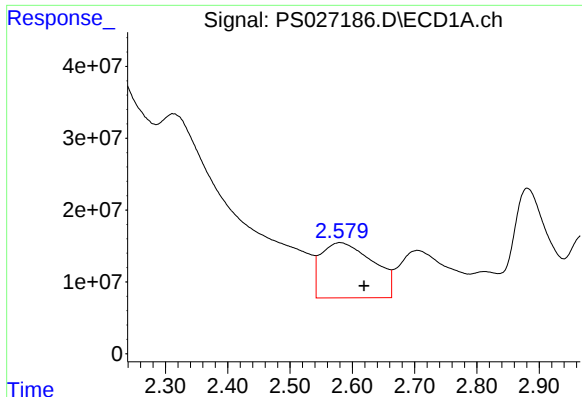

#1 Dalapon


R.T.: 2.579 min
Delta R.T.: -0.040 min
Response: 445493139
Conc: 134.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
WC-CTW2-BL-03

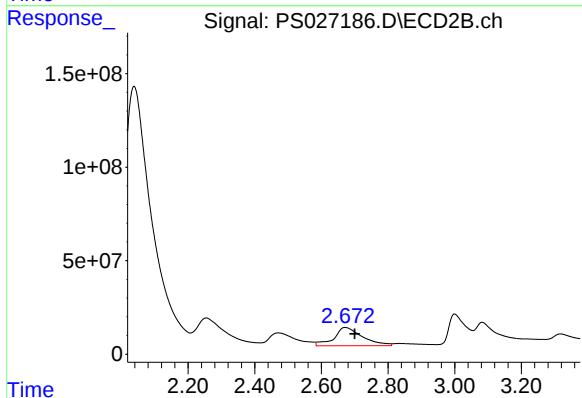


#1 Dalapon

R.T.: 2.671 min
Delta R.T.: -0.029 min
Response: 579512394
Conc: 139.64 ng/ml

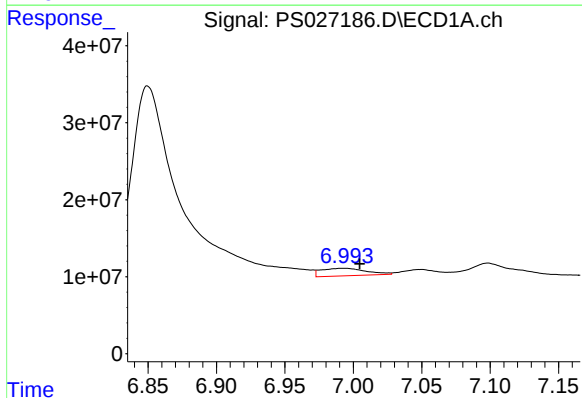


#3 4-Nitrophenol

R.T.: 6.993 min
Delta R.T.: -0.012 min
Response: 22458305
Conc: 14.01 ng/ml

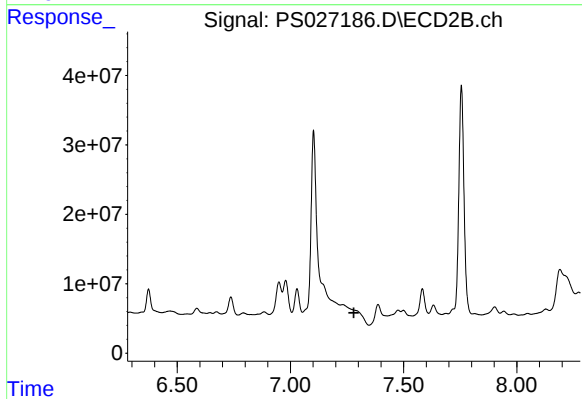

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 7.280 min
Response: 0
Conc: N.D.

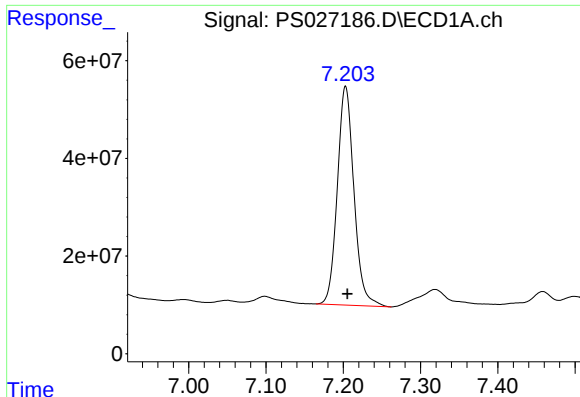

#4 2,4-DCAA


R.T.: 7.203 min
Delta R.T.: -0.002 min
Response: 670633163
Conc: 265.20 ng/ml

Instrument :
ECD_S
ClientSampleId :
WC-CTW2-BL-03

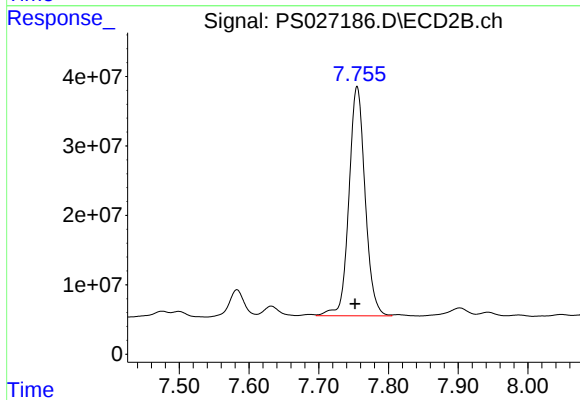


#4 2,4-DCAA

R.T.: 7.755 min
Delta R.T.: 0.003 min
Response: 532125638
Conc: 229.49 ng/ml

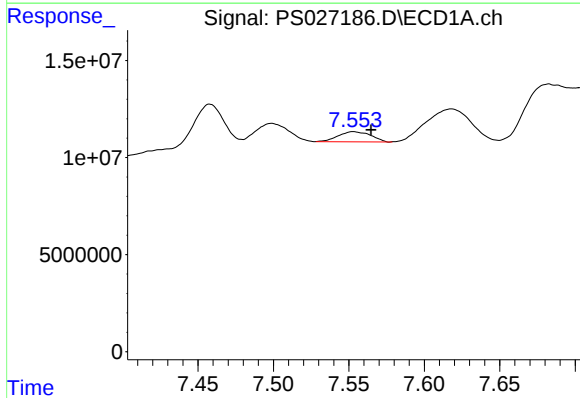


#6 MCP

R.T.: 7.553 min
Delta R.T.: -0.011 min
Response: 7756509
Conc: 1.01 ug/ml

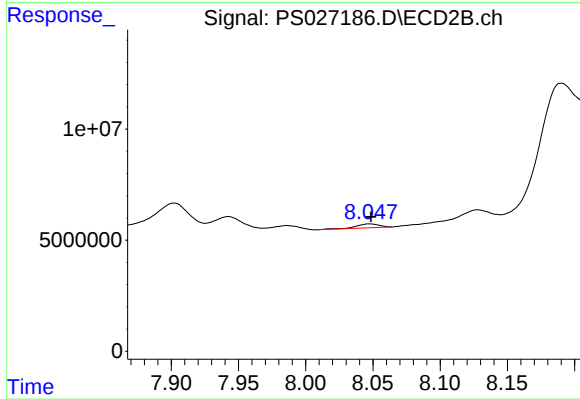

#6 MCP


R.T.: 8.048 min
Delta R.T.: -0.001 min
Response: 2130577
Conc: N.D.

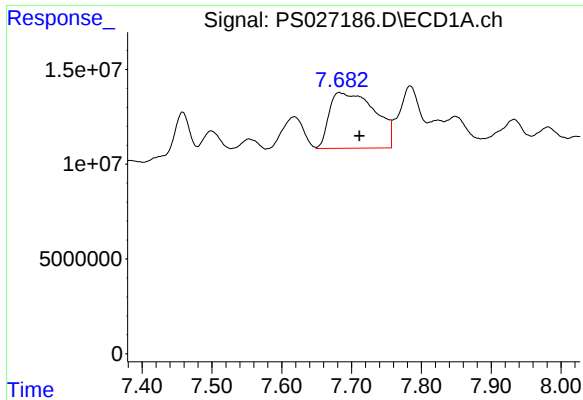

#7 MCPA


R.T.: 7.683 min
Delta R.T.: -0.028 min
Response: 133653544
Conc: 13.12 ug/ml

Instrument :
ECD_S
ClientSampleId :
WC-CTW2-BL-03

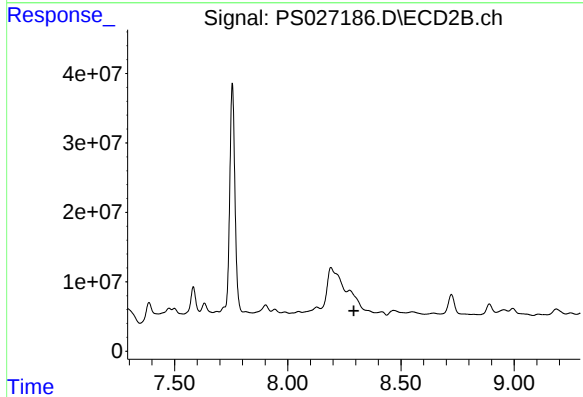


#7 MCPA

R.T.: 8.273 min
Delta R.T.: -0.019 min
Response: -28501702
Conc: N.D.

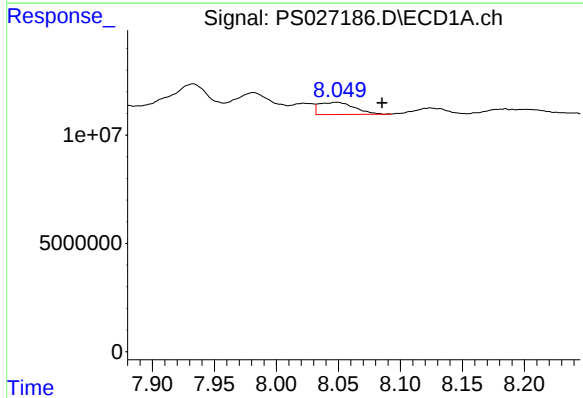


#8 DICHLORPROP

R.T.: 8.048 min
Delta R.T.: -0.037 min
Response: 11068986
Conc: 4.13 ng/ml

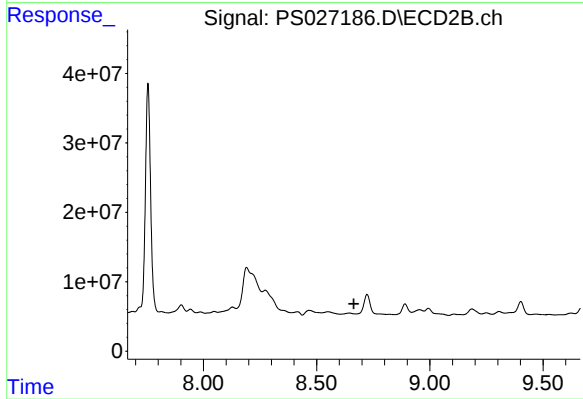

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.664 min
Response: 0
Conc: N.D.

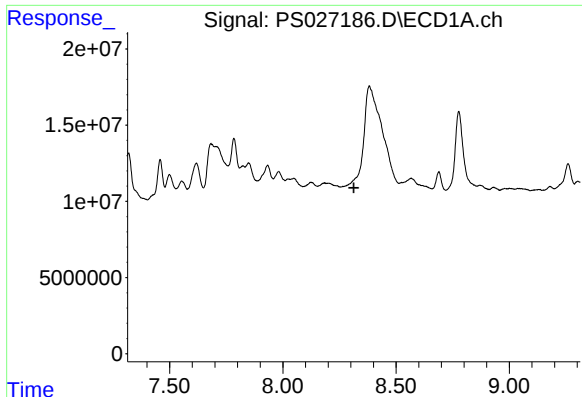

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.314 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
WC-CTW2-BL-03

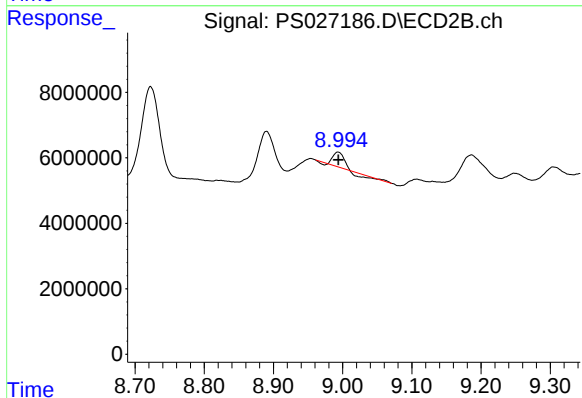


#9 2,4-D

R.T.: 8.993 min
Delta R.T.: 0.000 min
Response: 2963875
Conc: 1.03 ng/ml

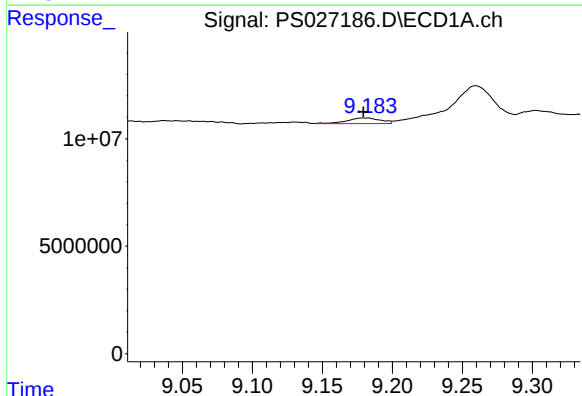


#11 2,4,5-TP (SILVEX)

R.T.: 9.180 min
Delta R.T.: 0.000 min
Response: 4295738
Conc: N.D.

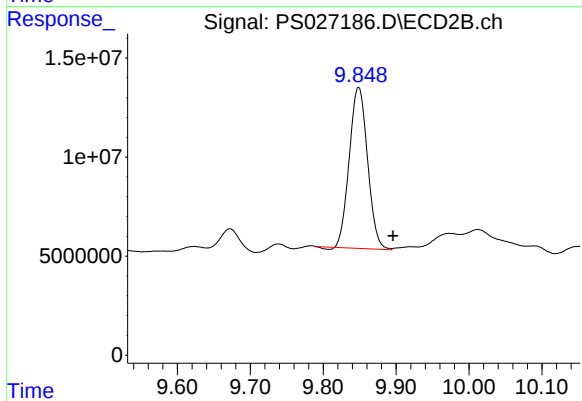

#11 2,4,5-TP (SILVEX)


R.T.: 9.848 min
Delta R.T.: -0.048 min
Response: 140928487
Conc: 8.84 ng/ml

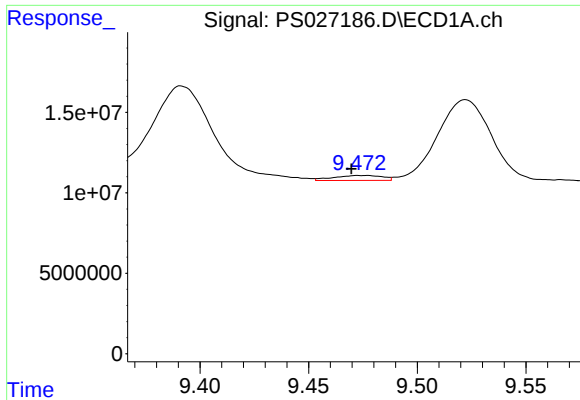

#12 2,4,5-T


R.T.: 9.475 min
Delta R.T.: 0.005 min
Response: 4815707
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
WC-CTW2-BL-03

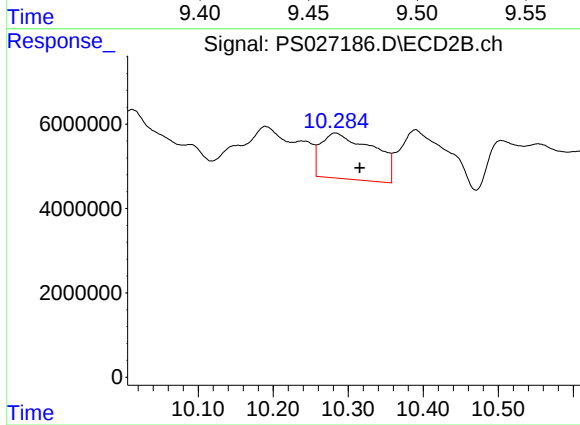


#12 2,4,5-T

R.T.: 10.283 min
Delta R.T.: -0.032 min
Response: 52558660
Conc: 3.29 ng/ml

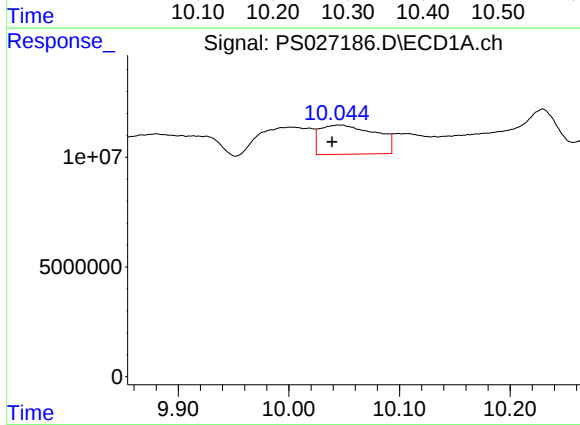


#13 2,4-DB

R.T.: 10.045 min
Delta R.T.: 0.006 min
Response: 46623254
Conc: 21.58 ng/ml

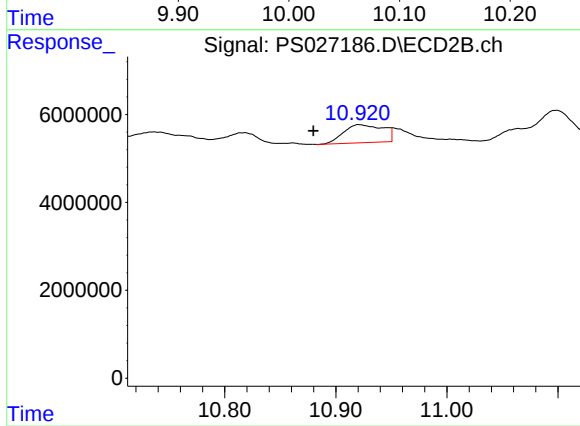

#13 2,4-DB


R.T.: 10.922 min
Delta R.T.: 0.042 min
Response: 10356074
Conc: 5.12 ng/ml

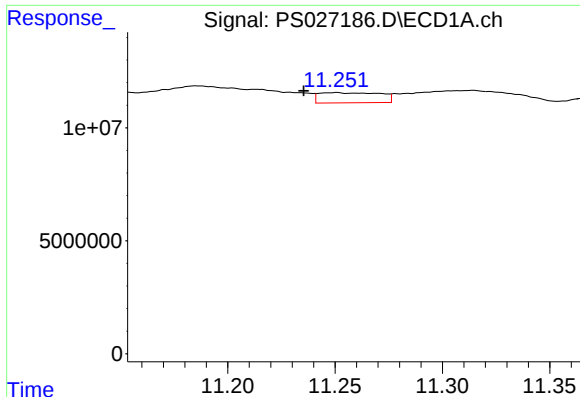

#14 DINOSEB


R.T.: 11.250 min
Delta R.T.: 0.014 min
Response: 8895095
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
WC-CTW2-BL-03

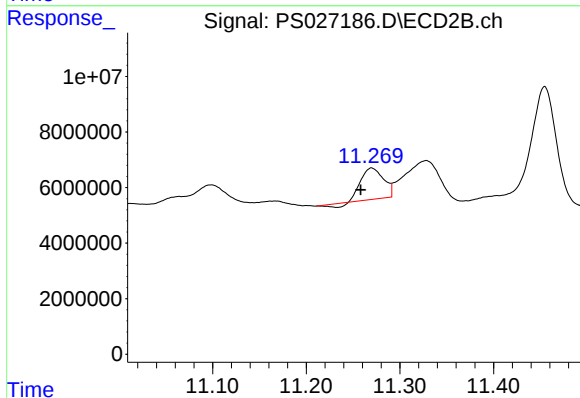


#14 DINOSEB

R.T.: 11.270 min
Delta R.T.: 0.012 min
Response: 17836352
Conc: 1.60 ng/ml

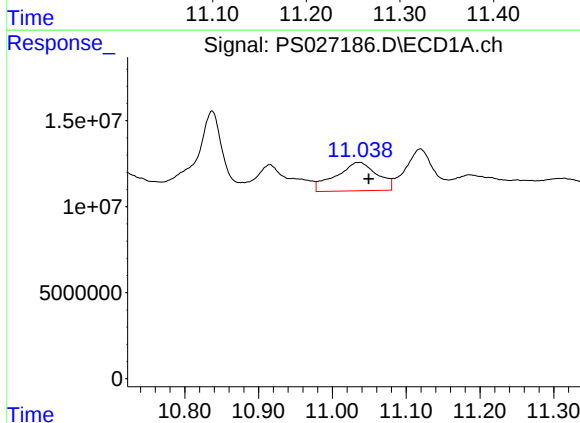


#15 Picloram

R.T.: 11.036 min
Delta R.T.: -0.014 min
Response: 64056915
Conc: 3.29 ng/ml

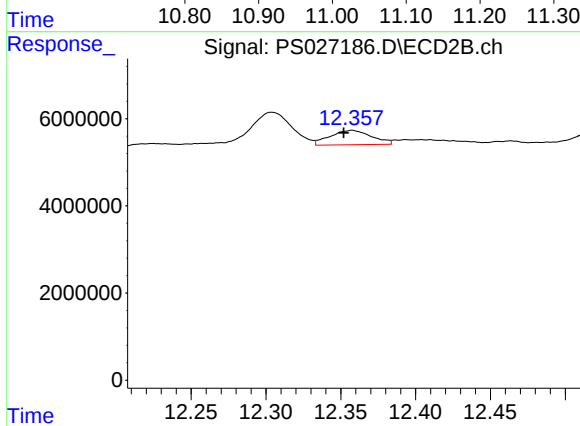

#15 Picloram


R.T.: 12.357 min
Delta R.T.: 0.005 min
Response: 6447193
Conc: N.D.

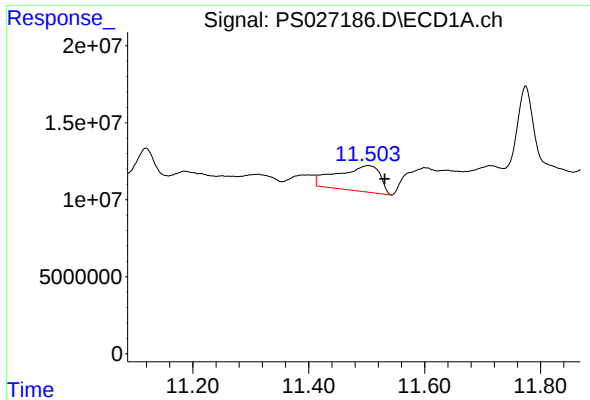

#16 DCPA

R.T.: 11.502 min
Delta R.T.: -0.029 min
Response: 85277609
Conc: 4.75 ng/ml

Instrument :
ECD_S
ClientSampleId :
WC-CTW2-BL-03

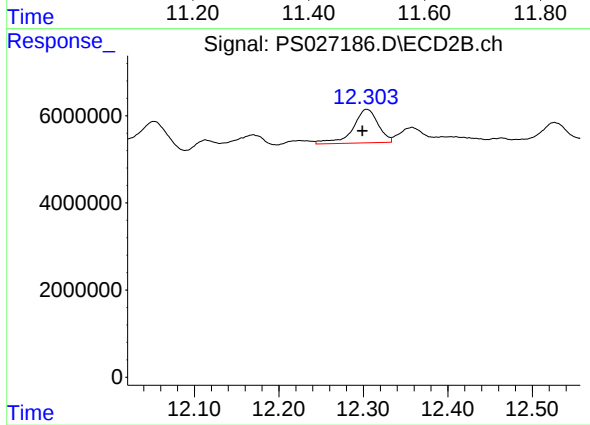

#16 DCPA

R.T.: 12.304 min
Delta R.T.: 0.005 min
Response: 16037700
Conc: N.D.