

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071724\
 Data File : PS027179.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jul 2024 10:41
 Operator : AR\AJ
 Sample : HSTDCCC750
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDCCC750

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 07/19/2024
 Supervised By :Ankita Jodhani 07/19/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 18 02:58:31 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071224.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 27 04:33:52 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.203	7.753	1924.6E6	1685.9E6	761.087	727.078
Target Compounds							
1) T	Dalapon	2.616	2.702	2311.7E6	2770.3E6	695.343	667.517
2) T	3,5-DICHL...	6.379	6.706	2828.5E6	2295.3E6	715.215m	676.730
3) T	4-Nitroph...	7.003	7.281	1167.1E6	1099.7E6	728.001	665.052
5) T	DICAMBA	7.387	7.952	7877.2E6	7379.4E6	716.936	700.364
6) T	MCPD	7.567	8.054	567.3E6	539.5E6	73.910	69.639
7) T	MCPA	7.714	8.299	746.3E6	719.9E6	73.238	68.766
8) T	DICHLORPROP	8.084	8.666	1925.2E6	1806.0E6	717.464	698.308m
9) T	2,4-D	8.311	8.995	2134.4E6	2032.5E6	741.848	704.929m
10) T	Pentachlo...	8.605	9.524	29632.7E6	28177.1E6	749.985	722.086
11) T	2,4,5-TP ...	9.178	9.898	11234.9E6	11317.2E6	742.197	709.679
12) T	2,4,5-T	9.467	10.317	11313.7E6	11353.2E6	765.427	710.520
13) T	2,4-DB	10.037	10.882	1647.0E6	1418.2E6	762.174	701.742
14) T	DINOSEB	11.233	11.260	8282.8E6	8049.5E6	735.437m	720.516m
15) T	Picloram	11.047	12.354	15197.1E6	16785.1E6	780.178	717.863
16) T	DCPA	11.528	12.302	13536.0E6	12485.8E6	753.974	713.725

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071724\
Data File : PS027179.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jul 2024 10:41
Operator : AR\AJ
Sample : HSTDCCC750
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :

ECD_S

ClientSampleId :

HSTDCCC750



Manual Integrations

APPROVED

Reviewed By :Abdul Mirza 07/19/2024
Supervised By :Ankita Jodhani 07/19/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 18 02:58:31 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071224.M
Quant Title : 8080.M
QLast Update : Thu Jun 27 04:33:52 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

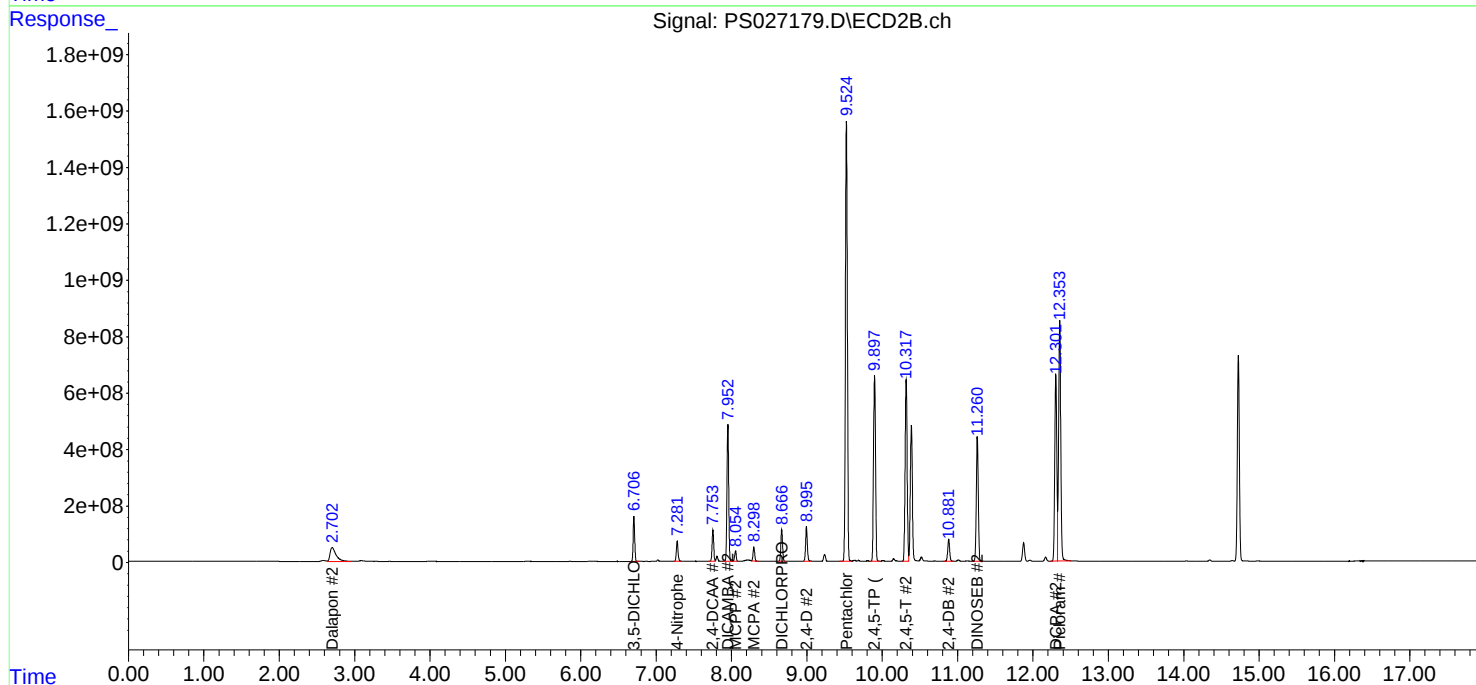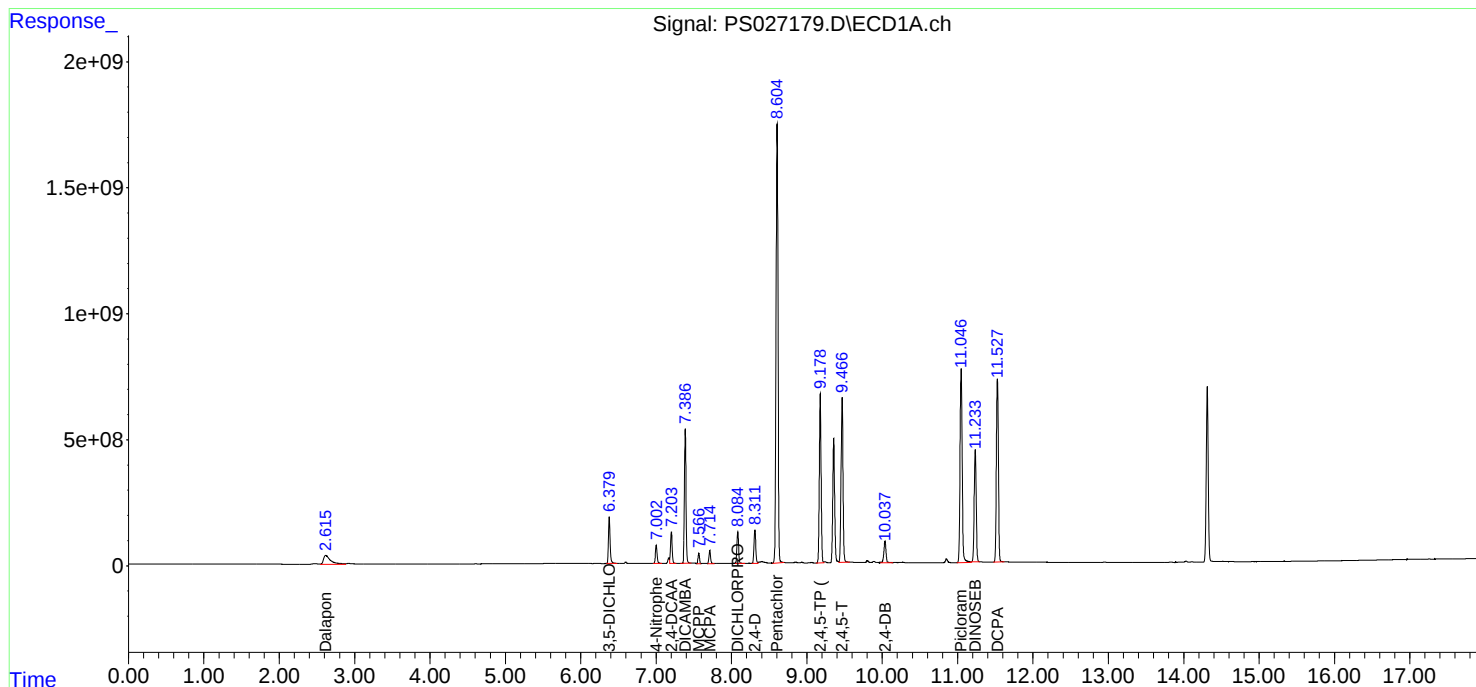

Instrument :
ECD_S
ClientSampleId :
HSTDCCCT50

**Manual Integrations
APPROVED**

Reviewed By :Abdul Miza 07/19/2024
Supervised By :Ankita Jodhani 07/19/2024

The printer must be in Portrait mode.