

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071724\
 Data File : PS027181.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jul 2024 11:48
 Operator : AR\AJ
 Sample : PB162109BS
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB162109BS

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 07/19/2024
 Supervised By :Ankita Jodhani 07/19/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 18 03:11:33 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071224.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 27 04:33:52 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.203	7.754	1397.6E6	1189.6E6	552.689	513.021
Target Compounds							
1) T	Dalapon	2.618	2.701	1582.4E6	1986.9E6	475.962	478.757
2) T	3,5-DICHL...	6.379	6.706	2029.5E6	1642.8E6	513.194m	484.369
3) T	4-Nitroph...	7.003	7.281	830.8E6	762.9E6	518.245	461.392
5) T	DICAMBA	7.387	7.953	5655.0E6	5093.7E6	514.681	483.436
6) T	MCPD	7.565	8.052	383.9E6	356.1E6	50.013	45.969
7) T	MCPA	7.712	8.296	511.7E6	478.4E6	50.218	45.698
8) T	DICHLORPROP	8.084	8.666	1402.6E6	1281.2E6	522.682	495.401m
9) T	2,4-D	8.311	8.995	1552.2E6	1446.9E6	539.496	501.828m
10) T	Pentachlo...	8.605	9.524	21505.1E6	20350.3E6	544.280	521.512
11) T	2,4,5-TP ...	9.178	9.898	8152.7E6	8167.6E6	538.578	512.175
12) T	2,4,5-T	9.467	10.317	8157.1E6	8139.2E6	551.868	509.377
13) T	2,4-DB	10.037	10.881	1176.2E6	996.2E6	544.306	492.944
14) T	DINOSEB	11.233	11.260	6039.0E6	5706.7E6	536.209	510.813
15) T	Picloram	11.045	12.354	10555.3E6	11812.1E6	541.881m	505.180
16) T	DCPA	11.528	12.301	9768.3E6	9082.3E6	544.112	519.170

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071724\
Data File : PS027181.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jul 2024 11:48
Operator : AR\AJ
Sample : PB162109BS
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :

ECD_S

ClientSampleId :

PB162109BS



Manual Integrations

APPROVED

Reviewed By :Abdul Mirza 07/19/2024
Supervised By :Ankita Jodhani 07/19/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 18 03:11:33 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071224.M
Quant Title : 8080.M
QLast Update : Thu Jun 27 04:33:52 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

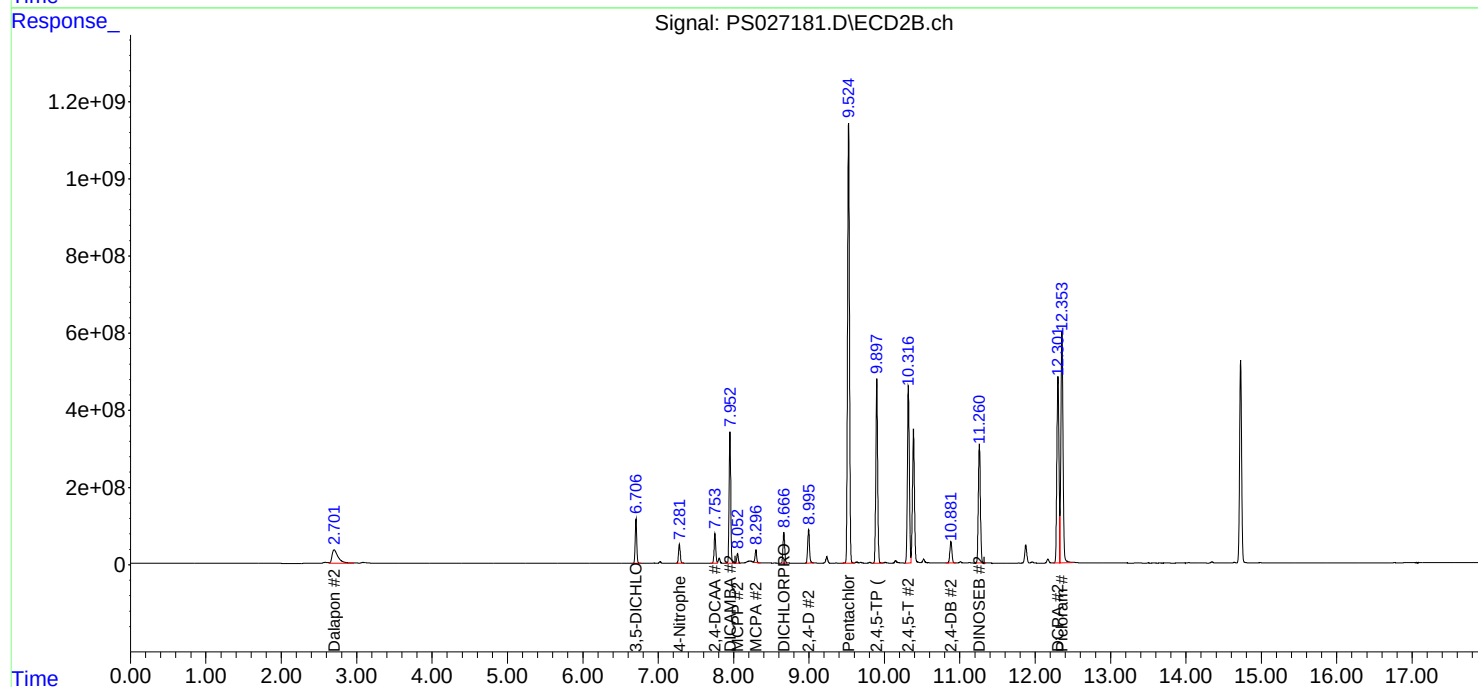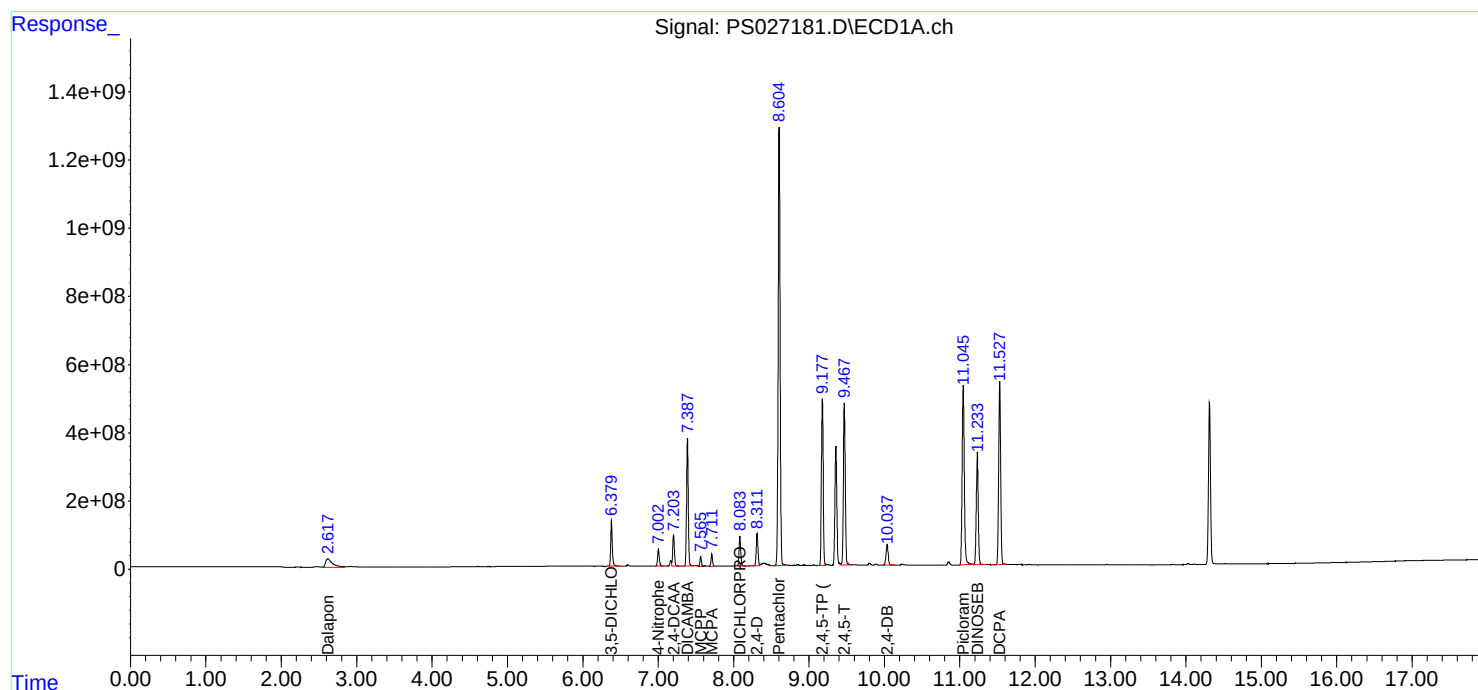

Instrument :
ECD_S
ClientSampleId :
PB162109BS

**Manual Integrations
APPROVED**

Reviewed By :Abdul Mirza 07/19/2024
Supervised By :Ankita Jodhani 07/19/2024

The printer must be in Portrait mode.