

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071724\
 Data File : PS027183.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jul 2024 12:37
 Operator : AR\AJ
 Sample : P3246-02MS
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 WC-CTW2-BL-01MS

Manual Integrations
 APPROVED

Reviewed By :Abdul
 Mirza
 07/18/2024

Supervised By :Ankita
 Jodhani
 07/19/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 18 03:13:27 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071224.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 27 04:33:52 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	7.203	7.754	504.8E6	393.5E6	199.604m	169.715
Target Compounds						
1) T Dalapon	2.617	2.702	618.6E6	1530.7E6	186.057m	368.840m#
2) T 3,5-DICHL...	6.380	6.707	1270.2E6	1043.0E6	321.178	307.507
5) T DICAMBA	7.387	7.954	4127.0E6	3954.7E6	375.615	375.337m
6) T MCPP	7.564	8.053	326.0E6	281.1E6	42.474m	36.290
7) T MCPA	7.710	8.296	408.5E6	492.1E6	40.084m	47.005m
8) T DICHLORPROP	8.083	8.667	1179.0E6	1075.6E6	439.370	415.895m
9) T 2,4-D	8.311	8.997	1526.9E6	1368.5E6	530.723	474.643
10) T Pentachlo...	8.604	9.525	6845.3E6	6569.1E6	173.251	168.343
11) T 2,4,5-TP ...	9.177	9.900	7110.7E6	13088.7E6	469.744	820.770 #
12) T 2,4,5-T	9.466	10.317	6781.5E6	6813.8E6	458.799m	426.429m
13) T 2,4-DB	10.036	10.882	873.3E6	819.6E6	404.149m	405.572
14) T DINOSEB	11.232	11.261	1385.5E6	1494.9E6	123.021	133.813
15) T Picloram	11.045	12.353	7775.6E6	8578.1E6	399.176	366.866
16) T DCPA	11.526	12.302	8881.2E6	8444.3E6	494.696	482.703

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071724\
Data File : PS027183.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jul 2024 12:37
Operator : AR\AJ
Sample : P3246-02MS
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
WC-CTW2-BL-01MS

Manual Integrations
APPROVED

Reviewed By :Abdul
Mirza
07/18/2024
Supervised By :Ankita
Jodhani
07/19/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 18 03:13:27 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071224.M
Quant Title : 8080.M
QLast Update : Thu Jun 27 04:33:52 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

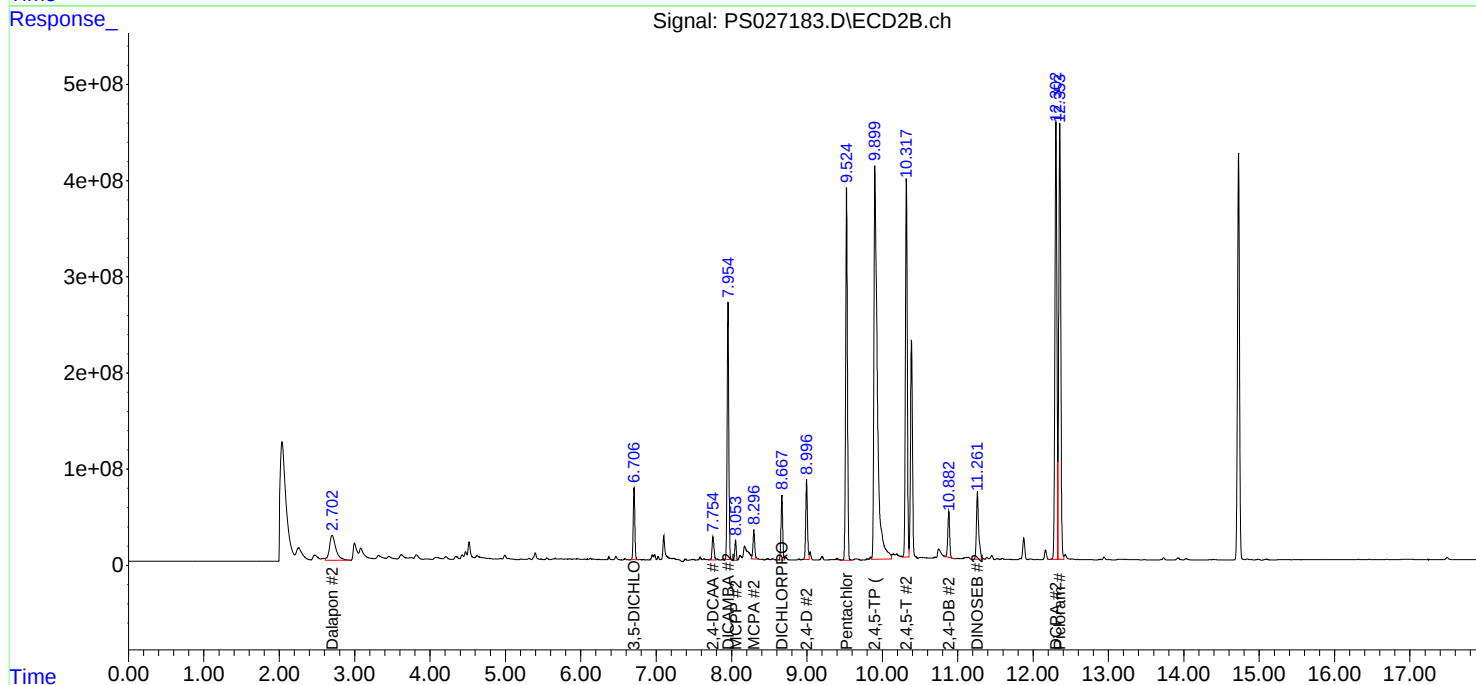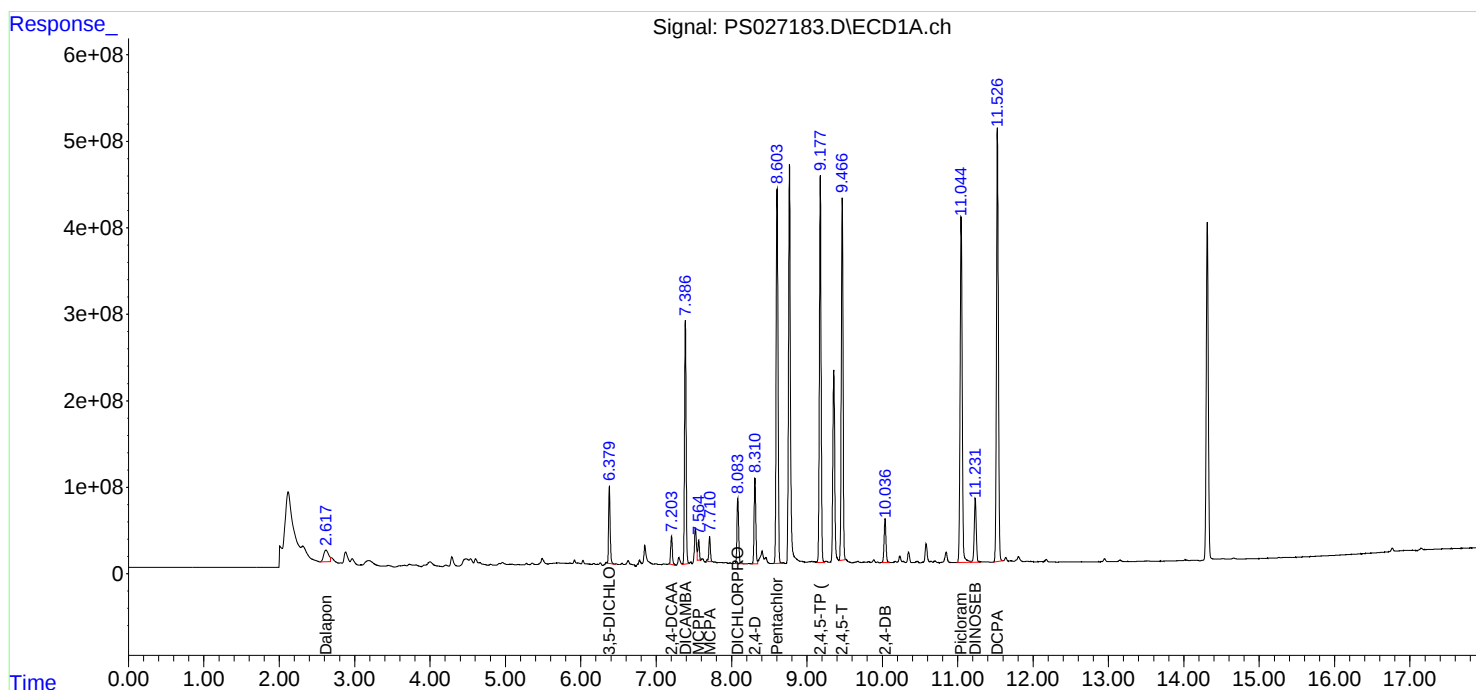

Instrument :
ECD_S
ClientSampled :
WC-CTW2-BL-01MS

**Manual Integrations
APPROVED**

Reviewed By :Abdul
Mitza
07/18/2024

Supervised By :Ankita
Jodhani
07/19/2024

The printer must be in Portrait mode.