

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071724\
 Data File : PS027184.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jul 2024 13:01
 Operator : AR\AJ
 Sample : P3246-02MSD
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 WC-CTW2-BL-01MSD

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 07/18/2024
 Supervised By :Ankita Jodhani 07/19/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 18 03:14:27 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071224.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 27 04:33:52 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.204	7.754	538.1E6	386.6E6	212.795m	166.719m
Target Compounds							
1) T	Dalapon	2.616	2.701	616.7E6	1483.1E6	185.481m	357.357m#
2) T	3,5-DICHL...	6.380	6.707	1255.3E6	1026.4E6	317.426	302.623
5) T	DICAMBA	7.387	7.954	4086.6E6	3953.9E6	371.939	375.260m
6) T	MCPD	7.563	8.053	323.3E6	283.0E6	42.121m	36.527m
7) T	MCPA	7.711	8.296	406.7E6	494.7E6	39.913m	47.253m
8) T	DICHLORPROP	8.083	8.666	1147.9E6	1076.3E6	427.780m	416.173m
9) T	2,4-D	8.311	8.996	1518.5E6	1363.9E6	527.797	473.049
10) T	Pentachlo...	8.604	9.525	6730.1E6	6538.5E6	170.335	167.561
11) T	2,4,5-TP ...	9.177	9.900	7002.0E6	13213.9E6	462.562m	828.623m#
12) T	2,4,5-T	9.466	10.317	6759.4E6	6776.1E6	457.308m	424.068m
13) T	2,4-DB	10.037	10.882	855.1E6	903.5E6	395.736m	447.067m
14) T	DINOSEB	11.232	11.261	1311.5E6	1470.0E6	116.452m	131.581
15) T	Picloram	11.045	12.353	7728.6E6	8435.0E6	396.765	360.745
16) T	DCPA	11.527	12.302	8804.8E6	8291.8E6	490.441	473.984

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071724\
Data File : PS027184.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jul 2024 13:01
Operator : AR\AJ
Sample : P3246-02MSD
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
WC-CTW2-BL-01MSD

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/18/2024
Supervised By :Ankita Jodhani 07/19/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 18 03:14:27 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071224.M
Quant Title : 8080.M
QLast Update : Thu Jun 27 04:33:52 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

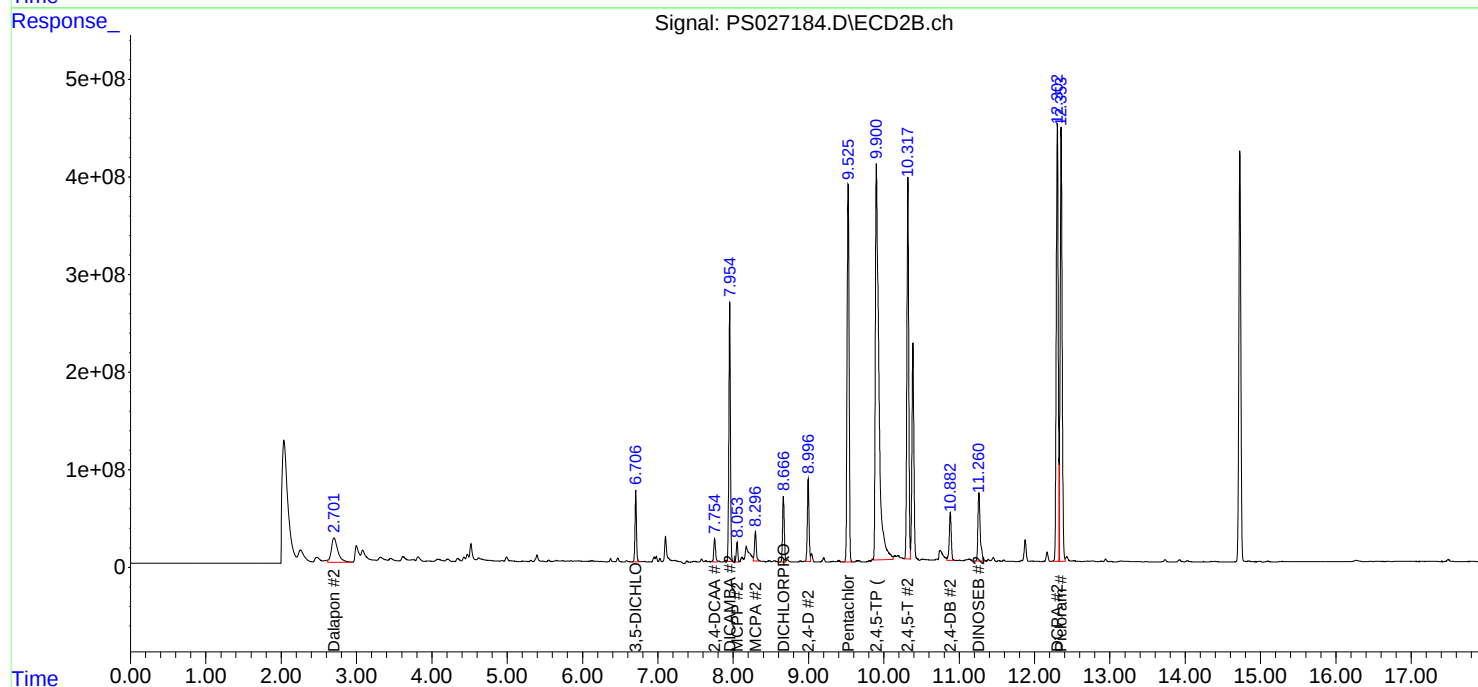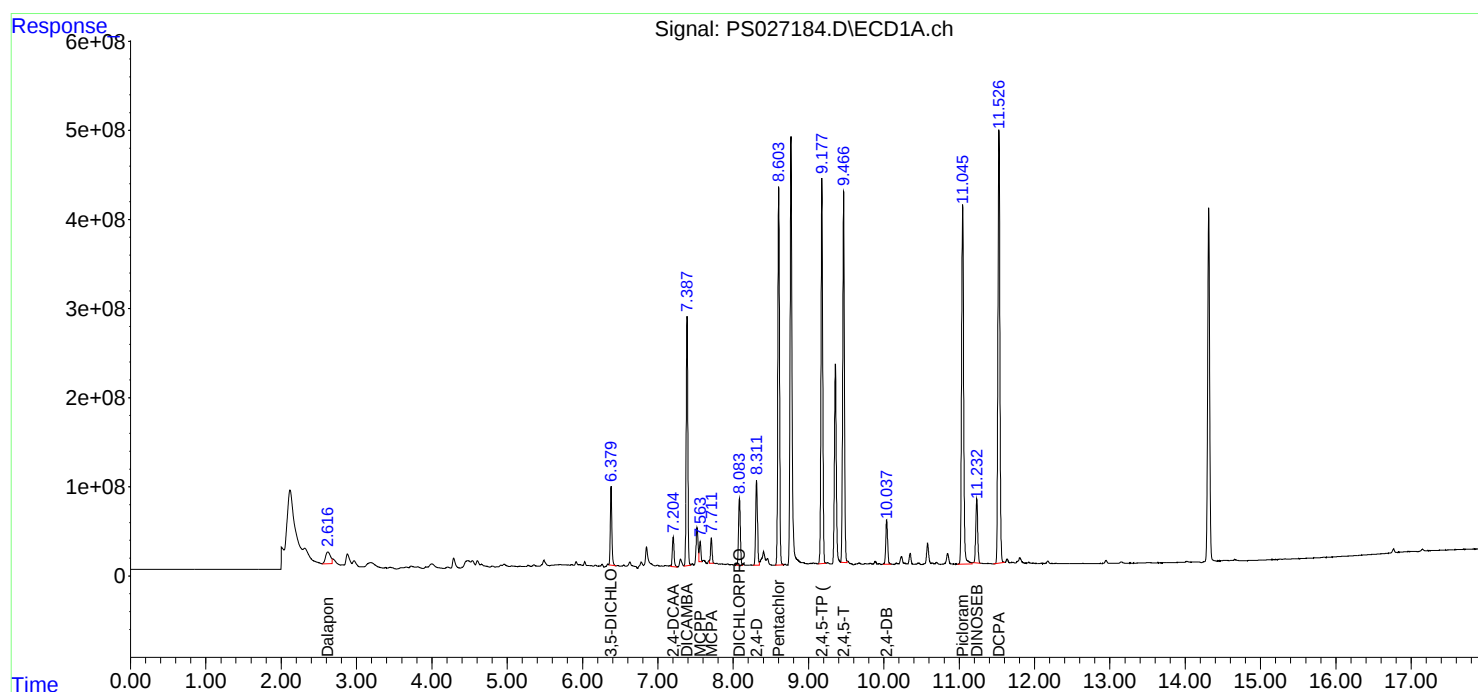

Instrument :
ECD_S
ClientSampleId :
WC-CTW2-BL-01MSD

**Manual Integrations
APPROVED**

Reviewed By :Abdul Miiza 07/18/2024
Supervised By :Ankita Jodhani 07/19/2024

The printer must be in Portrait mode.