

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS071724\  
 Data File : PS027185.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 17 Jul 2024 13:26  
 Operator : AR\AJ  
 Sample : P3246-07  
 Misc :  
 ALS Vial : 9 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :  
 WC-CTW2-BL-02

Manual Integrations  
 APPROVED

Reviewed By :Abdul Mirza 07/18/2024  
 Supervised By :Ankita Jodhani 07/19/2024

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Jul 18 03:15:46 2024  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS071224.M  
 Quant Title : 8080.M  
 QLast Update : Thu Jun 27 04:33:52 2024  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

|      |          |       |       |         |         |         |          |
|------|----------|-------|-------|---------|---------|---------|----------|
| 4) S | 2,4-DCAA | 7.204 | 7.754 | 602.3E6 | 456.8E6 | 238.186 | 197.016m |
|------|----------|-------|-------|---------|---------|---------|----------|

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS071724\  
Data File : PS027185.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 17 Jul 2024 13:26  
Operator : AR\AJ  
Sample : P3246-07  
Misc :  
ALS Vial : 9 Sample Multiplier: 1



Instrument :  
ECD\_S  
ClientSampleId :  
WC-CTW2-BL-02

Manual Integrations  
APPROVED

Reviewed By : Abdul Mirza 07/18/2024  
Supervised By : Ankita Jodhani 07/19/2024

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Jul 18 03:15:46 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS071224.M  
Quant Title : 8080.M  
QLast Update : Thu Jun 27 04:33:52 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

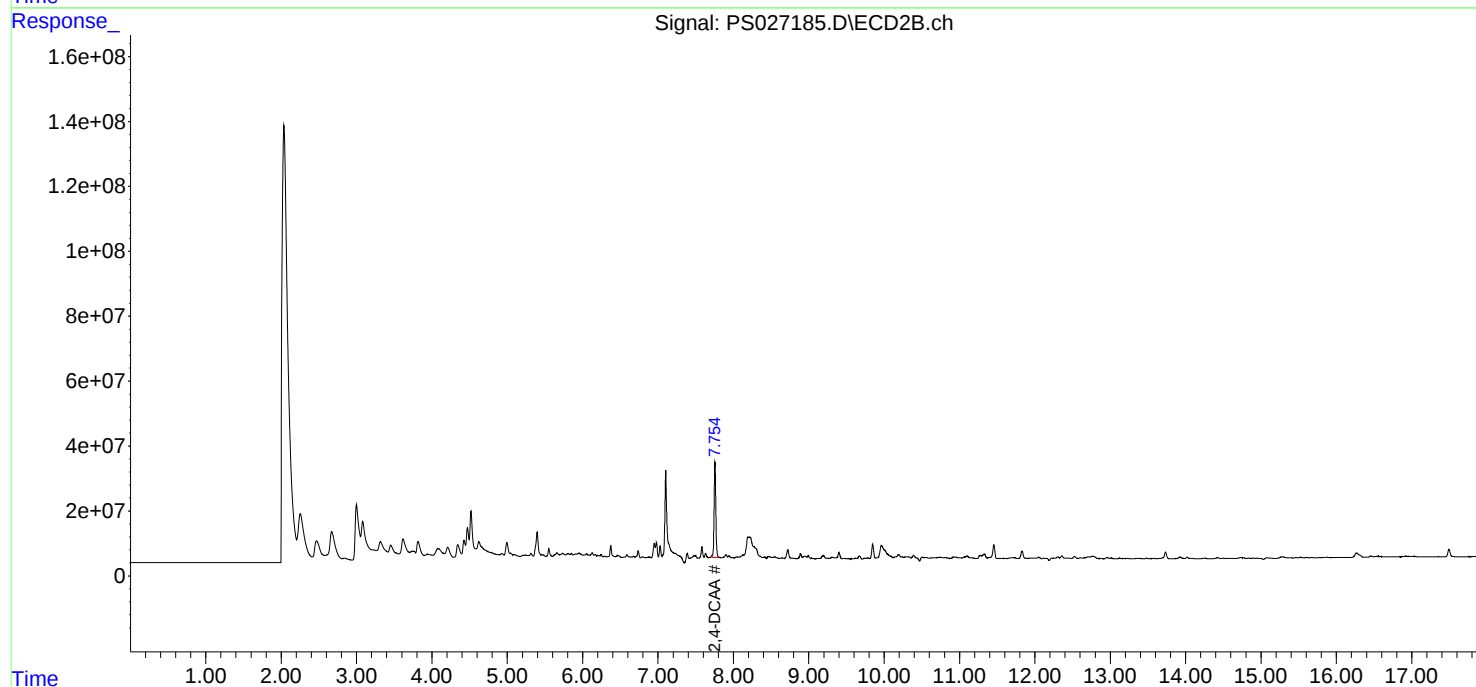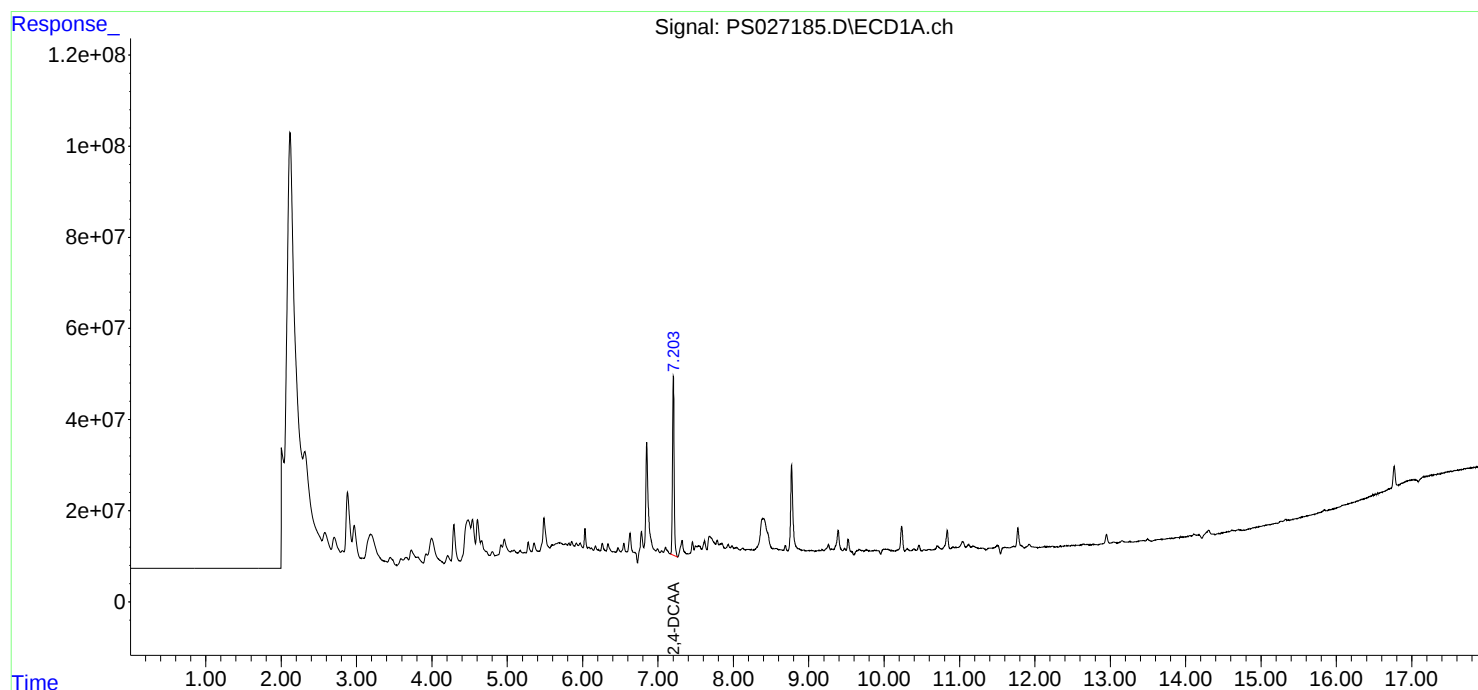

**Instrument :**  
ECD\_S  
**ClientSampled :**  
WC-CTW2-BL-02

**Manual Integrations  
APPROVED**

Reviewed By :Abdul Miza    07/18/2024  
Supervised By :Ankita Jodhani    07/19/2024

The printer must be in Portrait mode.