

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071818\
 Data File : PS001122.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jul 2018 11:47
 Operator : UA
 Sample : J3819-08
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 18 12:12:49 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 09 02:00:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.664	11.077	35558983	30238155	172.349	138.836
Target Compounds							
2) T	3,5-DICHL...	0.000	9.162	0	5812409	N.D.	19.760 #
5) T	DICAMBA	0.000	11.321	0	4969723	N.D.	6.331 #
6) T	MCP	12.355	0.000	7823713	0	14.243	N.D. #
8) T	DICHLORPROP	0.000	12.445	0	1279938	N.D.	6.337 #
15) T	Picloram	0.000	17.019	0	83906	N.D.	0.055 #
16) T	DCPA	0.000	17.019	0	83906	N.D.	0.049 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071818\
Data File : PS001122.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jul 2018 11:47
Operator : UA
Sample : J3819-08
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 18 12:12:49 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
Quant Title : 8080.M
QLast Update : Mon Jul 09 02:00:25 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

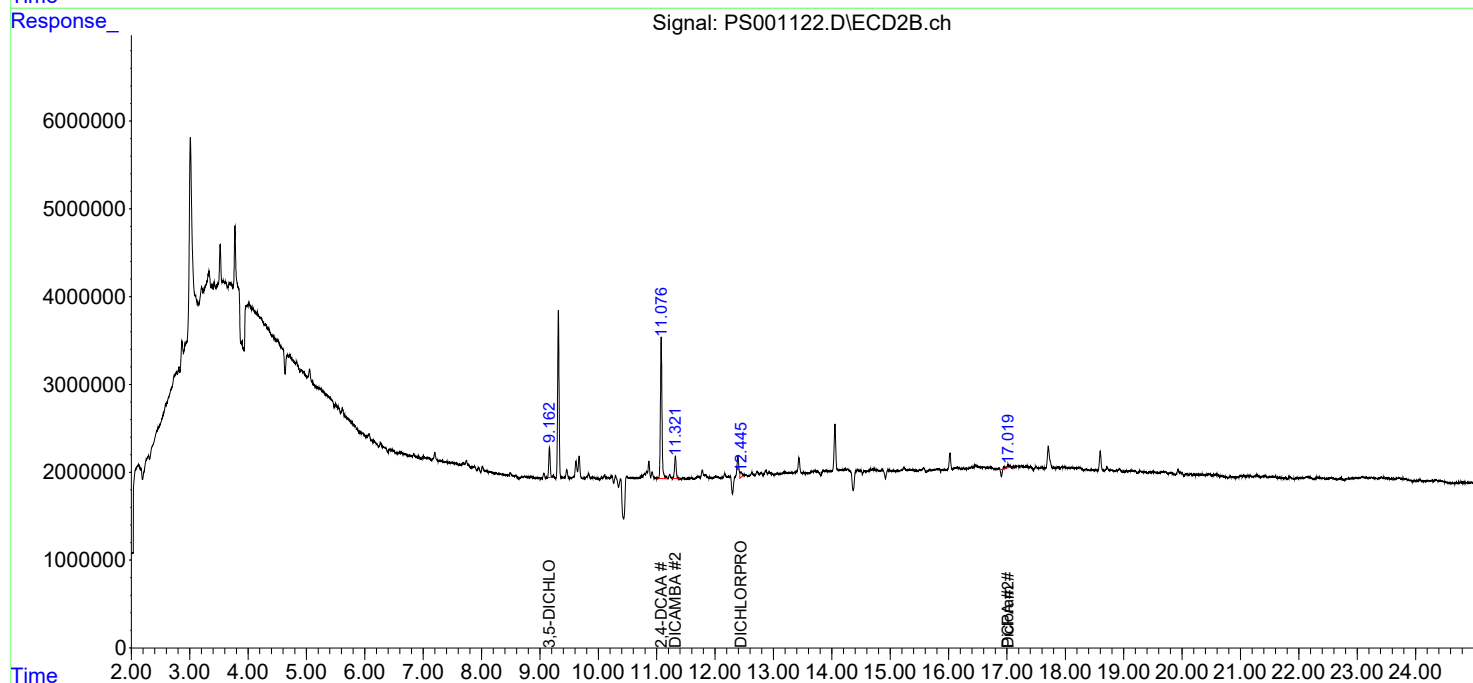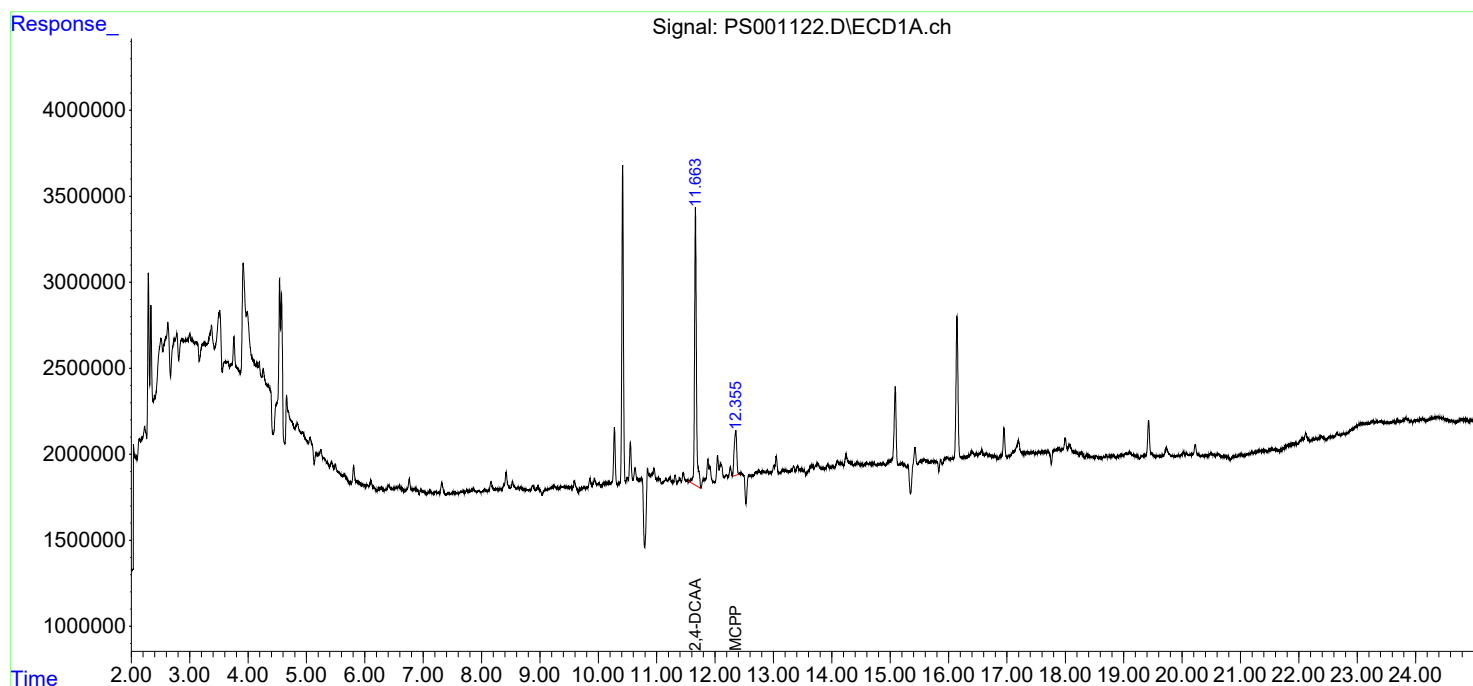


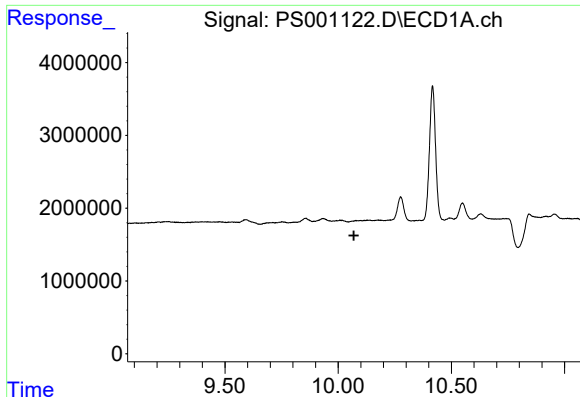

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 10.070 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

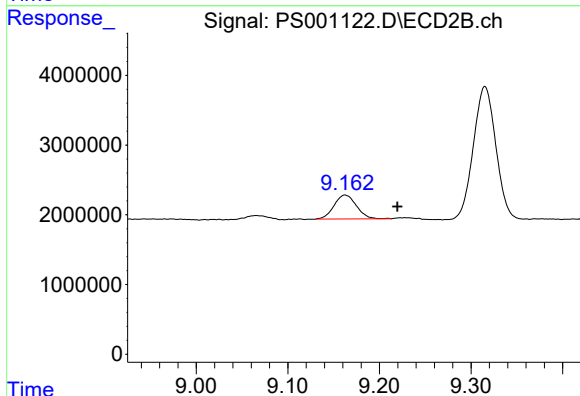


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.162 min
Delta R.T.: -0.057 min
Response: 5812409
Conc: 19.76 ng/ml

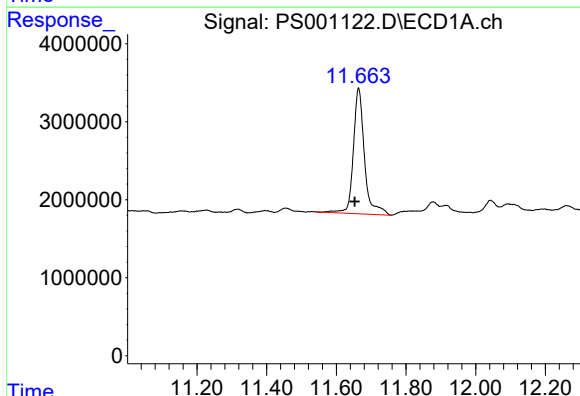


#4 2,4-DCAA

R.T.: 11.664 min
Delta R.T.: 0.010 min
Response: 35558983
Conc: 172.35 ng/ml

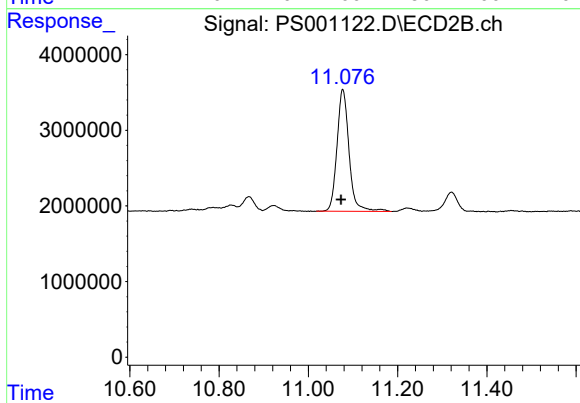

#4 2,4-DCAA


R.T.: 11.077 min
Delta R.T.: 0.004 min
Response: 30238155
Conc: 138.84 ng/ml

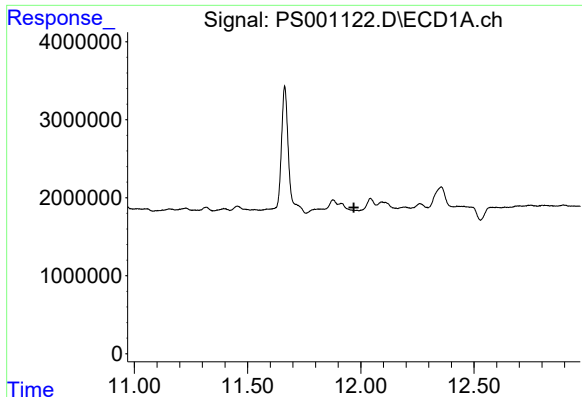

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.970 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

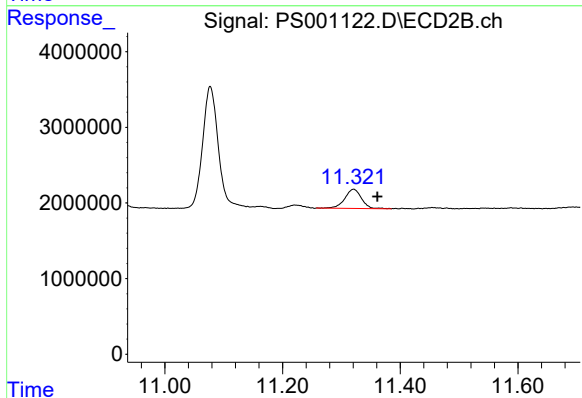


#5 DICAMBA

R.T.: 11.321 min
Delta R.T.: -0.040 min
Response: 4969723
Conc: 6.33 ng/ml

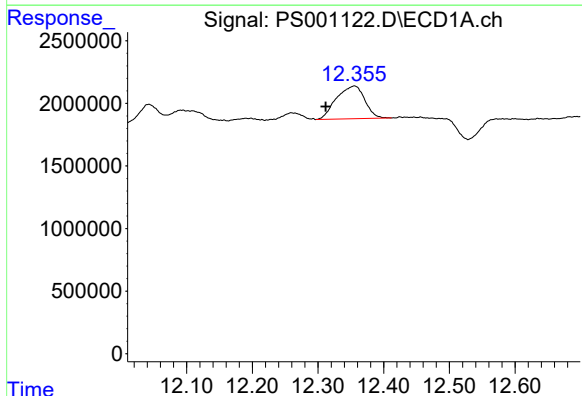


#6 MCP

R.T.: 12.355 min
Delta R.T.: 0.043 min
Response: 7823713
Conc: 14.24 ug/ml

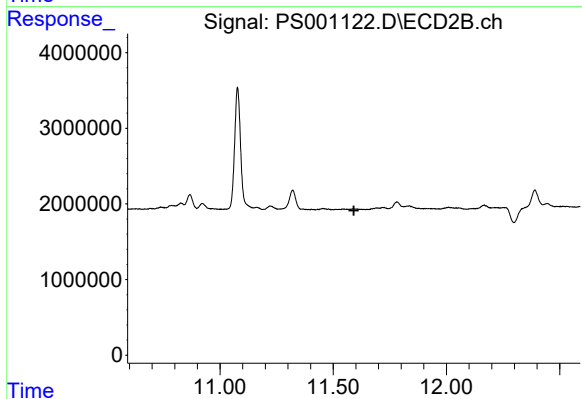

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.591 min
Response: 0
Conc: N.D.

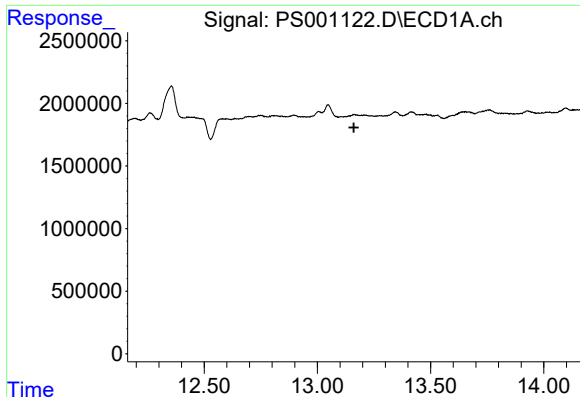

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 13.161 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

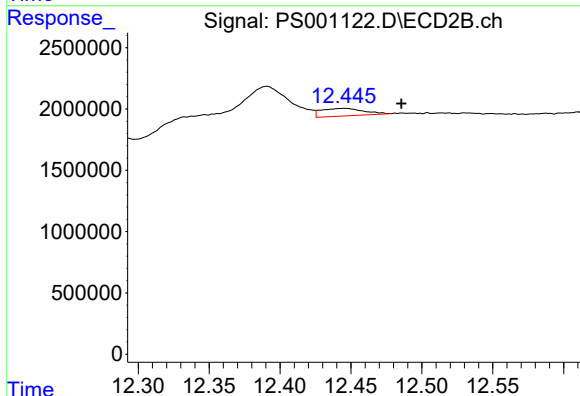


#8 DICHLORPROP

R.T.: 12.445 min
Delta R.T.: -0.040 min
Response: 1279938
Conc: 6.34 ng/ml

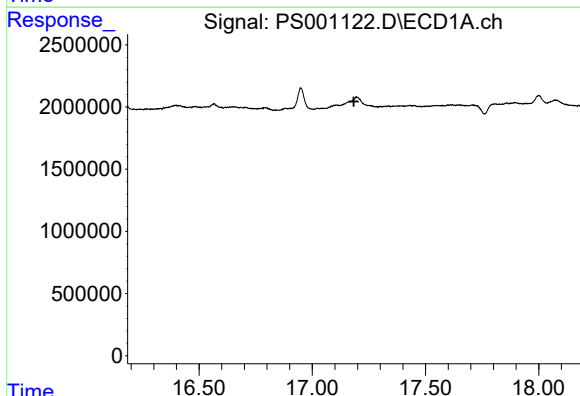


#15 Picloram

R.T.: 0.000 min
Exp R.T.: 17.184 min
Response: 0
Conc: N.D.

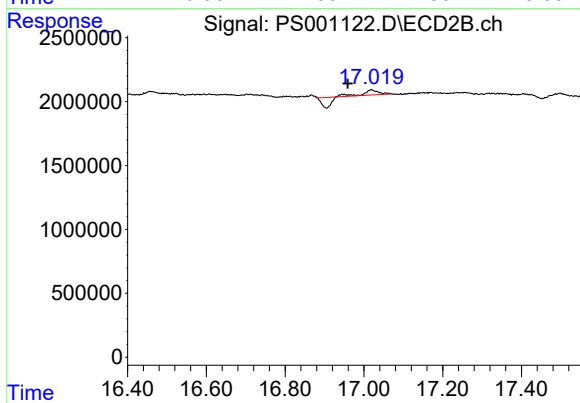

#15 Picloram


R.T.: 17.019 min
Delta R.T.: 0.060 min
Response: 83906
Conc: 0.06 ng/ml

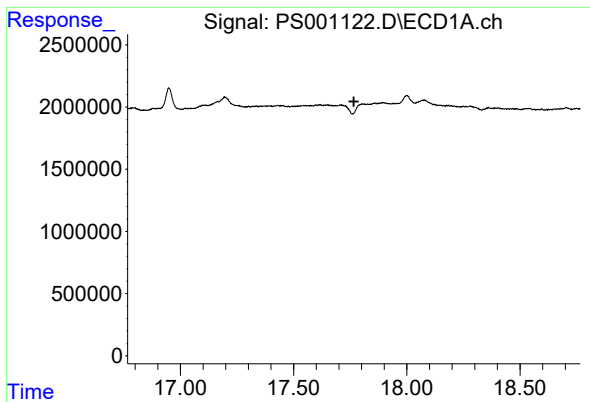

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.766 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

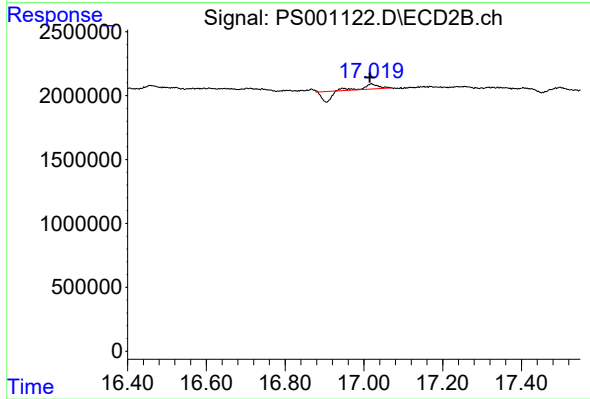

#16 DCPA

R.T.: 17.019 min
Delta R.T.: 0.004 min
Response: 83906
Conc: 0.05 ng/ml