

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071818\
 Data File : PS001128.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jul 2018 15:25
 Operator : UA
 Sample : PB111101TB
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 18 16:08:06 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 09 02:00:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.646	11.061	89589045	80033408	434.224	367.468
Target Compounds							
1) T	Dalapon	2.986	2.448	3349094	53154	12.473	0.197 #
5) T	DICAMBA	0.000	11.304	0	7303799	N.D.	9.305 #
6) T	MCPD	12.340	0.000	11401468	0	20.756	N.D. #
7) T	MCPA	12.614	0.000	11454348	0	12.551	N.D. #
8) T	DICHLORPROP	0.000	12.496	0	5833071	N.D.	28.880 #
9) T	2,4-D	0.000	12.951	0	2234506	N.D.	8.068 #
12) T	2,4,5-T	0.000	14.693	0	2225755	N.D.	2.151 #
13) T	2,4-DB	15.864	0.000	2191233	0	13.536	N.D. #
15) T	Picloram	0.000	17.003	0	21911606	N.D.	14.390 #
16) T	DCPA	17.802	17.003	-1067164	21911606	N.D.	12.746



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071818\
Data File : PS001128.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jul 2018 15:25
Operator : UA
Sample : PB111101TB
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 18 16:08:06 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
Quant Title : 8080.M
QLast Update : Mon Jul 09 02:00:25 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

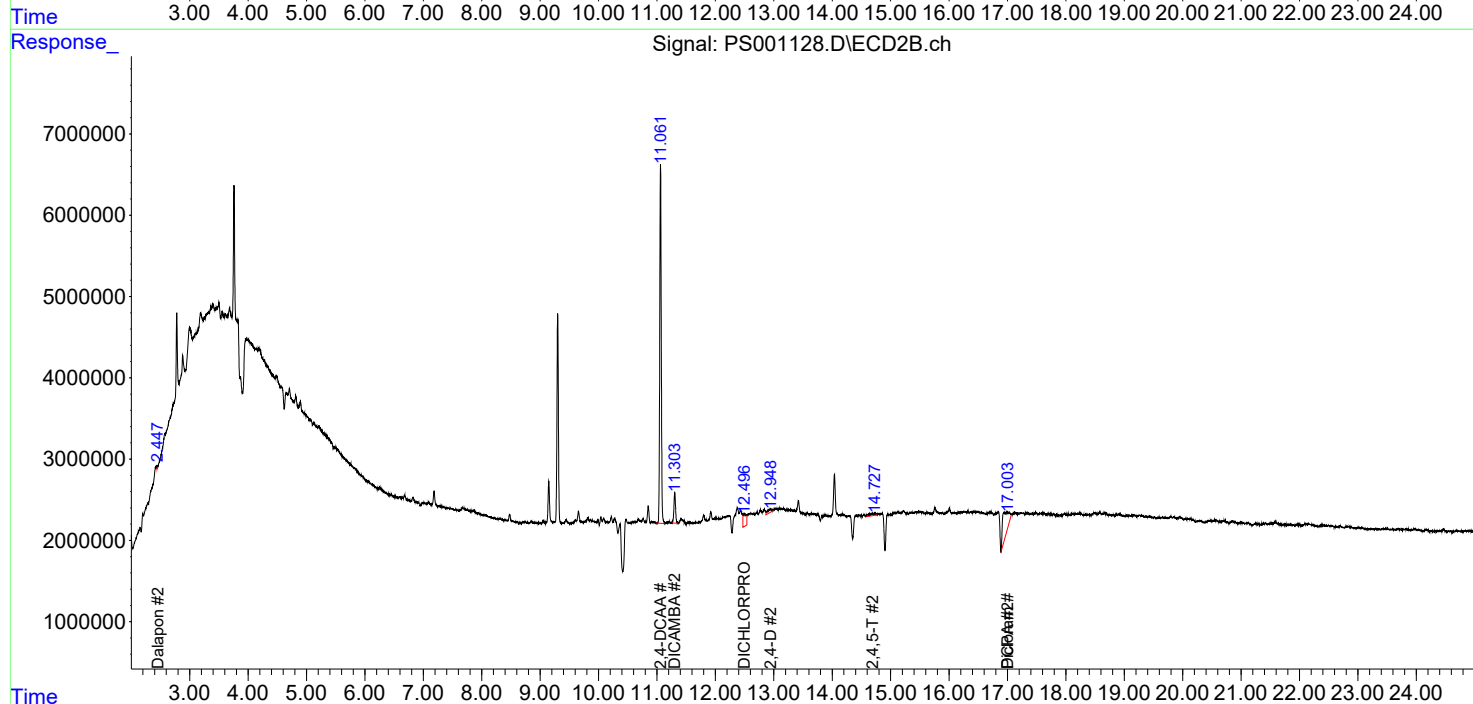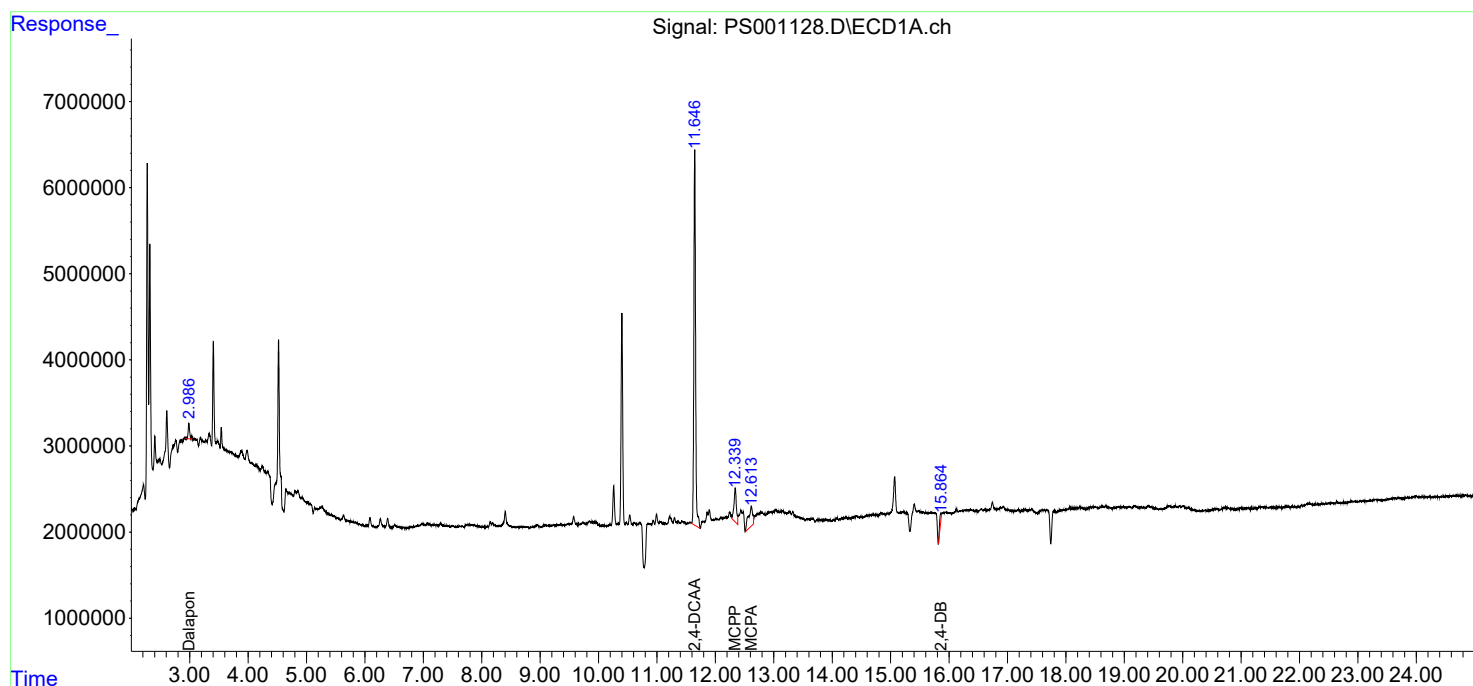


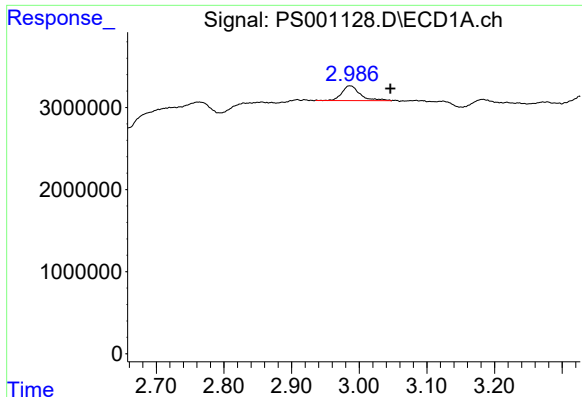

#1 Dalapon


R.T.: 2.986 min
Delta R.T.: -0.060 min
Response: 3349094
Conc: 12.47 ng/ml

Instrument :
ECD_S
ClientSampleId :

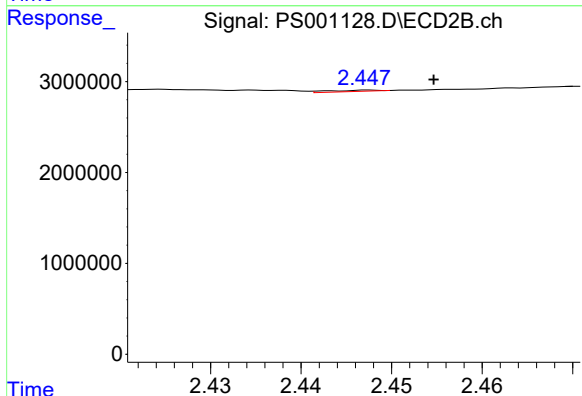


#1 Dalapon

R.T.: 2.448 min
Delta R.T.: -0.007 min
Response: 53154
Conc: 0.20 ng/ml

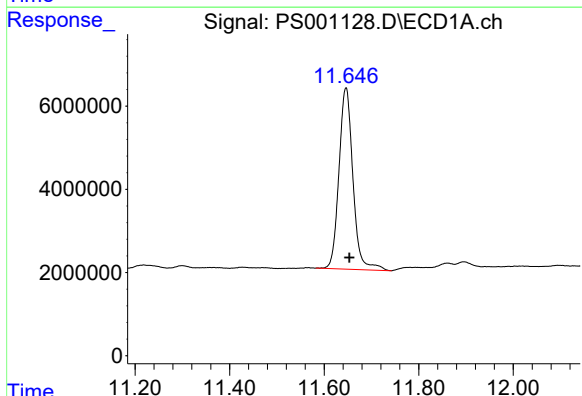


#4 2,4-DCAA

R.T.: 11.646 min
Delta R.T.: -0.007 min
Response: 89589045
Conc: 434.22 ng/ml

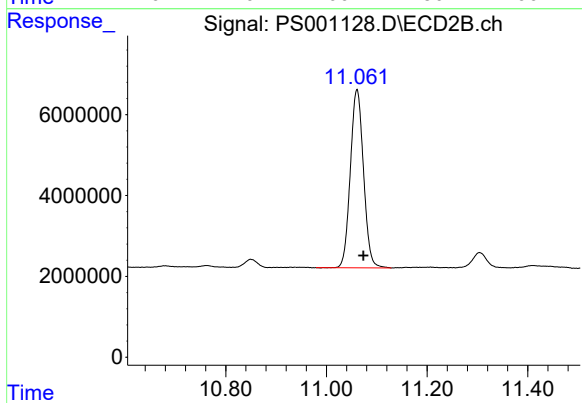

#4 2,4-DCAA


R.T.: 11.061 min
Delta R.T.: -0.013 min
Response: 80033408
Conc: 367.47 ng/ml

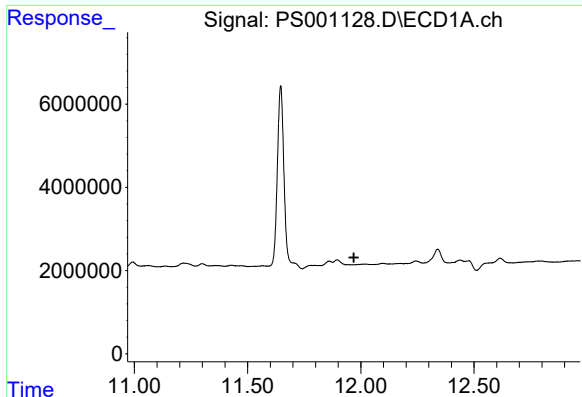

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.970 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

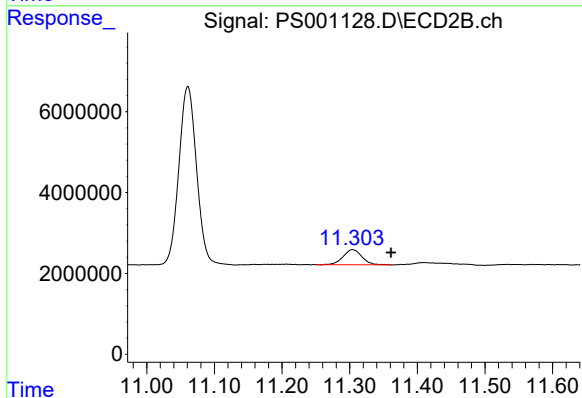


#5 DICAMBA

R.T.: 11.304 min
Delta R.T.: -0.057 min
Response: 7303799
Conc: 9.30 ng/ml

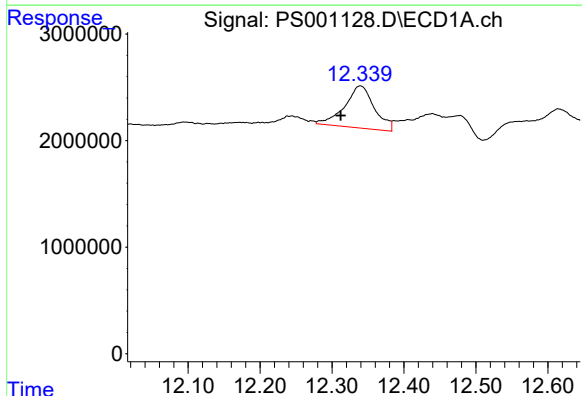


#6 MCP

R.T.: 12.340 min
Delta R.T.: 0.027 min
Response: 11401468
Conc: 20.76 ug/ml

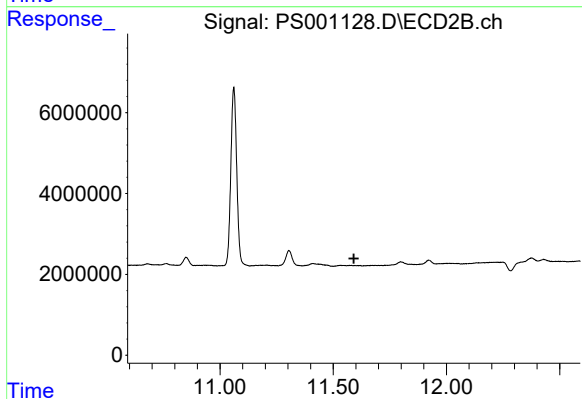

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.591 min
Response: 0
Conc: N.D.

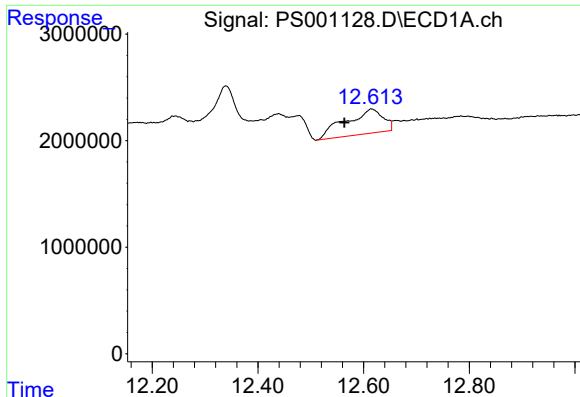

#7 MCPA


R.T.: 12.614 min
Delta R.T.: 0.050 min
Response: 11454348
Conc: 12.55 ug/ml

Instrument :
ECD_S
ClientSampleId :

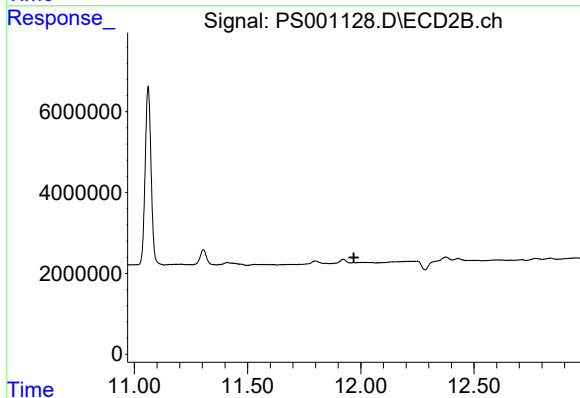


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 11.969 min
Response: 0
Conc: N.D.

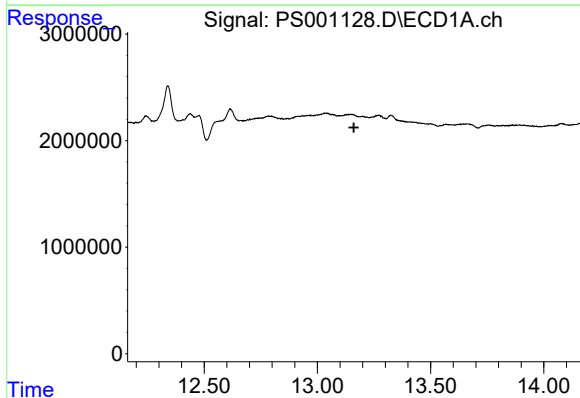


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 13.161 min
Response: 0
Conc: N.D.

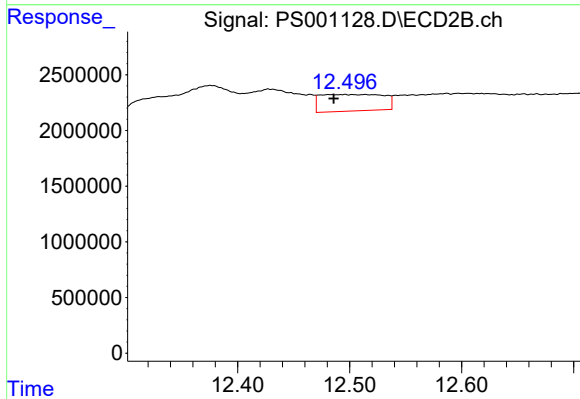

#8 DICHLORPROP


R.T.: 12.496 min
Delta R.T.: 0.010 min
Response: 5833071
Conc: 28.88 ng/ml

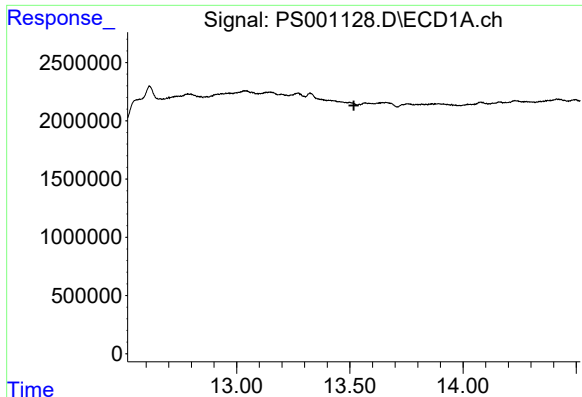

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.518 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

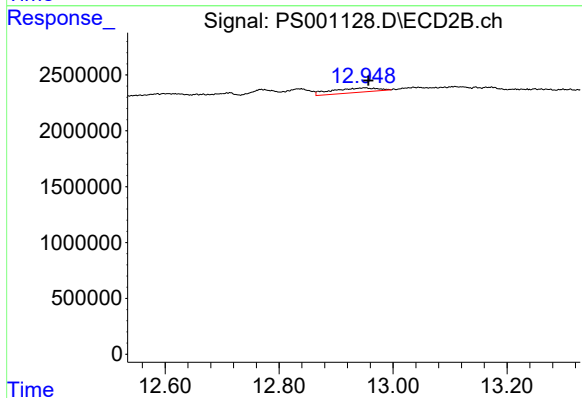


#9 2,4-D

R.T.: 12.951 min
Delta R.T.: -0.006 min
Response: 2234506
Conc: 8.07 ng/ml

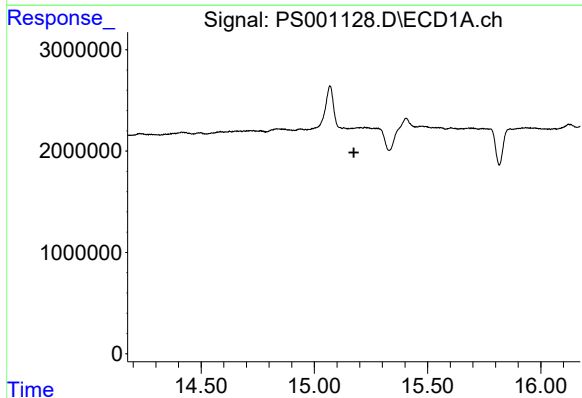


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 15.174 min
Response: 0
Conc: N.D.

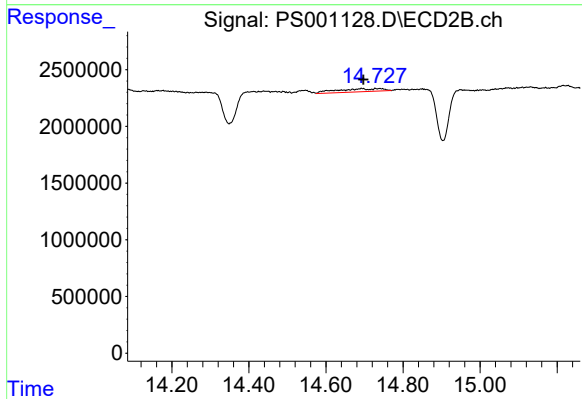

#12 2,4,5-T


R.T.: 14.693 min
Delta R.T.: -0.004 min
Response: 2225755
Conc: 2.15 ng/ml

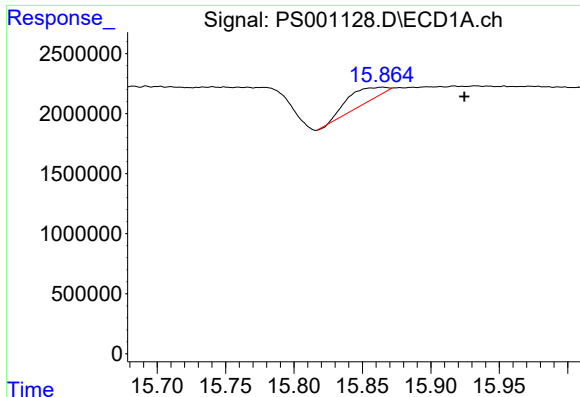

#13 2,4-DB


R.T.: 15.864 min
Delta R.T.: -0.060 min
Response: 2191233
Conc: 13.54 ng/ml

Instrument :
ECD_S
ClientSampleId :

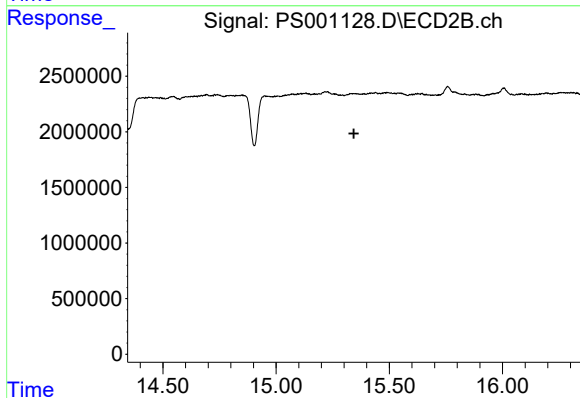


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 15.344 min
Response: 0
Conc: N.D.

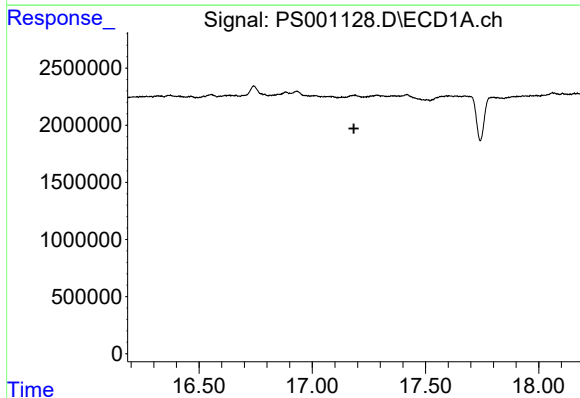


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 17.184 min
Response: 0
Conc: N.D.

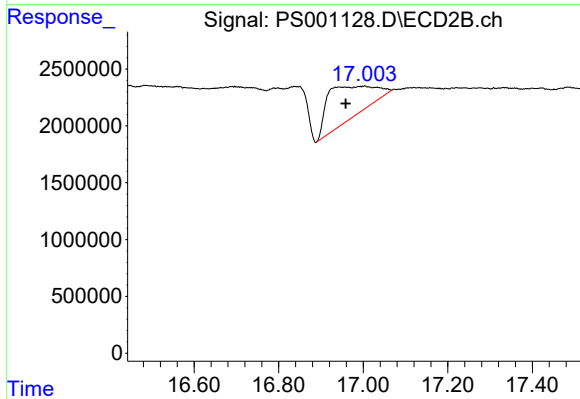

#15 Picloram


R.T.: 17.003 min
Delta R.T.: 0.044 min
Response: 21911606
Conc: 14.39 ng/ml

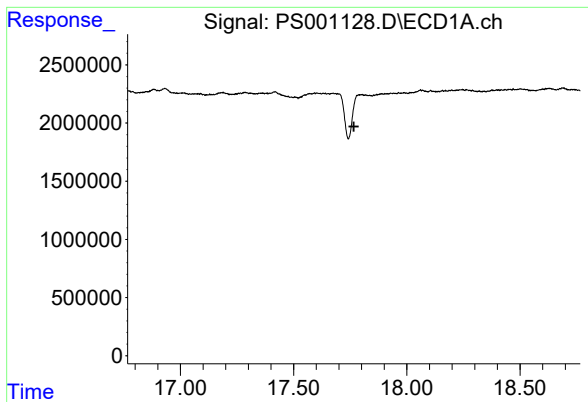

#16 DCPA

R.T.: 17.802 min
Delta R.T.: 0.036 min
Response: -1067164
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

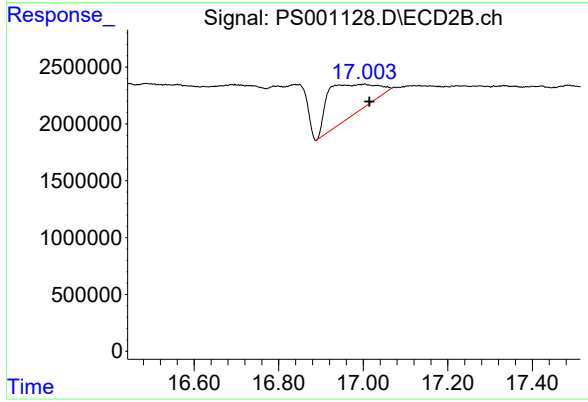

#16 DCPA

R.T.: 17.003 min
Delta R.T.: -0.012 min
Response: 21911606
Conc: 12.75 ng/ml