

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071818\
 Data File : PS001134.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jul 2018 18:31
 Operator : UA
 Sample : J3826-04
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 19 03:41:46 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 09 02:00:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.643	11.057	61450868	54056449	297.842	248.196
Target Compounds							
5) T	DICAMBA	0.000	11.301	0	4898393	N.D.	6.240 #
6) T	MCPD	12.320	0.000	12691040	0	23.104	N.D. #
8) T	DICHLORPROP	0.000	12.468	0	388209	N.D.	1.922 #
10) T	Pentachlo...	13.900	0.000	2400505	0	0.790	N.D. #
11) T	2,4,5-TP ...	0.000	14.111	0	2602068	N.D.	2.073 #
12) T	2,4,5-T	0.000	14.680	0	5570142	N.D.	5.383 #
14) T	DINOSEB	0.000	15.757	0	6983090	N.D.	8.338 #
15) T	Picloram	17.178	16.938	14502756	6121565	8.008	4.020 #
16) T	DCPA	17.768	16.996	-40449	16534431	N.D.	9.618



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071818\
Data File : PS001134.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jul 2018 18:31
Operator : UA
Sample : J3826-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 19 03:41:46 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
Quant Title : 8080.M
QLast Update : Mon Jul 09 02:00:25 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

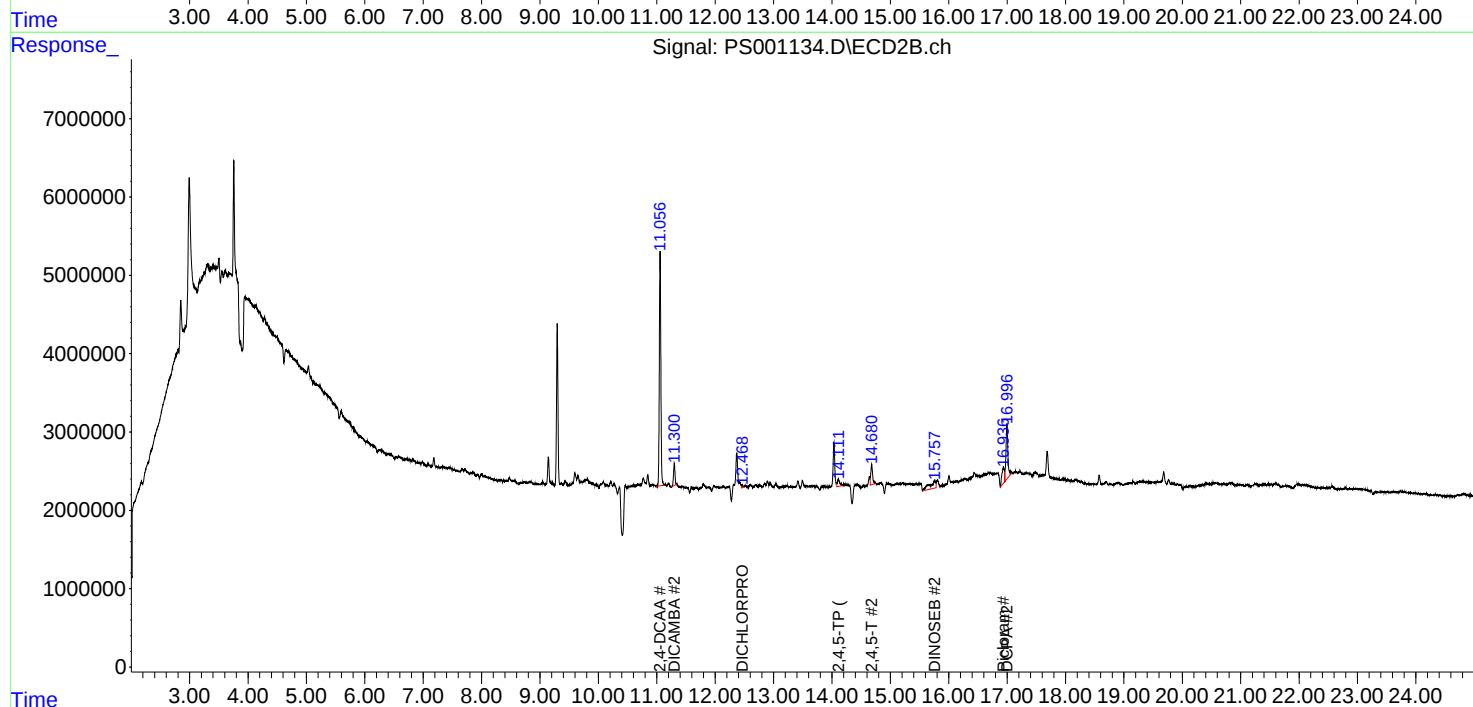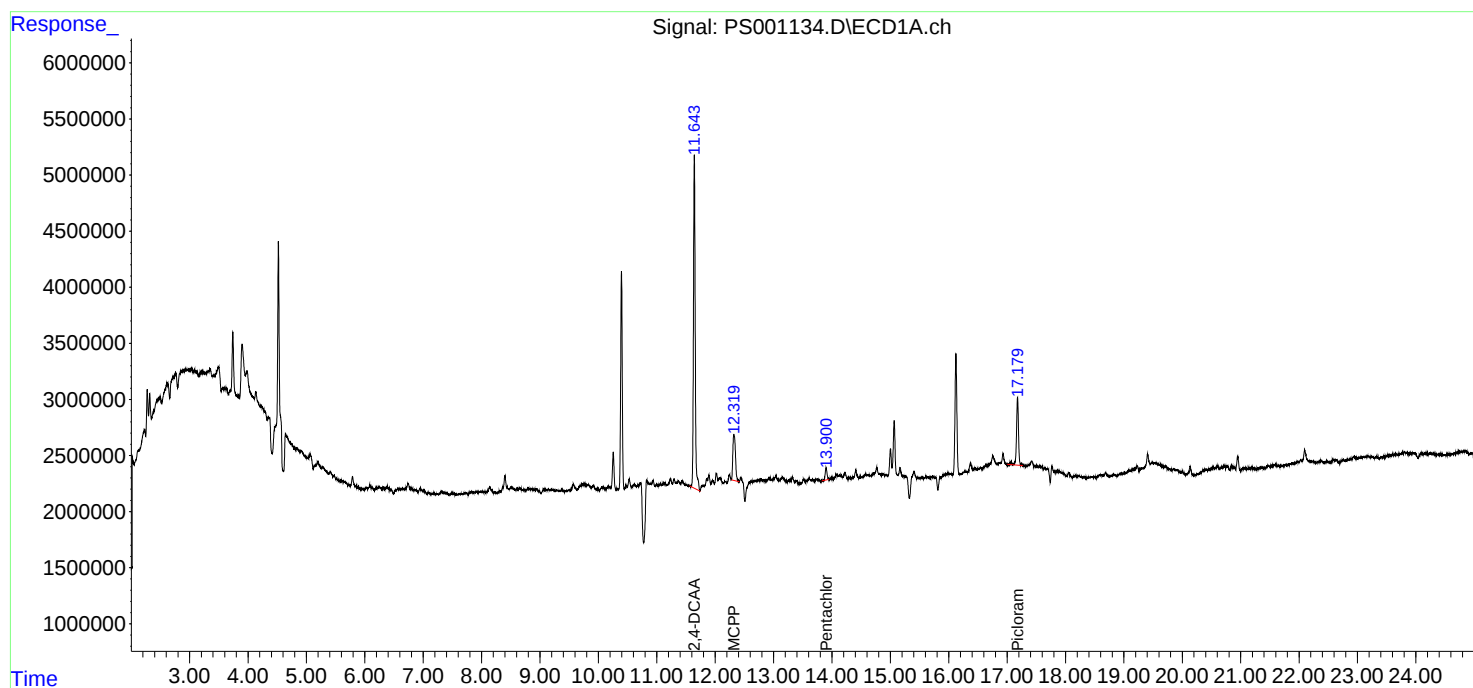


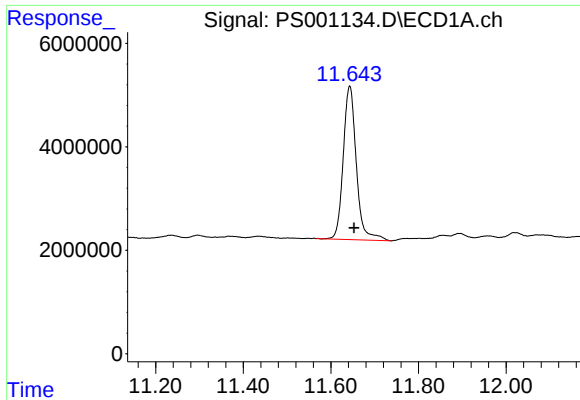

#4 2,4-DCAA


R.T.: 11.643 min
Delta R.T.: -0.010 min
Response: 61450868
Conc: 297.84 ng/ml

Instrument :
ECD_S
ClientSampleId :

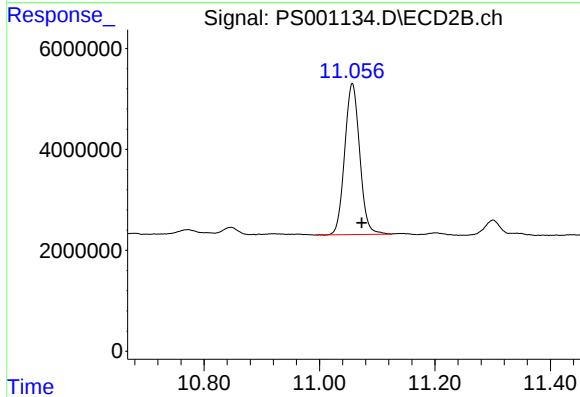


#4 2,4-DCAA

R.T.: 11.057 min
Delta R.T.: -0.017 min
Response: 54056449
Conc: 248.20 ng/ml

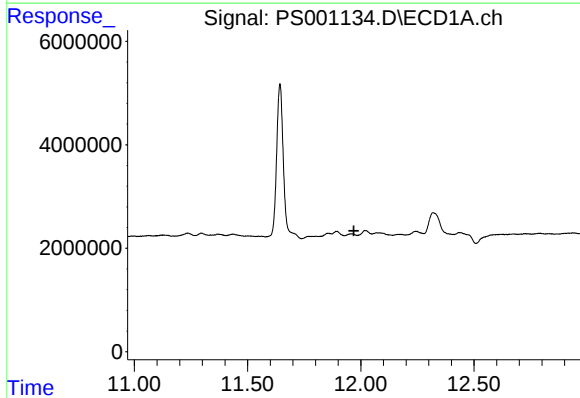


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.970 min
Response: 0
Conc: N.D.

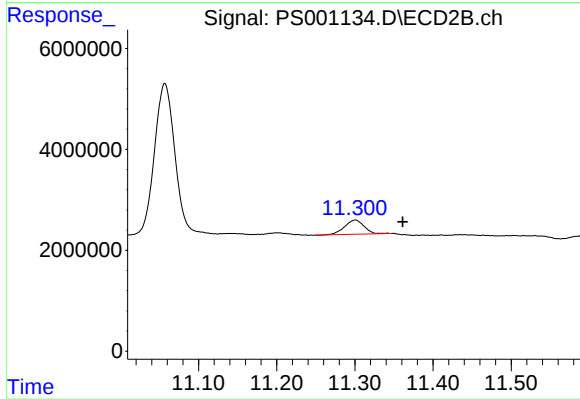

#5 DICAMBA


R.T.: 11.301 min
Delta R.T.: -0.060 min
Response: 4898393
Conc: 6.24 ng/ml

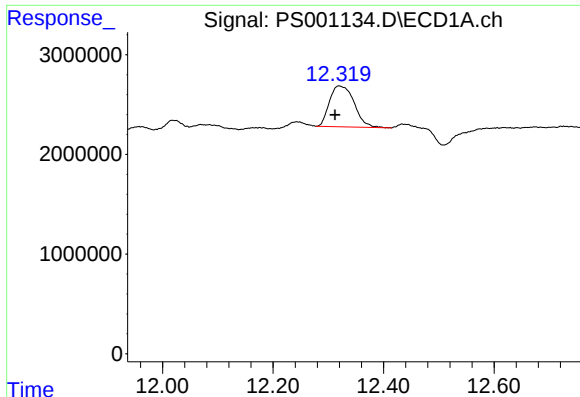

#6 MCP


R.T.: 12.320 min
Delta R.T.: 0.008 min
Response: 12691040
Conc: 23.10 ug/ml

Instrument :
ECD_S
ClientSampleId :

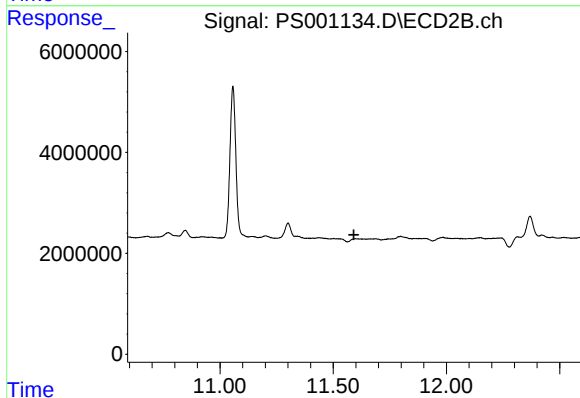


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.591 min
Response: 0
Conc: N.D.

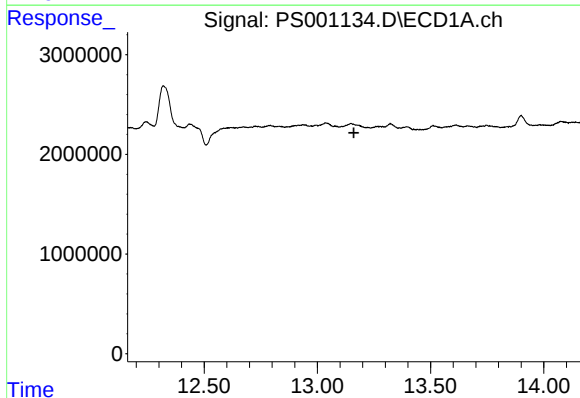


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 13.161 min
Response: 0
Conc: N.D.

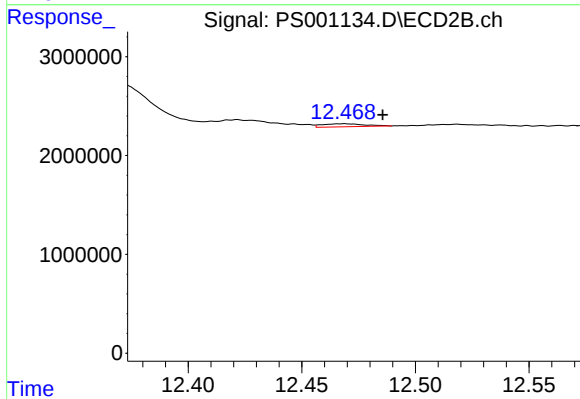

#8 DICHLORPROP


R.T.: 12.468 min
Delta R.T.: -0.018 min
Response: 388209
Conc: 1.92 ng/ml

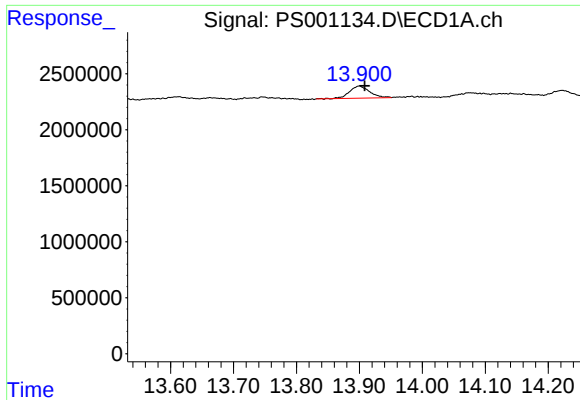

#10 Pentachlorophenol


R.T.: 13.900 min
Delta R.T.: -0.009 min
Response: 2400505
Conc: 0.79 ng/ml

Instrument :
ECD_S
ClientSampleId :

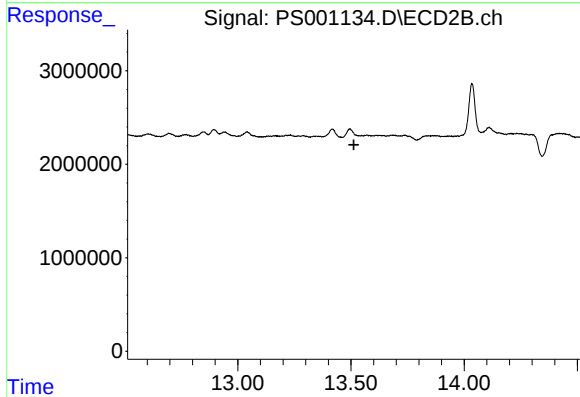


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 13.513 min
Response: 0
Conc: N.D.

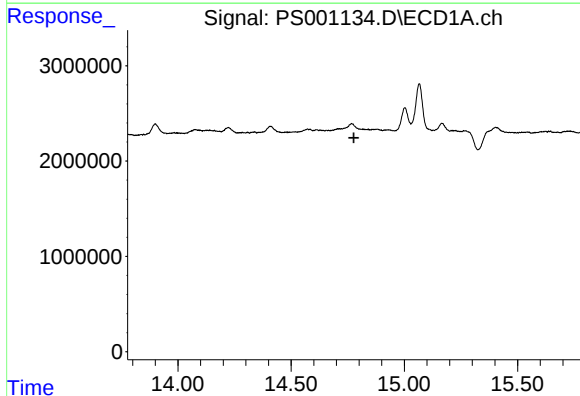


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 14.777 min
Response: 0
Conc: N.D.

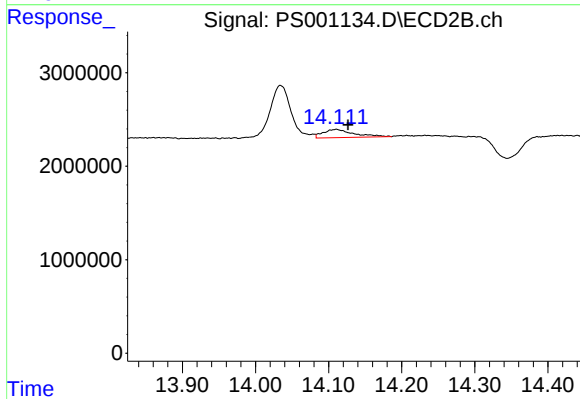

#11 2,4,5-TP (SILVEX)


R.T.: 14.111 min
Delta R.T.: -0.016 min
Response: 2602068
Conc: 2.07 ng/ml

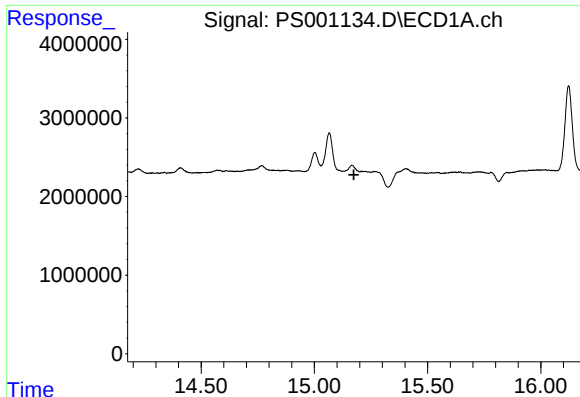

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 15.174 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

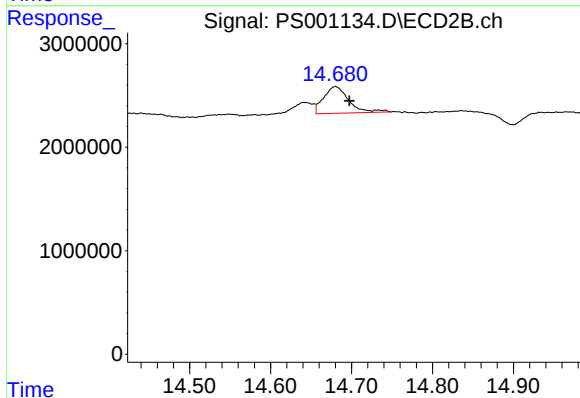


#12 2,4,5-T

R.T.: 14.680 min
Delta R.T.: -0.017 min
Response: 5570142
Conc: 5.38 ng/ml

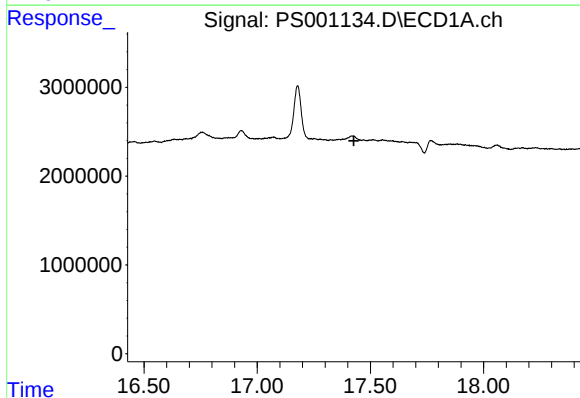


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 17.427 min
Response: 0
Conc: N.D.

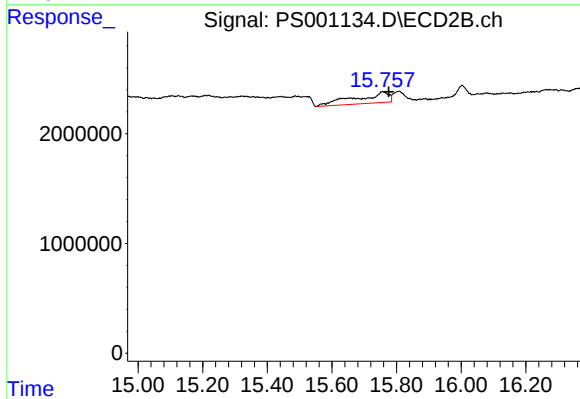

#14 DINOSEB


R.T.: 15.757 min
Delta R.T.: -0.019 min
Response: 6983090
Conc: 8.34 ng/ml

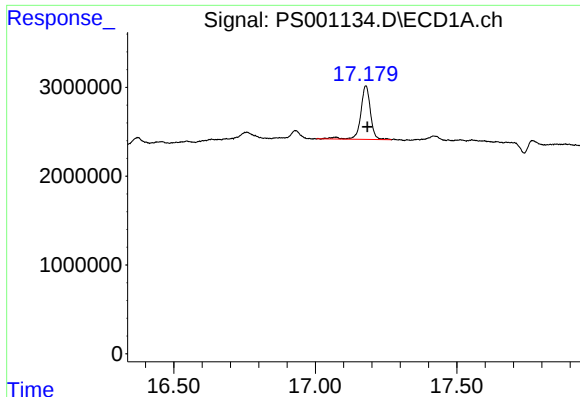

#15 Picloram


R.T.: 17.178 min
Delta R.T.: -0.005 min
Response: 14502756
Conc: 8.01 ng/ml

Instrument :
ECD_S
ClientSampleId :

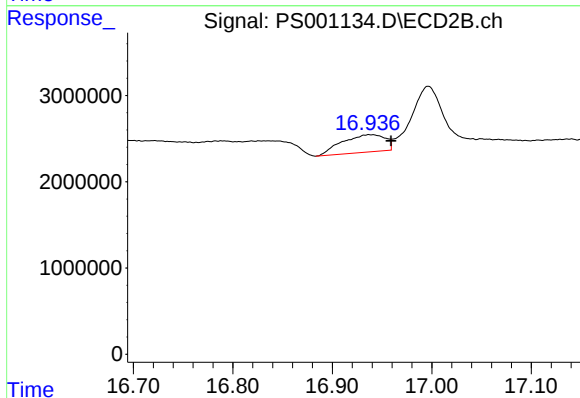


#15 Picloram

R.T.: 16.938 min
Delta R.T.: -0.021 min
Response: 6121565
Conc: 4.02 ng/ml

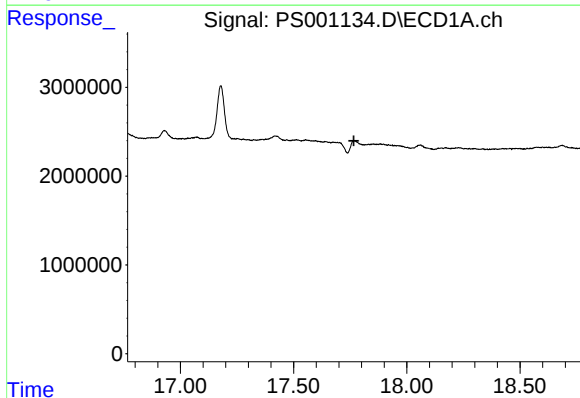

#16 DCPA

R.T.: 17.768 min
Delta R.T.: 0.002 min
Response: -40449
Conc: N.D.

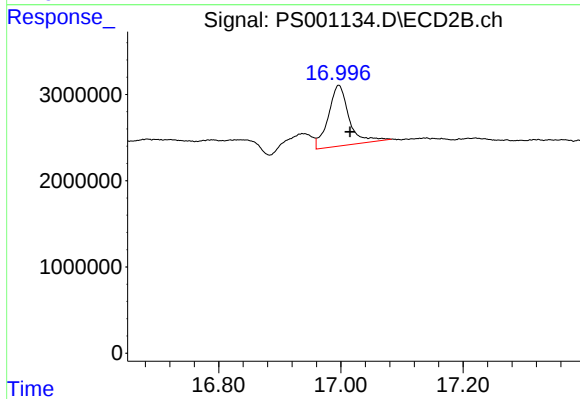

#16 DCPA

R.T.: 16.996 min
Delta R.T.: -0.019 min
Response: 16534431
Conc: 9.62 ng/ml