

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071818\
 Data File : PS001138.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jul 2018 20:35
 Operator : UA
 Sample : J4013-06
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 19 03:43:04 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 09 02:00:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.644	11.059	64689254	57073225	313.538	262.048
Target Compounds							
1) T	Dalapon	0.000	2.432	0	531009	N.D.	1.971 #
5) T	DICAMBA	12.023	11.302	1179594	5136019	1.498	6.543 #
6) T	MCPD	12.326	0.000	14297124	0	26.028	N.D. #
7) T	MCPA	12.591	0.000	4949345	0	5.423	N.D. #
8) T	DICHLORPROP	0.000	12.422	0	1073753	N.D.	5.316 #
14) T	DINOSEB	0.000	15.819	0	4218133	N.D.	5.037 #
15) T	Picloram	17.173	16.924	2379112	-804340	1.314	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071818\
Data File : PS001138.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jul 2018 20:35
Operator : UA
Sample : J4013-06
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 19 03:43:04 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
Quant Title : 8080.M
QLast Update : Mon Jul 09 02:00:25 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

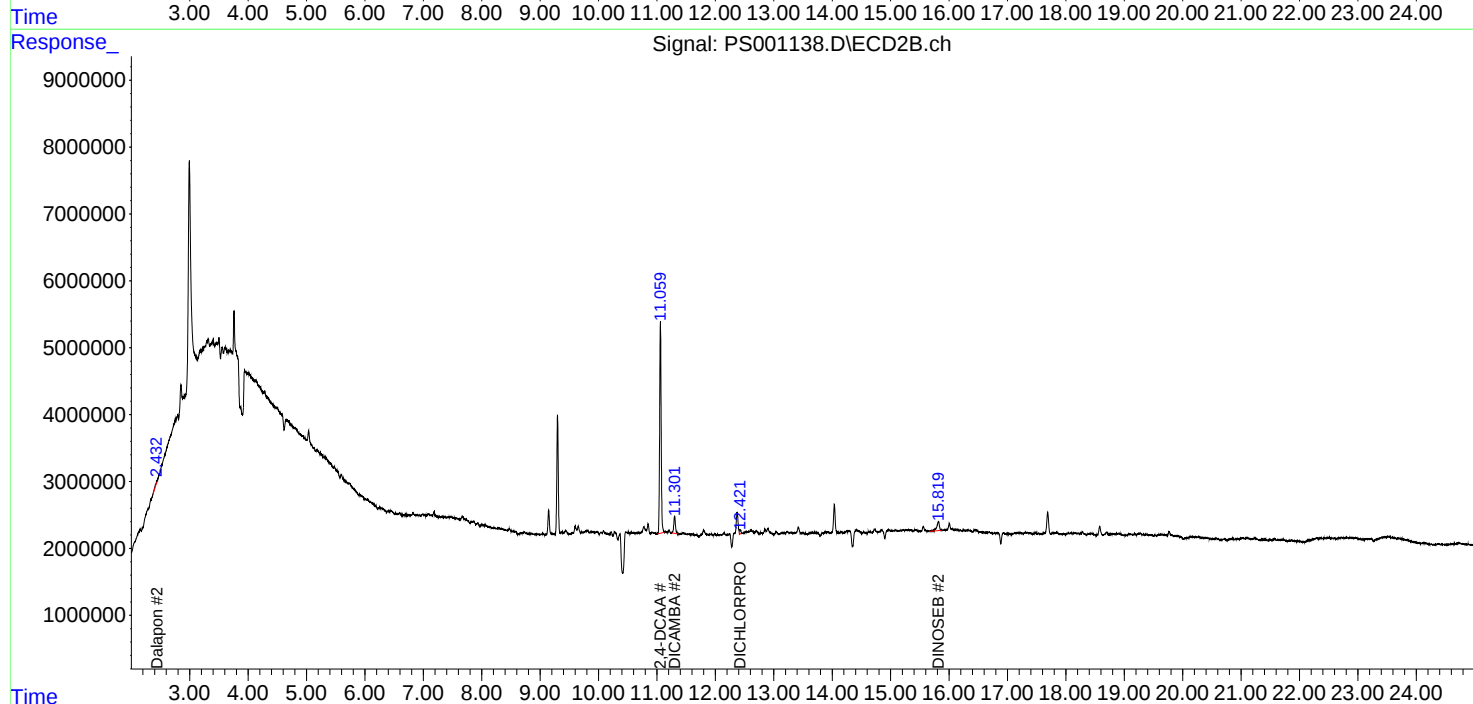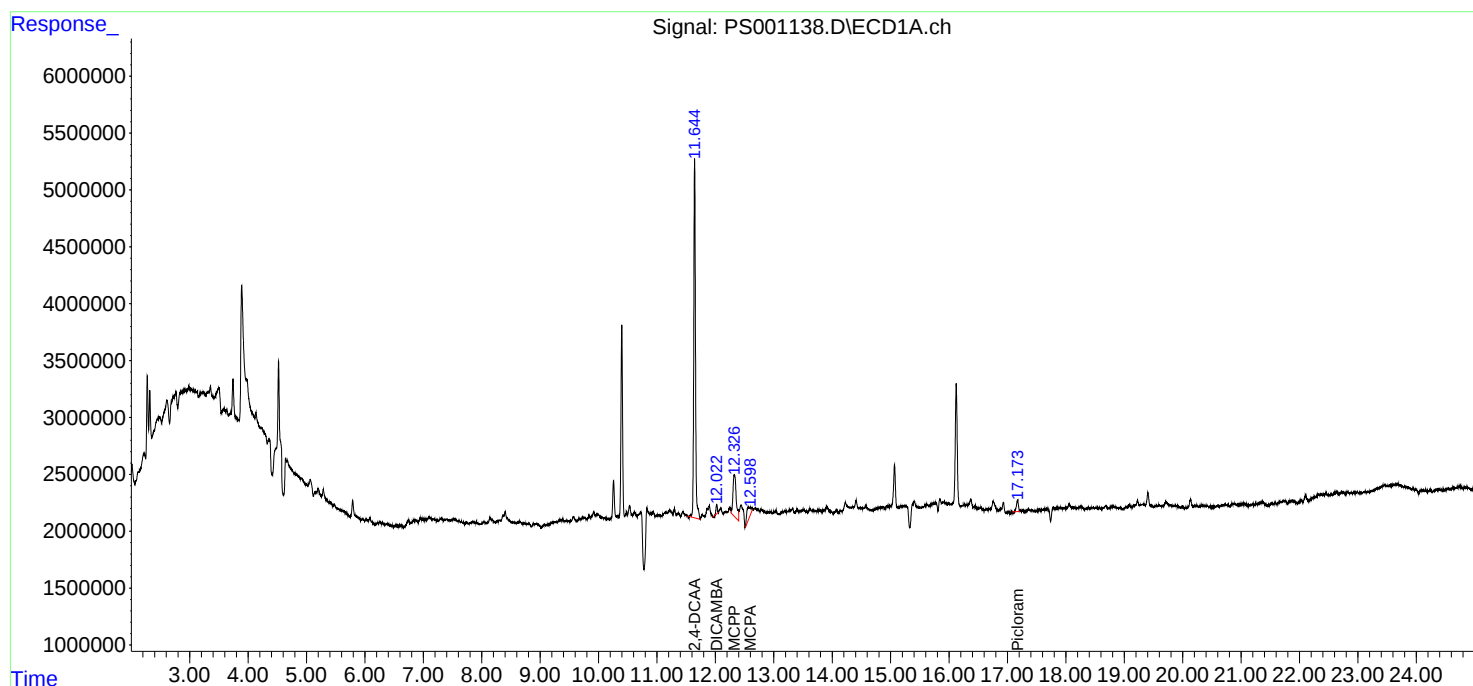


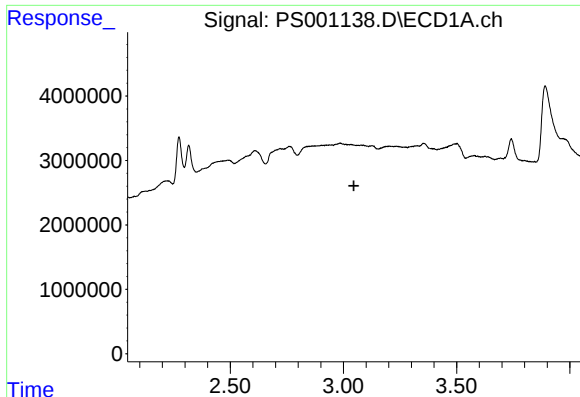

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 3.046 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

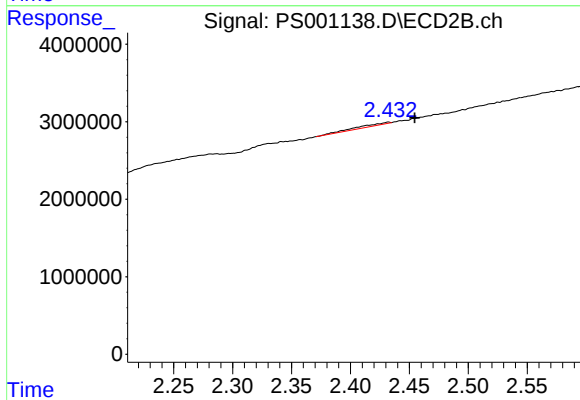


#1 Dalapon

R.T.: 2.432 min
Delta R.T.: -0.022 min
Response: 531009
Conc: 1.97 ng/ml

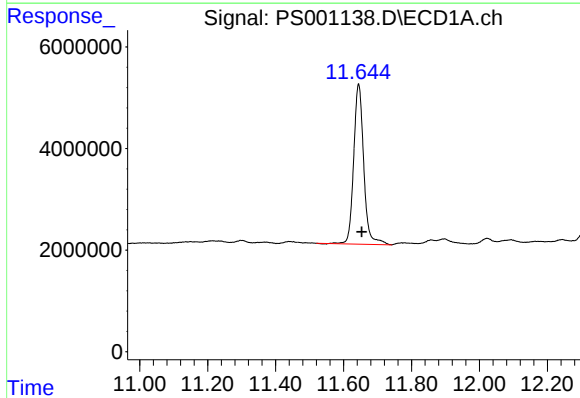


#4 2,4-DCAA

R.T.: 11.644 min
Delta R.T.: -0.009 min
Response: 64689254
Conc: 313.54 ng/ml

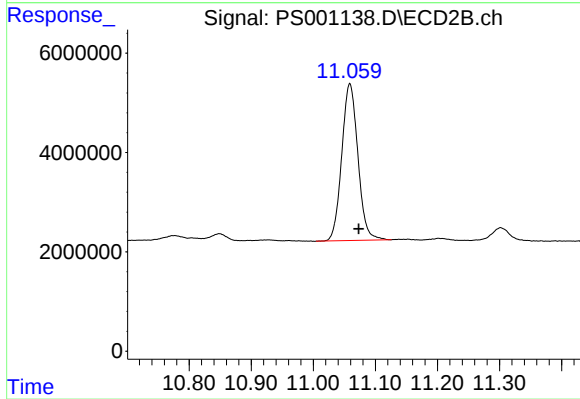

#4 2,4-DCAA


R.T.: 11.059 min
Delta R.T.: -0.015 min
Response: 57073225
Conc: 262.05 ng/ml

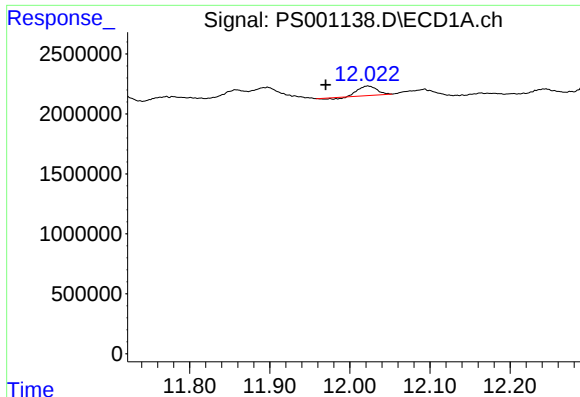

#5 DICAMBA


R.T.: 12.023 min
Delta R.T.: 0.053 min
Response: 1179594
Conc: 1.50 ng/ml

Instrument :
ECD_S
ClientSampleId :

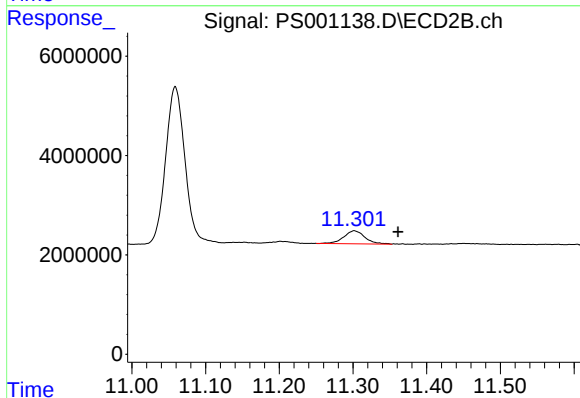


#5 DICAMBA

R.T.: 11.302 min
Delta R.T.: -0.059 min
Response: 5136019
Conc: 6.54 ng/ml

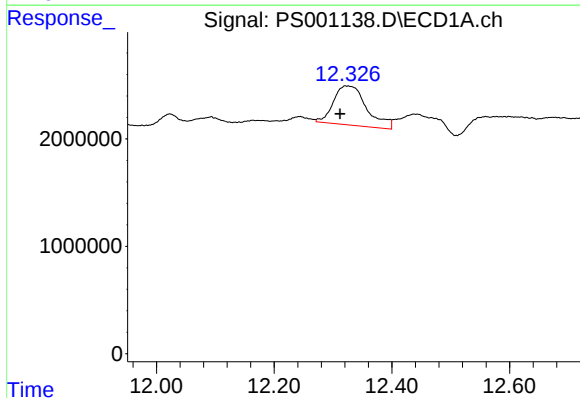


#6 MCP

R.T.: 12.326 min
Delta R.T.: 0.014 min
Response: 14297124
Conc: 26.03 ug/ml

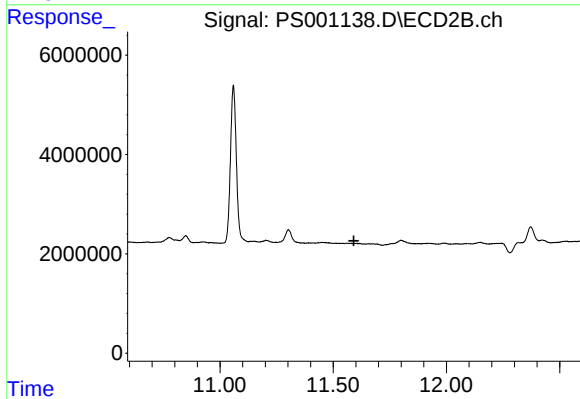

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.591 min
Response: 0
Conc: N.D.

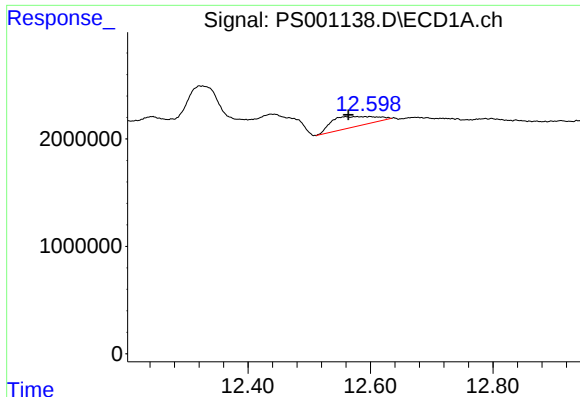

#7 MCPA


R.T.: 12.591 min
Delta R.T.: 0.027 min
Response: 4949345
Conc: 5.42 ug/ml

Instrument :
ECD_S
ClientSampleId :

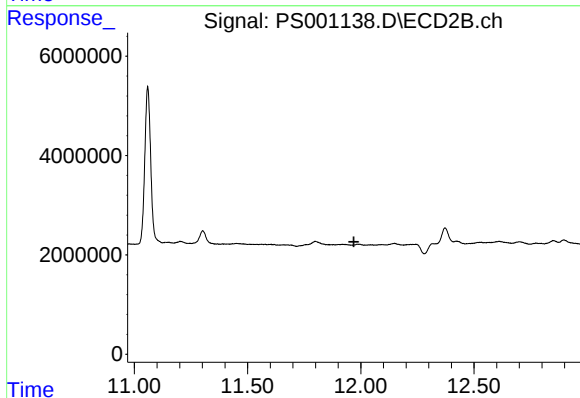


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 11.969 min
Response: 0
Conc: N.D.

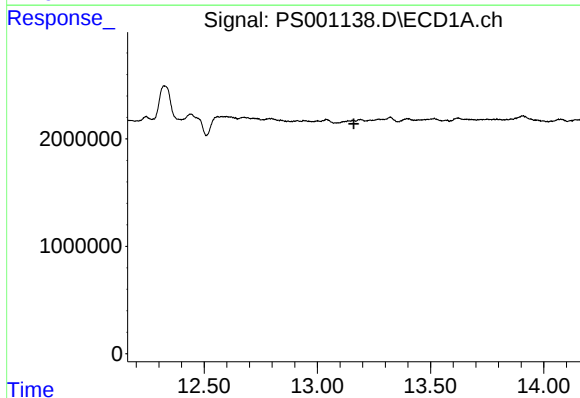


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 13.161 min
Response: 0
Conc: N.D.

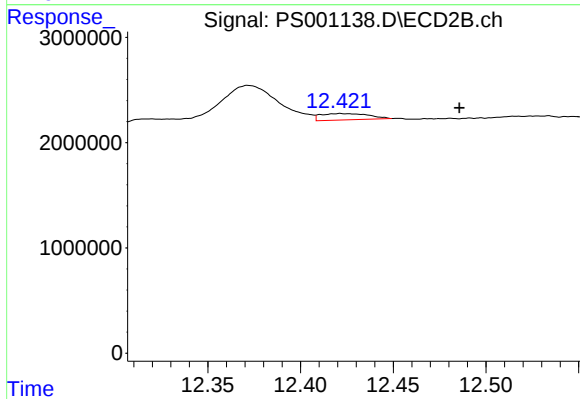

#8 DICHLORPROP


R.T.: 12.422 min
Delta R.T.: -0.064 min
Response: 1073753
Conc: 5.32 ng/ml

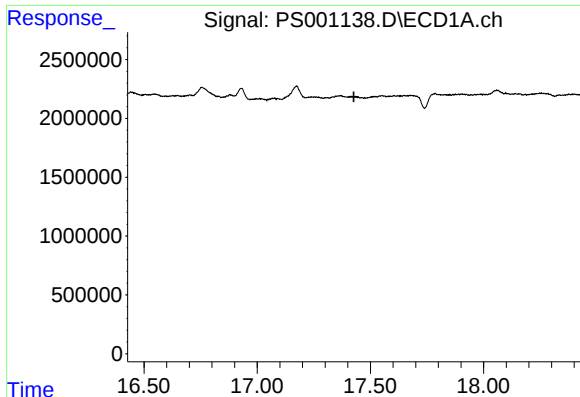

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 17.427 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

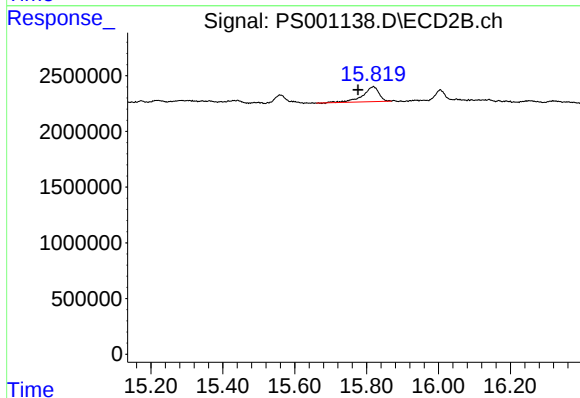


#14 DINOSEB

R.T.: 15.819 min
Delta R.T.: 0.043 min
Response: 4218133
Conc: 5.04 ng/ml

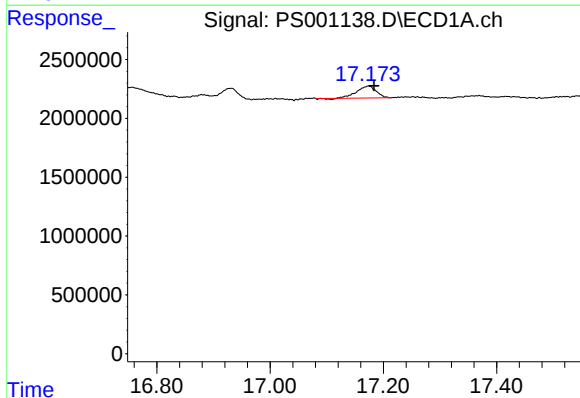

#15 Picloram

R.T.: 17.173 min
Delta R.T.: -0.010 min
Response: 2379112
Conc: 1.31 ng/ml

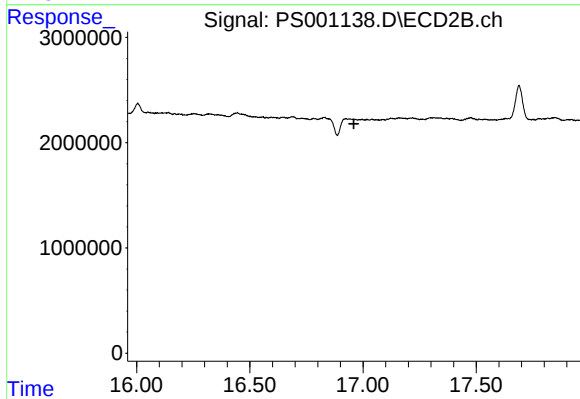

#15 Picloram

R.T.: 16.924 min
Delta R.T.: -0.035 min
Response: -804340
Conc: N.D.