

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071918\
 Data File : PS001144.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jul 2018 11:14
 Operator : UA
 Sample : J3832-04RE
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 19 12:45:40 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 09 02:00:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.632	11.037	50504878	43992344	244.789	201.988
Target Compounds							
1) T	Dalapon	0.000	2.457	0	1084671	N.D.	4.026 #
2) T	3,5-DICHL...	0.000	9.274	0	38398026	N.D.	130.537 #
6) T	MCP	12.324	0.000	7701529	0	14.021	N.D. #
7) T	MCPA	12.617	0.000	1162711	0	1.274	N.D. #
14) T	DINOSEB	0.000	15.796	0	3913375	N.D.	4.673 #
15) T	Picloram	17.165	16.981	7310808	14648083	4.037	9.620 #
16) T	DCPA	0.000	16.981	0	14648083	N.D.	8.521 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071918\
Data File : PS001144.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jul 2018 11:14
Operator : UA
Sample : J3832-04RE
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 19 12:45:40 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
Quant Title : 8080.M
QLast Update : Mon Jul 09 02:00:25 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

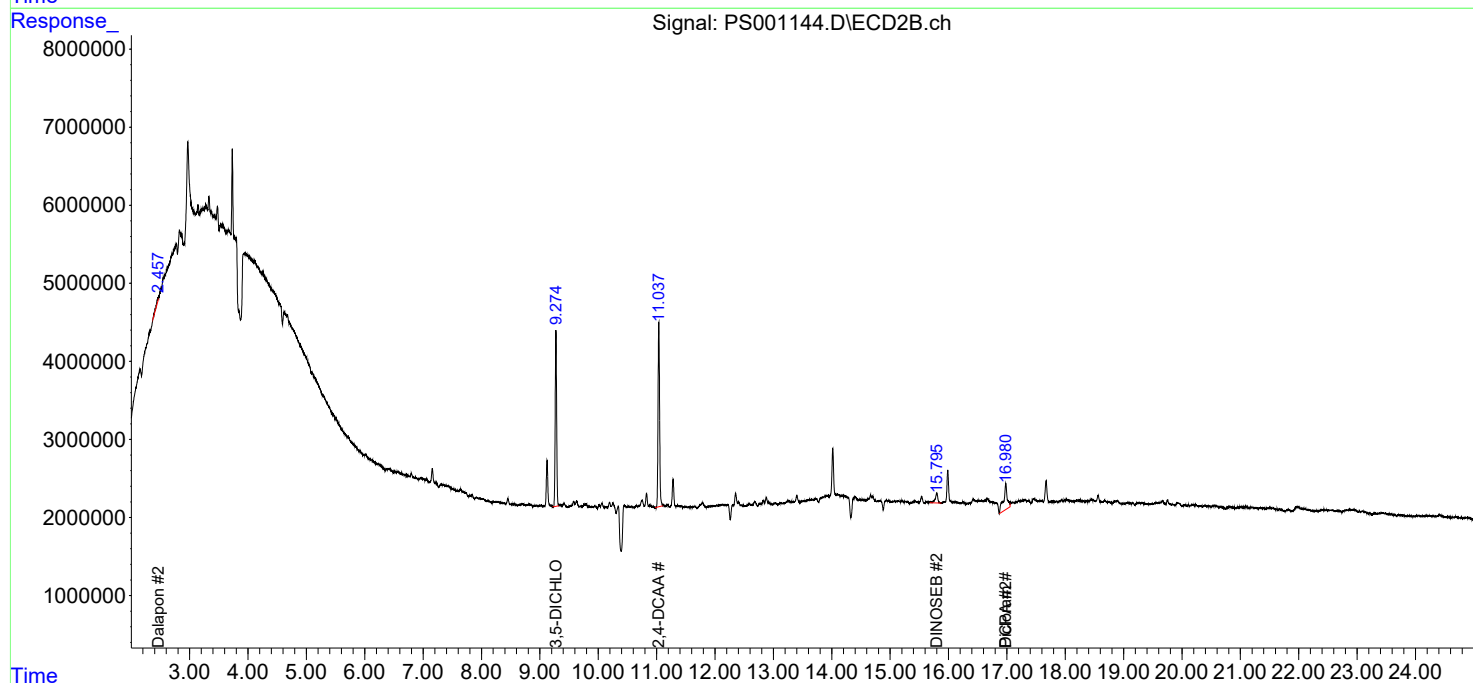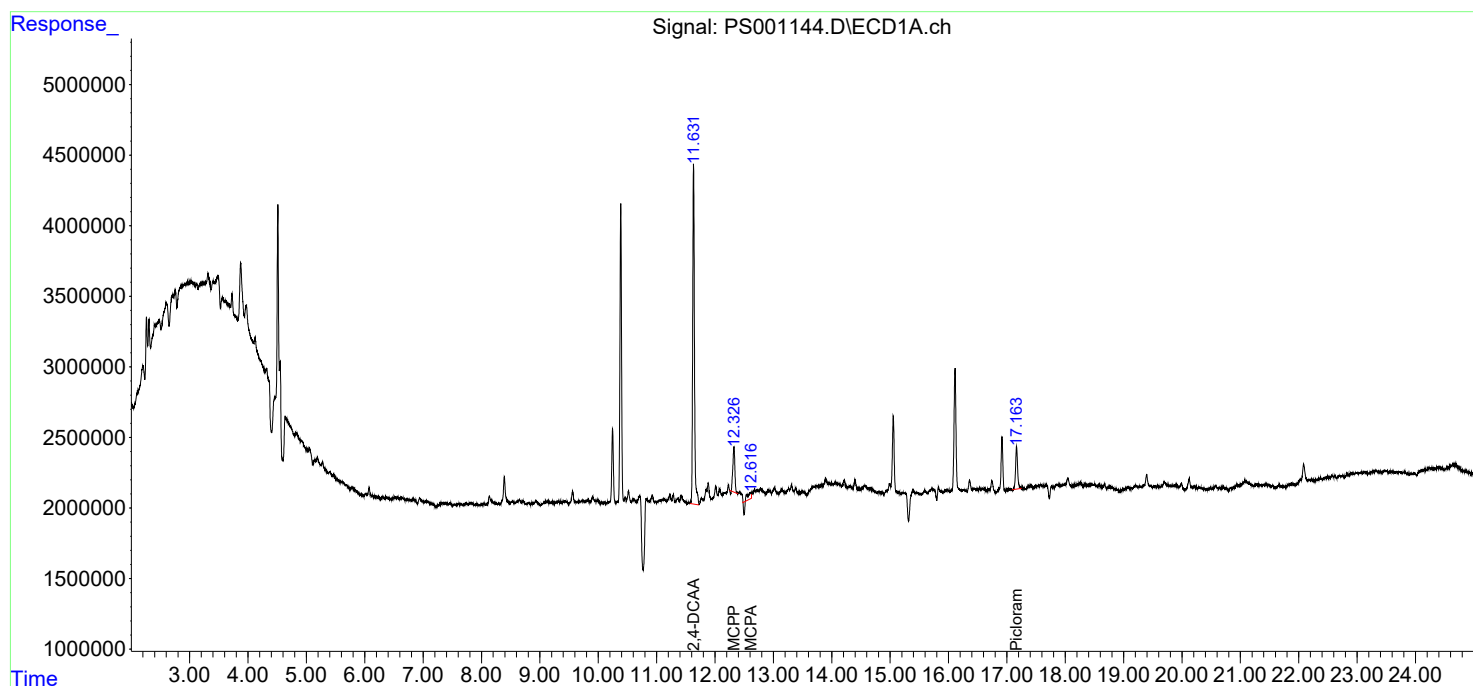


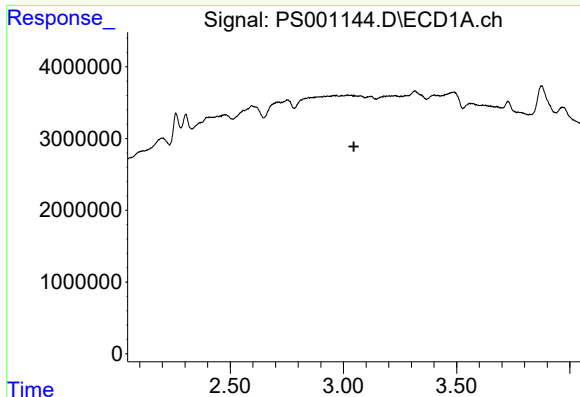

#1 Dalapon


R.T.: 0.000 min
Exp R.T. : 3.046 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

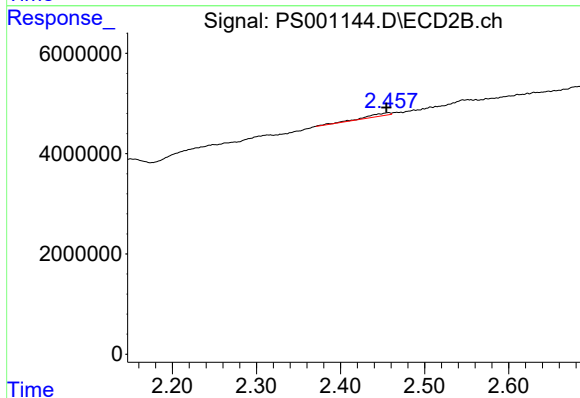


#1 Dalapon

R.T.: 2.457 min
Delta R.T.: 0.003 min
Response: 1084671
Conc: 4.03 ng/ml

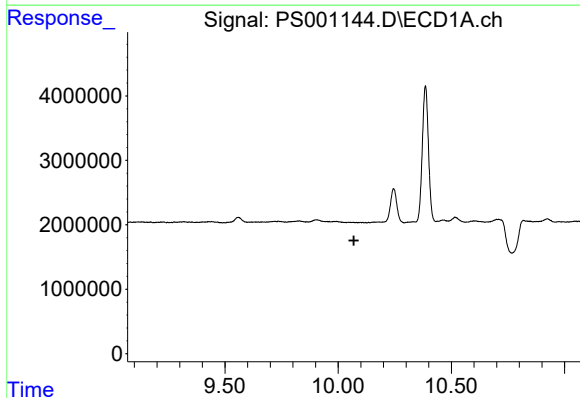


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 10.070 min
Response: 0
Conc: N.D.

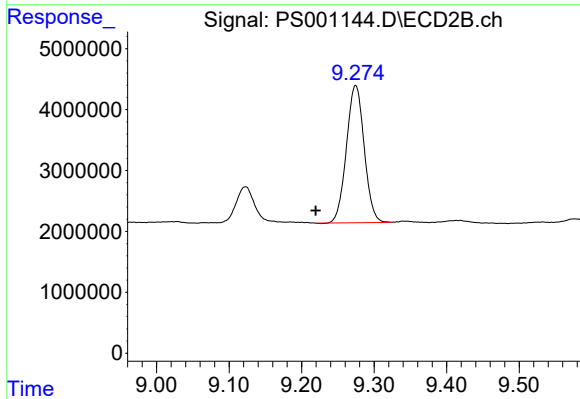

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.274 min
Delta R.T.: 0.055 min
Response: 38398026
Conc: 130.54 ng/ml

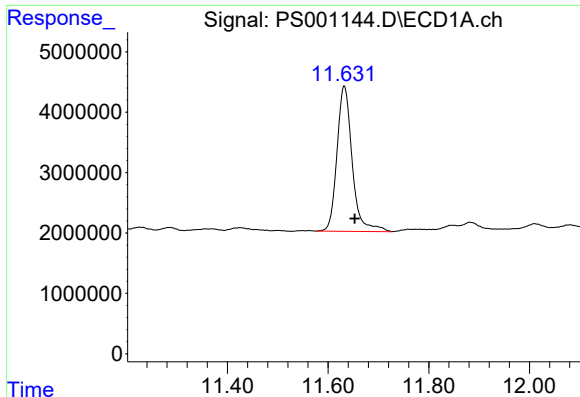

#4 2,4-DCAA


R.T.: 11.632 min
Delta R.T.: -0.021 min
Response: 50504878
Conc: 244.79 ng/ml

Instrument :
ECD_S
ClientSampleId :

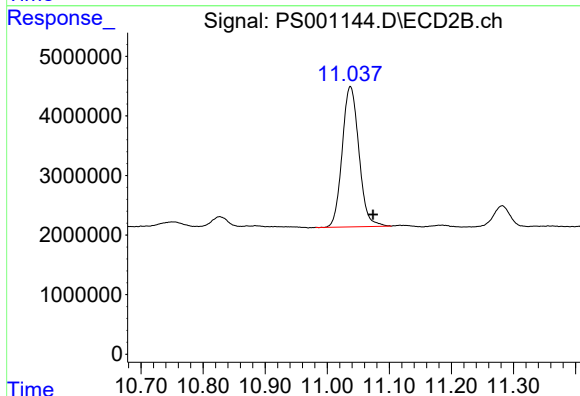


#4 2,4-DCAA

R.T.: 11.037 min
Delta R.T.: -0.036 min
Response: 43992344
Conc: 201.99 ng/ml

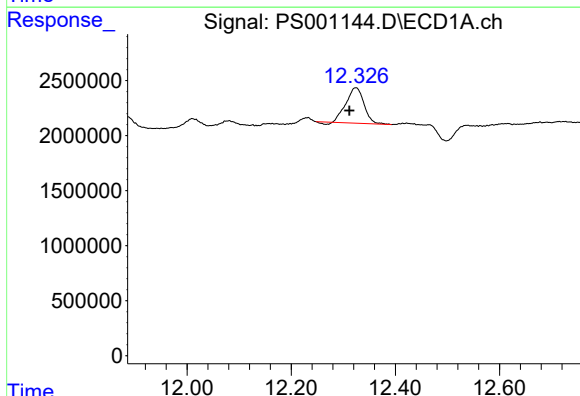


#6 MCPP

R.T.: 12.324 min
Delta R.T.: 0.012 min
Response: 7701529
Conc: 14.02 ug/ml

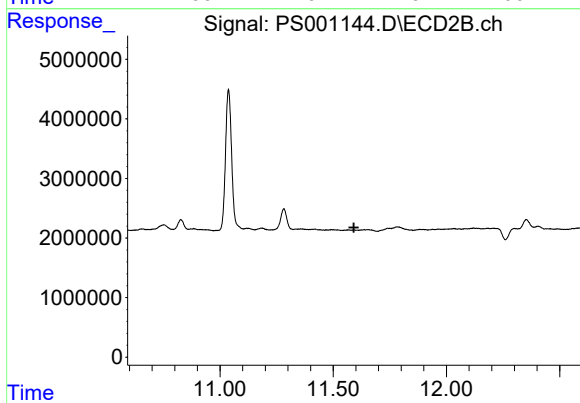

#6 MCPP


R.T.: 0.000 min
Exp R.T. : 11.591 min
Response: 0
Conc: N.D.

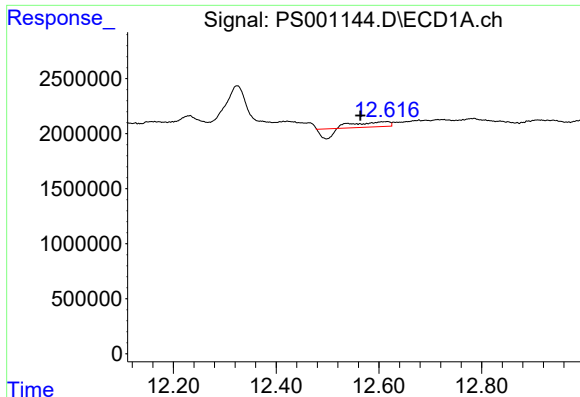

#7 MCPA


R.T.: 12.617 min
Delta R.T.: 0.053 min
Response: 1162711
Conc: 1.27 ug/ml

Instrument :
ECD_S
ClientSampleId :

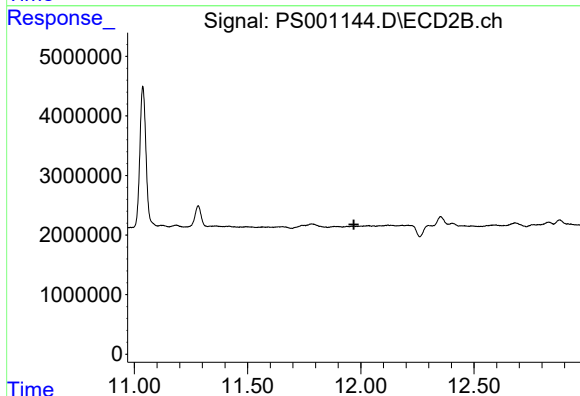


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 11.969 min
Response: 0
Conc: N.D.

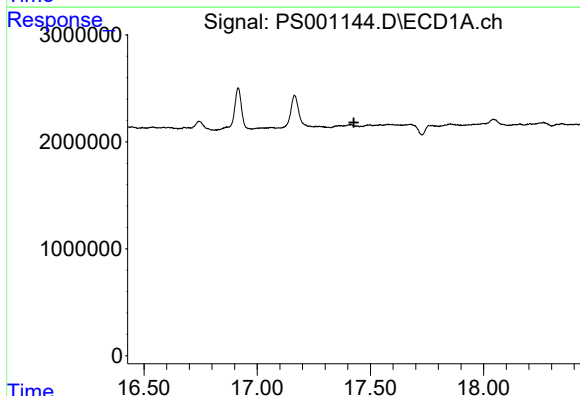


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 17.427 min
Response: 0
Conc: N.D.

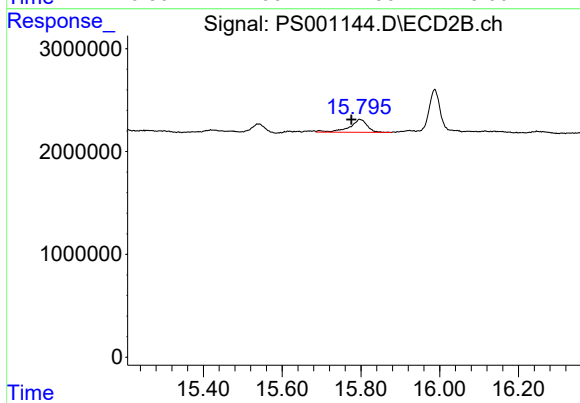

#14 DINOSEB


R.T.: 15.796 min
Delta R.T.: 0.020 min
Response: 3913375
Conc: 4.67 ng/ml

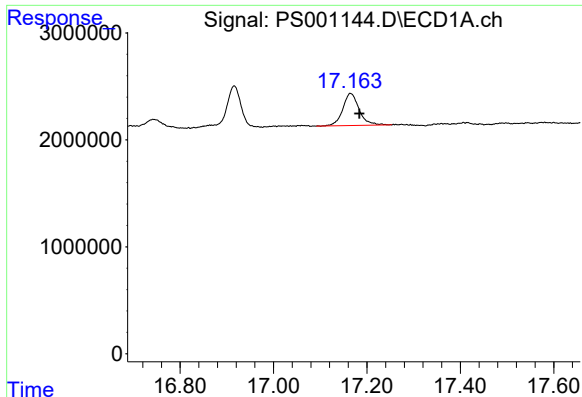

#15 Picloram


R.T.: 17.165 min
Delta R.T.: -0.019 min
Response: 7310808
Conc: 4.04 ng/ml

Instrument :
ECD_S
ClientSampleId :

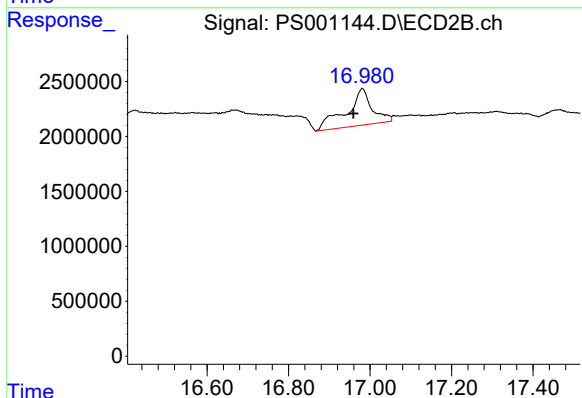


#15 Picloram

R.T.: 16.981 min
Delta R.T.: 0.022 min
Response: 14648083
Conc: 9.62 ng/ml

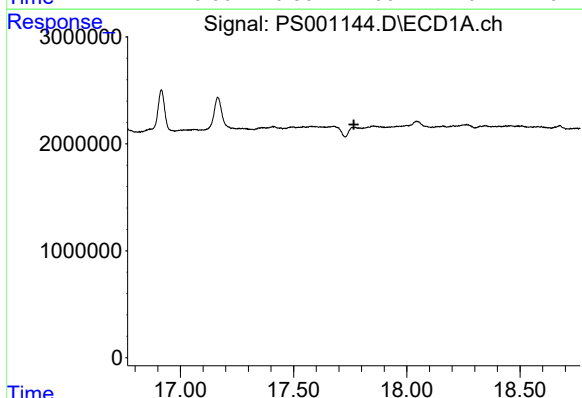

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.766 min
Response: 0
Conc: N.D.

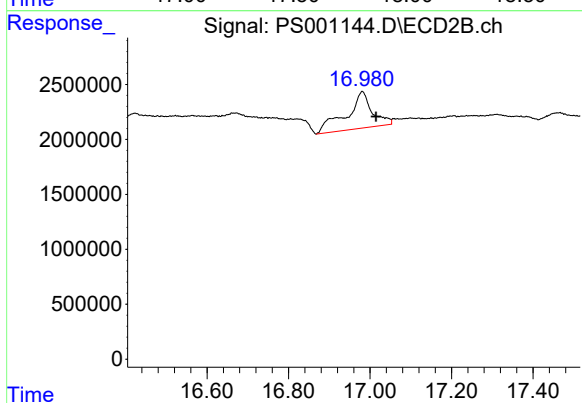

#16 DCPA

R.T.: 16.981 min
Delta R.T.: -0.034 min
Response: 14648083
Conc: 8.52 ng/ml