

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071918\
 Data File : PS001145.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jul 2018 11:45
 Operator : UA
 Sample : J4012-03RE
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 19 12:46:01 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 09 02:00:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.623	11.039	52325638	45815355	253.614	210.358
Target Compounds							
2) T	3,5-DICHL...	0.000	9.276	0	31354905	N.D.	106.594 #
6) T	MCPP	12.315	0.000	6991124	0	12.727	N.D. #
12) T	2,4,5-T	0.000	14.706	0	3007924	N.D.	2.907 #
15) T	Picloram	17.156	16.978	2867094	4283194	1.583	2.813 #
16) T	DCPA	0.000	16.978	0	4283194	N.D.	2.491 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071918\
Data File : PS001145.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jul 2018 11:45
Operator : UA
Sample : J4012-03RE
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 19 12:46:01 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
Quant Title : 8080.M
QLast Update : Mon Jul 09 02:00:25 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

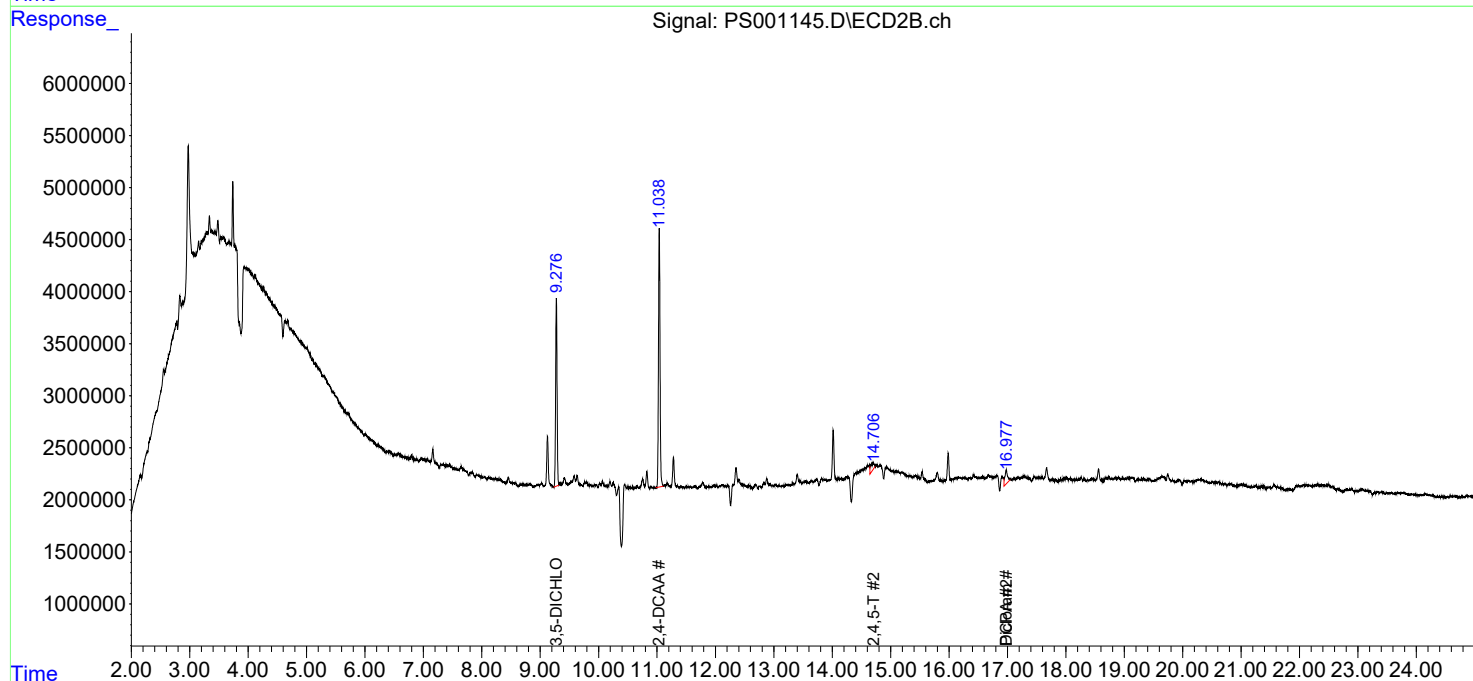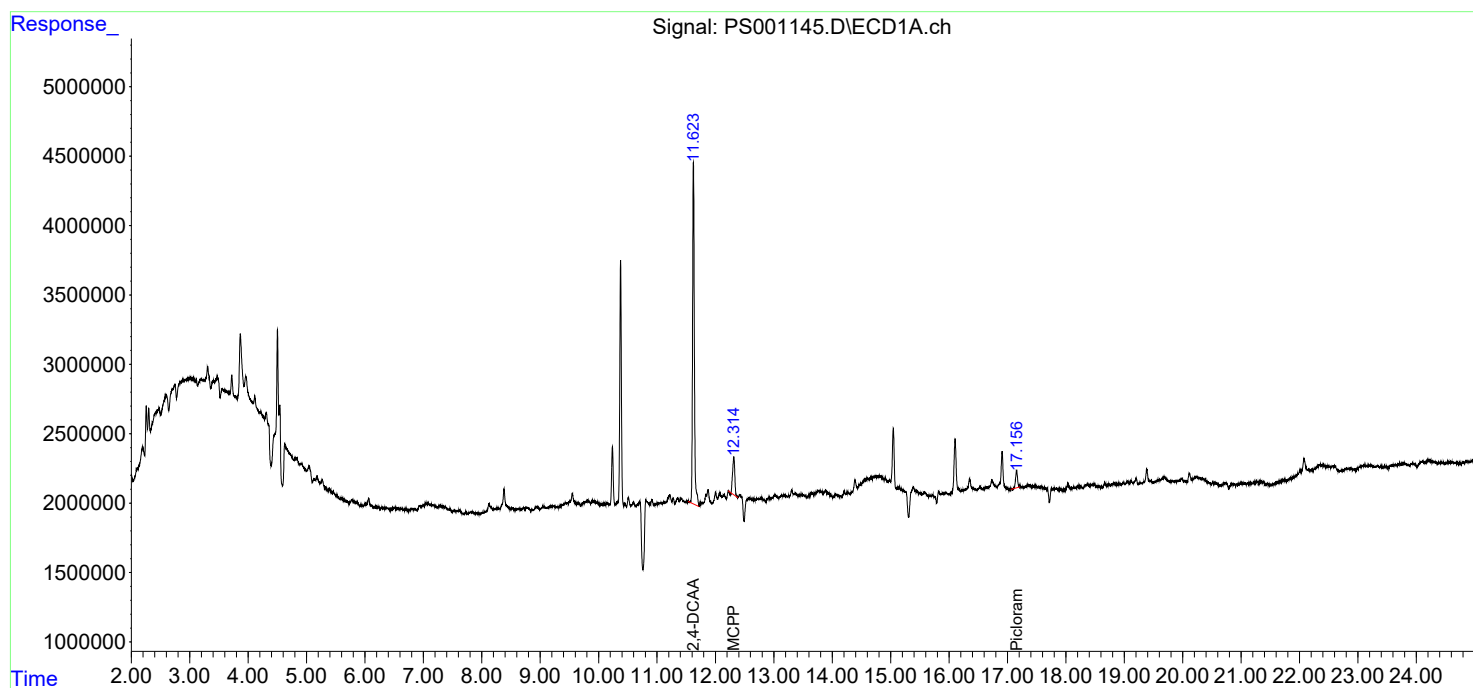


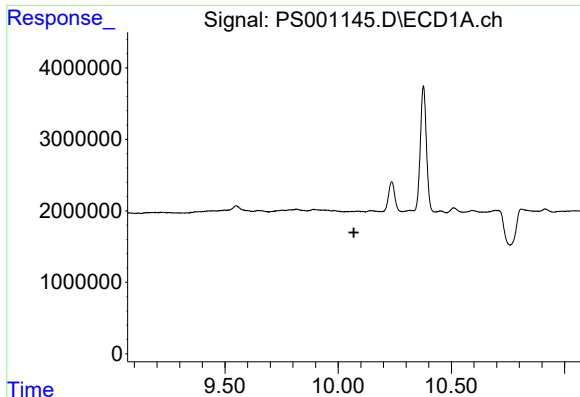

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 10.070 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

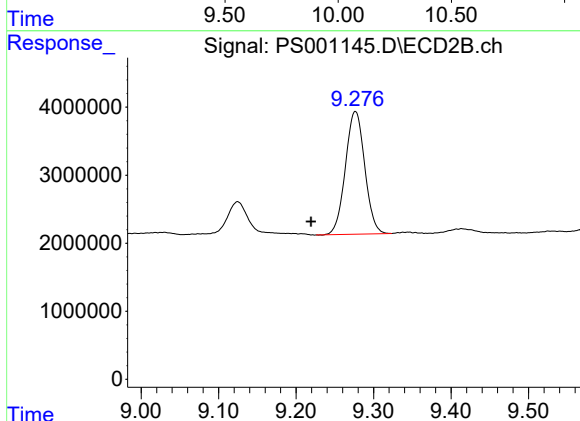


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.276 min
Delta R.T.: 0.057 min
Response: 31354905
Conc: 106.59 ng/ml

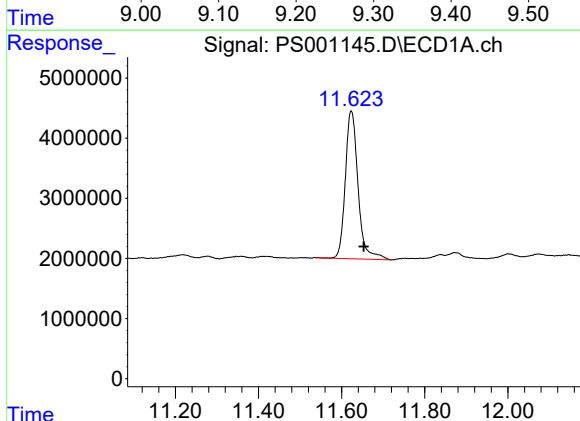


#4 2,4-DCAA

R.T.: 11.623 min
Delta R.T.: -0.030 min
Response: 52325638
Conc: 253.61 ng/ml

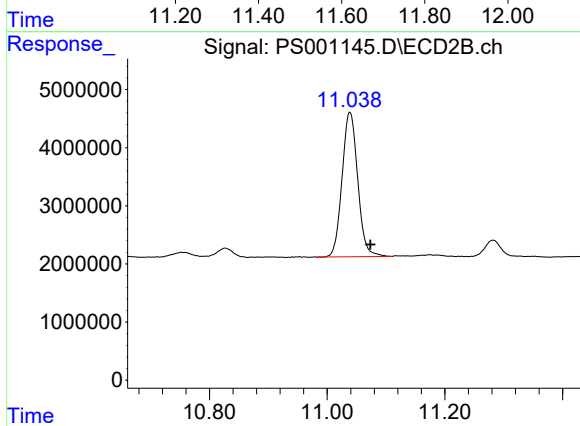

#4 2,4-DCAA


R.T.: 11.039 min
Delta R.T.: -0.035 min
Response: 45815355
Conc: 210.36 ng/ml

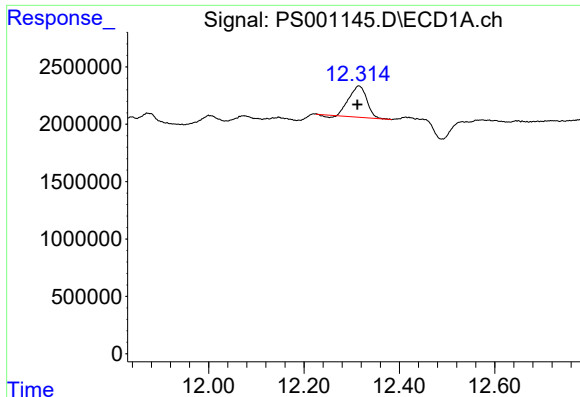

#6 MCPP


R.T.: 12.315 min
Delta R.T.: 0.003 min
Response: 6991124
Conc: 12.73 ug/ml

Instrument :
ECD_S
ClientSampleId :

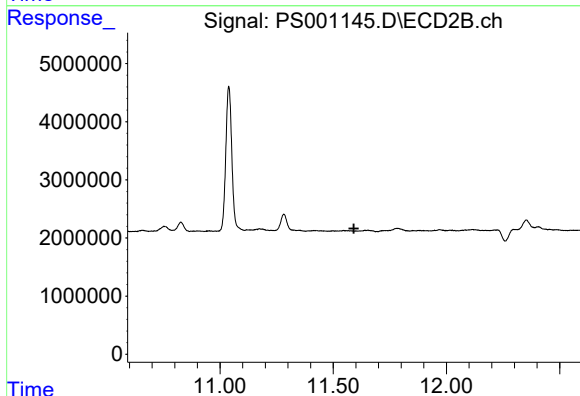


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 11.591 min
Response: 0
Conc: N.D.

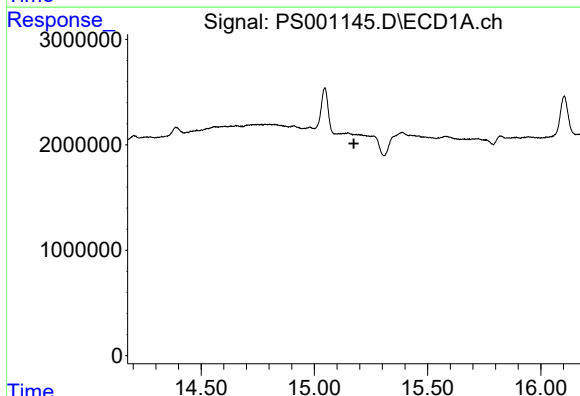


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 15.174 min
Response: 0
Conc: N.D.

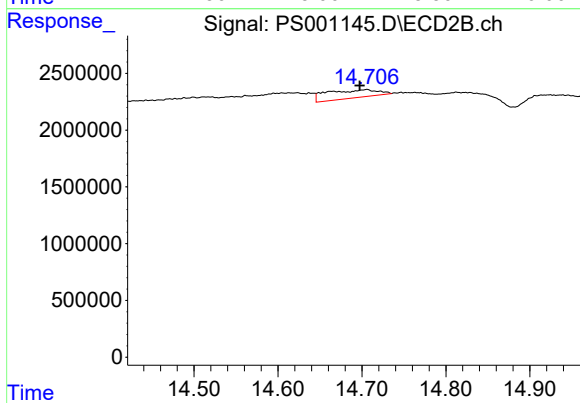

#12 2,4,5-T


R.T.: 14.706 min
Delta R.T.: 0.008 min
Response: 3007924
Conc: 2.91 ng/ml

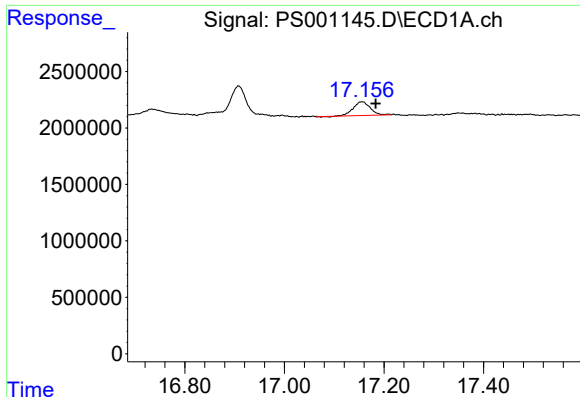

#15 Picloram


R.T.: 17.156 min
Delta R.T.: -0.028 min
Response: 2867094
Conc: 1.58 ng/ml

Instrument :
ECD_S
ClientSampleId :

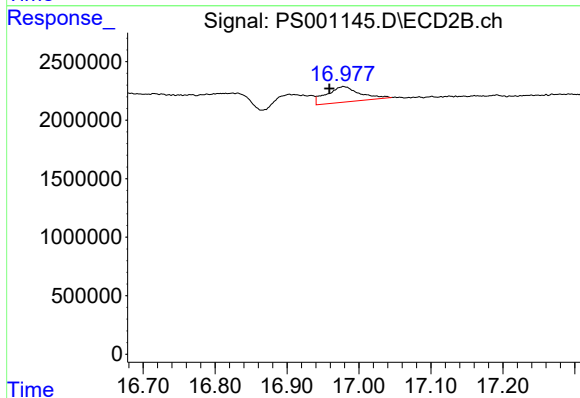


#15 Picloram

R.T.: 16.978 min
Delta R.T.: 0.019 min
Response: 4283194
Conc: 2.81 ng/ml

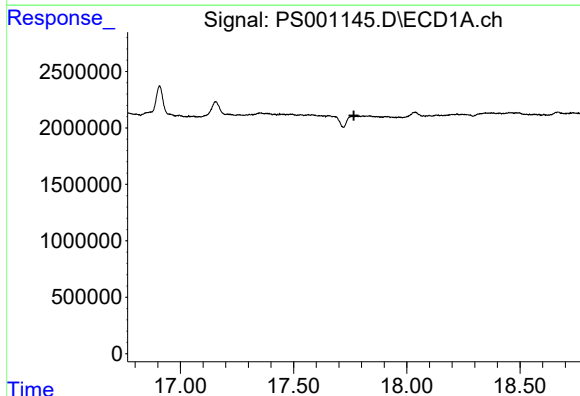

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.766 min
Response: 0
Conc: N.D.

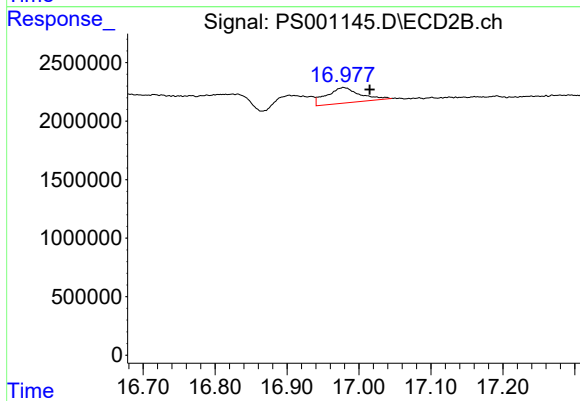

#16 DCPA

R.T.: 16.978 min
Delta R.T.: -0.037 min
Response: 4283194
Conc: 2.49 ng/ml