

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071918\
 Data File : PS001150.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jul 2018 14:53
 Operator : UA
 Sample : J4030-06
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 20 02:28:25 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 09 02:00:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.640	11.056	56341174	45830786	273.077	210.429
Target Compounds							
1) T	Dalapon	2.982	2.416	5263951	3797851	19.604	14.096 #
3) T	4-Nitroph...	0.000	10.212	0	6278491	N.D.	52.032 #
5) T	DICAMBA	12.019	11.300	4393218	7761966	5.580	9.889 #
6) T	MCP	12.333	0.000	8820523	0	16.058	N.D. #
15) T	Picloram	0.000	16.993	0	3535235	N.D.	2.322 #
16) T	DCPA	0.000	16.993	0	3535235	N.D.	2.056 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071918\
Data File : PS001150.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jul 2018 14:53
Operator : UA
Sample : J4030-06
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 20 02:28:25 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
Quant Title : 8080.M
QLast Update : Mon Jul 09 02:00:25 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

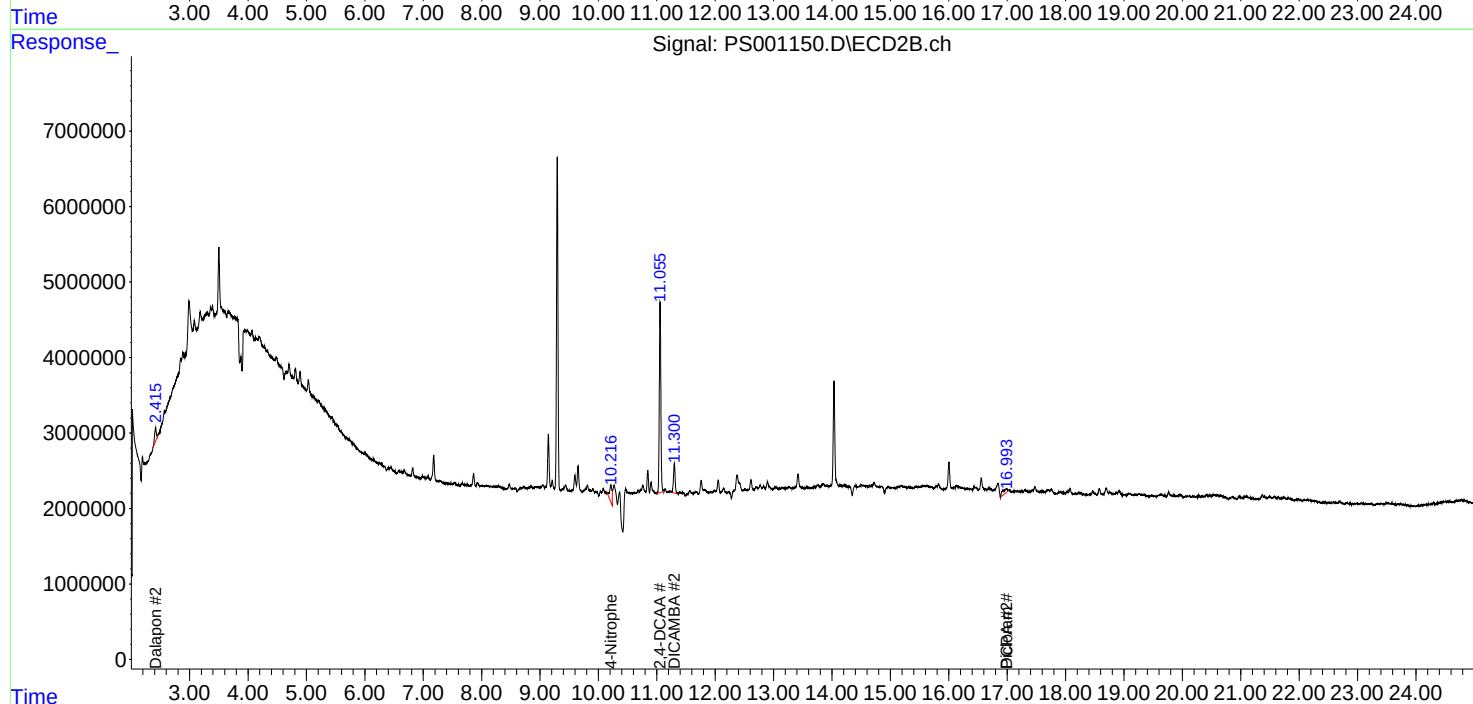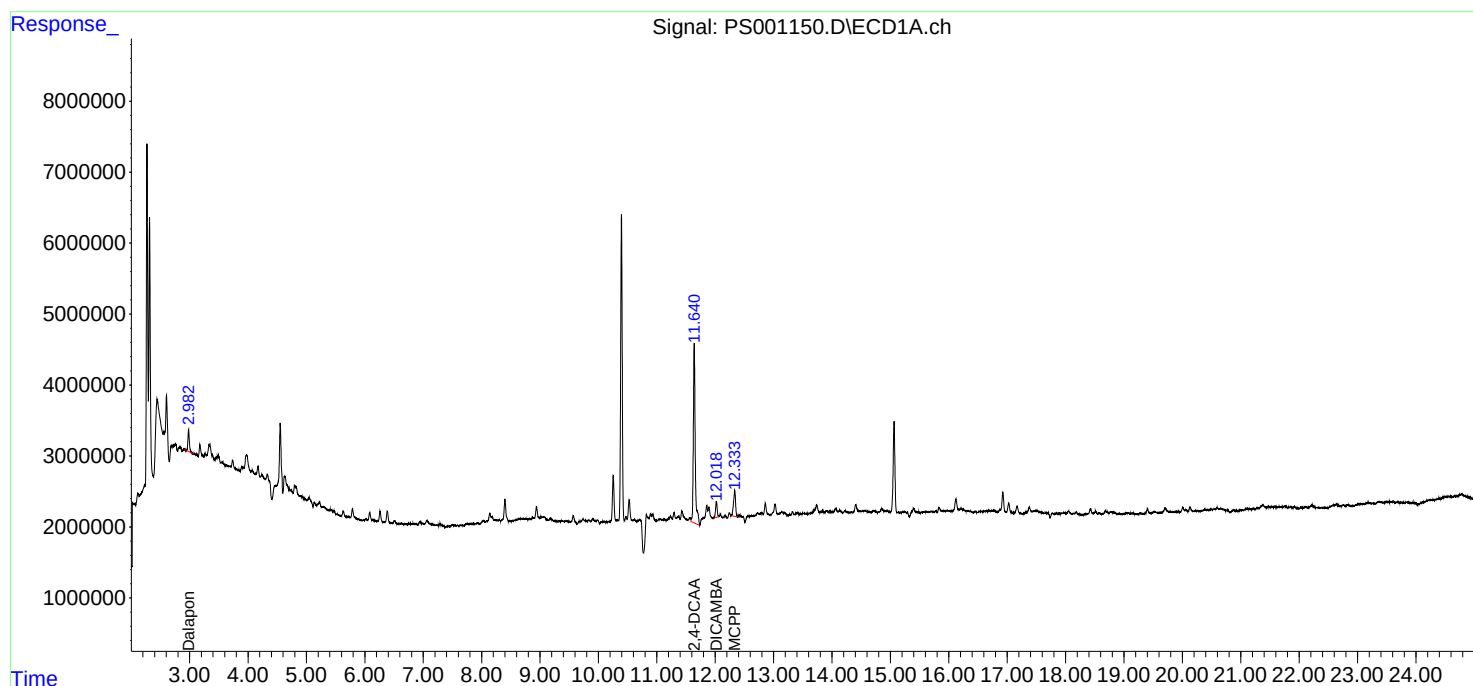


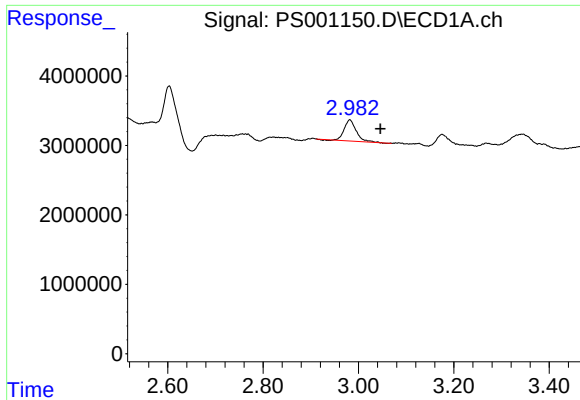

#1 Dalapon


R.T.: 2.982 min
Delta R.T.: -0.064 min
Response: 5263951
Conc: 19.60 ng/ml

Instrument :
ECD_S
ClientSampleId :

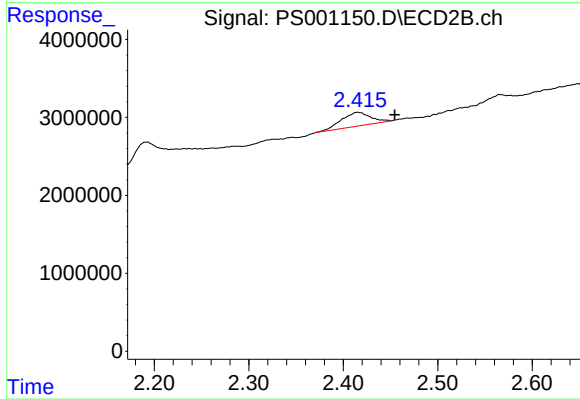


#1 Dalapon

R.T.: 2.416 min
Delta R.T.: -0.039 min
Response: 3797851
Conc: 14.10 ng/ml

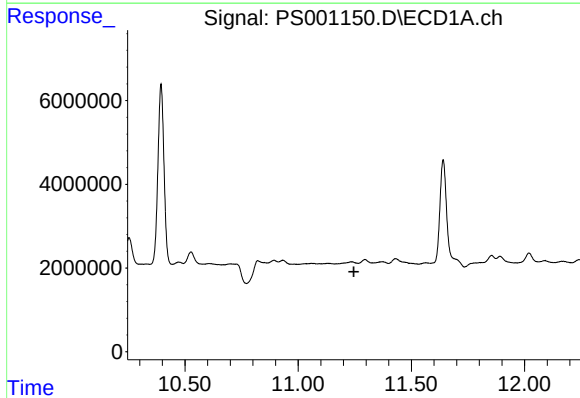


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 11.246 min
Response: 0
Conc: N.D.

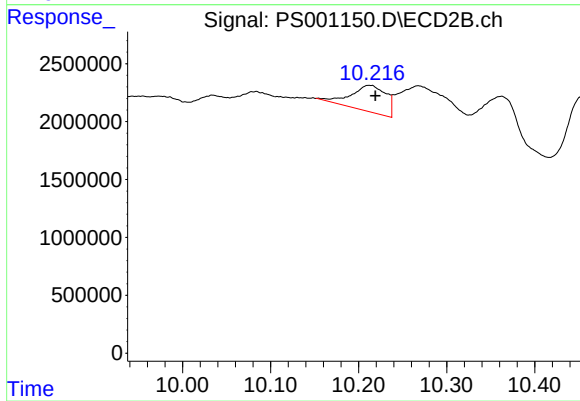

#3 4-Nitrophenol


R.T.: 10.212 min
Delta R.T.: -0.007 min
Response: 6278491
Conc: 52.03 ng/ml

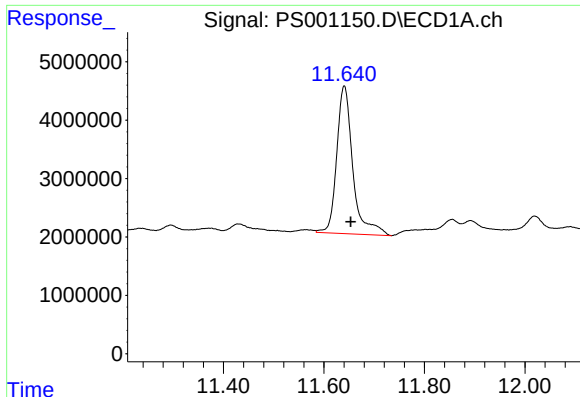

#4 2,4-DCAA


R.T.: 11.640 min
Delta R.T.: -0.013 min
Response: 56341174
Conc: 273.08 ng/ml

Instrument :
ECD_S
ClientSampleId :

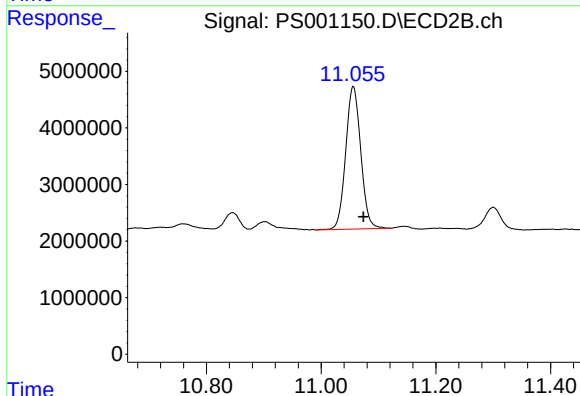


#4 2,4-DCAA

R.T.: 11.056 min
Delta R.T.: -0.018 min
Response: 45830786
Conc: 210.43 ng/ml

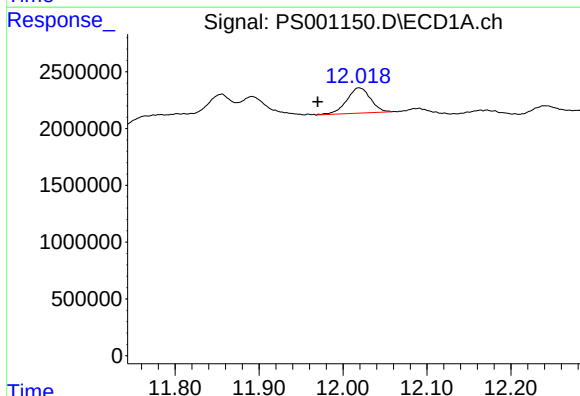


#5 DICAMBA

R.T.: 12.019 min
Delta R.T.: 0.049 min
Response: 4393218
Conc: 5.58 ng/ml

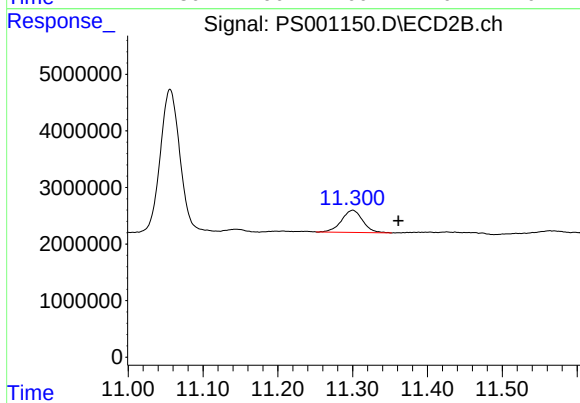

#5 DICAMBA


R.T.: 11.300 min
Delta R.T.: -0.061 min
Response: 7761966
Conc: 9.89 ng/ml

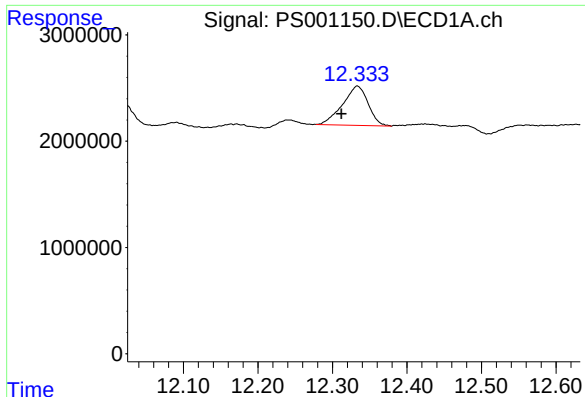

#6 MCP


R.T.: 12.333 min
Delta R.T.: 0.021 min
Response: 8820523
Conc: 16.06 ug/ml

Instrument :
ECD_S
ClientSampleId :

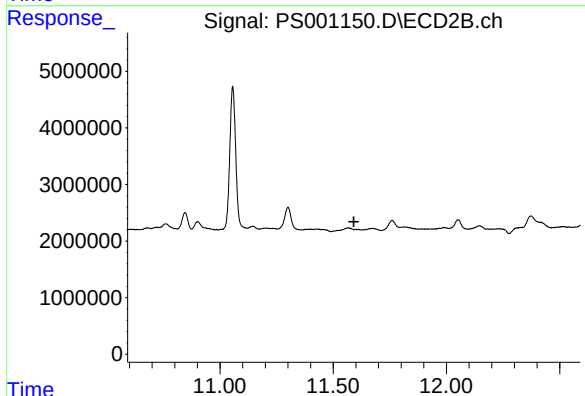


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.591 min
Response: 0
Conc: N.D.

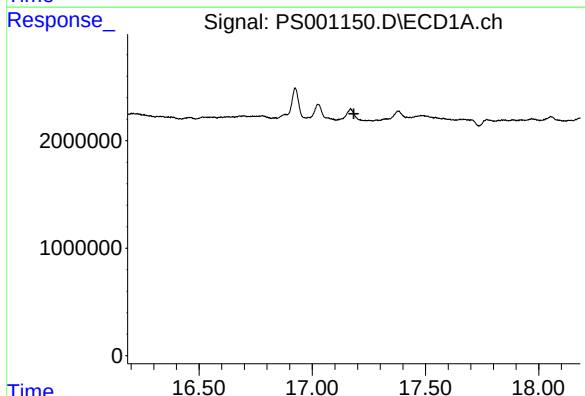


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 17.184 min
Response: 0
Conc: N.D.

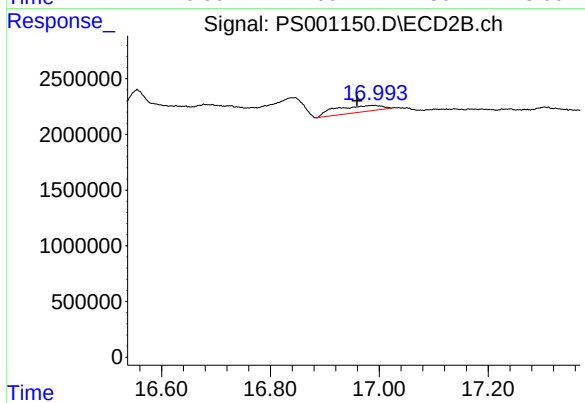

#15 Picloram


R.T.: 16.993 min
Delta R.T.: 0.033 min
Response: 3535235
Conc: 2.32 ng/ml

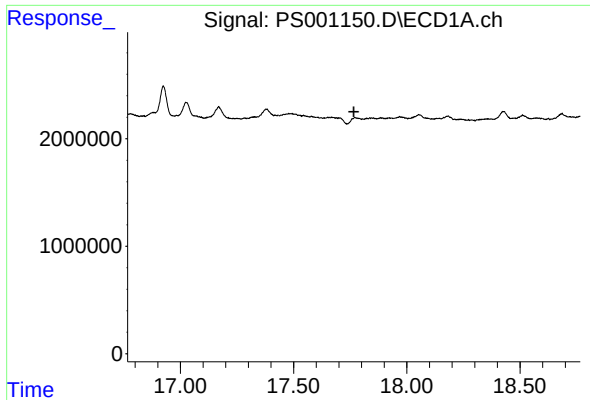

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.766 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

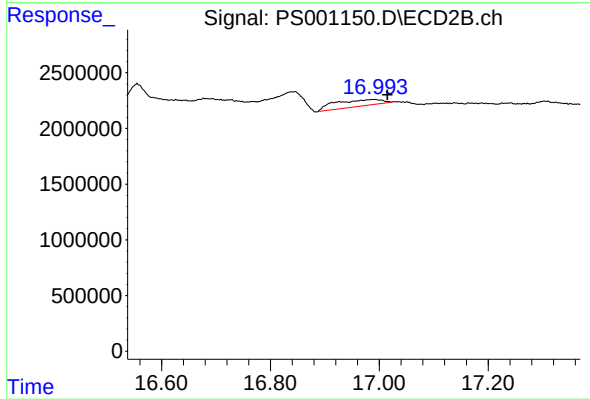

#16 DCPA

R.T.: 16.993 min
Delta R.T.: -0.023 min
Response: 3535235
Conc: 2.06 ng/ml