

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS071918\  
 Data File : PS001151.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 19 Jul 2018 15:24  
 Operator : UA  
 Sample : J4030-09  
 Misc :  
 ALS Vial : 9 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Jul 20 02:28:45 2018  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS070818.M  
 Quant Title : 8080.M  
 QLast Update : Mon Jul 09 02:00:25 2018  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

|                             | Compound     | RT#1   | RT#2   | Resp#1   | Resp#2   | ng/ml   | ng/ml     |
|-----------------------------|--------------|--------|--------|----------|----------|---------|-----------|
| -----                       |              |        |        |          |          |         |           |
| System Monitoring Compounds |              |        |        |          |          |         |           |
| 4) S                        | 2,4-DCAA     | 11.630 | 11.047 | 52311934 | 43339794 | 253.547 | 198.992   |
| Target Compounds            |              |        |        |          |          |         |           |
| 1) T                        | Dalapon      | 0.000  | 2.407  | 0        | 3314763  | N.D.    | 12.303 #  |
| 2) T                        | 3,5-DICHL... | 0.000  | 9.284  | 0        | 43266552 | N.D.    | 147.088 # |
| 5) T                        | DICAMBA      | 12.008 | 0.000  | 2960406  | 0        | 3.760   | N.D. #    |
| 6) T                        | MCP          | 12.323 | 0.000  | 8078390  | 0        | 14.707  | N.D. #    |
| 15) T                       | Picloram     | 0.000  | 16.973 | 0        | 3830613  | N.D.    | 2.516 #   |
| 16) T                       | DCPA         | 0.000  | 16.973 | 0        | 3830613  | N.D.    | 2.228 #   |
| -----                       |              |        |        |          |          |         |           |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS071918\  
Data File : PS001151.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 19 Jul 2018 15:24  
Operator : UA  
Sample : J4030-09  
Misc :  
ALS Vial : 9 Sample Multiplier: 1

Instrument :  
ECD\_S  
ClientSampleId :

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Jul 20 02:28:45 2018  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS070818.M  
Quant Title : 8080.M  
QLast Update : Mon Jul 09 02:00:25 2018  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

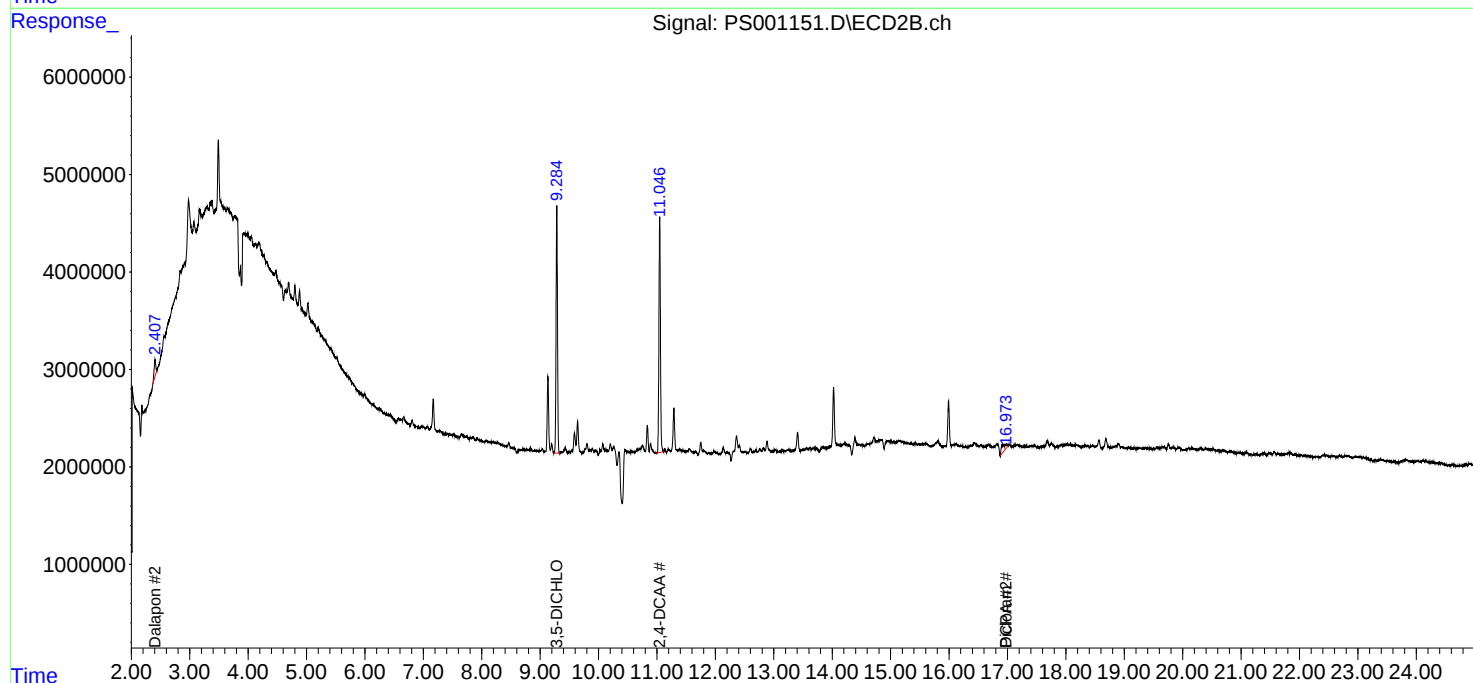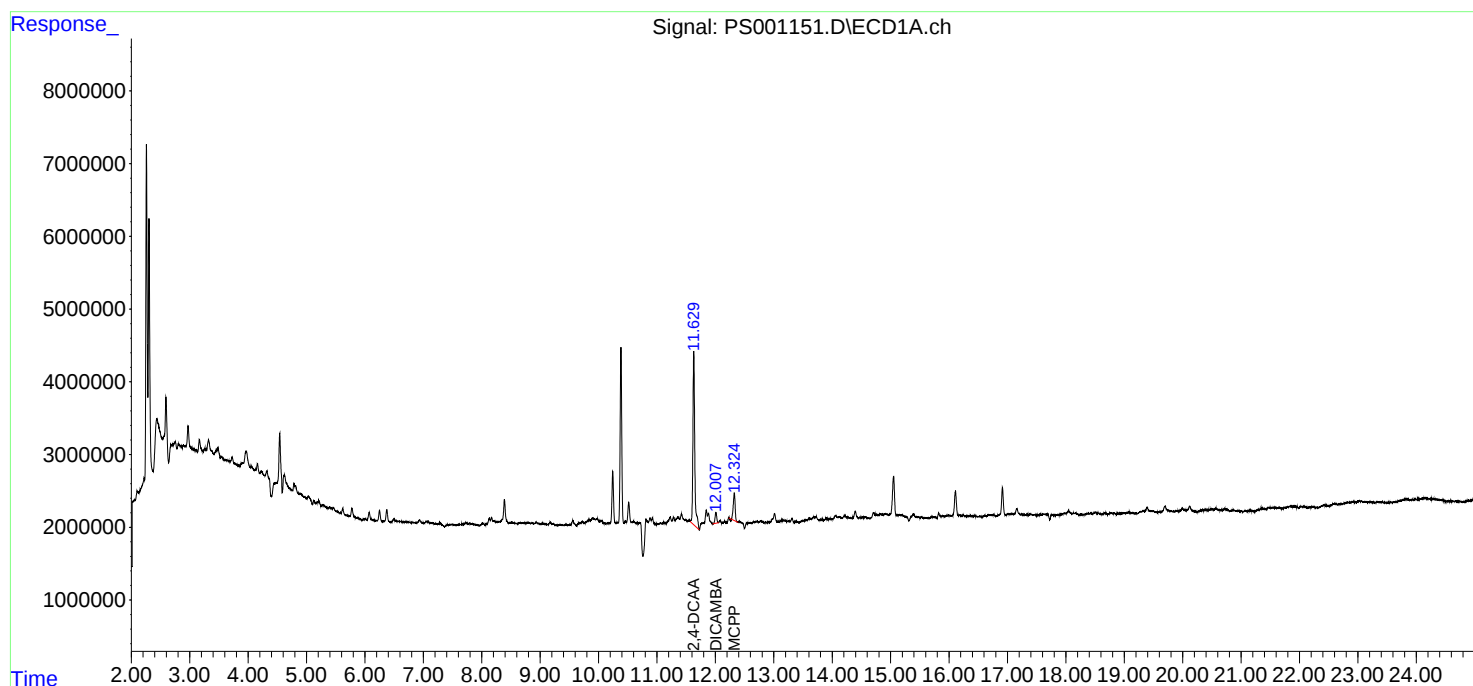


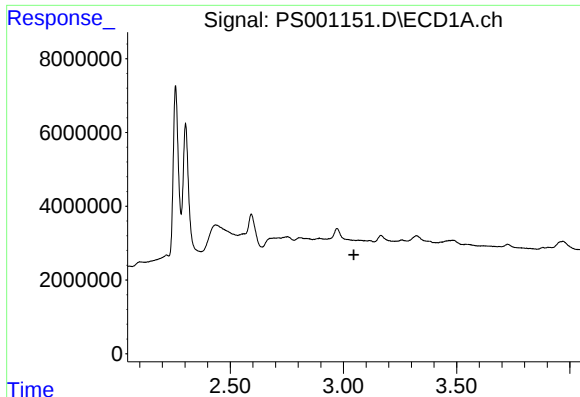

#1 Dalapon


R.T.: 0.000 min  
Exp R.T. : 3.046 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_S  
ClientSampleId :

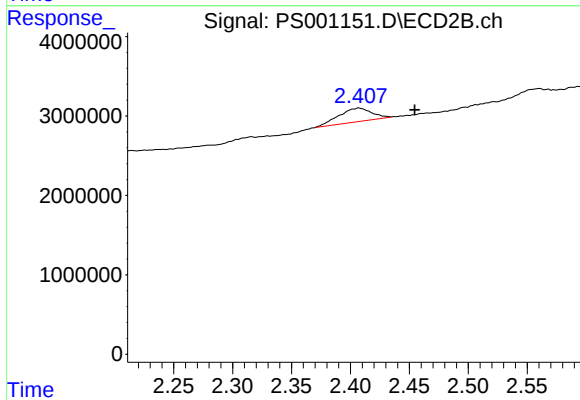


#1 Dalapon

R.T.: 2.407 min  
Delta R.T.: -0.048 min  
Response: 3314763  
Conc: 12.30 ng/ml

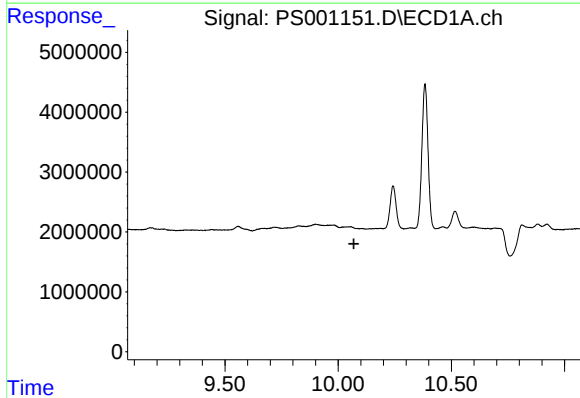


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min  
Exp R.T. : 10.070 min  
Response: 0  
Conc: N.D.

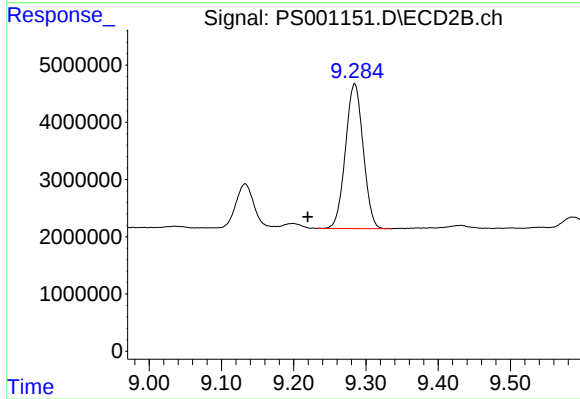

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.284 min  
Delta R.T.: 0.065 min  
Response: 43266552  
Conc: 147.09 ng/ml

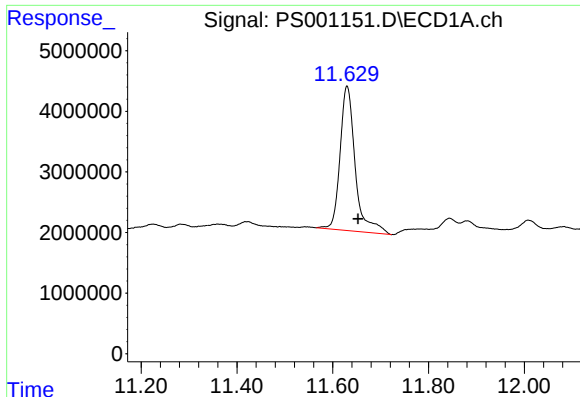

#4 2,4-DCAA


R.T.: 11.630 min  
Delta R.T.: -0.024 min  
Response: 52311934  
Conc: 253.55 ng/ml

Instrument :  
ECD\_S  
ClientSampleId :

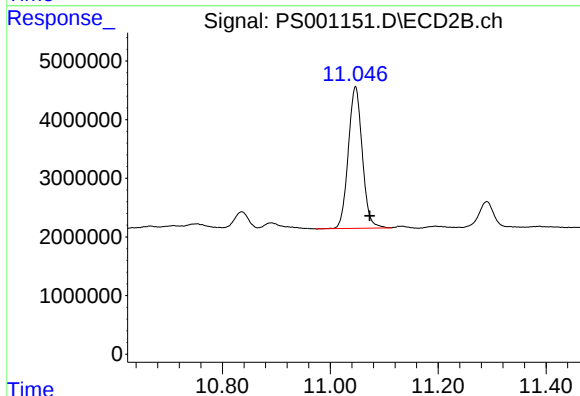


#4 2,4-DCAA

R.T.: 11.047 min  
Delta R.T.: -0.027 min  
Response: 43339794  
Conc: 198.99 ng/ml

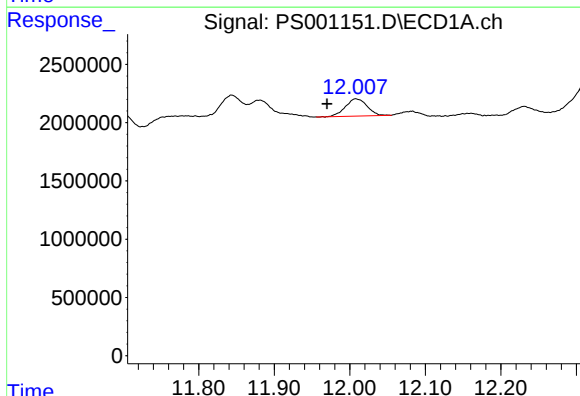


#5 DICAMBA

R.T.: 12.008 min  
Delta R.T.: 0.038 min  
Response: 2960406  
Conc: 3.76 ng/ml

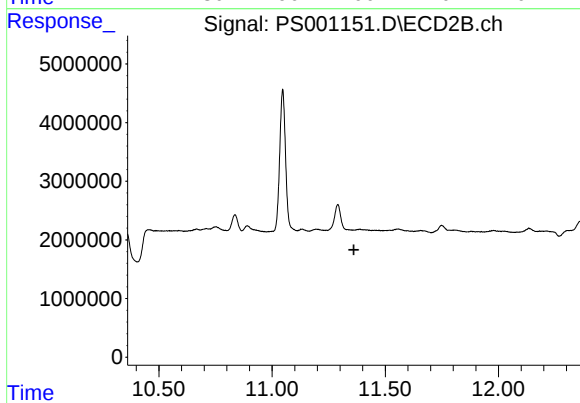

#5 DICAMBA


R.T.: 0.000 min  
Exp R.T.: 11.361 min  
Response: 0  
Conc: N.D.

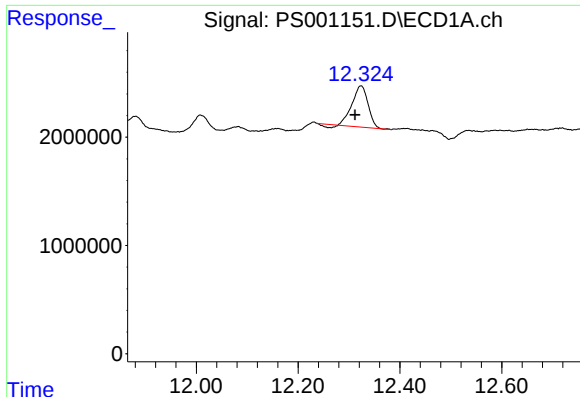

#6 MCP


R.T.: 12.323 min  
Delta R.T.: 0.011 min  
Response: 8078390  
Conc: 14.71 ug/ml

Instrument :  
ECD\_S  
ClientSampleId :

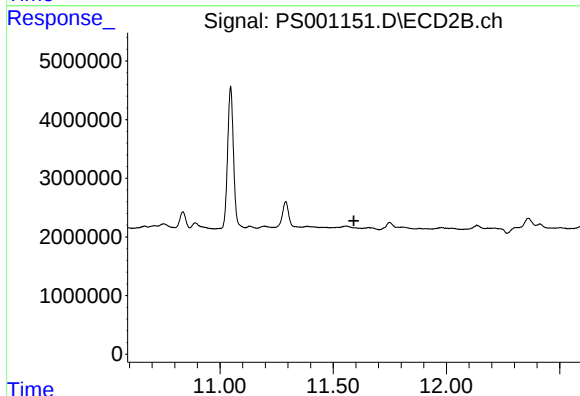


#6 MCP

R.T.: 0.000 min  
Exp R.T. : 11.591 min  
Response: 0  
Conc: N.D.

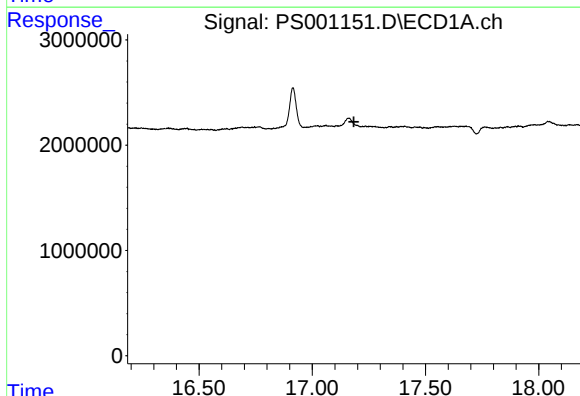


#15 Picloram

R.T.: 0.000 min  
Exp R.T. : 17.184 min  
Response: 0  
Conc: N.D.

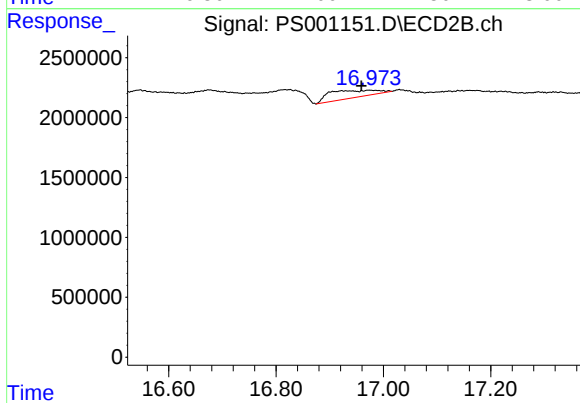

#15 Picloram


R.T.: 16.973 min  
Delta R.T.: 0.014 min  
Response: 3830613  
Conc: 2.52 ng/ml

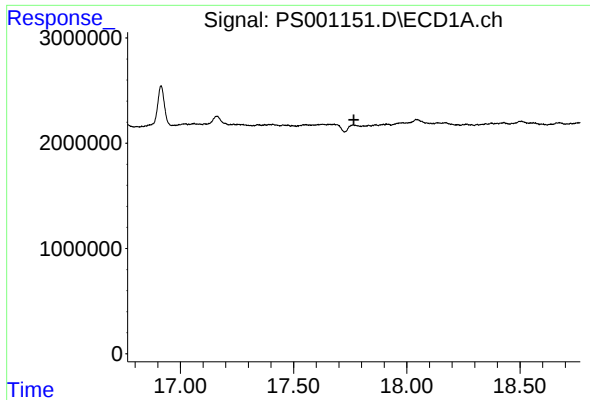

#16 DCPA

R.T.: 0.000 min  
Exp R.T.: 17.766 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_S  
ClientSampleId :

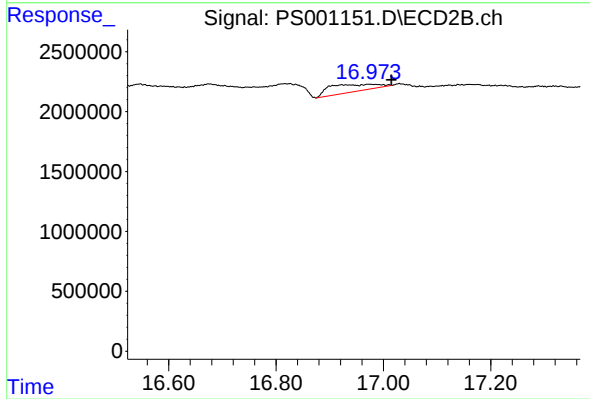

#16 DCPA

R.T.: 16.973 min  
Delta R.T.: -0.042 min  
Response: 3830613  
Conc: 2.23 ng/ml