

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071918\
 Data File : PS001153.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jul 2018 16:26
 Operator : UA
 Sample : J4016-21
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 20 02:29:23 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 09 02:00:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.626	11.042	54573840	42033218	264.511	192.993 #
Target Compounds							
1) T	Dalapon	0.000	2.410	0	733784	N.D.	2.723 #
2) T	3,5-DICHL...	0.000	9.280	0	67140726	N.D.	228.251 #
5) T	DICAMBA	12.004	0.000	4854147	0	6.165	N.D. #
6) T	MCP	12.319	0.000	6250063	0	11.378	N.D. #
15) T	Picloram	17.158	16.984	5039324	4010129	2.783	2.634
16) T	DCPA	0.000	16.984	0	4010129	N.D.	2.333 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071918\
Data File : PS001153.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jul 2018 16:26
Operator : UA
Sample : J4016-21
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 20 02:29:23 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
Quant Title : 8080.M
QLast Update : Mon Jul 09 02:00:25 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

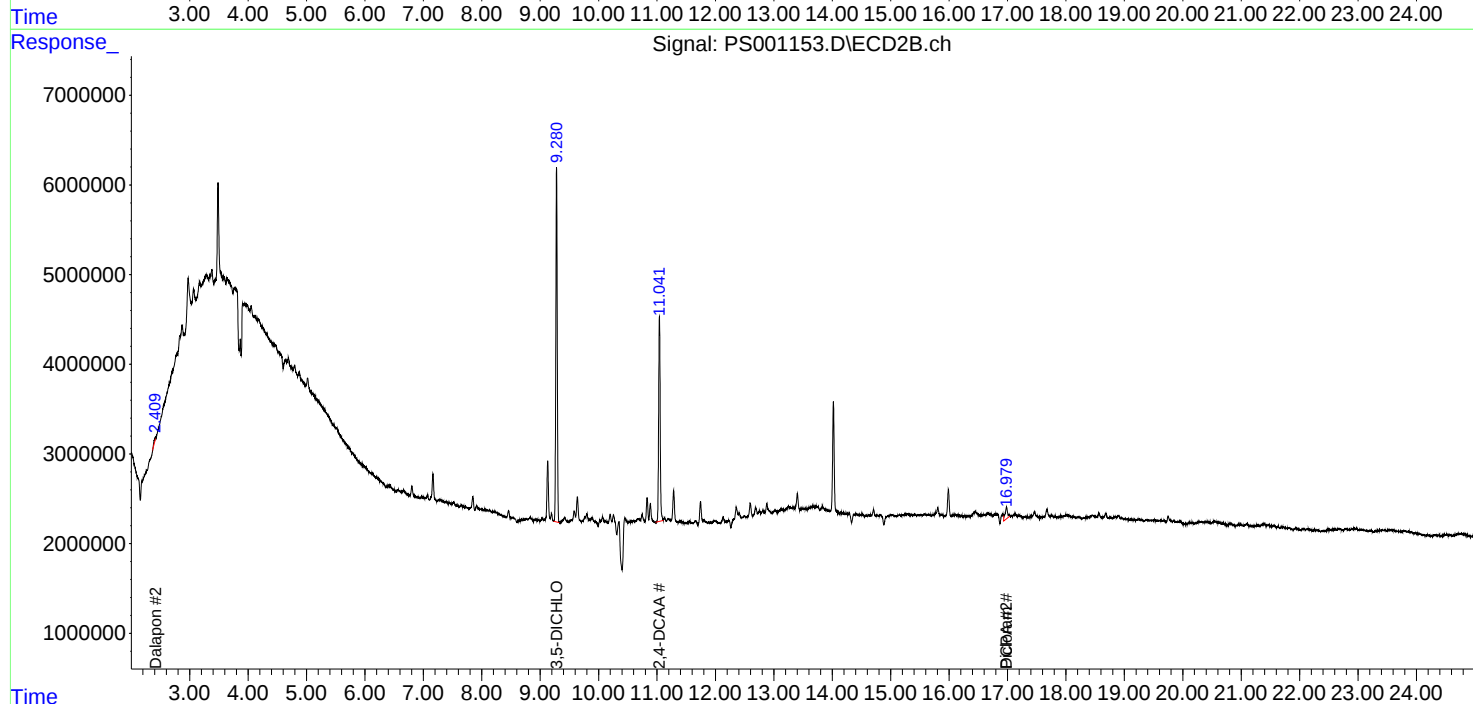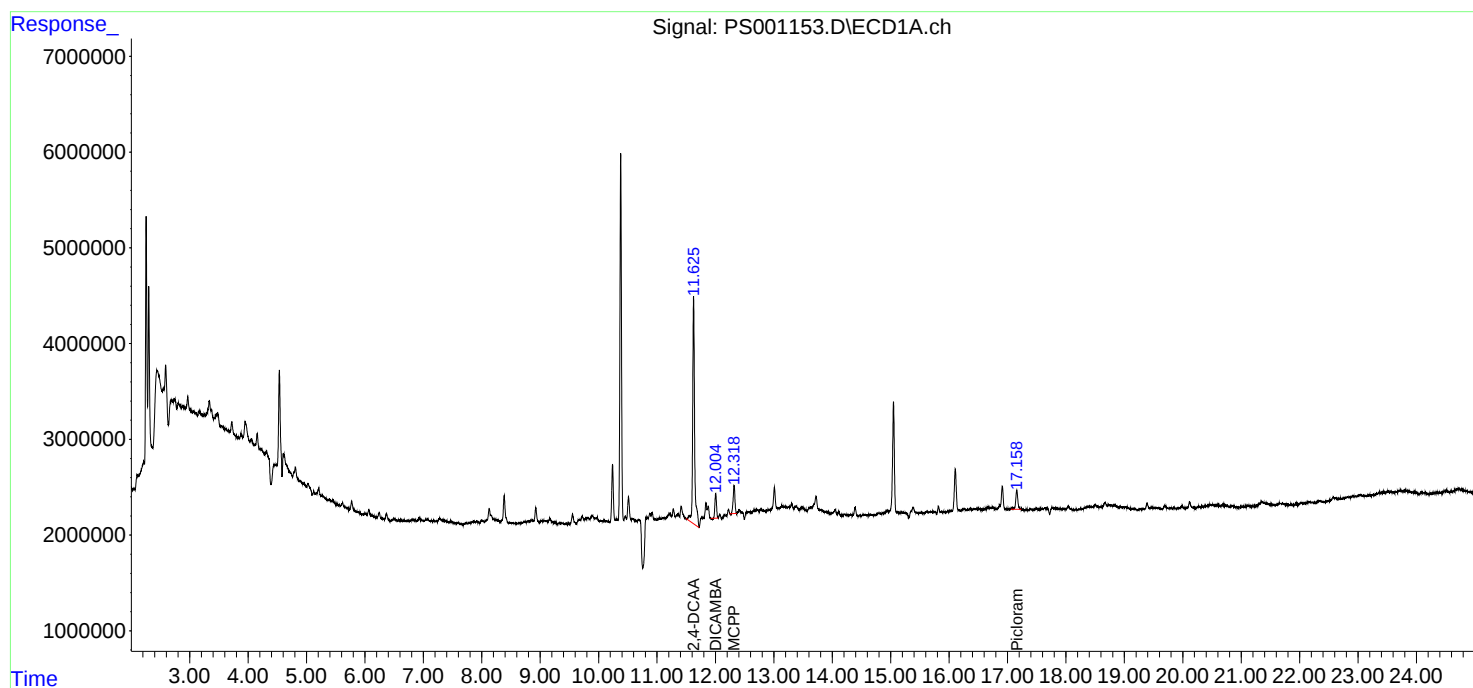


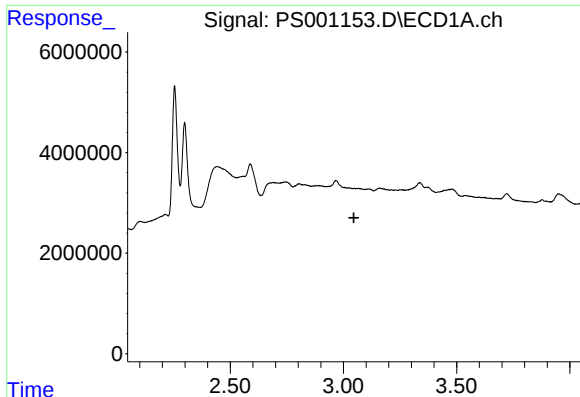

#1 Dalapon


R.T.: 0.000 min
Exp R.T. : 3.046 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

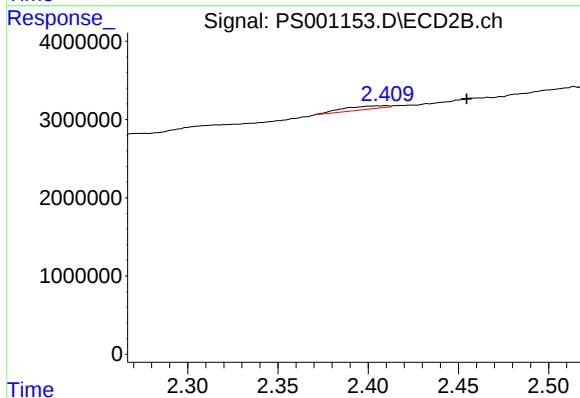


#1 Dalapon

R.T.: 2.410 min
Delta R.T.: -0.045 min
Response: 733784
Conc: 2.72 ng/ml

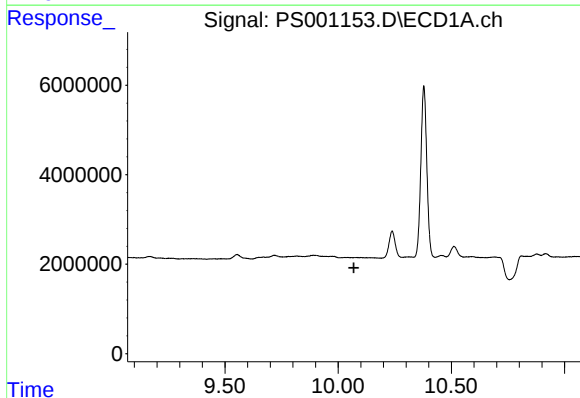


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 10.070 min
Response: 0
Conc: N.D.

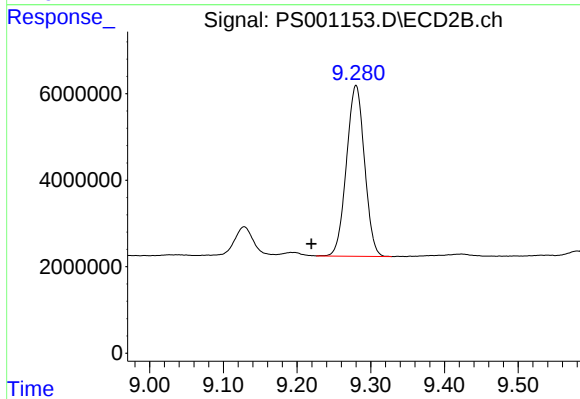

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.280 min
Delta R.T.: 0.061 min
Response: 67140726
Conc: 228.25 ng/ml

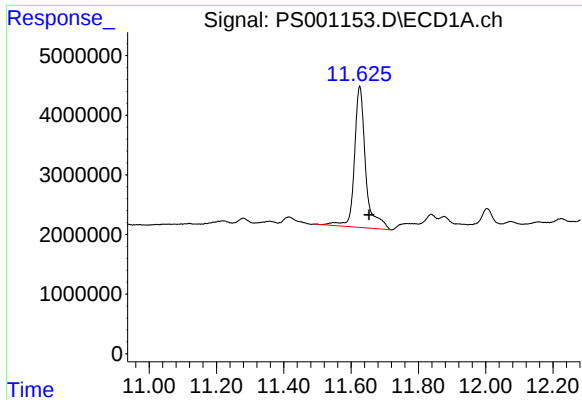

#4 2,4-DCAA


R.T.: 11.626 min
Delta R.T.: -0.028 min
Response: 54573840
Conc: 264.51 ng/ml

Instrument :
ECD_S
ClientSampleId :

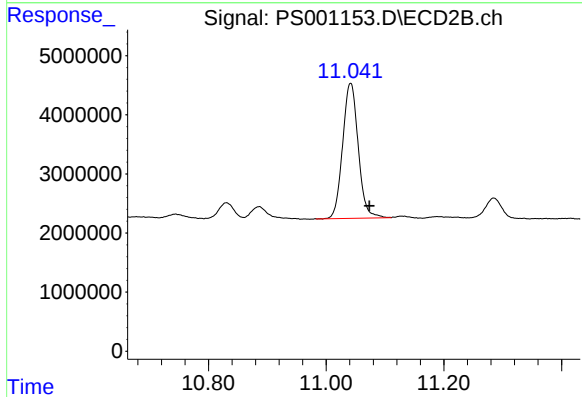


#4 2,4-DCAA

R.T.: 11.042 min
Delta R.T.: -0.032 min
Response: 42033218
Conc: 192.99 ng/ml

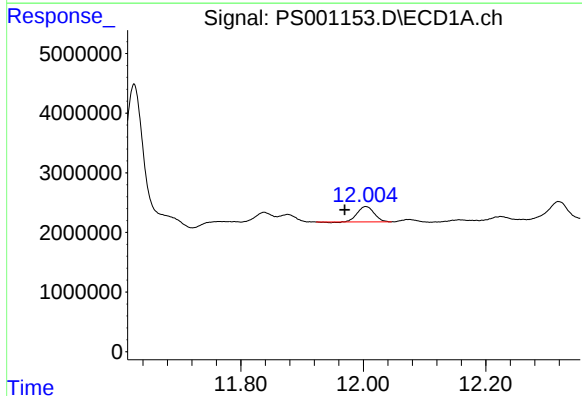


#5 DICAMBA

R.T.: 12.004 min
Delta R.T.: 0.034 min
Response: 4854147
Conc: 6.16 ng/ml

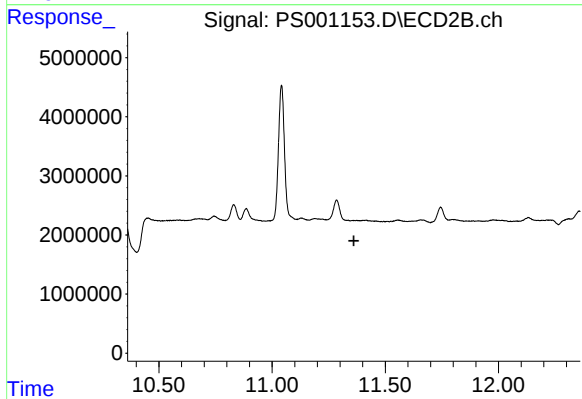

#5 DICAMBA


R.T.: 0.000 min
Exp R.T. : 11.361 min
Response: 0
Conc: N.D.

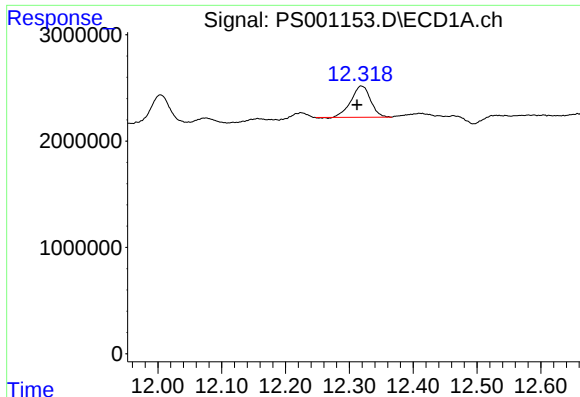

#6 MCPP


R.T.: 12.319 min
Delta R.T.: 0.007 min
Response: 6250063
Conc: 11.38 ug/ml

Instrument :
ECD_S
ClientSampleId :

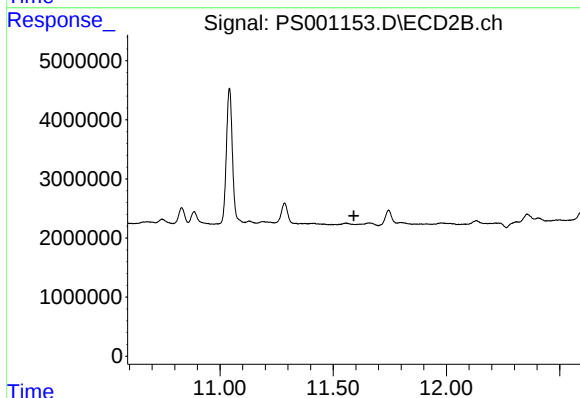


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 11.591 min
Response: 0
Conc: N.D.

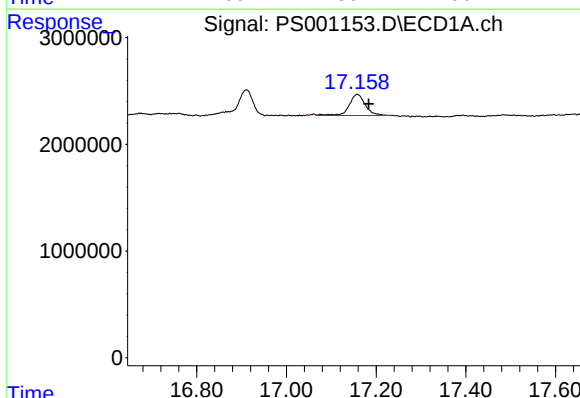


#15 Picloram

R.T.: 17.158 min
Delta R.T.: -0.026 min
Response: 5039324
Conc: 2.78 ng/ml

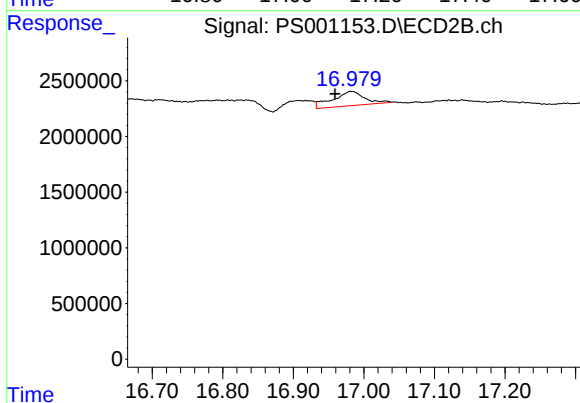

#15 Picloram


R.T.: 16.984 min
Delta R.T.: 0.025 min
Response: 4010129
Conc: 2.63 ng/ml

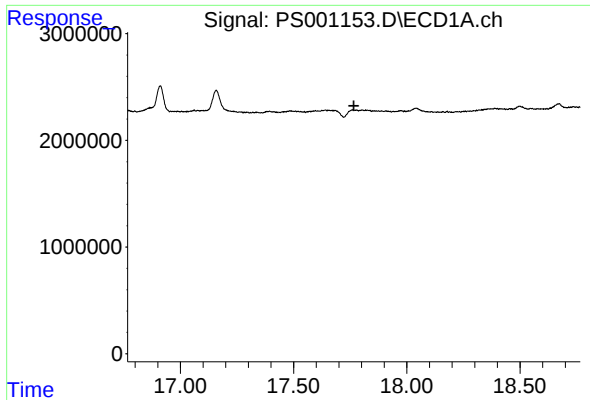

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.766 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

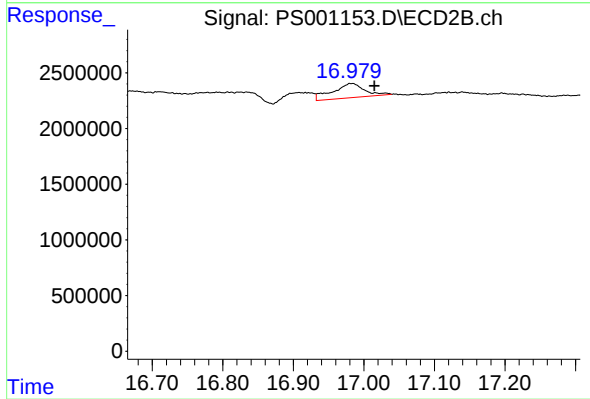

#16 DCPA

R.T.: 16.984 min
Delta R.T.: -0.031 min
Response: 4010129
Conc: 2.33 ng/ml