

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071918\
 Data File : PS001154.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jul 2018 16:57
 Operator : UA
 Sample : J4016-24
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 20 02:29:42 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 09 02:00:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.664	11.079	51494989	43191854	249.588	198.312
Target Compounds							
1) T	Dalapon	3.005	2.445	3055358	2110116	11.379	7.832 #
2) T	3,5-DICHL...	0.000	9.166	0	10045490	N.D.	34.150 #
5) T	DICAMBA	0.000	11.323	0	5864165	N.D.	7.471 #
6) T	MCP	12.357	0.000	5936131	0	10.807	N.D. #
8) T	DICHLORPROP	0.000	12.446	0	1705293	N.D.	8.443 #
11) T	2,4,5-TP ...	0.000	14.058	0	21739601	N.D.	17.323 #
12) T	2,4,5-T	0.000	14.747	0	2062950	N.D.	1.994 #
15) T	Picloram	17.195	0.000	2324133	0	1.283	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071918\
Data File : PS001154.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jul 2018 16:57
Operator : UA
Sample : J4016-24
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 20 02:29:42 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
Quant Title : 8080.M
QLast Update : Mon Jul 09 02:00:25 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

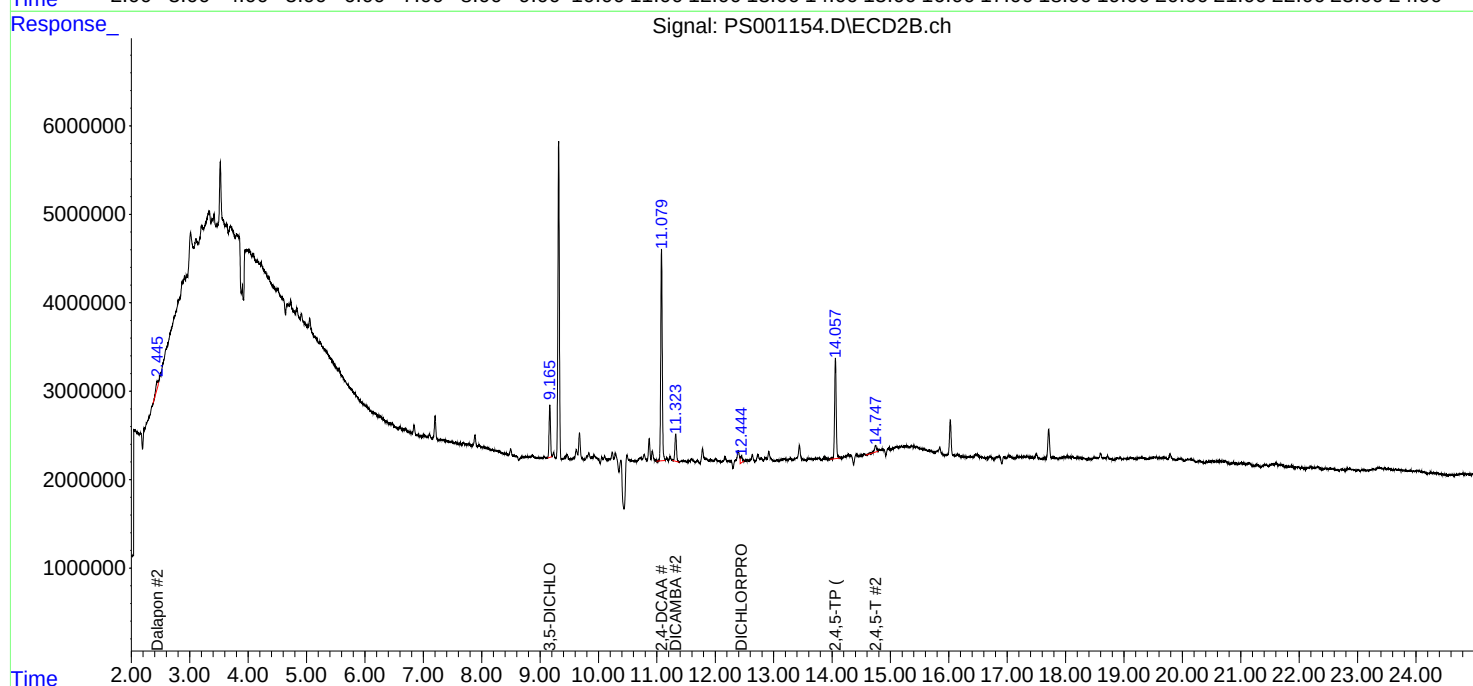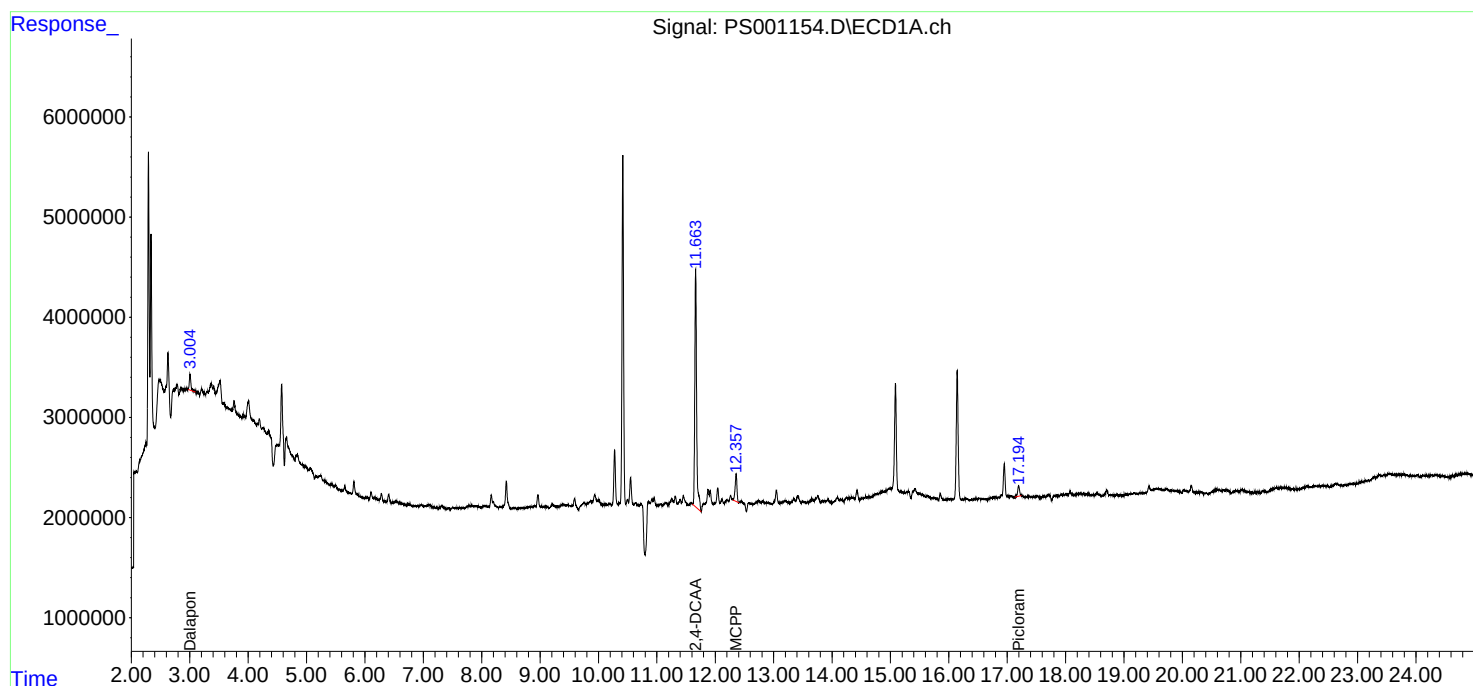


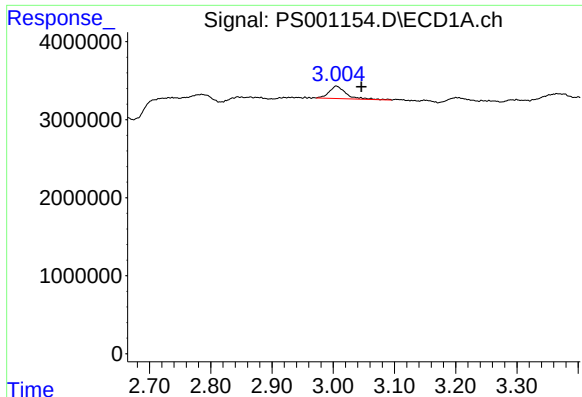

#1 Dalapon


R.T.: 3.005 min
Delta R.T.: -0.041 min
Response: 3055358
Conc: 11.38 ng/ml

Instrument :
ECD_S
ClientSampleId :

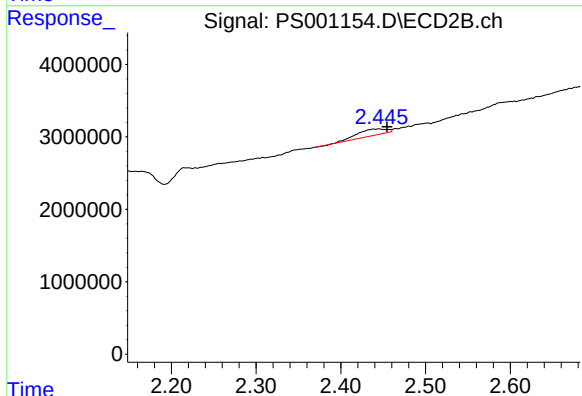


#1 Dalapon

R.T.: 2.445 min
Delta R.T.: -0.010 min
Response: 2110116
Conc: 7.83 ng/ml

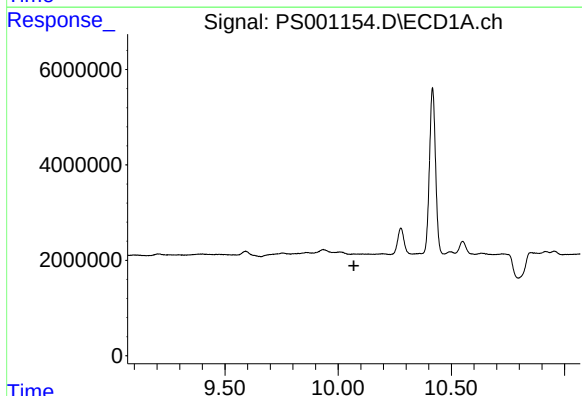


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 10.070 min
Response: 0
Conc: N.D.

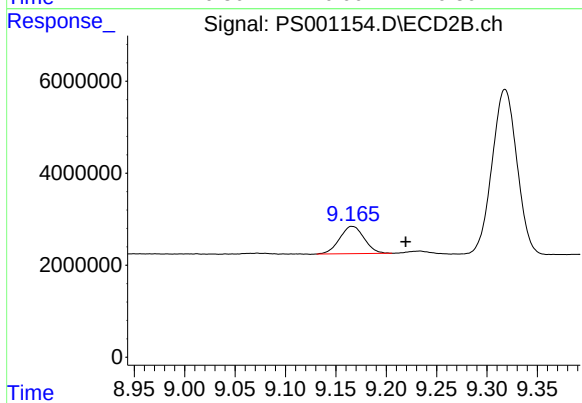

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.166 min
Delta R.T.: -0.053 min
Response: 10045490
Conc: 34.15 ng/ml

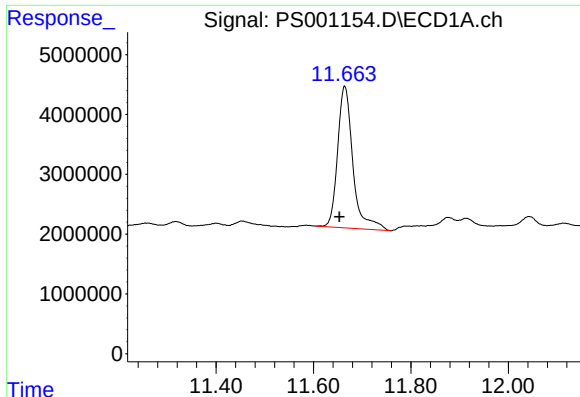

#4 2,4-DCAA


R.T.: 11.664 min
Delta R.T.: 0.011 min
Response: 51494989
Conc: 249.59 ng/ml

Instrument :
ECD_S
ClientSampleId :

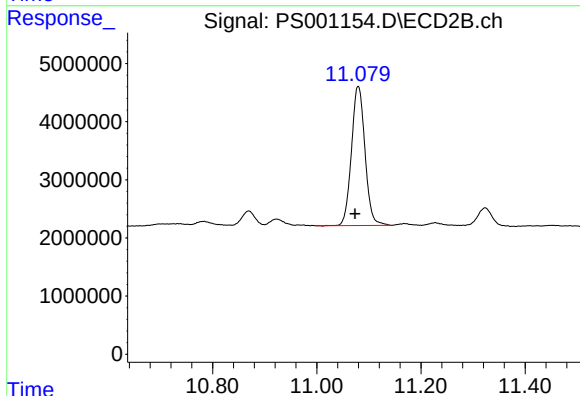


#4 2,4-DCAA

R.T.: 11.079 min
Delta R.T.: 0.006 min
Response: 43191854
Conc: 198.31 ng/ml

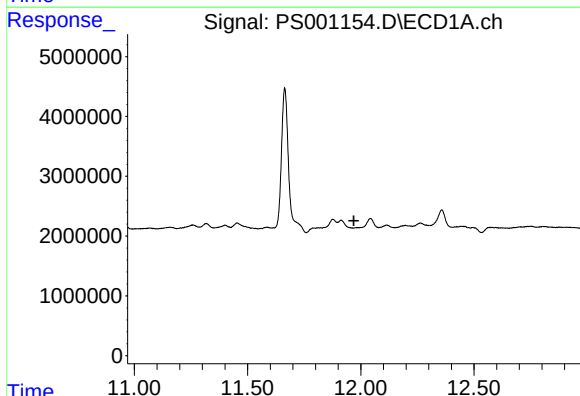


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.970 min
Response: 0
Conc: N.D.

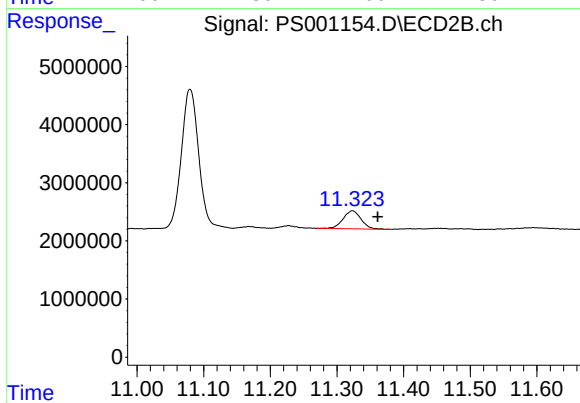

#5 DICAMBA


R.T.: 11.323 min
Delta R.T.: -0.038 min
Response: 5864165
Conc: 7.47 ng/ml

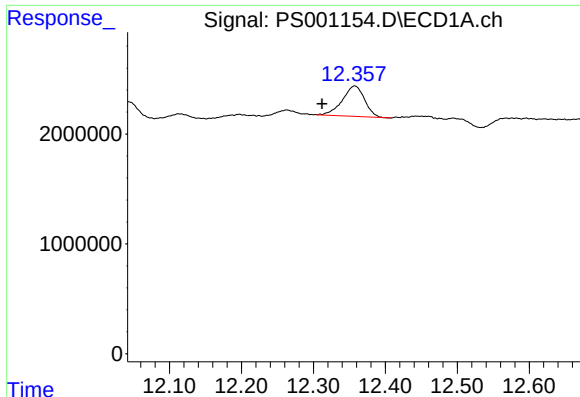

#6 MCP


R.T.: 12.357 min
Delta R.T.: 0.045 min
Response: 5936131
Conc: 10.81 ug/ml

Instrument :
ECD_S
ClientSampleId :

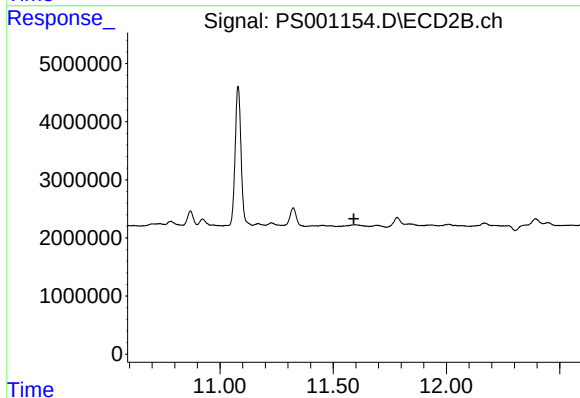


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.591 min
Response: 0
Conc: N.D.

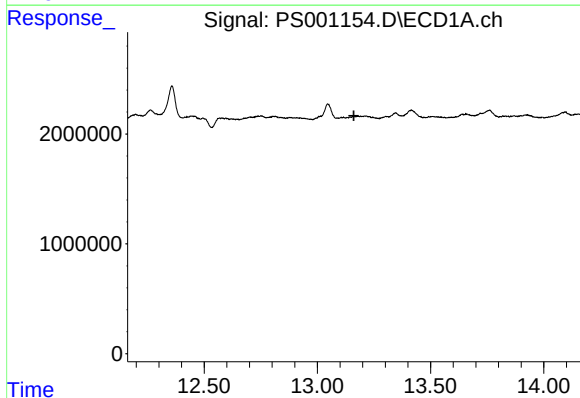


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 13.161 min
Response: 0
Conc: N.D.

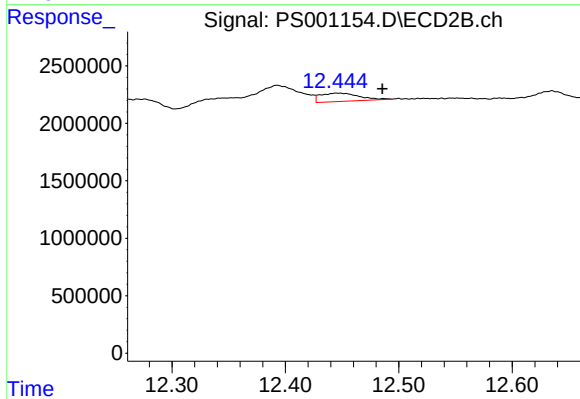

#8 DICHLORPROP


R.T.: 12.446 min
Delta R.T.: -0.040 min
Response: 1705293
Conc: 8.44 ng/ml

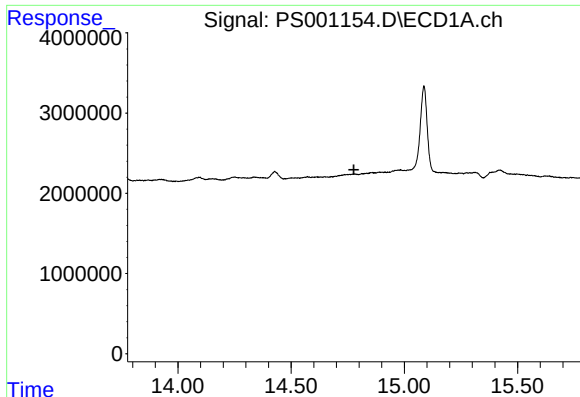

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.777 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

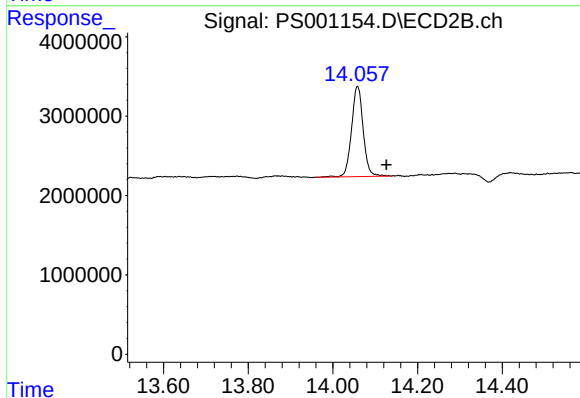


#11 2,4,5-TP (SILVEX)

R.T.: 14.058 min
Delta R.T.: -0.069 min
Response: 21739601
Conc: 17.32 ng/ml

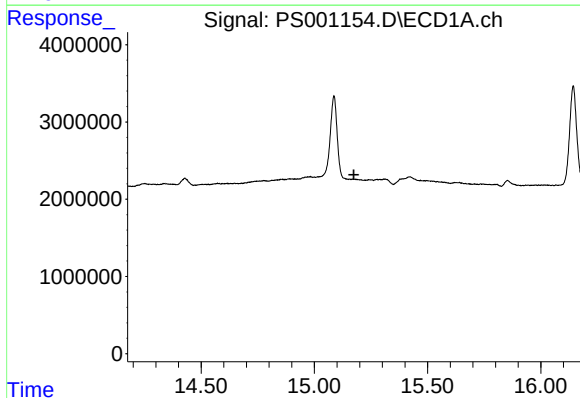


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 15.174 min
Response: 0
Conc: N.D.

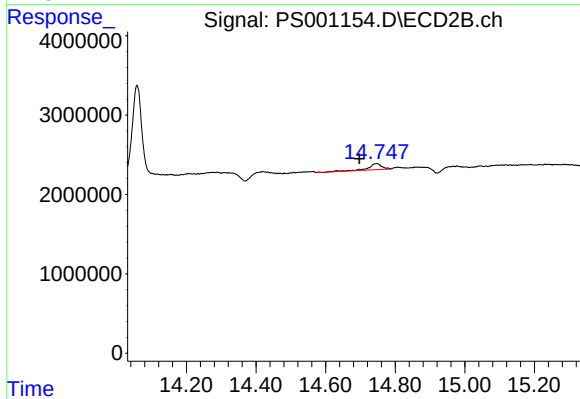

#12 2,4,5-T


R.T.: 14.747 min
Delta R.T.: 0.049 min
Response: 2062950
Conc: 1.99 ng/ml

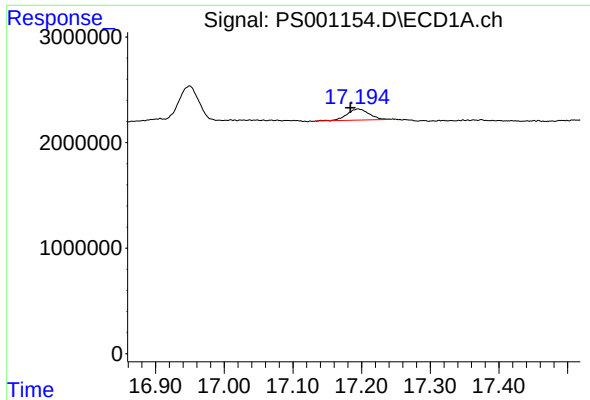

#15 Picloram

R.T.: 17.195 min
Delta R.T.: 0.011 min
Response: 2324133
Conc: 1.28 ng/ml

Instrument :
ECD_S
ClientSampleId :

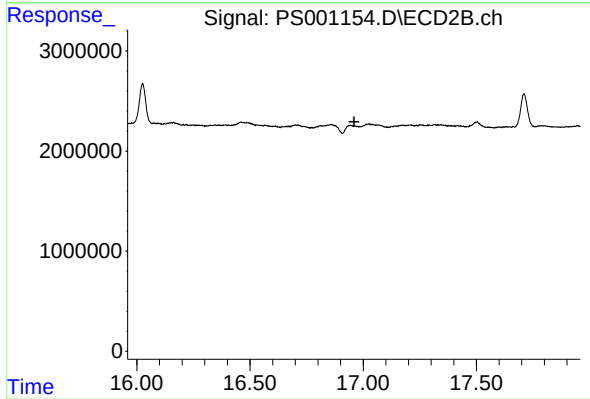

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 16.959 min
Response: 0
Conc: N.D.