

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071918\
 Data File : PS001156.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jul 2018 17:59
 Operator : UA
 Sample : J4030-15RE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 20 02:30:22 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 09 02:00:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.644	11.060	57576618	46043168	279.065	211.404
Target Compounds							
1) T	Dalapon	2.986	2.422	11048542	11634027	41.148	43.181
5) T	DICAMBA	12.023	11.302	2464564	8579492	3.130	10.930 #
6) T	MCPD	12.337	0.000	9219450	0	16.784	N.D. #
8) T	DICHLORPROP	0.000	12.423	0	1757149	N.D.	8.700 #
15) T	Picloram	17.174	17.003	2192159	3468218	1.210	2.278 #
16) T	DCPA	0.000	17.003	0	3468218	N.D.	2.017 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071918\
Data File : PS001156.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jul 2018 17:59
Operator : UA
Sample : J4030-15RE
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 20 02:30:22 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
Quant Title : 8080.M
QLast Update : Mon Jul 09 02:00:25 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

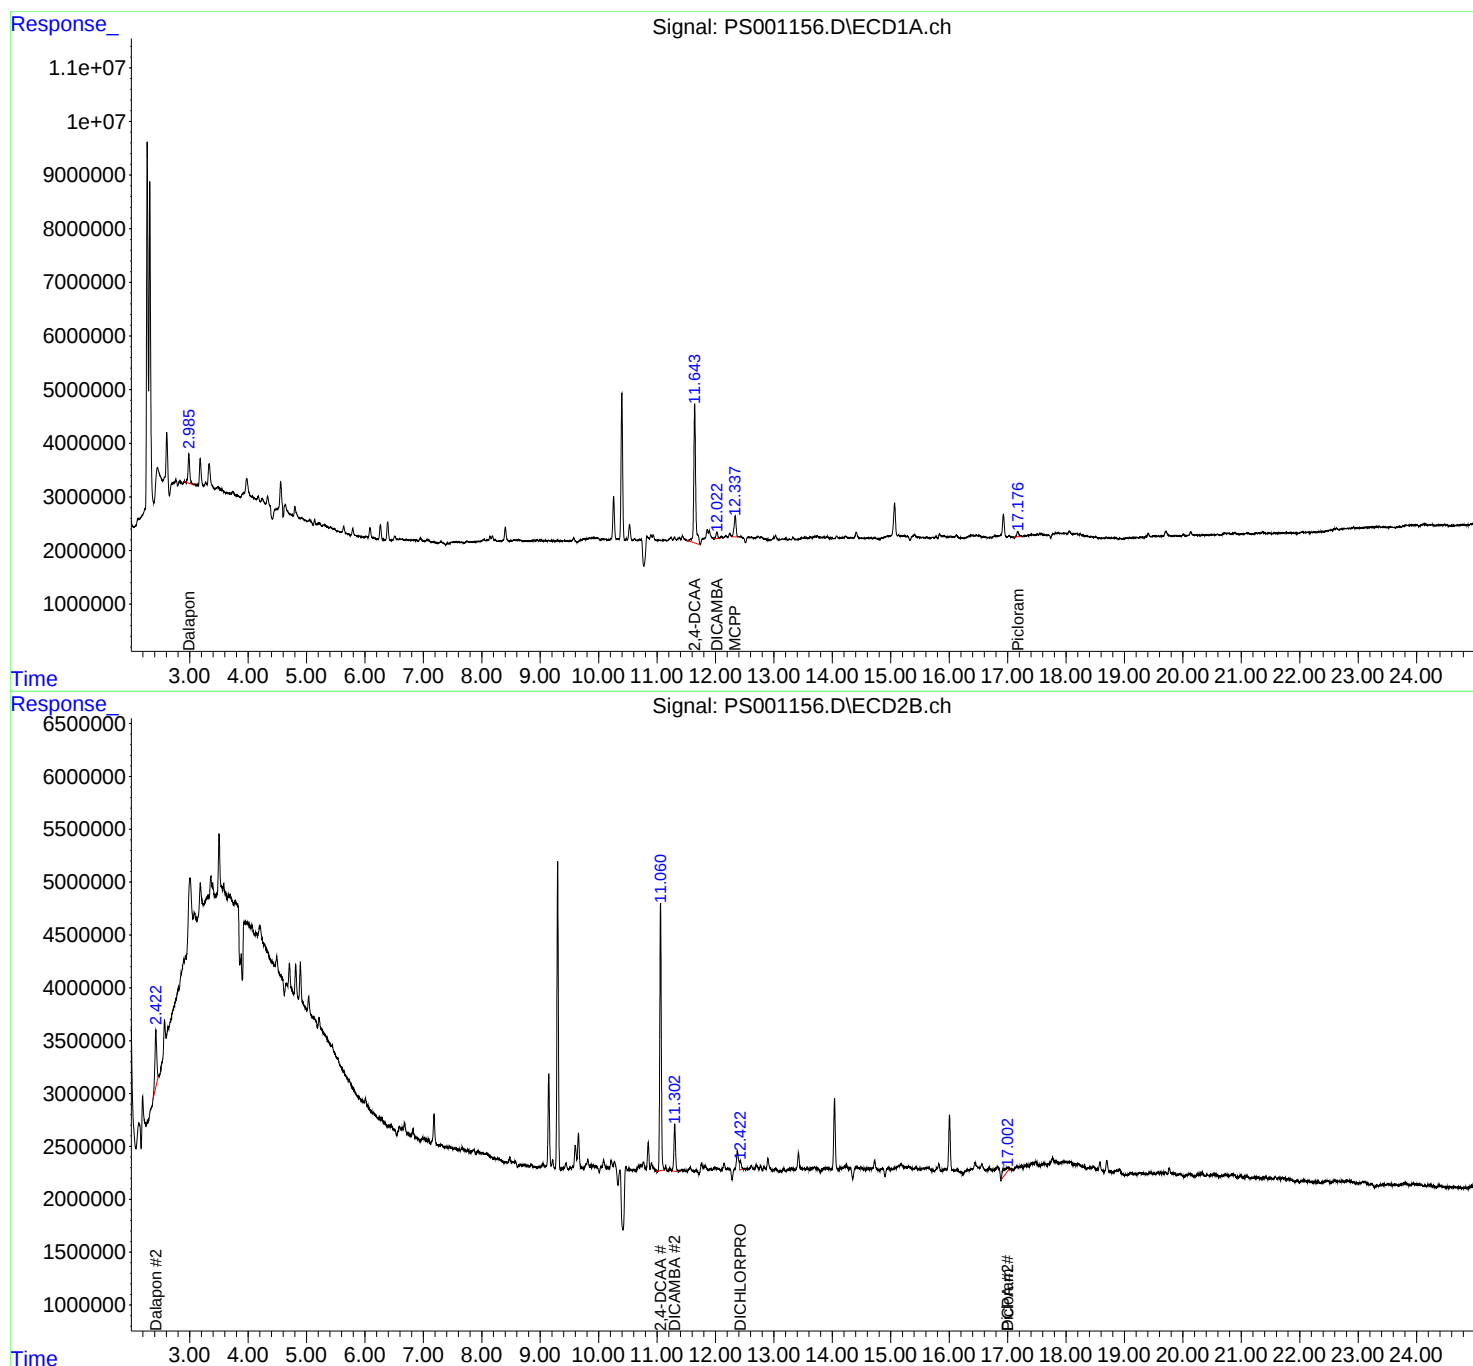


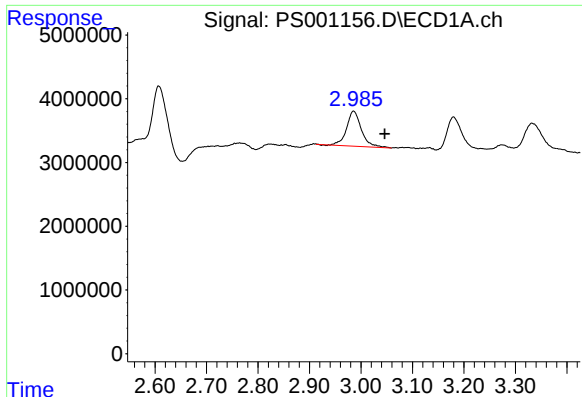

#1 Dalapon


R.T.: 2.986 min
Delta R.T.: -0.060 min
Response: 11048542
Conc: 41.15 ng/ml

Instrument :
ECD_S
ClientSampleId :

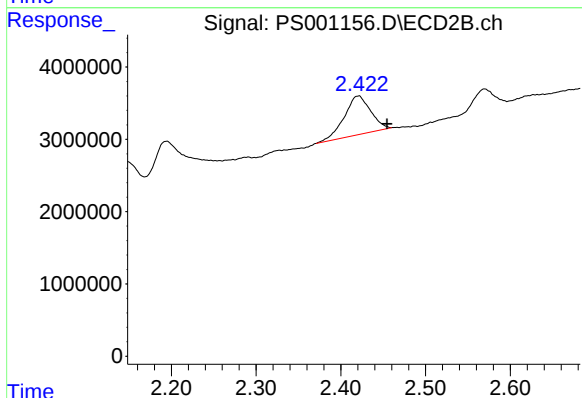


#1 Dalapon

R.T.: 2.422 min
Delta R.T.: -0.033 min
Response: 11634027
Conc: 43.18 ng/ml

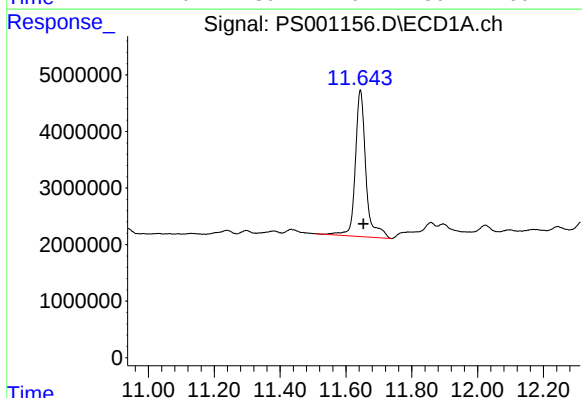


#4 2,4-DCAA

R.T.: 11.644 min
Delta R.T.: -0.010 min
Response: 57576618
Conc: 279.06 ng/ml

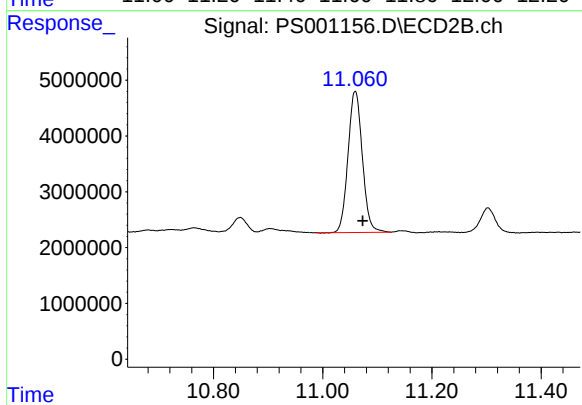

#4 2,4-DCAA


R.T.: 11.060 min
Delta R.T.: -0.014 min
Response: 46043168
Conc: 211.40 ng/ml

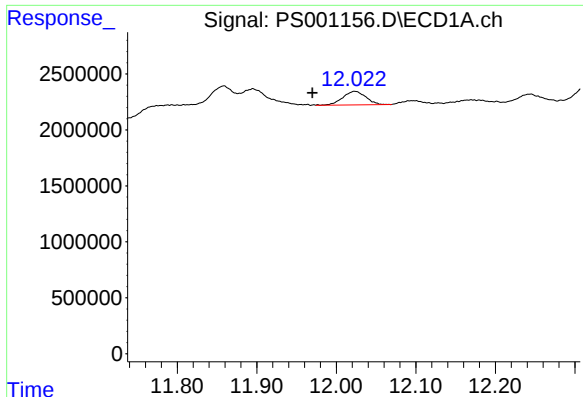

#5 DICAMBA


R.T.: 12.023 min
Delta R.T.: 0.054 min
Response: 2464564
Conc: 3.13 ng/ml

Instrument :
ECD_S
ClientSampleId :

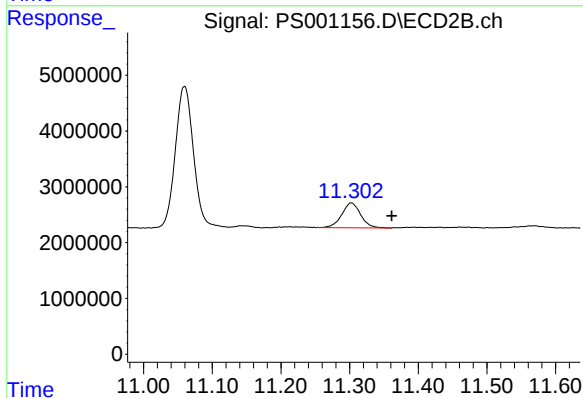


#5 DICAMBA

R.T.: 11.302 min
Delta R.T.: -0.059 min
Response: 8579492
Conc: 10.93 ng/ml

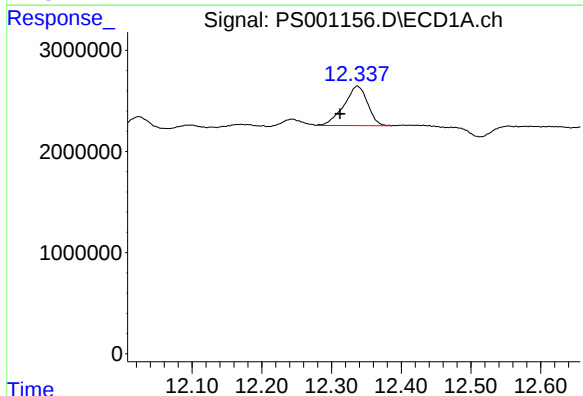


#6 MCP

R.T.: 12.337 min
Delta R.T.: 0.025 min
Response: 9219450
Conc: 16.78 ug/ml

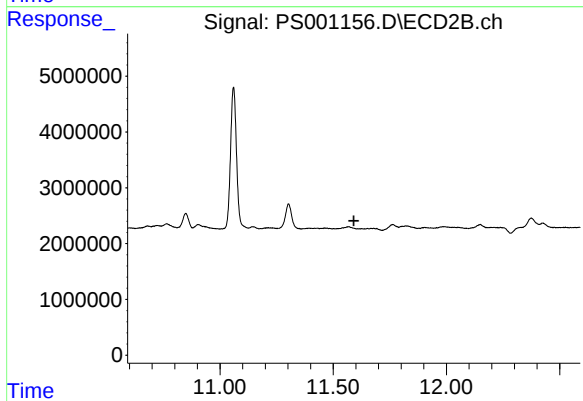

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.591 min
Response: 0
Conc: N.D.

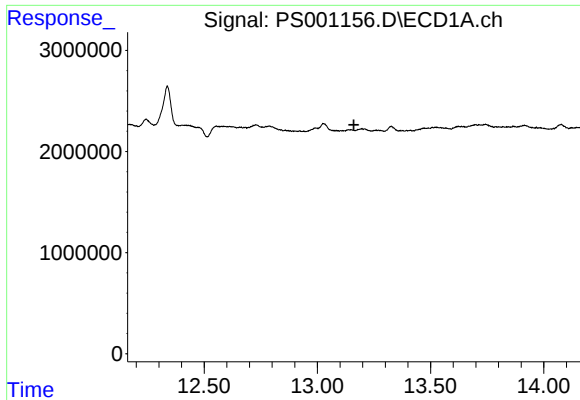

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 13.161 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

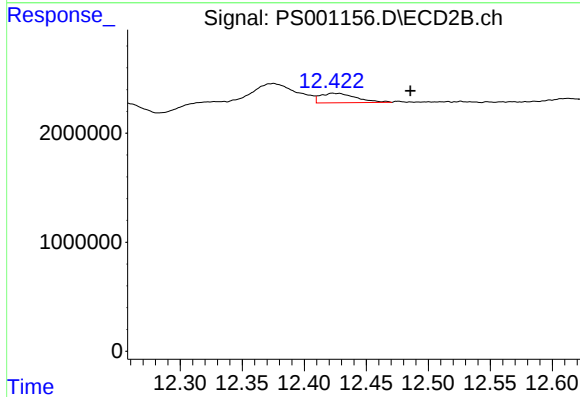


#8 DICHLORPROP

R.T.: 12.423 min
Delta R.T.: -0.063 min
Response: 1757149
Conc: 8.70 ng/ml

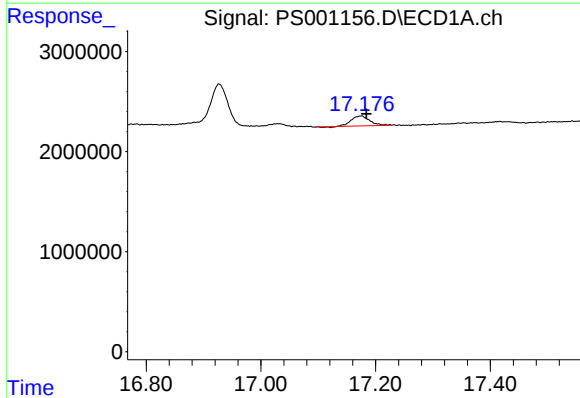


#15 Picloram

R.T.: 17.174 min
Delta R.T.: -0.010 min
Response: 2192159
Conc: 1.21 ng/ml

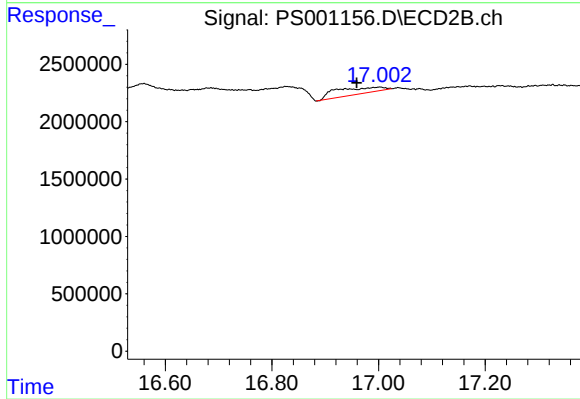

#15 Picloram


R.T.: 17.003 min
Delta R.T.: 0.043 min
Response: 3468218
Conc: 2.28 ng/ml

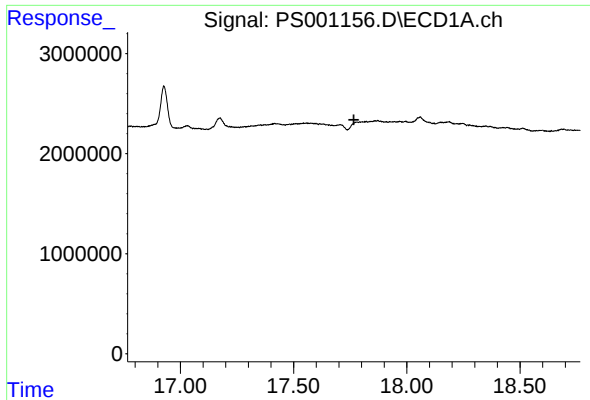

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.766 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

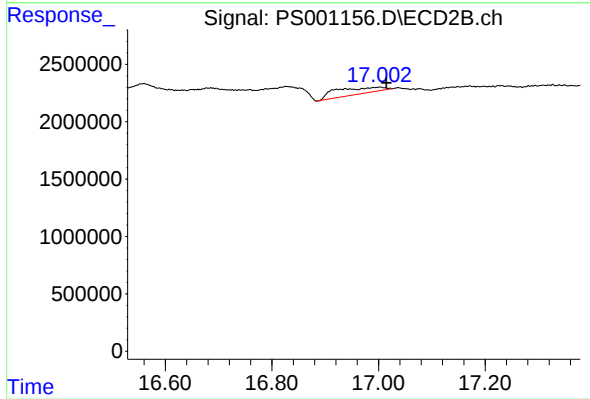

#16 DCPA

R.T.: 17.003 min
Delta R.T.: -0.012 min
Response: 3468218
Conc: 2.02 ng/ml