

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071923\
 Data File : PS023720.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jul 2023 08:31
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 19 13:24:02 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070723.M
 Quant Title : 8080.M
 QLast Update : Fri Jul 07 18:46:40 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.394	0.000	741956	0	<MDL	N.D. #
Target Compounds							
1) T	Dalapon	2.468	2.583	215264	3283558	<MDL	4.691 #
2) T	3,5-DICHL...	5.759	6.037f	1424667	560592	<MDL	<MDL #
3) T	4-Nitroph...	6.214	6.379f	5739358	137129	6.413	<MDL #
5) T	DICAMBA	6.514	7.020f	878635	10764155	<MDL	5.942 #
8) T	DICHLORPROP	7.125	7.605	1606789	917785	1.086	1.972 #
10) T	Pentachlo...	7.539	0.000	1168327	0	<MDL	N.D. #
12) T	2,4,5-T	8.328	9.076	2281944	1414843	<MDL	<MDL #
13) T	2,4-DB	8.778f	0.000	441225	0	<MDL	N.D. #
14) T	DINOSEB	9.890	0.000	1401268	0	<MDL	N.D. #
15) T	Picloram	9.694	10.828	36900352	5400646	3.147	1.277 #
16) T	DCPA	10.156	10.828	429573	5400646	<MDL	1.947 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071923\
Data File : PS023720.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jul 2023 08:31
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 19 13:24:02 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070723.M
Quant Title : 8080.M
QLast Update : Fri Jul 07 18:46:40 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

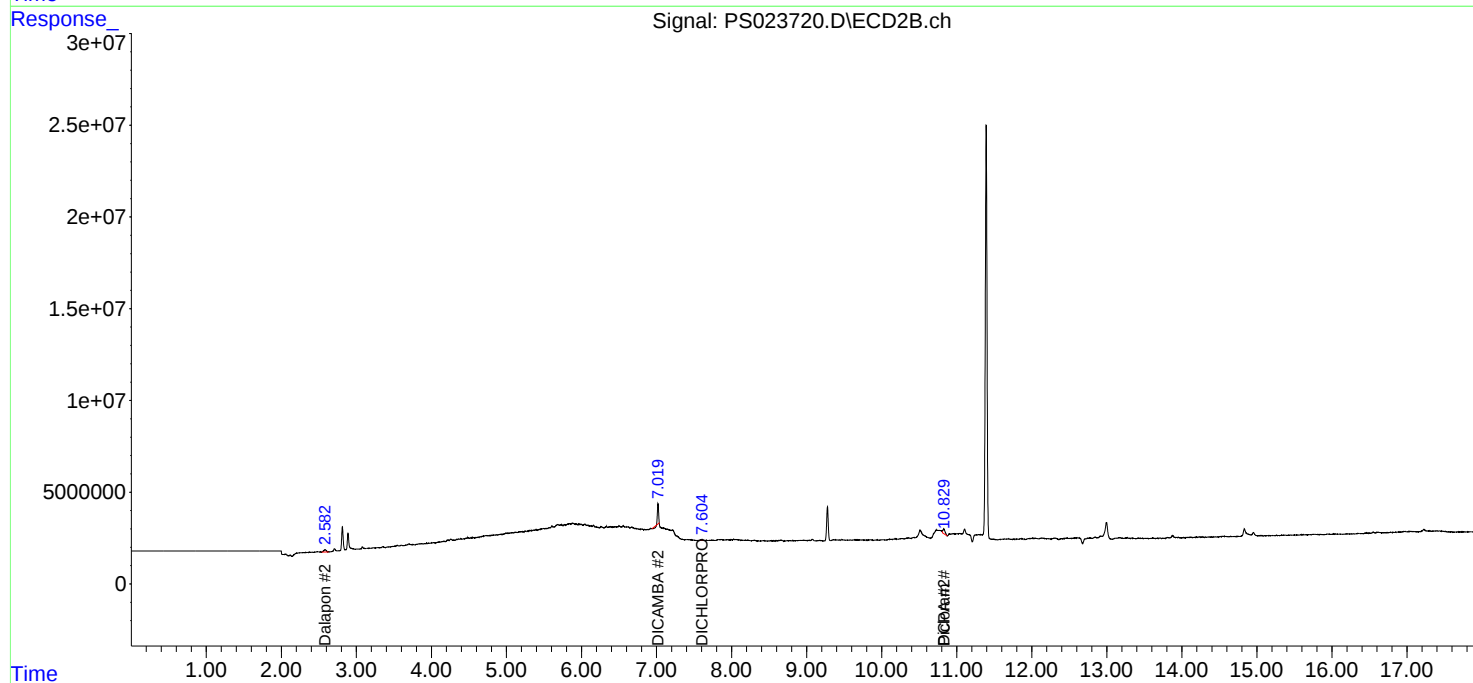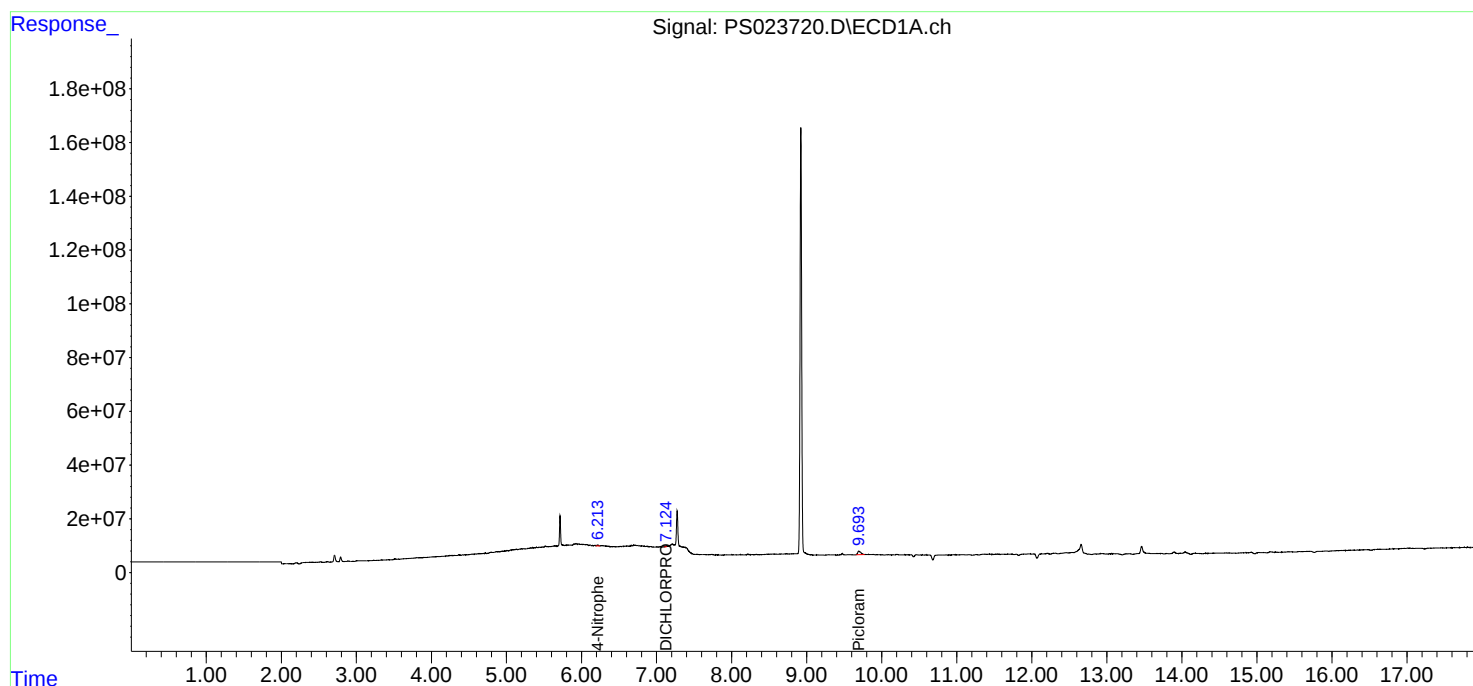


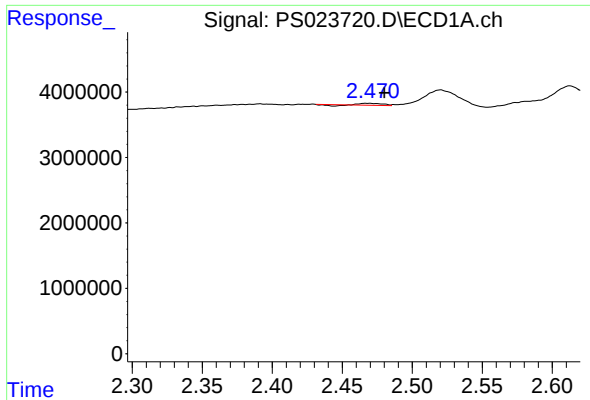

#1 Dalapon


R.T.: 2.468 min
Delta R.T.: -0.012 min
Response: 215264
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

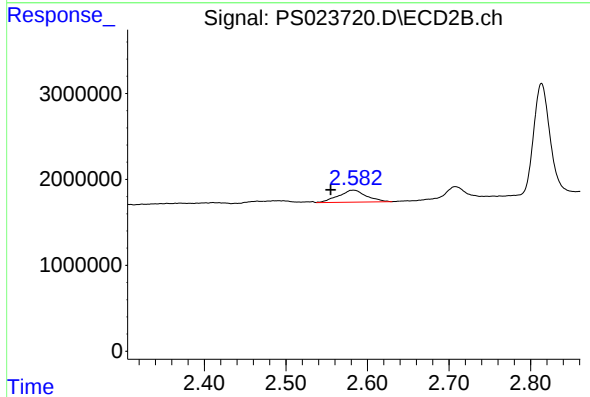


#1 Dalapon

R.T.: 2.583 min
Delta R.T.: 0.027 min
Response: 3283558
Conc: 4.69 ng/ml

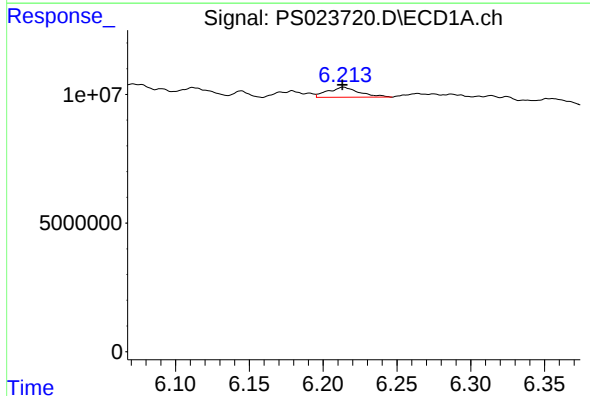


#3 4-Nitrophenol

R.T.: 6.214 min
Delta R.T.: 0.000 min
Response: 5739358
Conc: 6.41 ng/ml

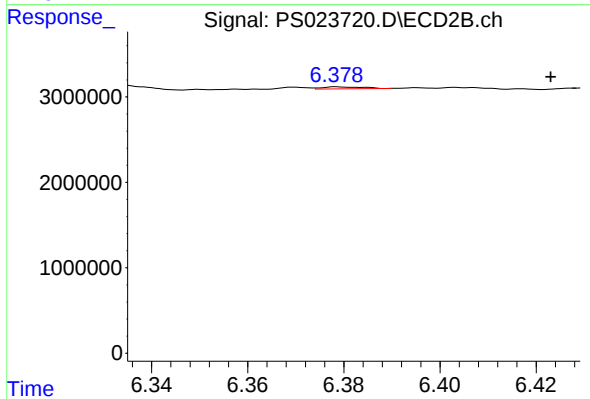

#3 4-Nitrophenol


R.T.: 6.379 min
Delta R.T.: -0.044 min
Response: 137129
Conc: N.D.

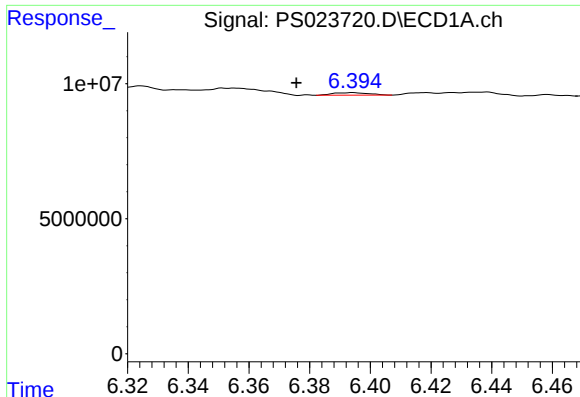

#4 2,4-DCAA


R.T.: 6.394 min
Delta R.T.: 0.019 min
Response: 741956
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

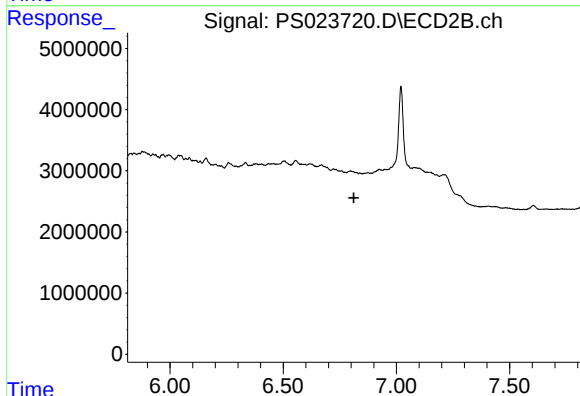


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.812 min
Response: 0
Conc: N.D.

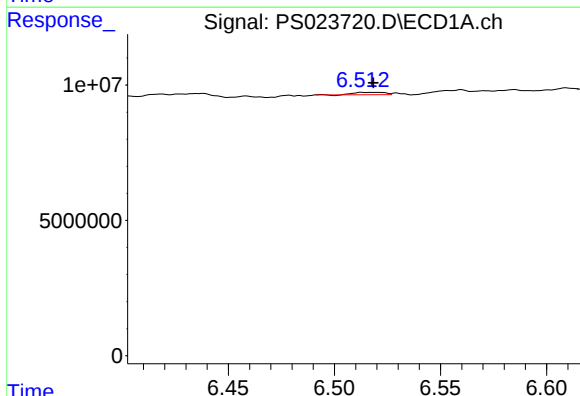


#5 DICAMBA

R.T.: 6.514 min
Delta R.T.: -0.005 min
Response: 878635
Conc: N.D.

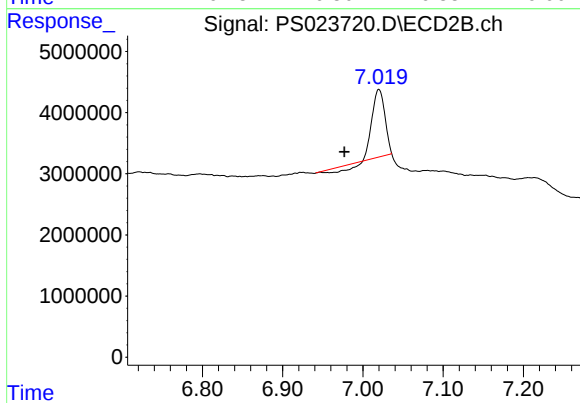

#5 DICAMBA


R.T.: 7.020 min
Delta R.T.: 0.043 min
Response: 10764155
Conc: 5.94 ng/ml

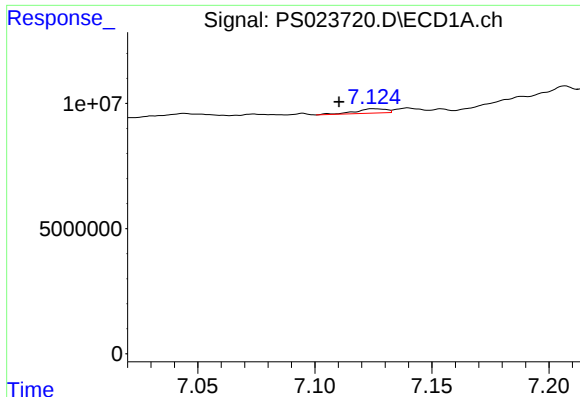

#8 DICHLORPROP


R.T.: 7.125 min
Delta R.T.: 0.015 min
Response: 1606789
Conc: 1.09 ng/ml

Instrument :
ECD_S
ClientSampleId :

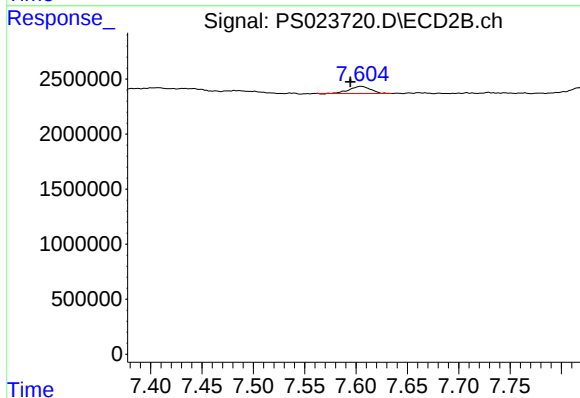


#8 DICHLORPROP

R.T.: 7.605 min
Delta R.T.: 0.010 min
Response: 917785
Conc: 1.97 ng/ml

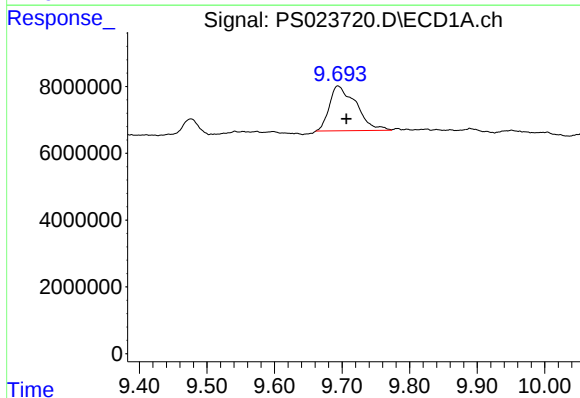


#15 Picloram

R.T.: 9.694 min
Delta R.T.: -0.012 min
Response: 36900352
Conc: 3.15 ng/ml

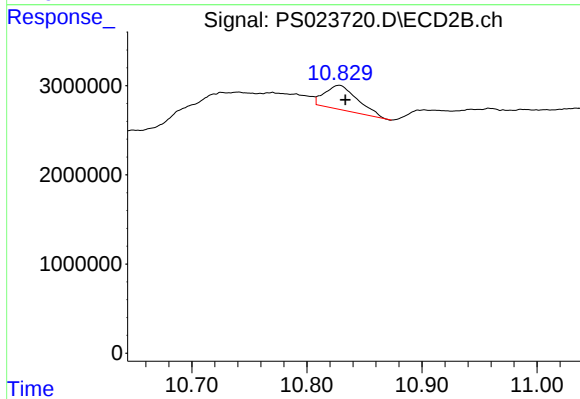

#15 Picloram


R.T.: 10.828 min
Delta R.T.: -0.005 min
Response: 5400646
Conc: 1.28 ng/ml

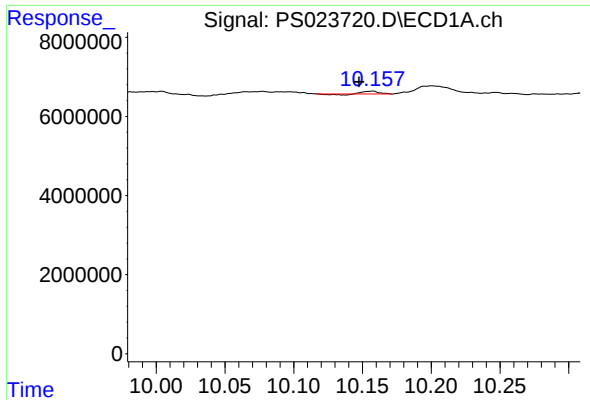

#16 DCPA

R.T.: 10.156 min
Delta R.T.: 0.008 min
Response: 429573
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

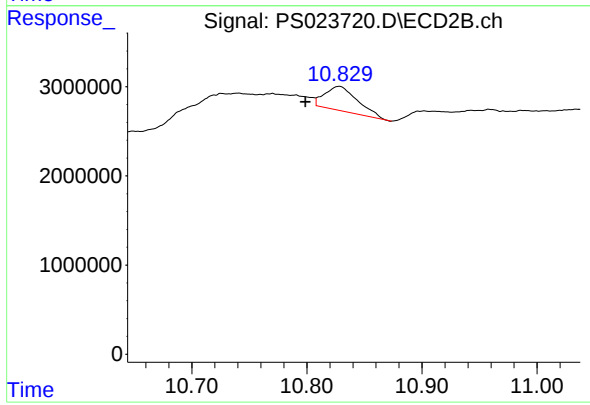

#16 DCPA

R.T.: 10.828 min
Delta R.T.: 0.029 min
Response: 5400646
Conc: 1.95 ng/ml