

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071923\
 Data File : PS023721.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jul 2023 08:55
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 19 13:24:22 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070723.M
 Quant Title : 8080.M
 QLast Update : Fri Jul 07 18:46:40 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.376	6.809	466.3E6	145.7E6	369.186	347.455
Target Compounds							
1) T	Dalapon	2.501	0.000	637805	0	<MDL	N.D. #
2) T	3,5-DICHL...	5.766	0.000	176023	0	<MDL	N.D. #
3) T	4-Nitroph...	6.215	0.000	4916039	0	5.493	N.D. #
5) T	DICAMBA	0.000	7.022f	0	961580	N.D.	<MDL
8) T	DICHLORPROP	7.062f	7.606	2399765	614581	1.623	1.321
9) T	2,4-D	0.000	7.820f	0	670217	N.D.	1.239
10) T	Pentachlo...	7.536	8.302	1087750	573303	<MDL	<MDL #
11) T	2,4,5-TP ...	8.064	0.000	728194	0	<MDL	N.D. #
12) T	2,4,5-T	8.319	0.000	418748	0	<MDL	N.D. #
13) T	2,4-DB	8.846	0.000	111486	0	<MDL	N.D. #
14) T	DINOSEB	9.884	0.000	875794	0	<MDL	N.D. #
15) T	Picloram	9.707	10.824	15434271	8520651	1.316	2.014 #
16) T	DCPA	10.149	10.824	1672701	8520651	<MDL	3.071 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071923\
Data File : PS023721.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jul 2023 08:55
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 19 13:24:22 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070723.M
Quant Title : 8080.M
QLast Update : Fri Jul 07 18:46:40 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

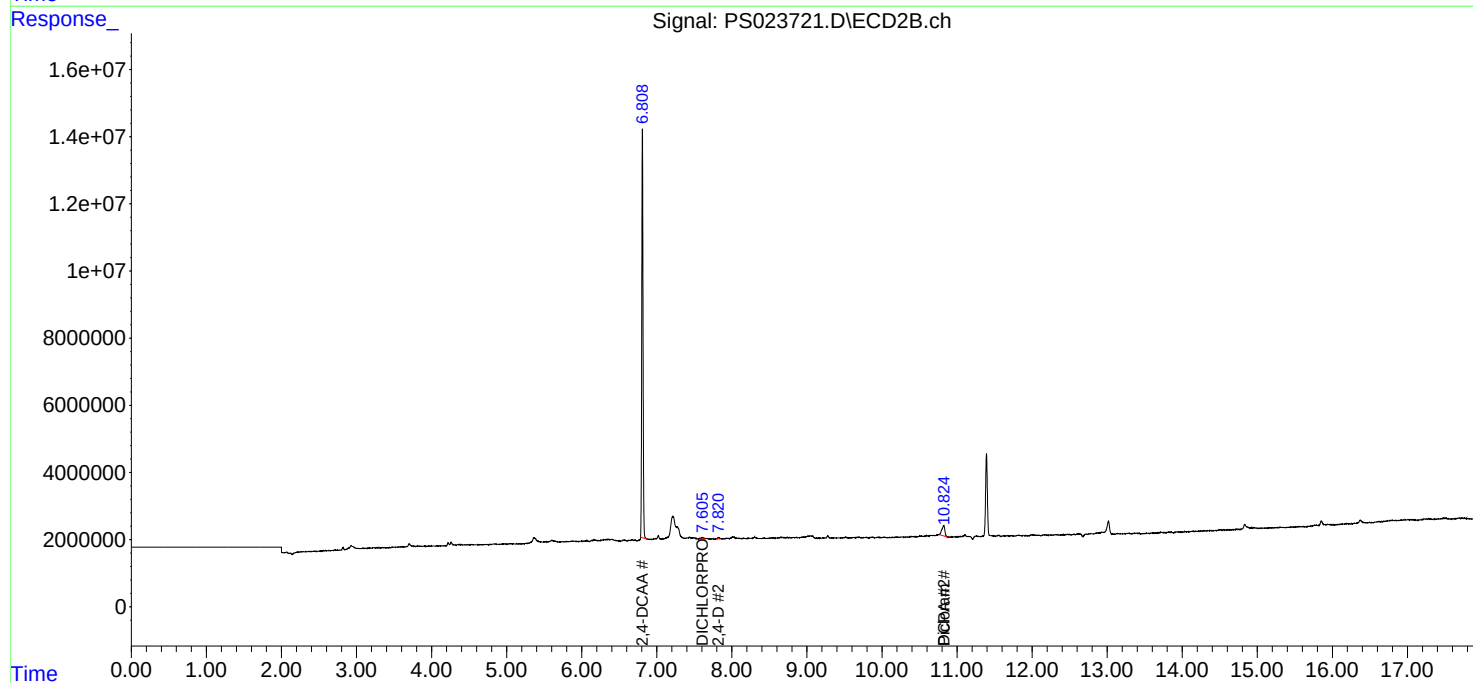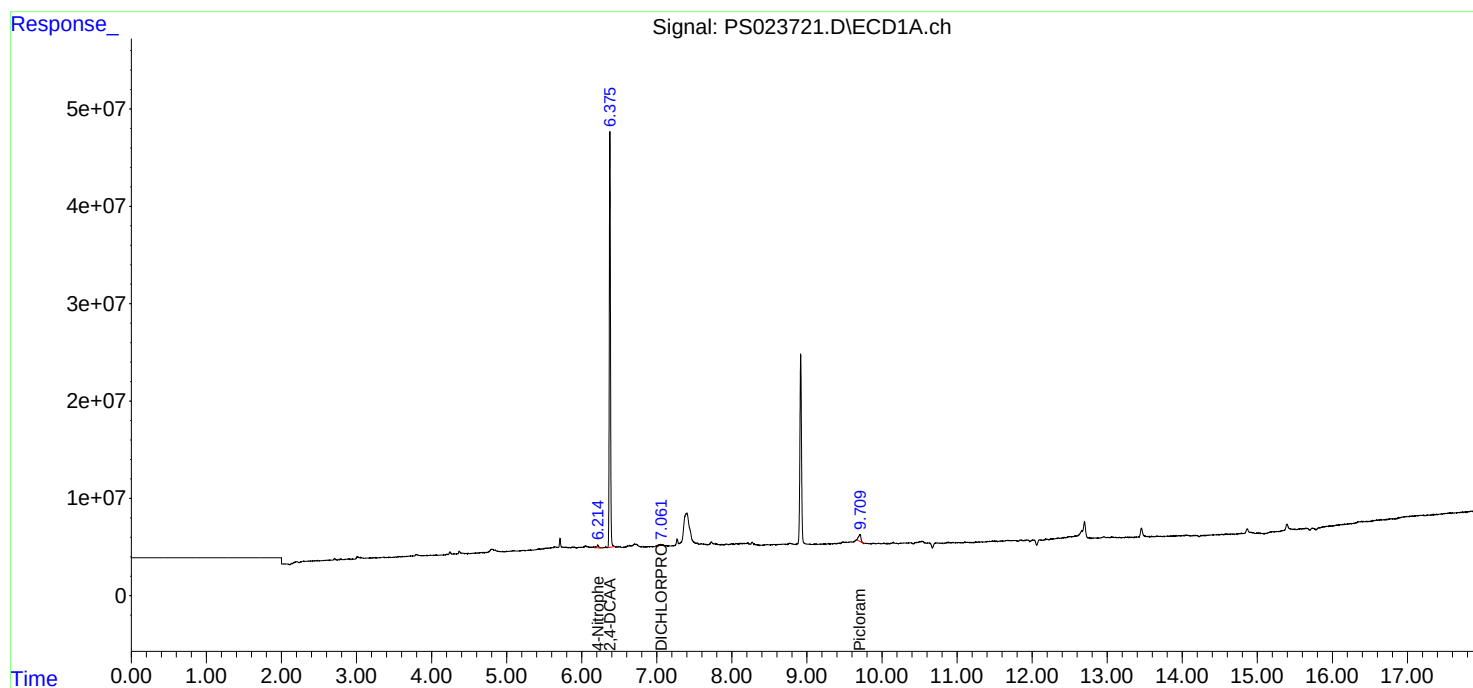


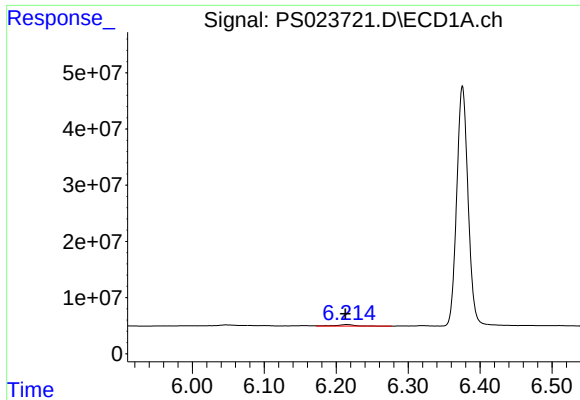

#3 4-Nitrophenol


R.T.: 6.215 min
Delta R.T.: 0.002 min
Response: 4916039
Conc: 5.49 ng/ml

Instrument :
ECD_S
ClientSampleId :

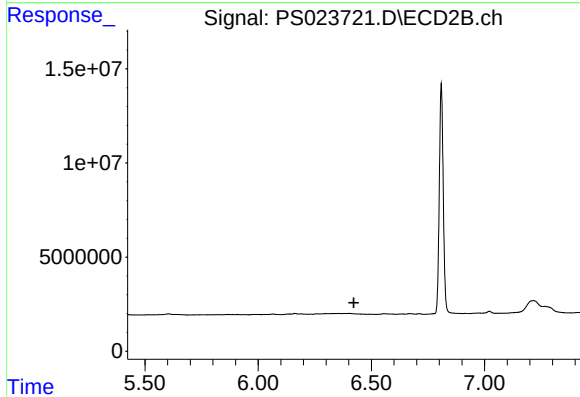


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.423 min
Response: 0
Conc: N.D.

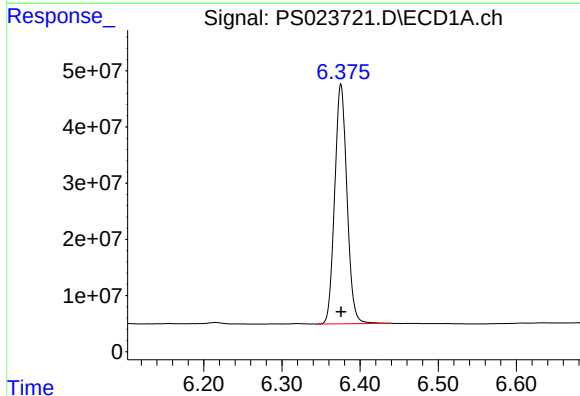


#4 2,4-DCAA

R.T.: 6.376 min
Delta R.T.: 0.000 min
Response: 466283896
Conc: 369.19 ng/ml

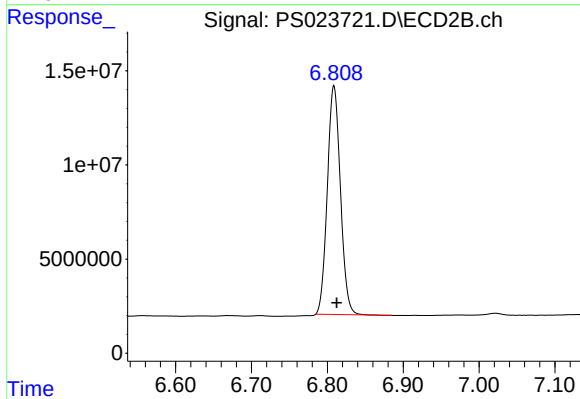

#4 2,4-DCAA


R.T.: 6.809 min
Delta R.T.: -0.003 min
Response: 145737203
Conc: 347.45 ng/ml

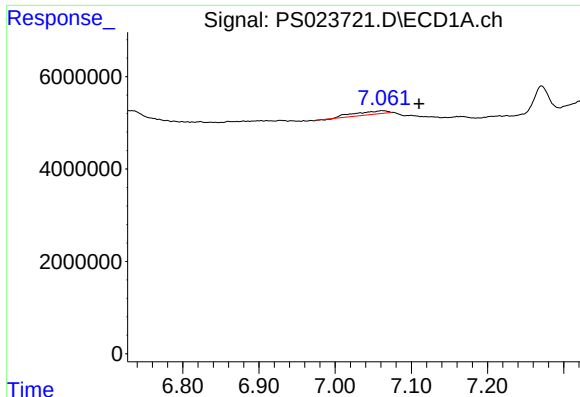

#8 DICHLORPROP


R.T.: 7.062 min
Delta R.T.: -0.049 min
Response: 2399765
Conc: 1.62 ng/ml

Instrument :
ECD_S
ClientSampleId :

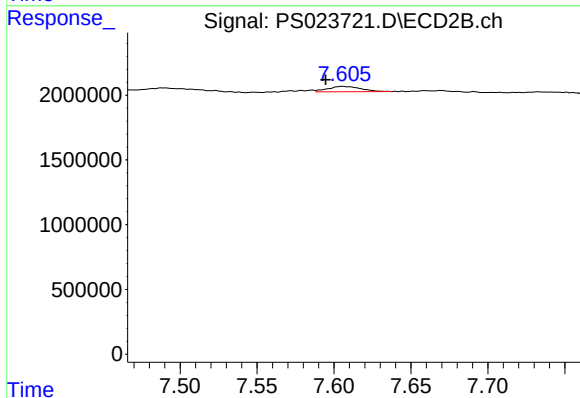


#8 DICHLORPROP

R.T.: 7.606 min
Delta R.T.: 0.011 min
Response: 614581
Conc: 1.32 ng/ml

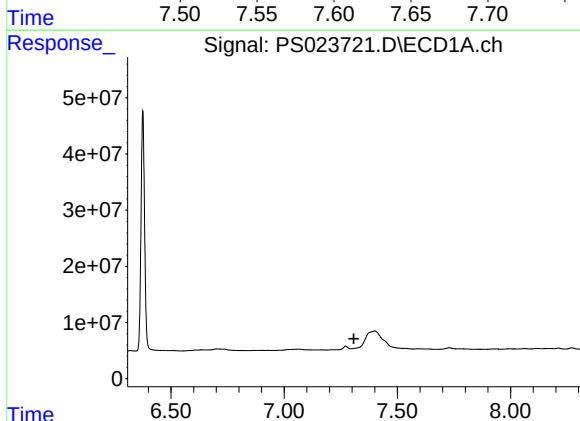


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.308 min
Response: 0
Conc: N.D.

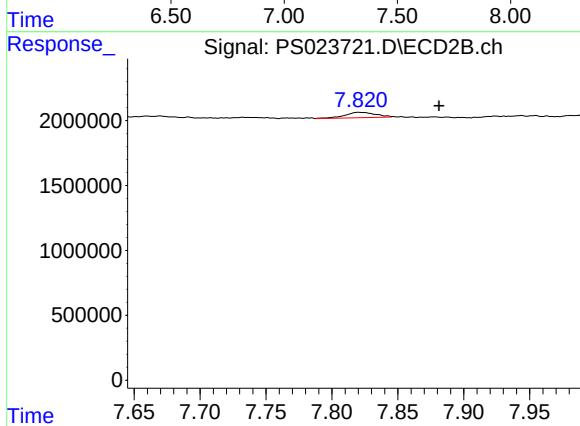

#9 2,4-D


R.T.: 7.820 min
Delta R.T.: -0.061 min
Response: 670217
Conc: 1.24 ng/ml

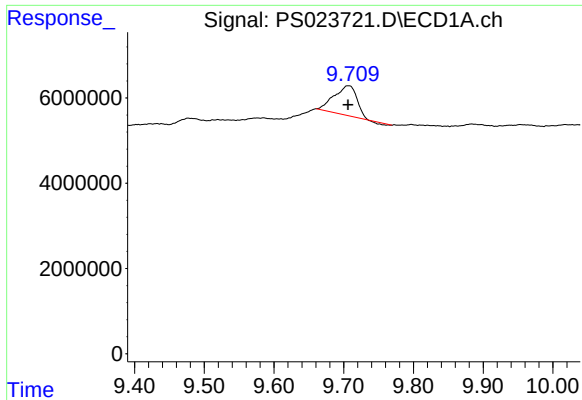

#15 Picloram


R.T.: 9.707 min
Delta R.T.: 0.000 min
Response: 15434271
Conc: 1.32 ng/ml

Instrument :
ECD_S
ClientSampleId :

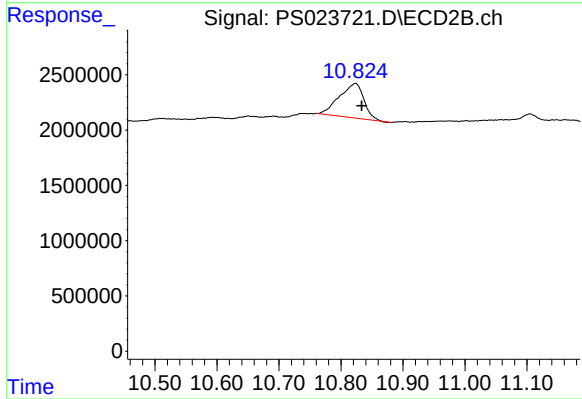


#15 Picloram

R.T.: 10.824 min
Delta R.T.: -0.009 min
Response: 8520651
Conc: 2.01 ng/ml

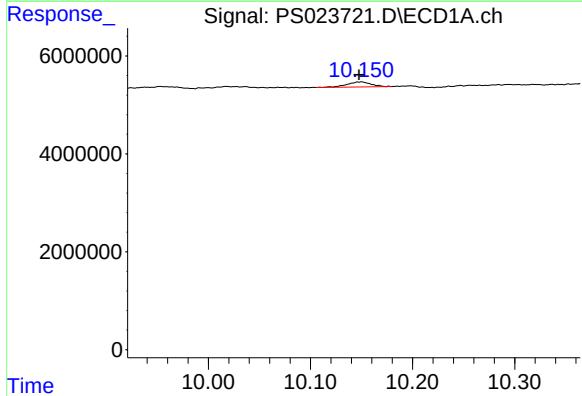

#16 DCPA

R.T.: 10.149 min
Delta R.T.: 0.001 min
Response: 1672701
Conc: N.D.

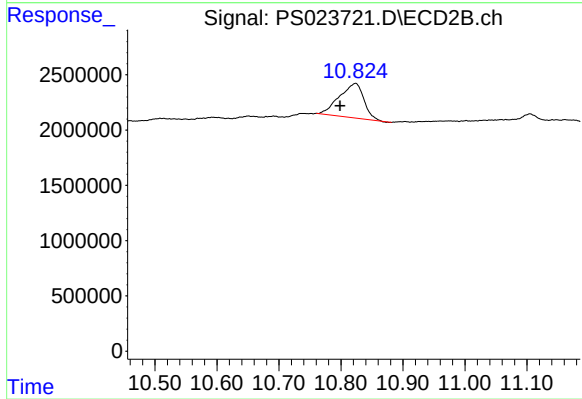

#16 DCPA

R.T.: 10.824 min
Delta R.T.: 0.025 min
Response: 8520651
Conc: 3.07 ng/ml