

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071923\
 Data File : PS023757.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jul 2023 02:15
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 20 03:05:32 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070723.M
 Quant Title : 8080.M
 QLast Update : Fri Jul 07 18:46:40 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.374	6.809	415.1E6	131.0E6	328.683	312.349
Target Compounds							
2) T	3,5-DICHL...	5.770	0.000	148238	0	<MDL	N.D. #
3) T	4-Nitroph...	6.213	6.383f	4020697	109546	4.493	<MDL #
5) T	DICAMBA	6.511	6.982	44615	542426	<MDL	<MDL #
8) T	DICHLORPROP	7.048f	7.607	5126438	2905854	3.466	6.245 #
9) T	2,4-D	0.000	7.822f	0	678959	N.D.	1.256
10) T	Pentachlo...	7.588f	8.302	550555	499196	<MDL	<MDL #
11) T	2,4,5-TP ...	8.063	0.000	846406	0	<MDL	N.D. #
12) T	2,4,5-T	8.324	9.078	1119857	508399	<MDL	<MDL #
13) T	2,4-DB	8.848	0.000	87437	0	<MDL	N.D. #
14) T	DINOSEB	9.883	0.000	1134269	0	<MDL	N.D. #
15) T	Picloram	9.705	10.827	8451065	3280708	<MDL	<MDL #
16) T	DCPA	10.146	10.794	976231	594664	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071923\
Data File : PS023757.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jul 2023 02:15
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 20 03:05:32 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070723.M
Quant Title : 8080.M
QLast Update : Fri Jul 07 18:46:40 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

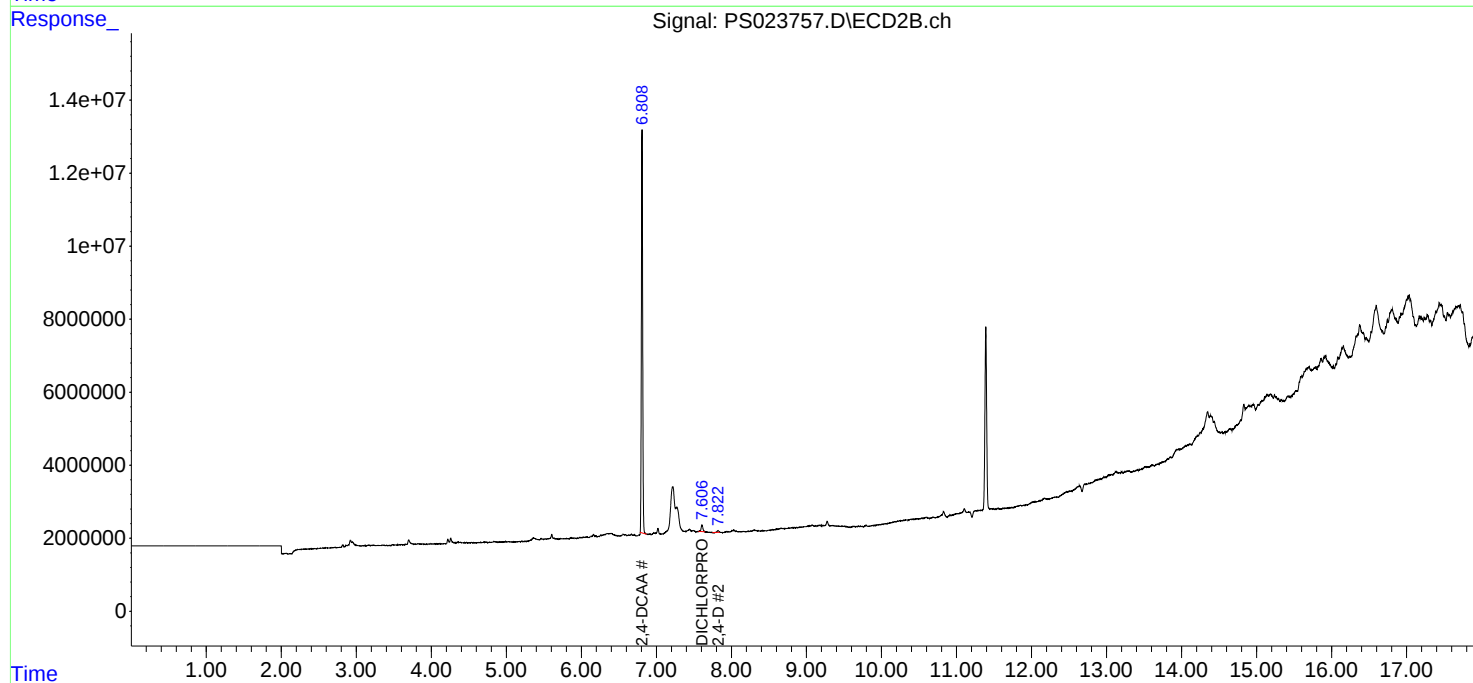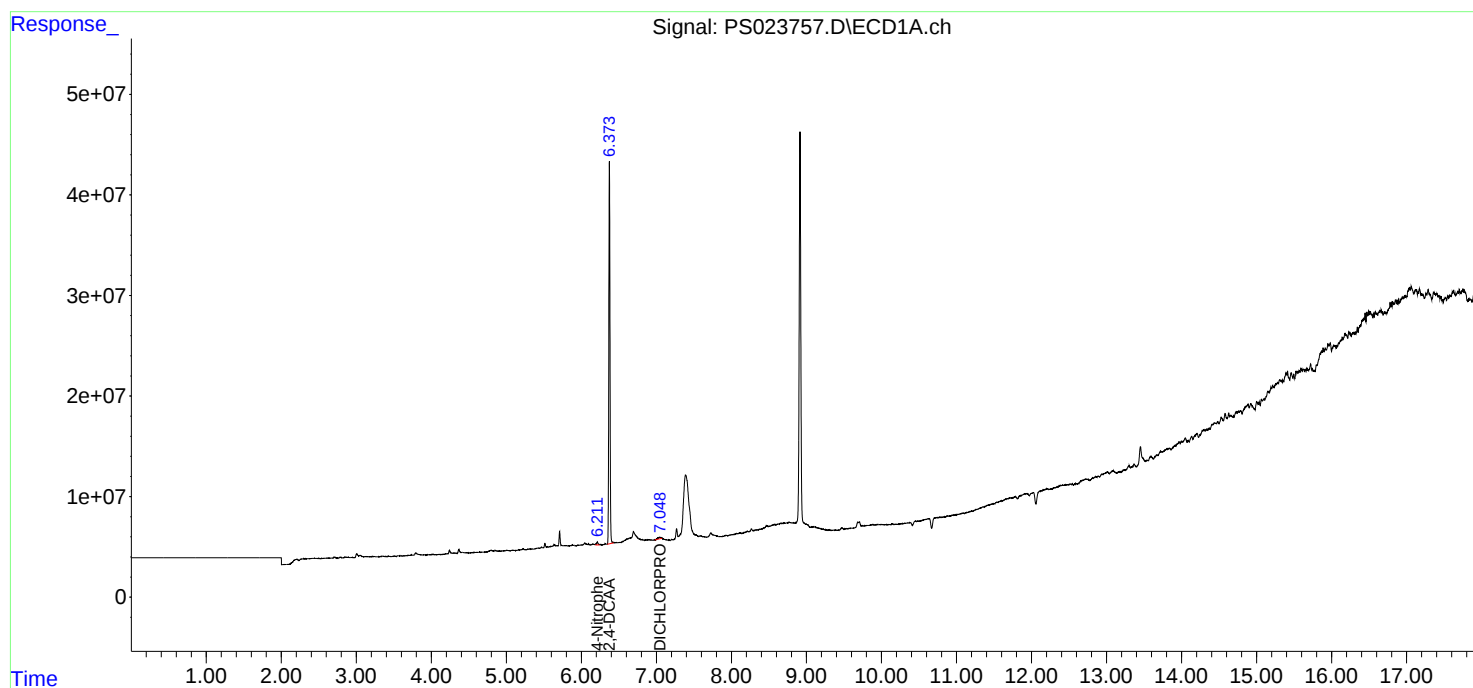


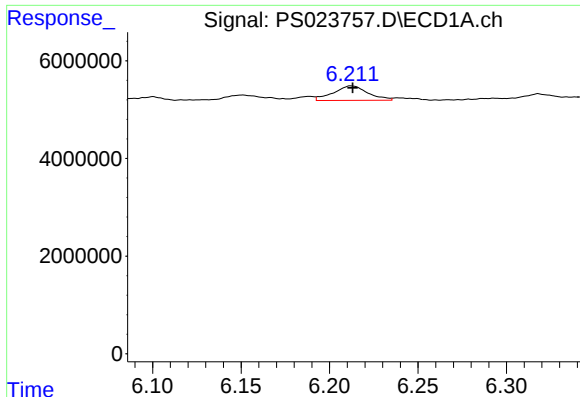

#3 4-Nitrophenol


R.T.: 6.213 min
Delta R.T.: 0.000 min
Response: 4020697
Conc: 4.49 ng/ml

Instrument :
ECD_S
ClientSampleId :

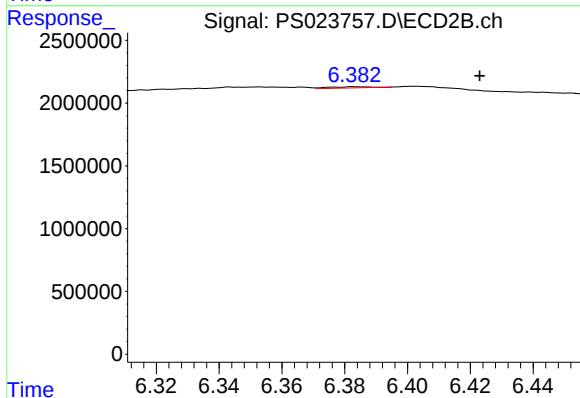


#3 4-Nitrophenol

R.T.: 6.383 min
Delta R.T.: -0.040 min
Response: 109546
Conc: N.D.

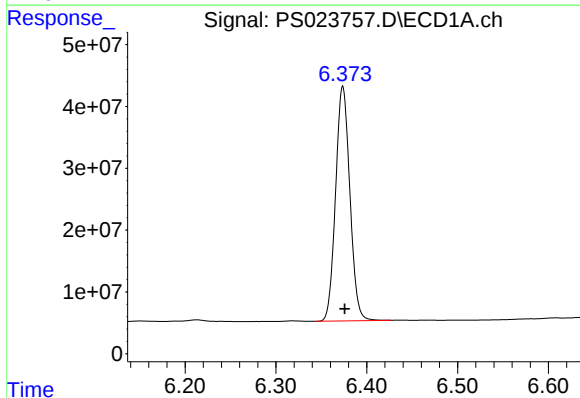


#4 2,4-DCAA

R.T.: 6.374 min
Delta R.T.: -0.002 min
Response: 415128412
Conc: 328.68 ng/ml

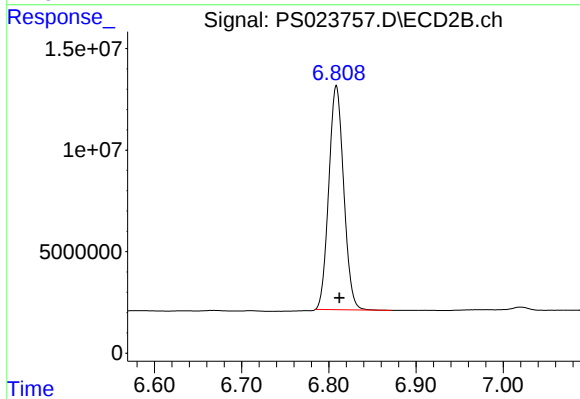

#4 2,4-DCAA


R.T.: 6.809 min
Delta R.T.: -0.003 min
Response: 131012335
Conc: 312.35 ng/ml

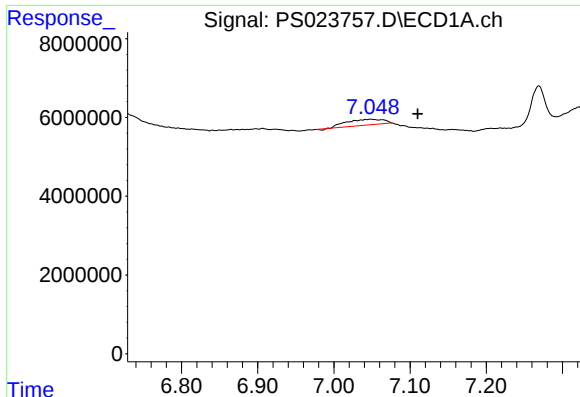

#8 DICHLORPROP


R.T.: 7.048 min
Delta R.T.: -0.062 min
Response: 5126438
Conc: 3.47 ng/ml

Instrument :
ECD_S
ClientSampleId :

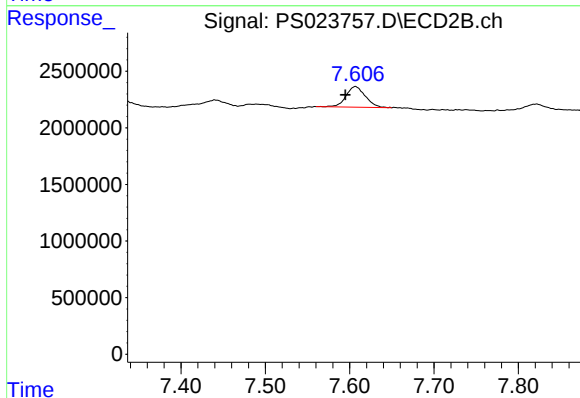


#8 DICHLORPROP

R.T.: 7.607 min
Delta R.T.: 0.012 min
Response: 2905854
Conc: 6.24 ng/ml

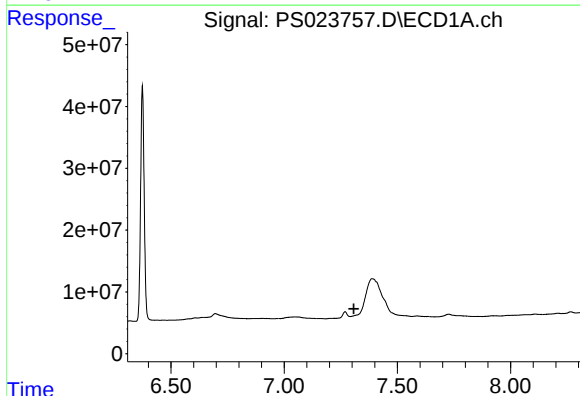

#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.308 min
Response: 0
Conc: N.D.

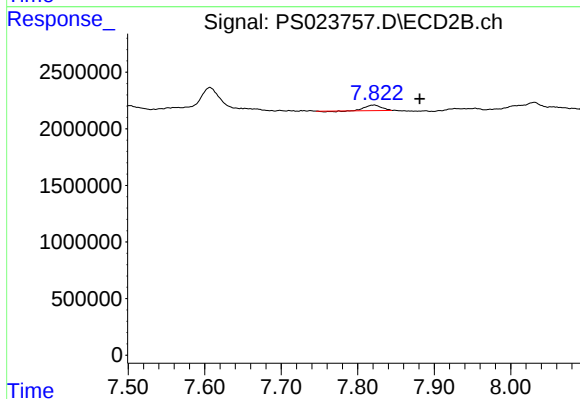

#9 2,4-D

R.T.: 7.822 min
Delta R.T.: -0.060 min
Response: 678959
Conc: 1.26 ng/ml