

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072018\
 Data File : PS001162.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jul 2018 12:56
 Operator : UA
 Sample : J4019-03RE
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 20 14:43:25 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 09 02:00:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.627	11.039	50804146	43415252	246.239	199.338
Target Compounds							
1) T	Dalapon	0.000	2.486	0	1054152	N.D.	3.913 #
2) T	3,5-DICHL...	0.000	9.277	0	62599761	N.D.	212.813 #
6) T	MCP	12.317	0.000	8608885	0	15.673	N.D. #
12) T	2,4,5-T	0.000	14.709	0	1692037	N.D.	1.635 #
15) T	Picloram	17.161	16.980	7602856	6584498	4.198	4.324
16) T	DCPA	0.000	16.980	0	6584498	N.D.	3.830 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072018\
Data File : PS001162.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jul 2018 12:56
Operator : UA
Sample : J4019-03RE
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 20 14:43:25 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
Quant Title : 8080.M
QLast Update : Mon Jul 09 02:00:25 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

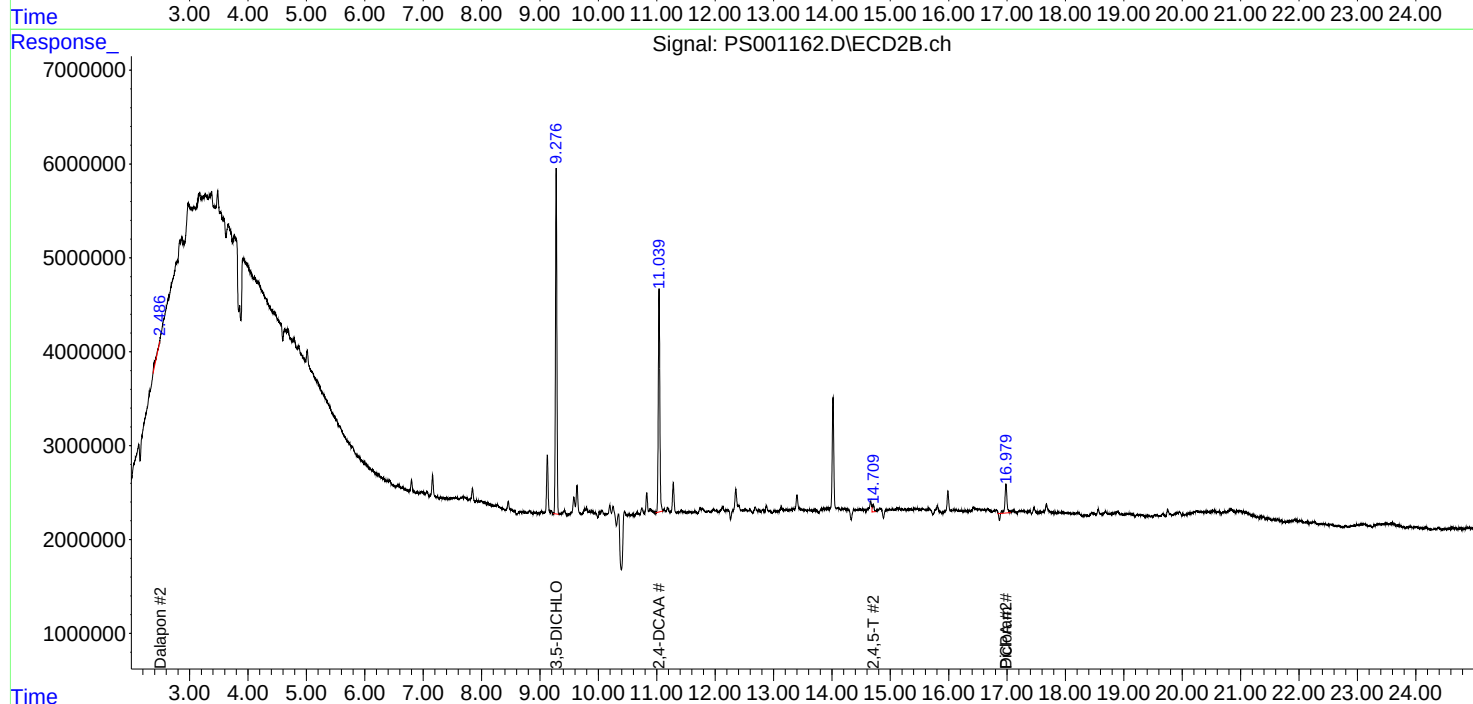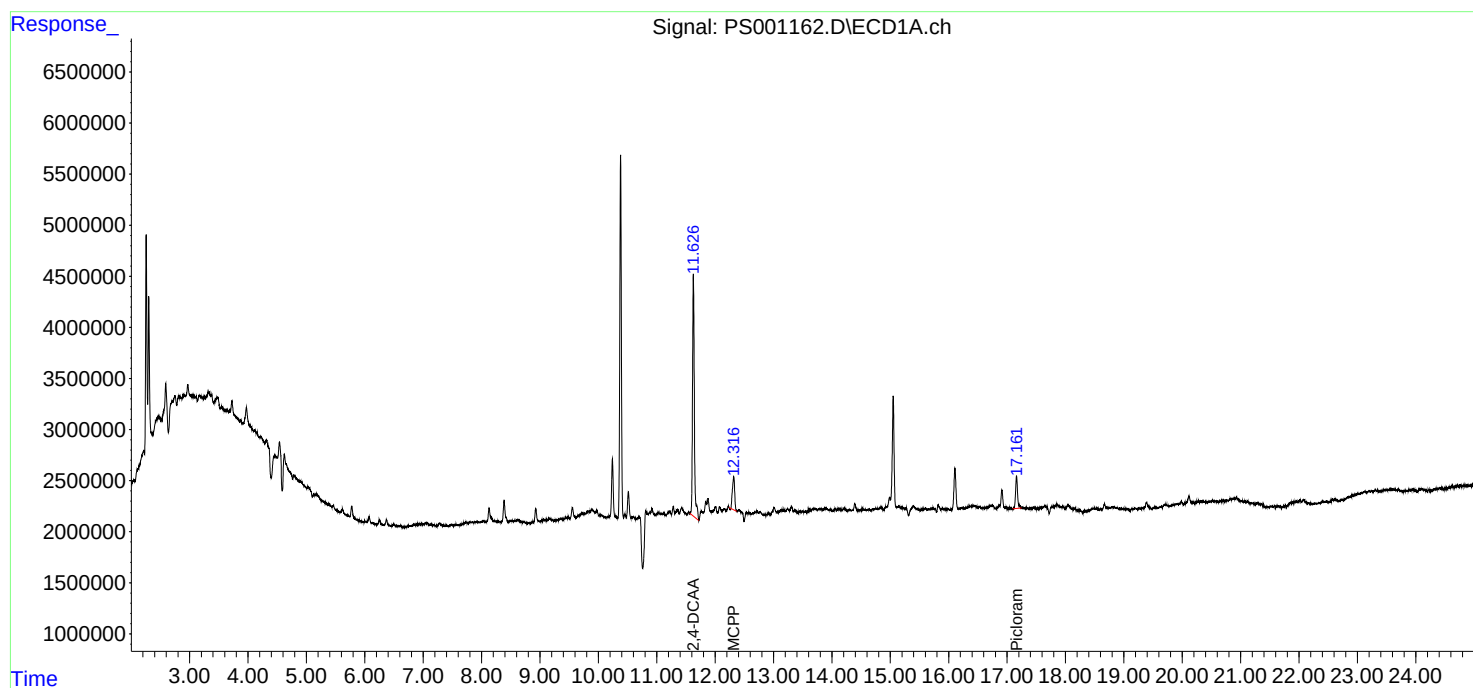


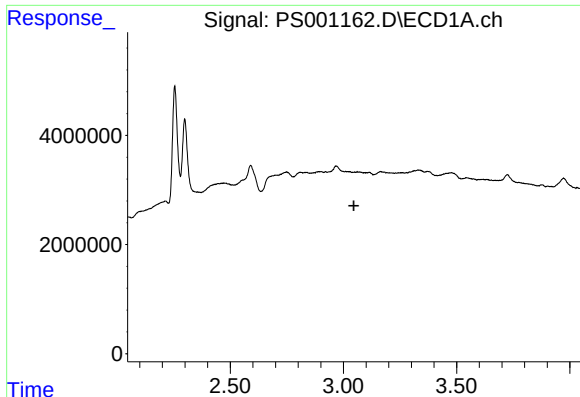

#1 Dalapon


R.T.: 0.000 min
Exp R.T. : 3.046 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

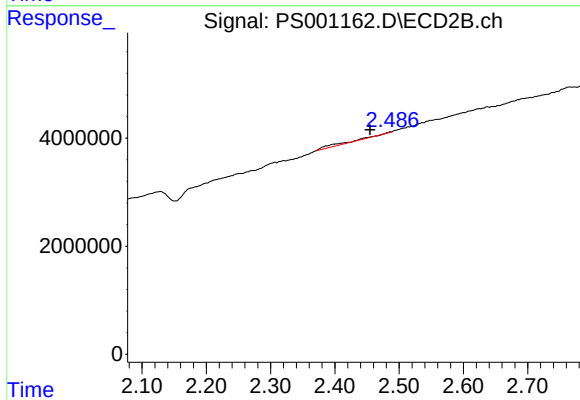


#1 Dalapon

R.T.: 2.486 min
Delta R.T.: 0.031 min
Response: 1054152
Conc: 3.91 ng/ml

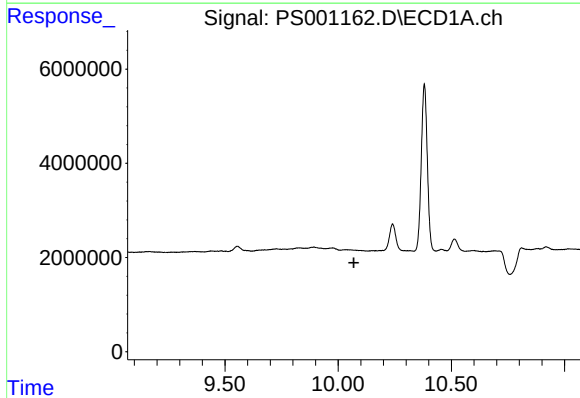


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 10.070 min
Response: 0
Conc: N.D.

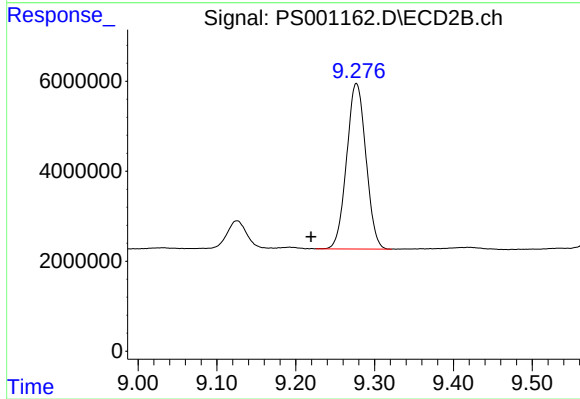

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.277 min
Delta R.T.: 0.058 min
Response: 62599761
Conc: 212.81 ng/ml

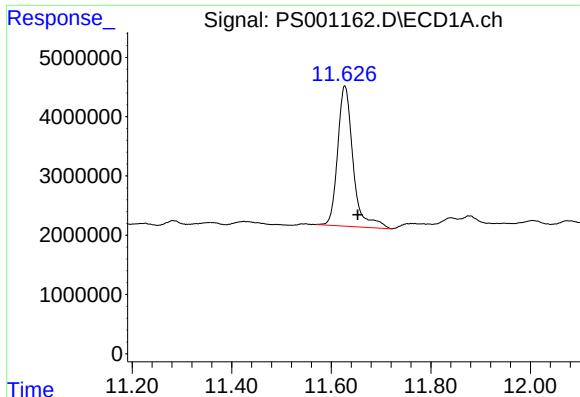

#4 2,4-DCAA


R.T.: 11.627 min
Delta R.T.: -0.026 min
Response: 50804146
Conc: 246.24 ng/ml

Instrument :
ECD_S
ClientSampleId :

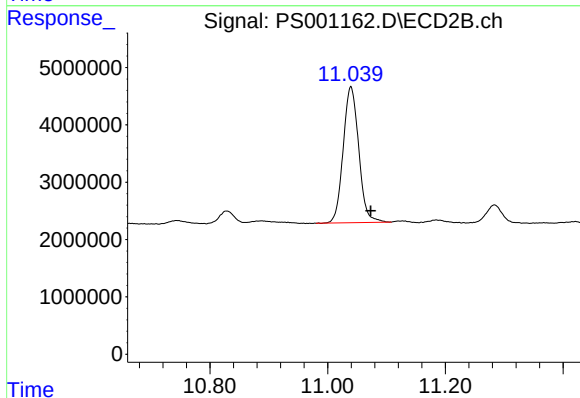


#4 2,4-DCAA

R.T.: 11.039 min
Delta R.T.: -0.034 min
Response: 43415252
Conc: 199.34 ng/ml

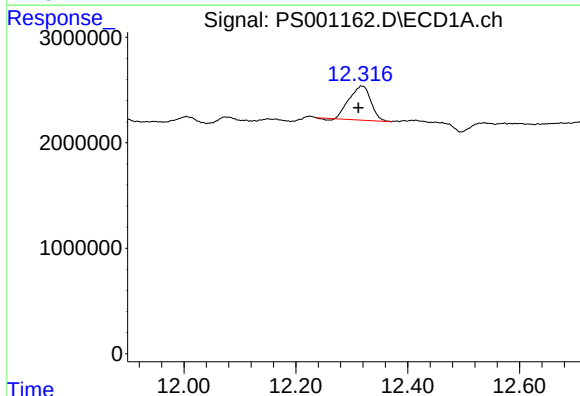


#6 MCPP

R.T.: 12.317 min
Delta R.T.: 0.005 min
Response: 8608885
Conc: 15.67 ug/ml

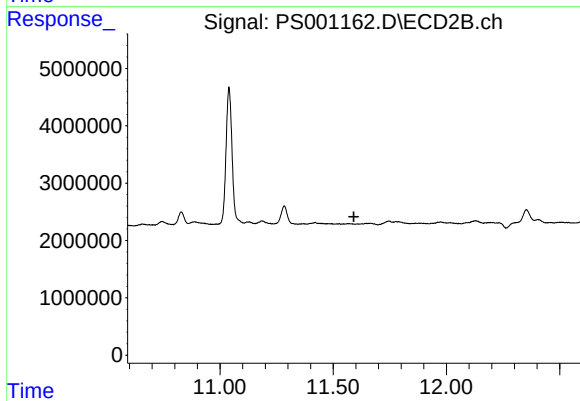

#6 MCPP


R.T.: 0.000 min
Exp R.T. : 11.591 min
Response: 0
Conc: N.D.

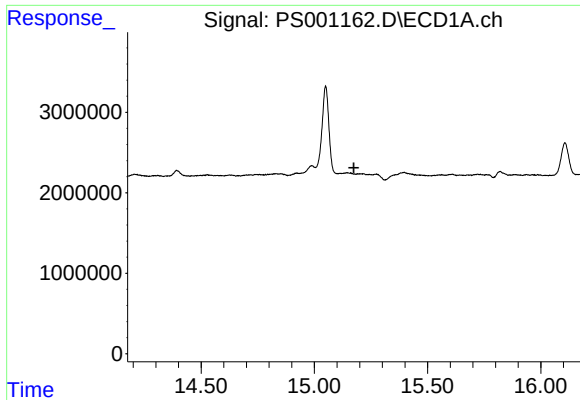

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 15.174 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

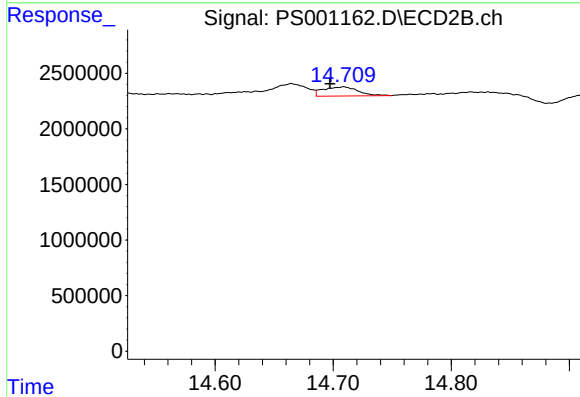


#12 2,4,5-T

R.T.: 14.709 min
Delta R.T.: 0.012 min
Response: 1692037
Conc: 1.64 ng/ml

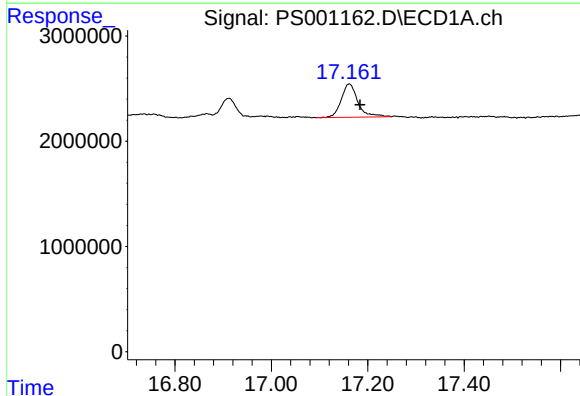


#15 Picloram

R.T.: 17.161 min
Delta R.T.: -0.022 min
Response: 7602856
Conc: 4.20 ng/ml

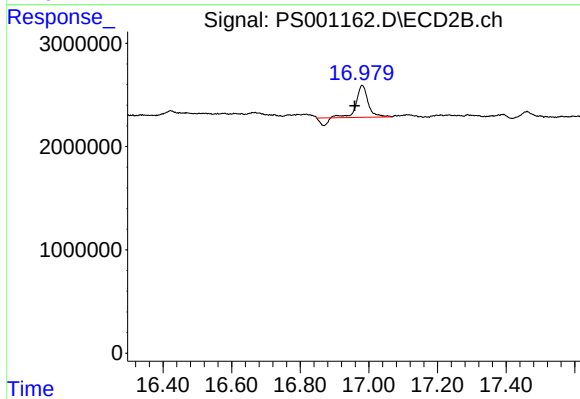

#15 Picloram


R.T.: 16.980 min
Delta R.T.: 0.021 min
Response: 6584498
Conc: 4.32 ng/ml

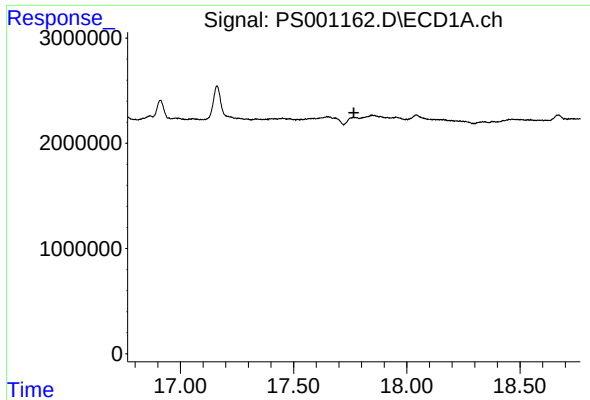

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.766 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

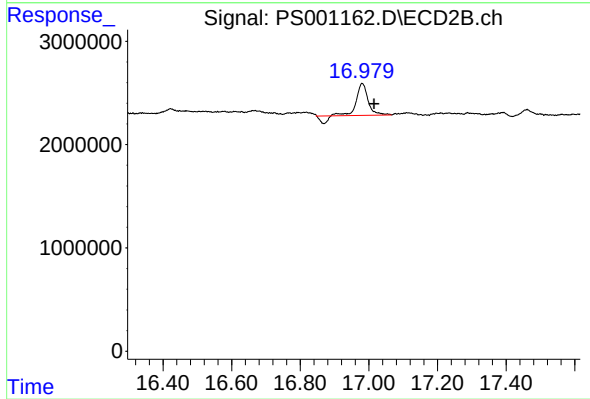

#16 DCPA

R.T.: 16.980 min
Delta R.T.: -0.035 min
Response: 6584498
Conc: 3.83 ng/ml