

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072018\
 Data File : PS001164.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jul 2018 13:58
 Operator : UA
 Sample : J4016-24RE
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 20 14:43:41 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 09 02:00:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.644	11.060	53020053	45505467	256.980	208.935
Target Compounds							
1) T	Dalapon	2.985	2.431	3228049	1199947	12.022	4.454 #
5) T	DICAMBA	12.023	11.305	3737558	5891830	4.747	7.506 #
6) T	MCPD	12.336	0.000	8508787	0	15.490	N.D. #
8) T	DICHLORPROP	0.000	12.429	0	1135348	N.D.	5.621 #
15) T	Picloram	17.172	0.000	4399364	0	2.429	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072018\
Data File : PS001164.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jul 2018 13:58
Operator : UA
Sample : J4016-24RE
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 20 14:43:41 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
Quant Title : 8080.M
QLast Update : Mon Jul 09 02:00:25 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

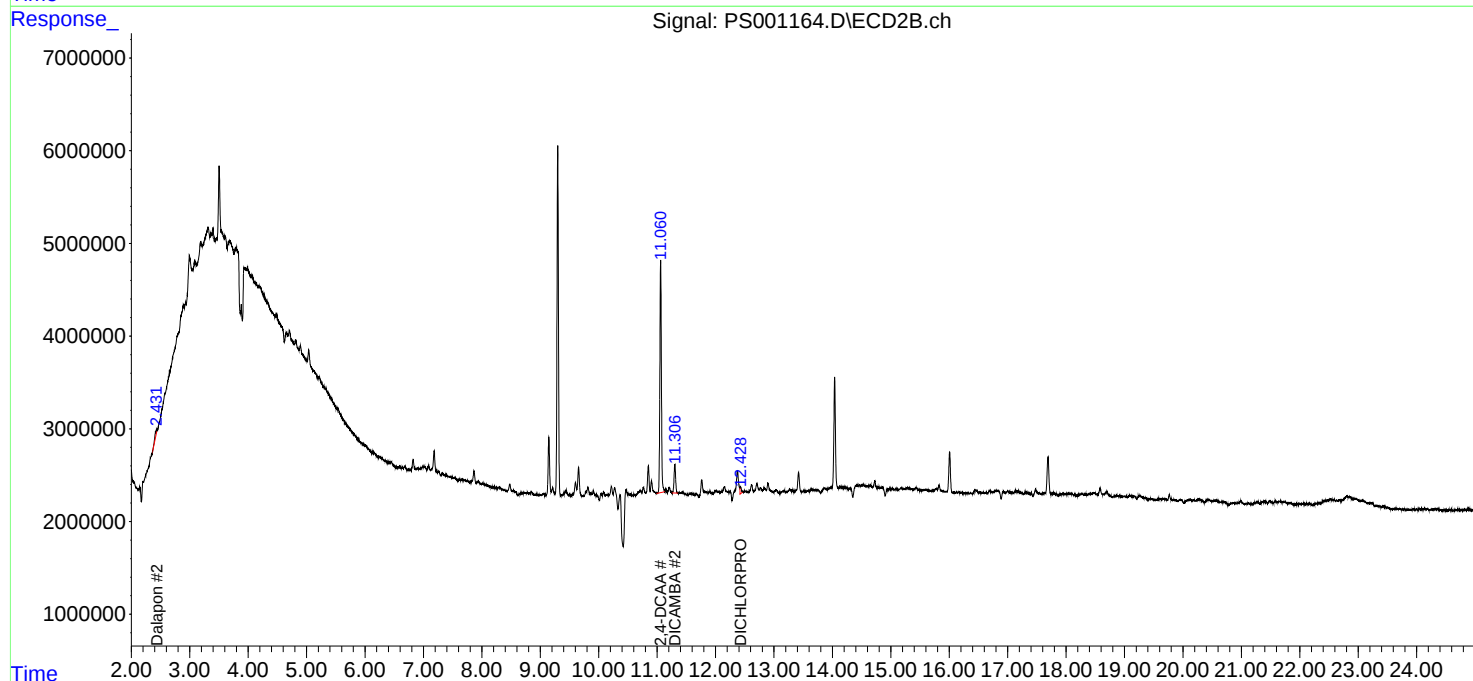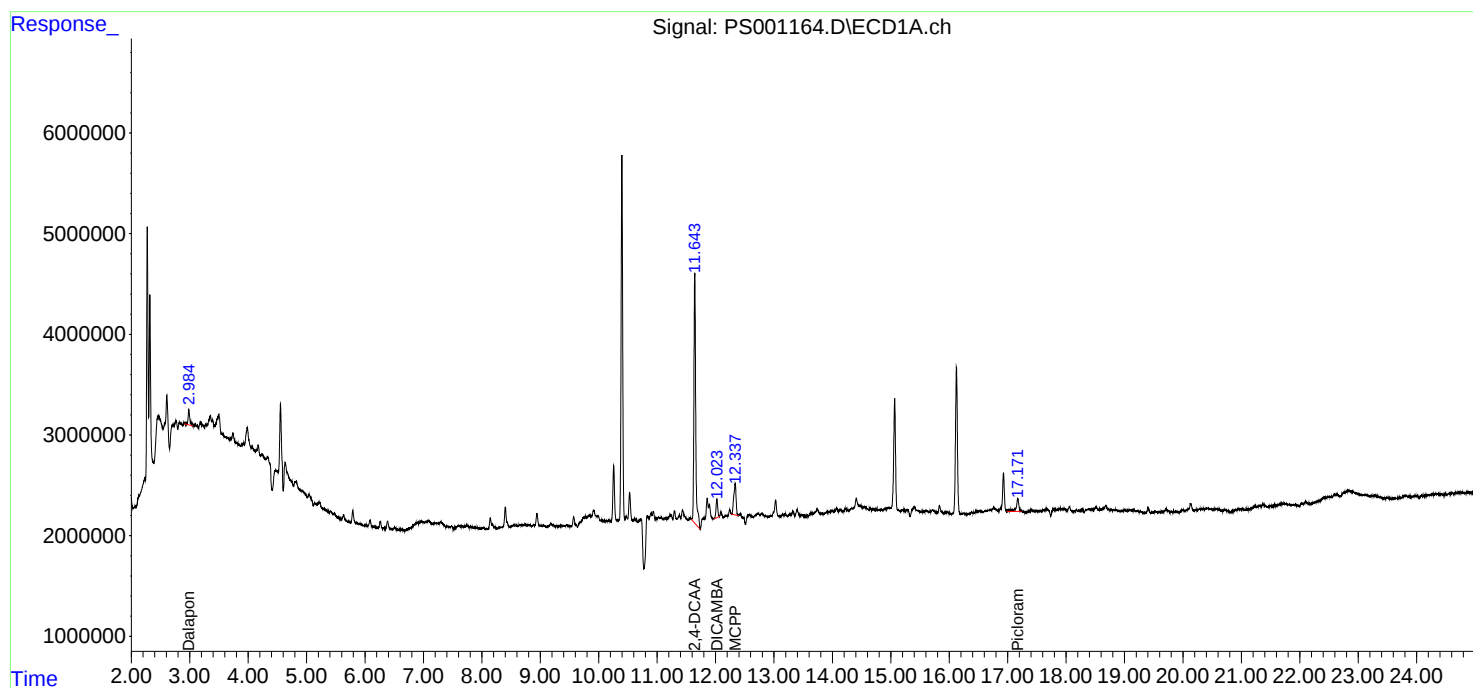


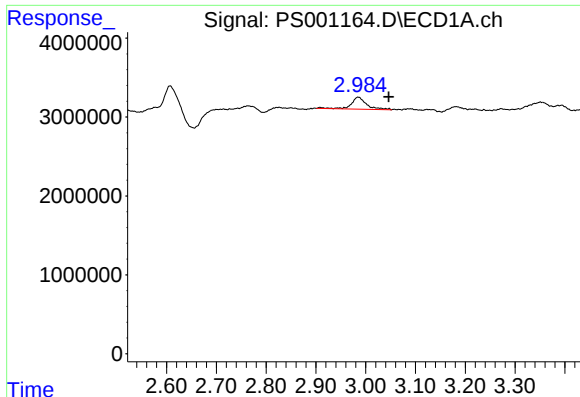

#1 Dalapon


R.T.: 2.985 min
Delta R.T.: -0.061 min
Response: 3228049
Conc: 12.02 ng/ml

Instrument :
ECD_S
ClientSampleId :

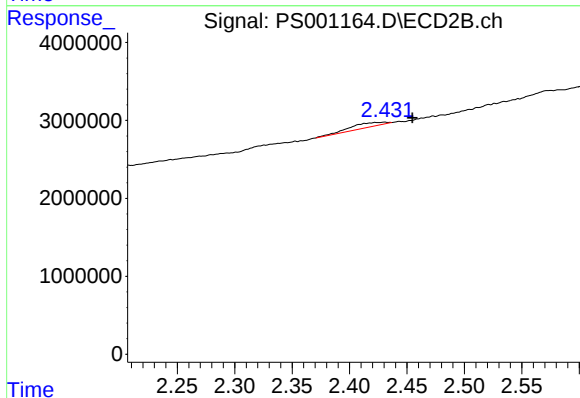


#1 Dalapon

R.T.: 2.431 min
Delta R.T.: -0.024 min
Response: 1199947
Conc: 4.45 ng/ml

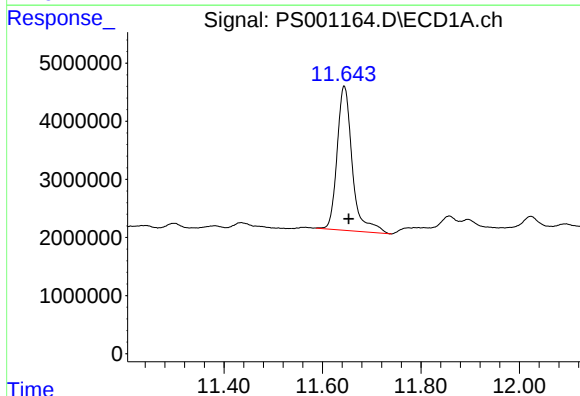


#4 2,4-DCAA

R.T.: 11.644 min
Delta R.T.: -0.009 min
Response: 53020053
Conc: 256.98 ng/ml

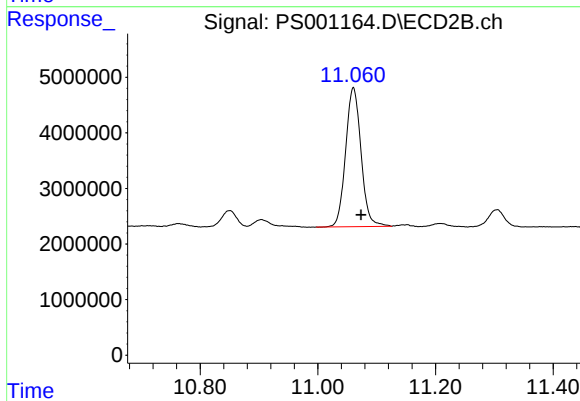

#4 2,4-DCAA


R.T.: 11.060 min
Delta R.T.: -0.013 min
Response: 45505467
Conc: 208.94 ng/ml

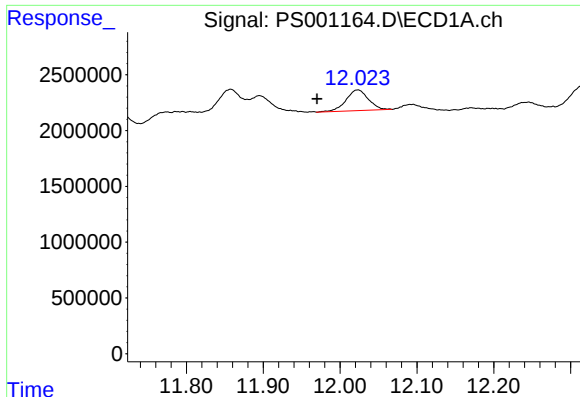

#5 DICAMBA


R.T.: 12.023 min
Delta R.T.: 0.053 min
Response: 3737558
Conc: 4.75 ng/ml

Instrument :
ECD_S
ClientSampleId :

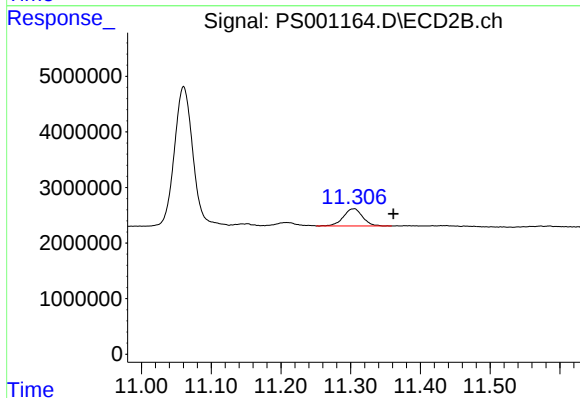


#5 DICAMBA

R.T.: 11.305 min
Delta R.T.: -0.056 min
Response: 5891830
Conc: 7.51 ng/ml

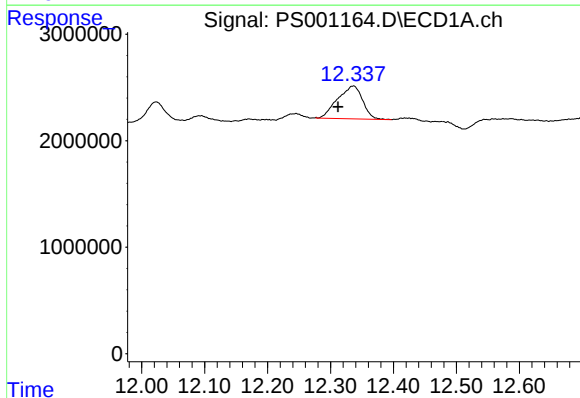


#6 MCP

R.T.: 12.336 min
Delta R.T.: 0.024 min
Response: 8508787
Conc: 15.49 ug/ml

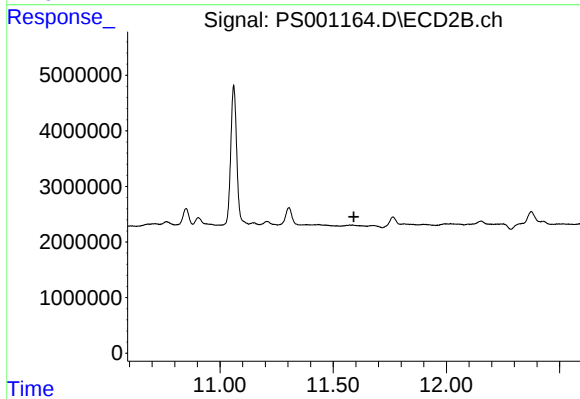

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.591 min
Response: 0
Conc: N.D.

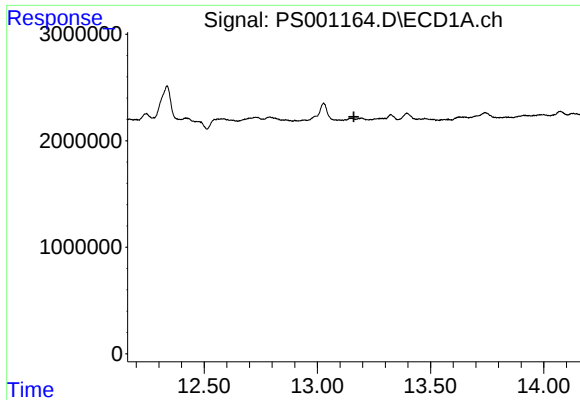

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 13.161 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

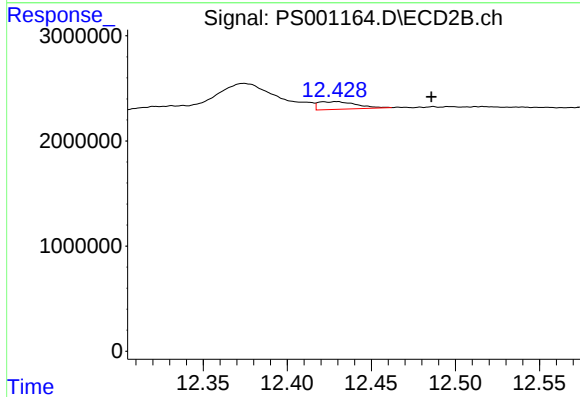


#8 DICHLORPROP

R.T.: 12.429 min
Delta R.T.: -0.056 min
Response: 1135348
Conc: 5.62 ng/ml

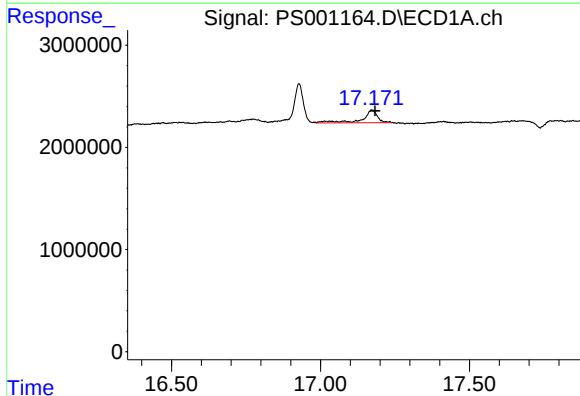

#15 Picloram

R.T.: 17.172 min
Delta R.T.: -0.011 min
Response: 4399364
Conc: 2.43 ng/ml

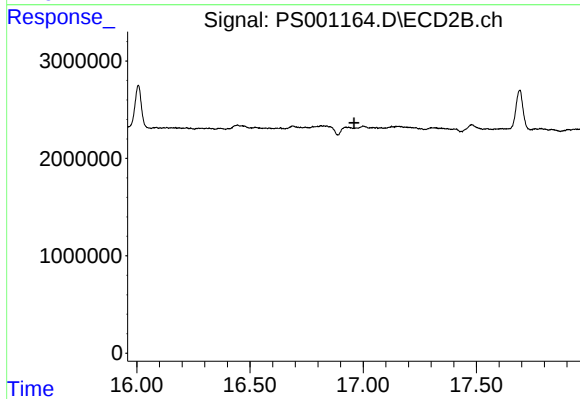

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 16.959 min
Response: 0
Conc: N.D.