

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072018\
 Data File : PS001167.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jul 2018 15:31
 Operator : UA
 Sample : J4030-09RE
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 21 00:05:01 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 09 02:00:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.644	11.059	55644724	45881546	269.701	210.662
Target Compounds							
1) T	Dalapon	2.985	2.420	5403026	3153023	20.122	11.703 #
5) T	DICAMBA	12.024	11.303	3316807	8504945	4.212	10.835 #
6) T	MCP	12.336	0.000	12291607	0	22.377	N.D. #
8) T	DICHLORPROP	0.000	12.423	0	2132758	N.D.	10.559 #
15) T	Picloram	0.000	16.982	0	4437079	N.D.	2.914 #
16) T	DCPA	0.000	17.042	0	1990973	N.D.	1.158 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072018\
Data File : PS001167.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jul 2018 15:31
Operator : UA
Sample : J4030-09RE
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 21 00:05:01 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
Quant Title : 8080.M
QLast Update : Mon Jul 09 02:00:25 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

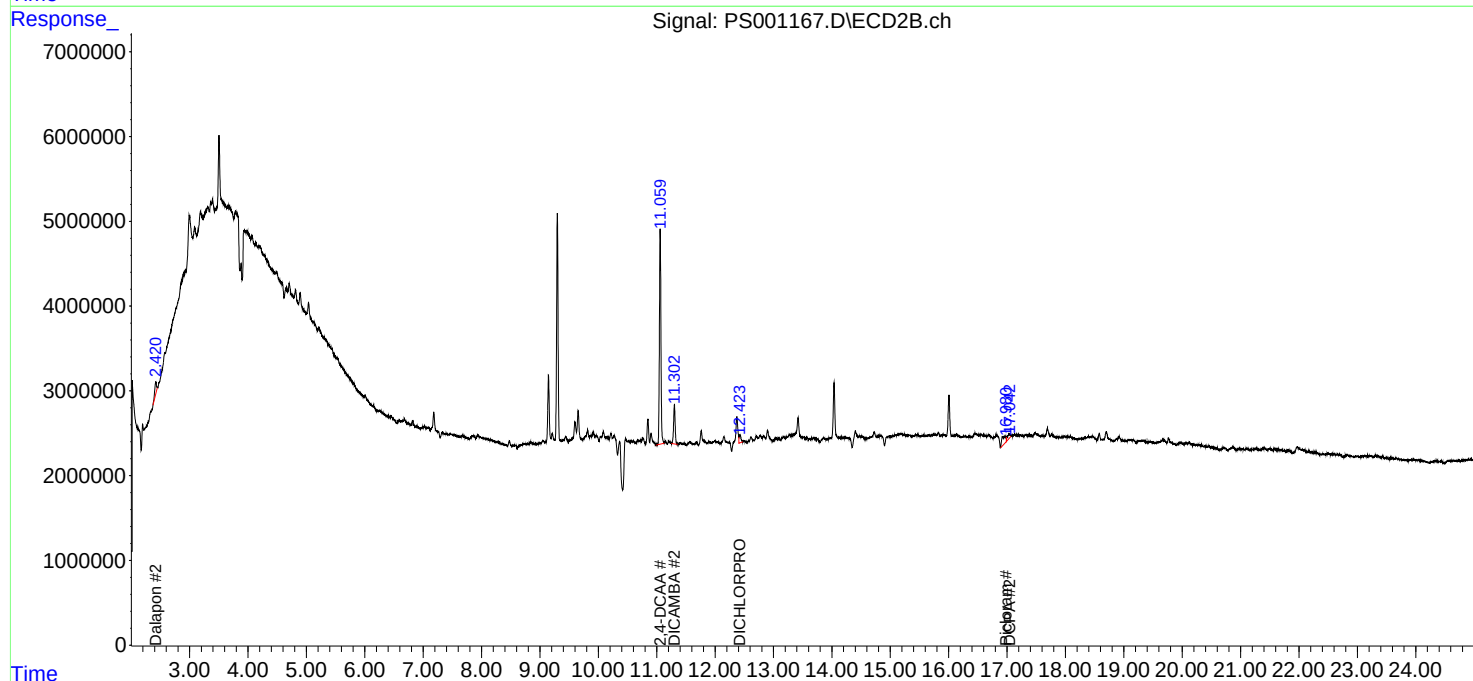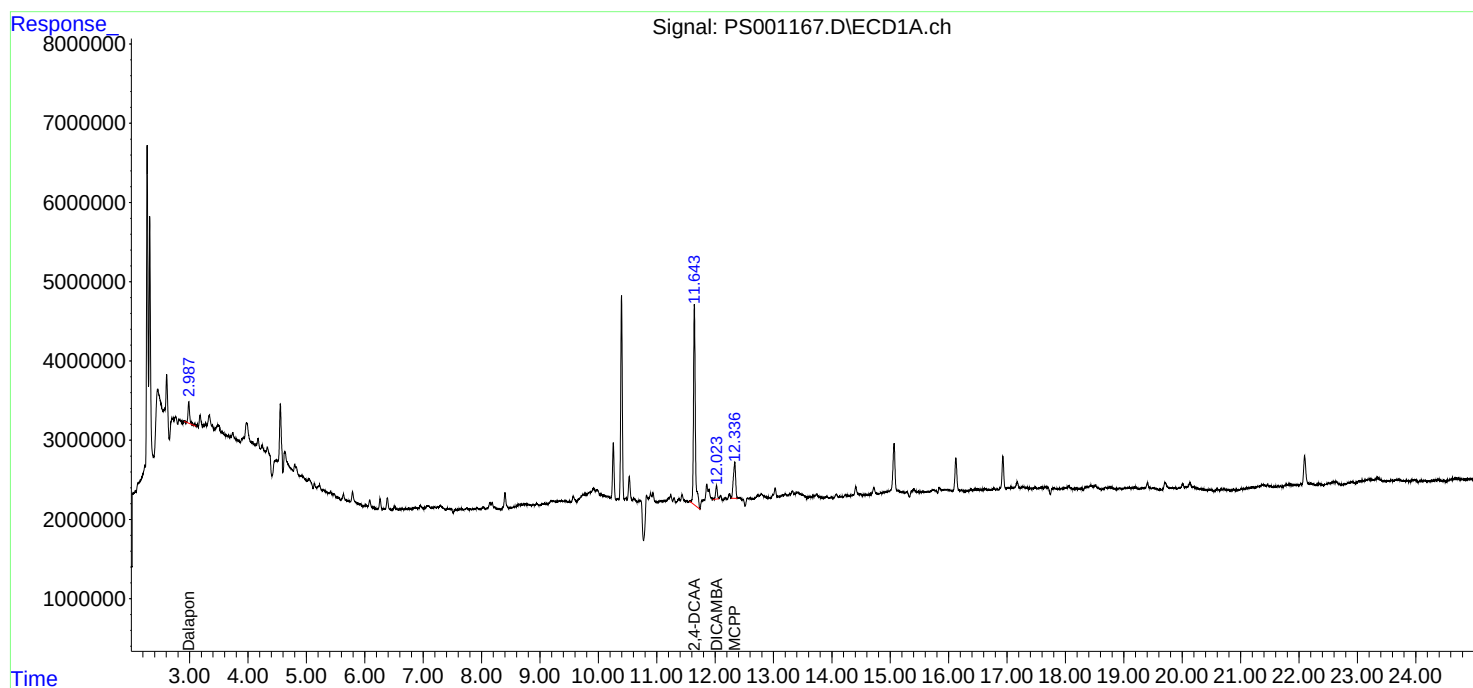


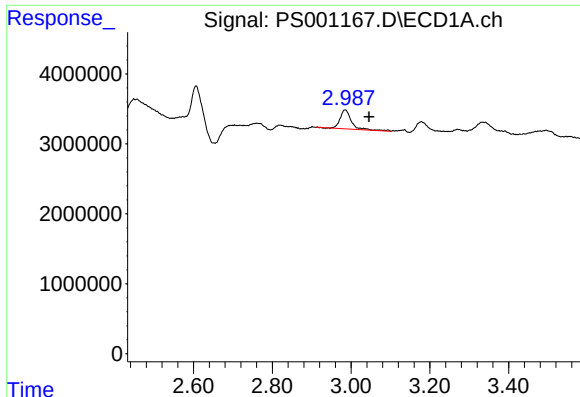

#1 Dalapon


R.T.: 2.985 min
Delta R.T.: -0.061 min
Response: 5403026
Conc: 20.12 ng/ml

Instrument :
ECD_S
ClientSampleId :

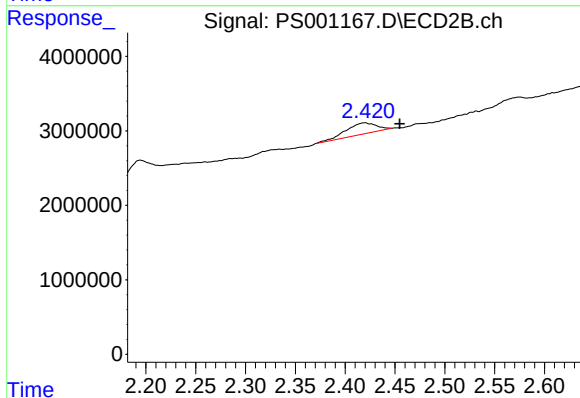


#1 Dalapon

R.T.: 2.420 min
Delta R.T.: -0.035 min
Response: 3153023
Conc: 11.70 ng/ml

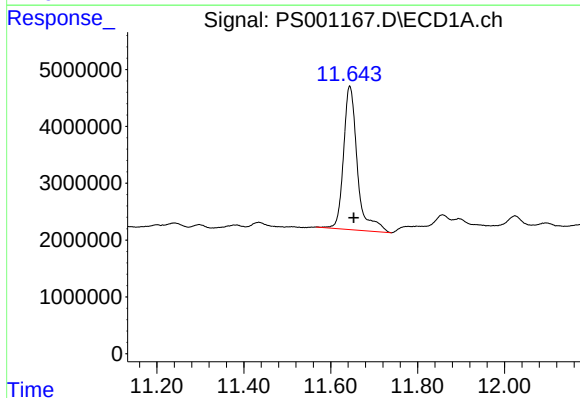


#4 2,4-DCAA

R.T.: 11.644 min
Delta R.T.: -0.009 min
Response: 55644724
Conc: 269.70 ng/ml

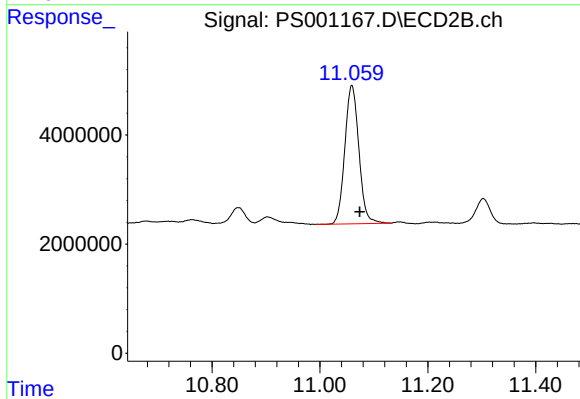

#4 2,4-DCAA


R.T.: 11.059 min
Delta R.T.: -0.014 min
Response: 45881546
Conc: 210.66 ng/ml

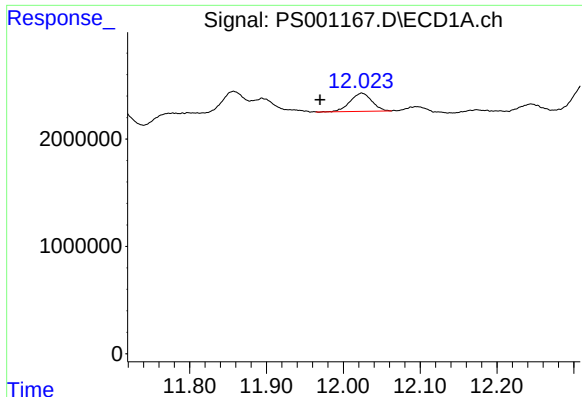

#5 DICAMBA


R.T.: 12.024 min
Delta R.T.: 0.054 min
Response: 3316807
Conc: 4.21 ng/ml

Instrument :
ECD_S
ClientSampleId :

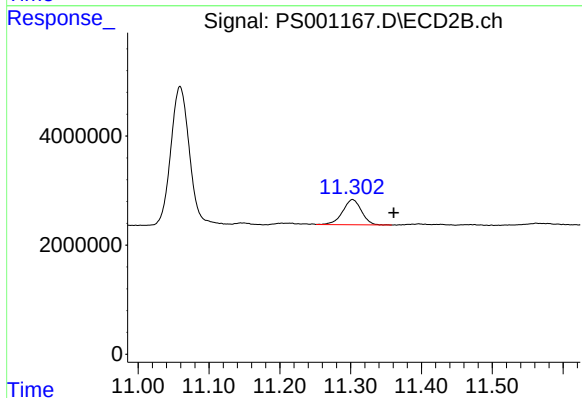


#5 DICAMBA

R.T.: 11.303 min
Delta R.T.: -0.059 min
Response: 8504945
Conc: 10.84 ng/ml

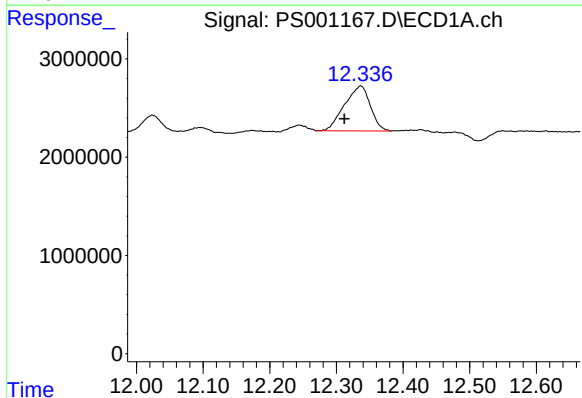


#6 MCP

R.T.: 12.336 min
Delta R.T.: 0.024 min
Response: 12291607
Conc: 22.38 ug/ml

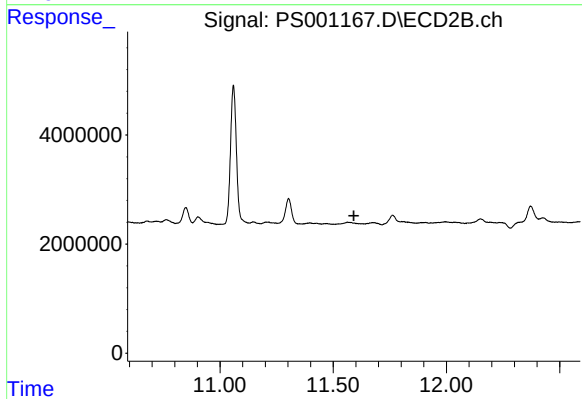

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.591 min
Response: 0
Conc: N.D.

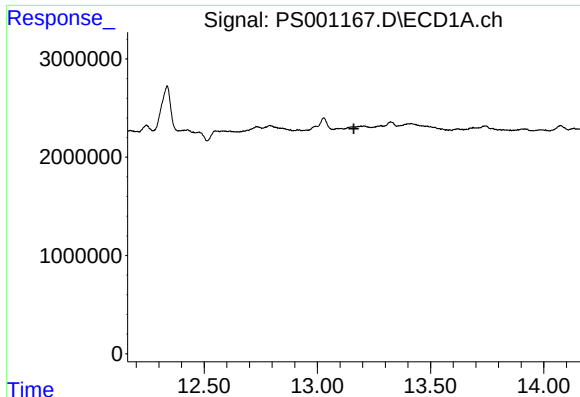

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 13.161 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

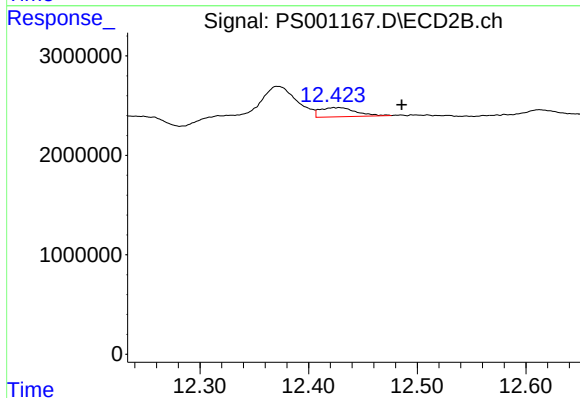


#8 DICHLORPROP

R.T.: 12.423 min
Delta R.T.: -0.063 min
Response: 2132758
Conc: 10.56 ng/ml

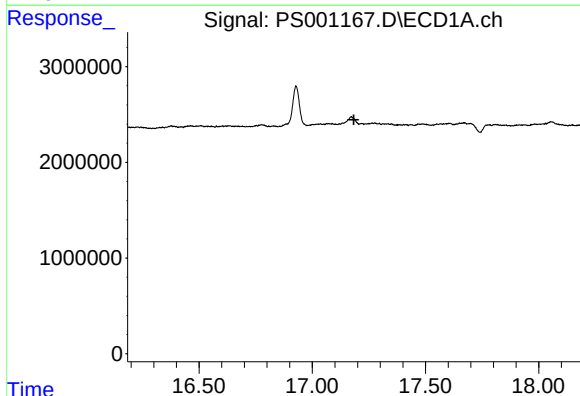


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 17.184 min
Response: 0
Conc: N.D.

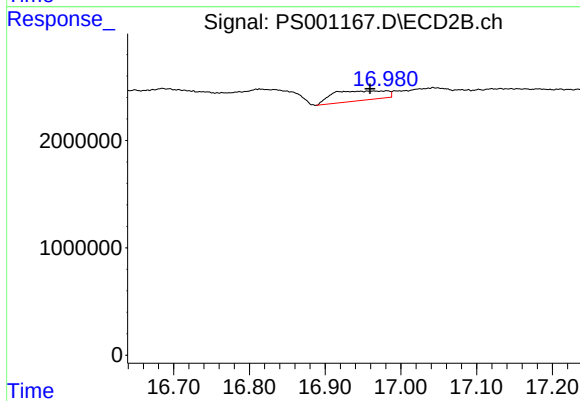

#15 Picloram


R.T.: 16.982 min
Delta R.T.: 0.022 min
Response: 4437079
Conc: 2.91 ng/ml

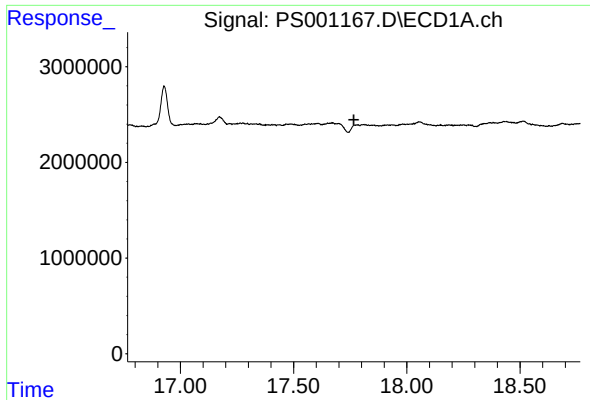

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.766 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

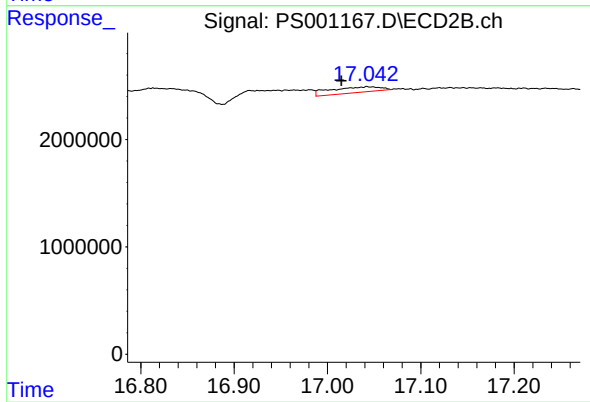

#16 DCPA

R.T.: 17.042 min
Delta R.T.: 0.027 min
Response: 1990973
Conc: 1.16 ng/ml