

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072020\
 Data File : PS011282.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jul 2020 10:08
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 21 00:54:25 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071320.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 13 16:10:29 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
2) T	3,5-DICHL...	6.482	0.000	163.8E6	0	122.404	N.D. #
5) T	DICAMBA	0.000	7.147	0	119.7E6	N.D.	52.254
6) T	MCCP	0.000	7.147	0	119.7E6	N.D.	62.711
10) T	Pentachlo...	8.655	0.000	7274441	0	<MDL	N.D. #
12) T	2,4,5-T	9.491	9.231	7847760	21183775	1.555	6.984 #
15) T	Picloram	11.027	10.999	90275576	77206399	14.307	17.654
16) T	DCPA	11.469	10.999	8991363	77206399	1.396	20.415 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072020\
Data File : PS011282.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jul 2020 10:08
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 21 00:54:25 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071320.M
Quant Title : 8080.M
QLast Update : Mon Jul 13 16:10:29 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

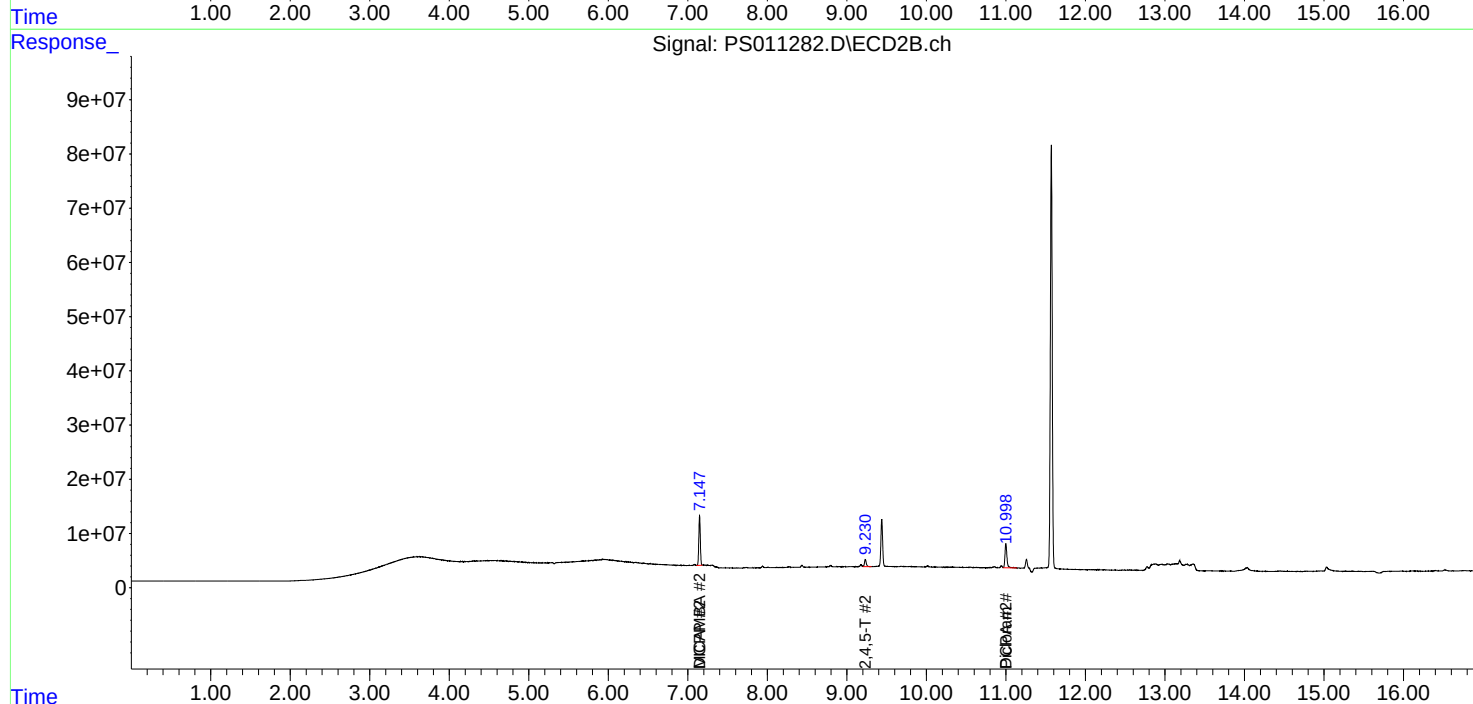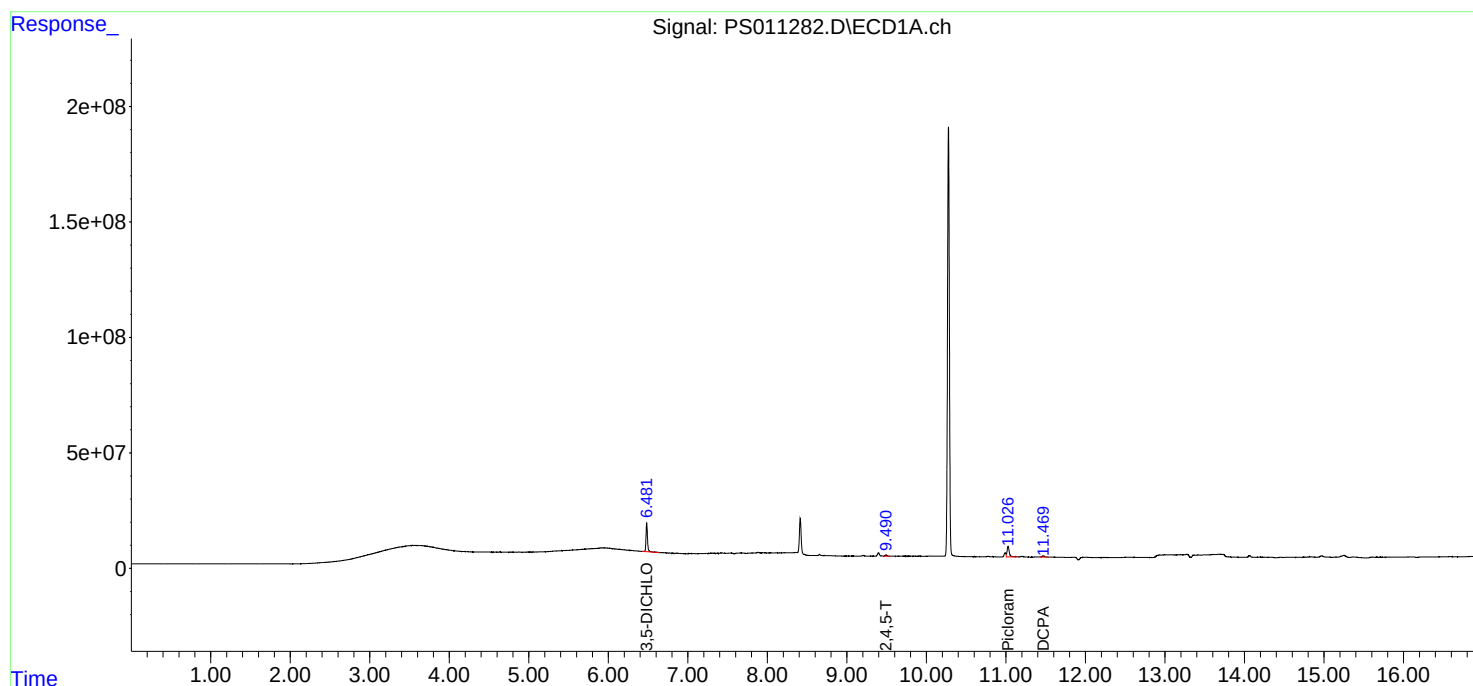


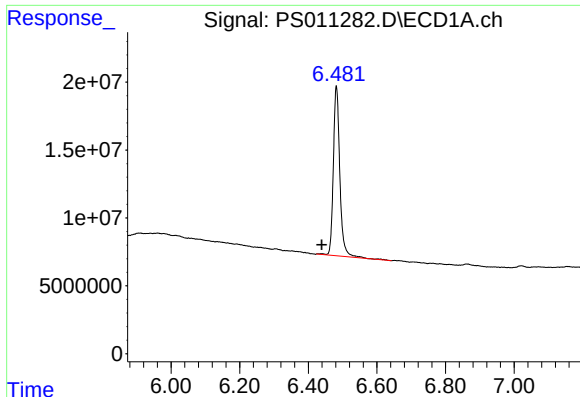

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.482 min
Delta R.T.: 0.043 min
Response: 163795508
Conc: 122.40 ng/ml

Instrument :
ECD_S
ClientSampleId :

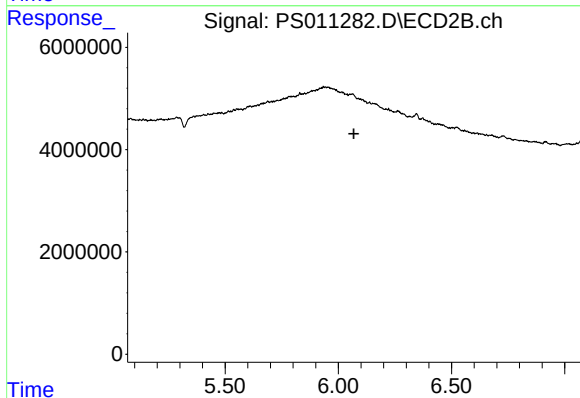


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.069 min
Response: 0
Conc: N.D.

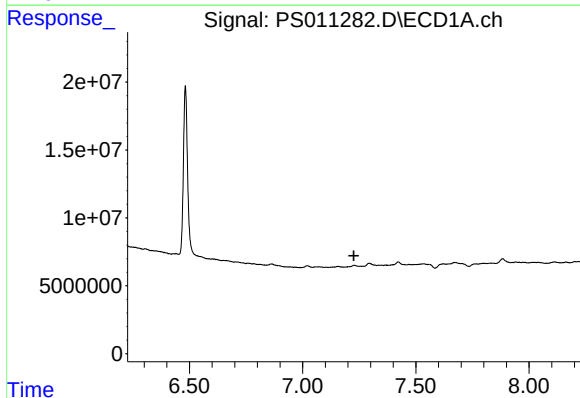


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 7.226 min
Response: 0
Conc: N.D.

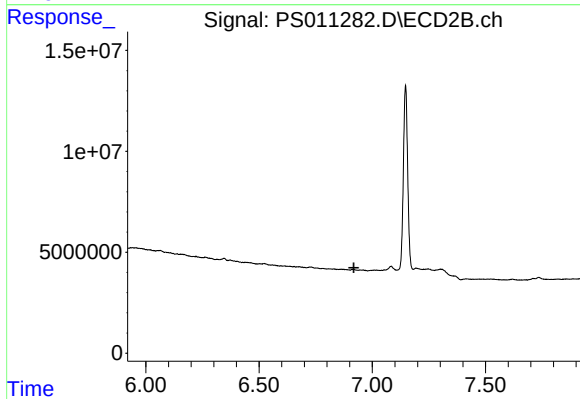

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.918 min
Response: 0
Conc: N.D.

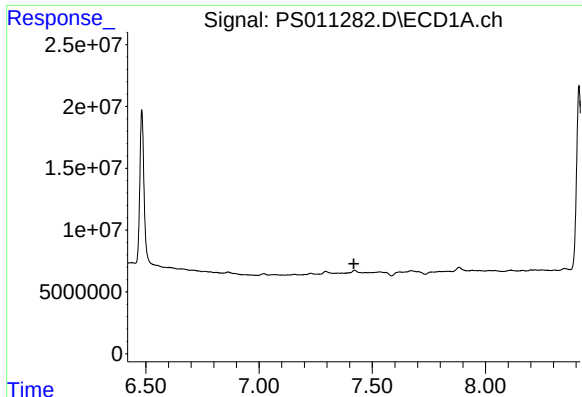

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 7.419 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

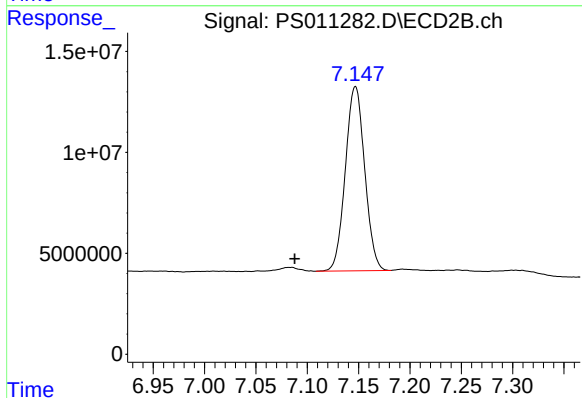


#5 DICAMBA

R.T.: 7.147 min
Delta R.T.: 0.059 min
Response: 119658968
Conc: 52.25 ng/ml

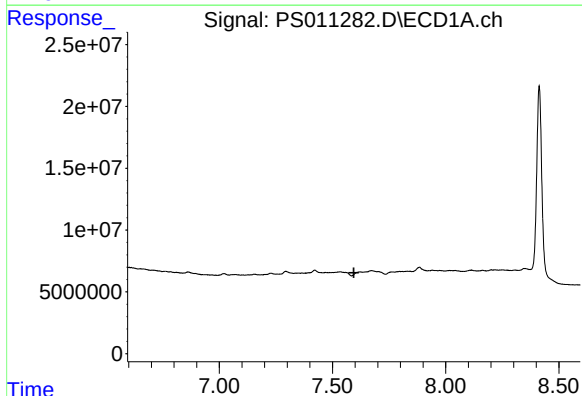


#6 MCP

R.T.: 0.000 min
Exp R.T.: 7.594 min
Response: 0
Conc: N.D.

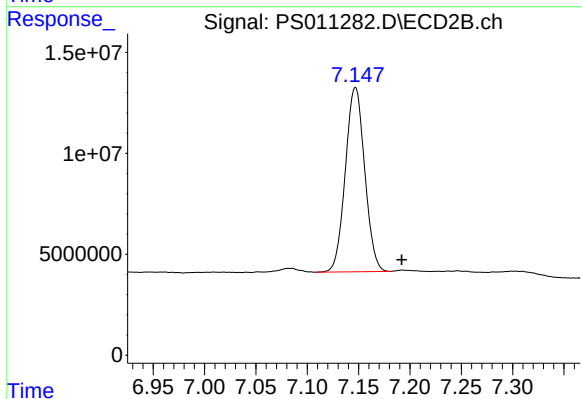

#6 MCP


R.T.: 7.147 min
Delta R.T.: -0.045 min
Response: 119658968
Conc: 62.71 ug/ml

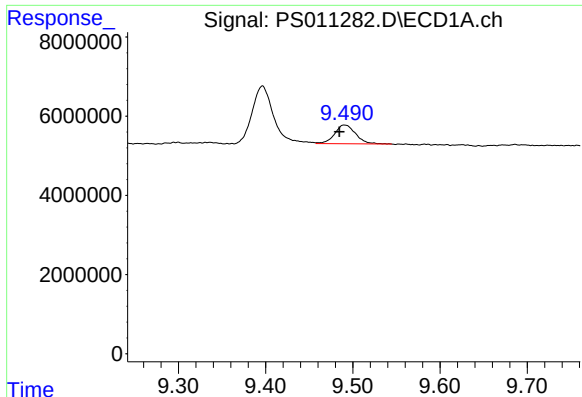

#12 2,4,5-T


R.T.: 9.491 min
Delta R.T.: 0.006 min
Response: 7847760
Conc: 1.56 ng/ml

Instrument :
ECD_S
ClientSampleId :

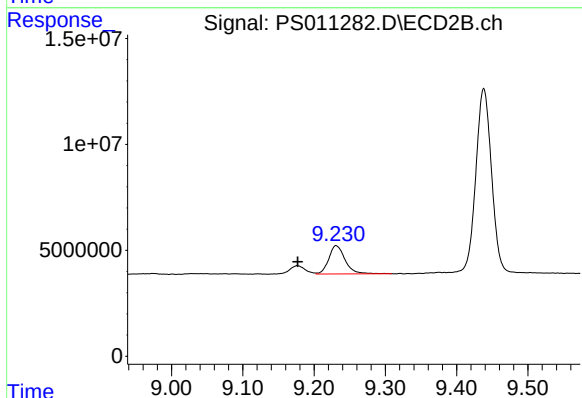


#12 2,4,5-T

R.T.: 9.231 min
Delta R.T.: 0.054 min
Response: 21183775
Conc: 6.98 ng/ml

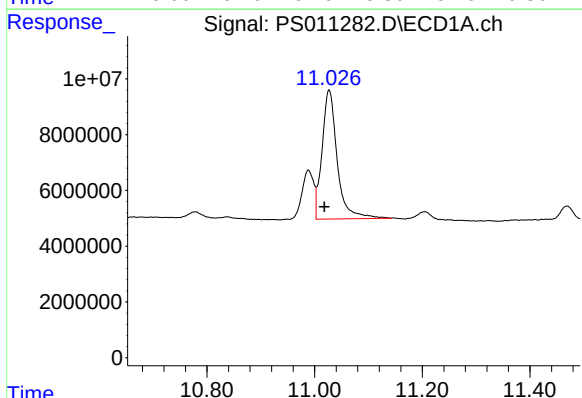


#15 Picloram

R.T.: 11.027 min
Delta R.T.: 0.009 min
Response: 90275576
Conc: 14.31 ng/ml

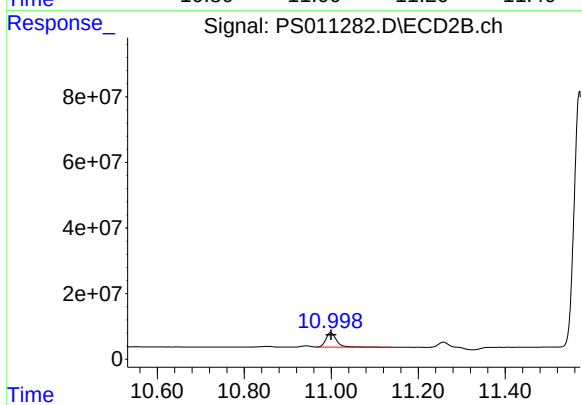

#15 Picloram


R.T.: 10.999 min
Delta R.T.: 0.000 min
Response: 77206399
Conc: 17.65 ng/ml

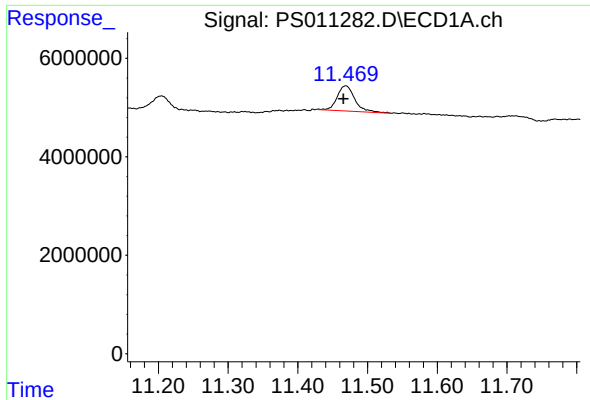

#16 DCPA

R.T.: 11.469 min
Delta R.T.: 0.003 min
Response: 8991363
Conc: 1.40 ng/ml

Instrument :
ECD_S
ClientSampleId :

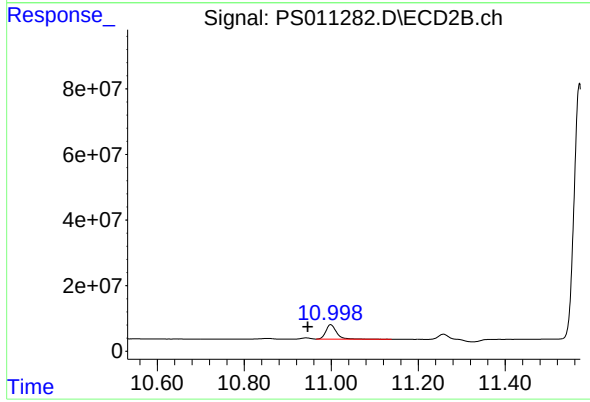

#16 DCPA

R.T.: 10.999 min
Delta R.T.: 0.053 min
Response: 77206399
Conc: 20.41 ng/ml