

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072021\
 Data File : PS016150.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jul 2021 09:53
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 21 03:58:36 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS063021.M
 Quant Title : 8080.M
 QLast Update : Wed Jun 30 00:31:48 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.187	6.766	622.5E6	249.1E6	405.503	485.194
Target Compounds							
12) T	2,4,5-T	9.380f	0.000	10828611	0	1.387	N.D. #
15) T	Picloram	11.006	10.833	70603639	26844319	6.418	6.452
16) T	DCPA	0.000	10.833f	0	26844319	N.D.	6.242



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072021\
Data File : PS016150.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jul 2021 09:53
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 21 03:58:36 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS063021.M
Quant Title : 8080.M
QLast Update : Wed Jun 30 00:31:48 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

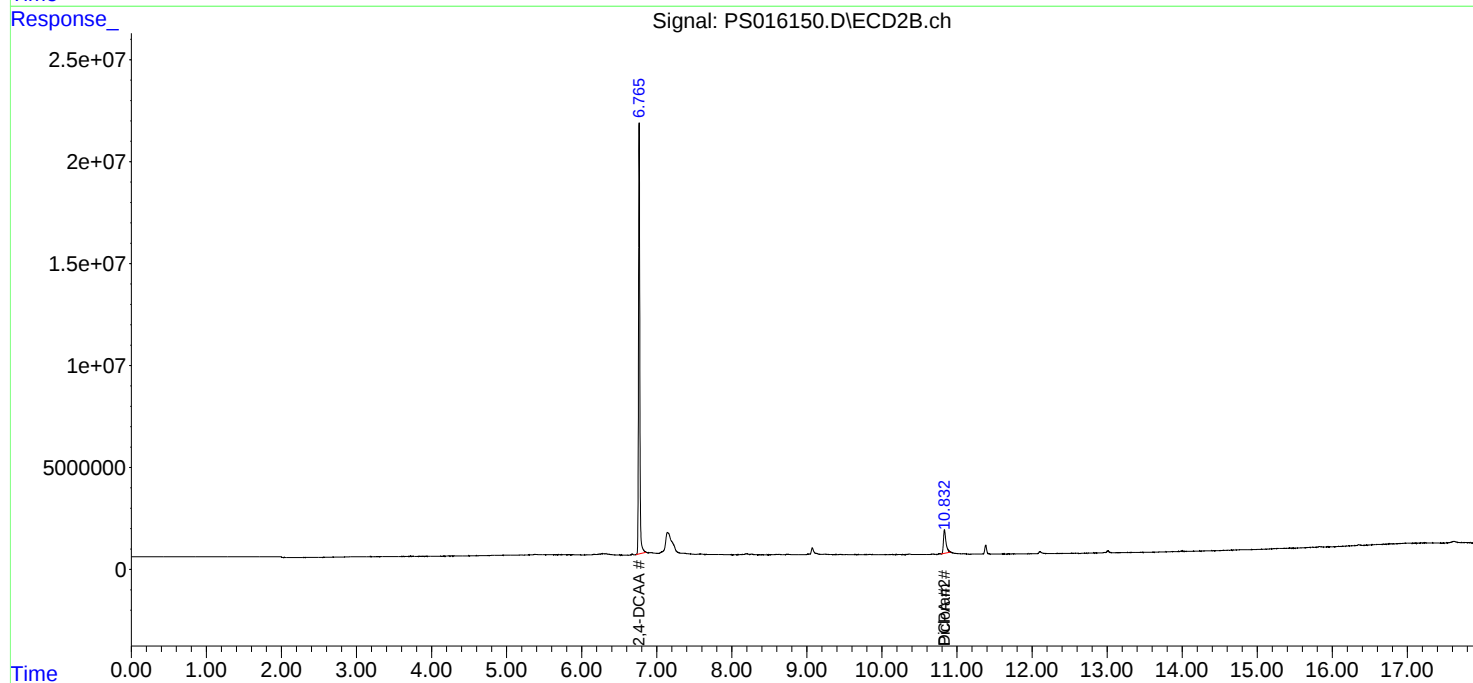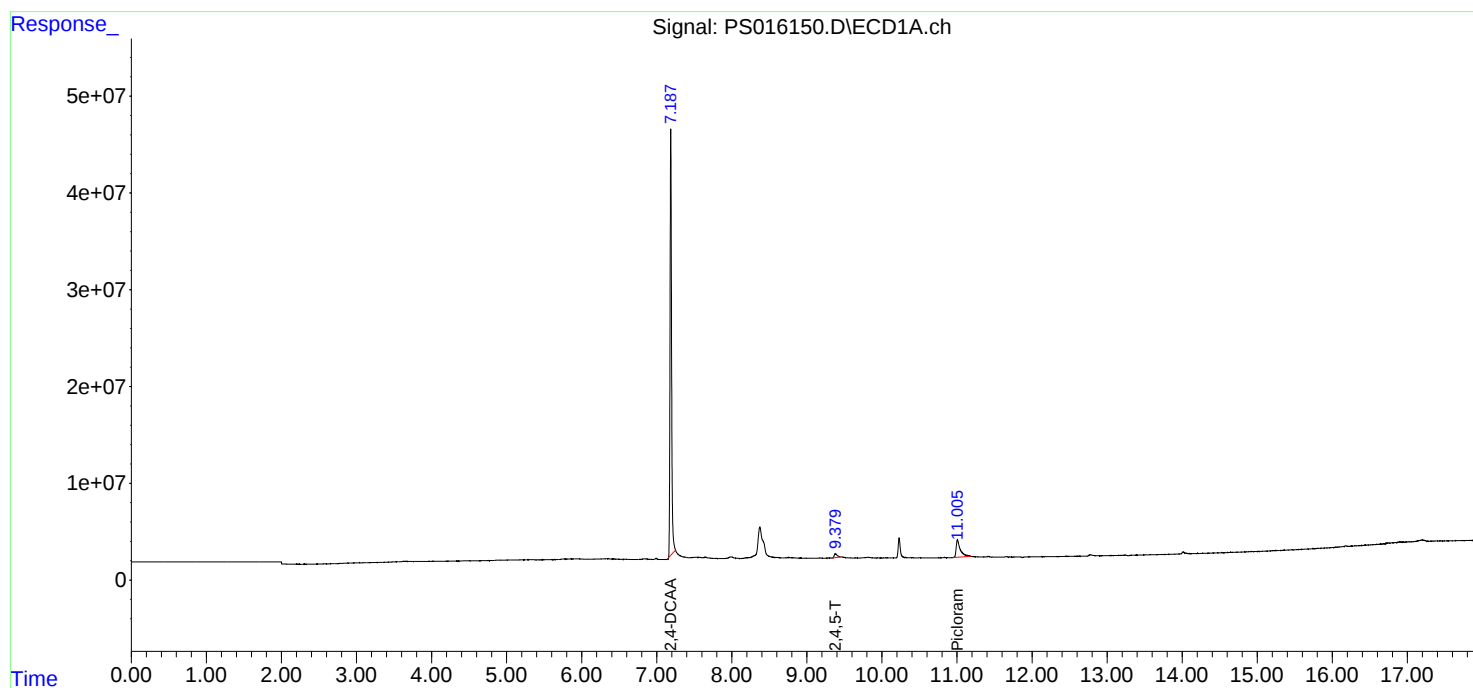


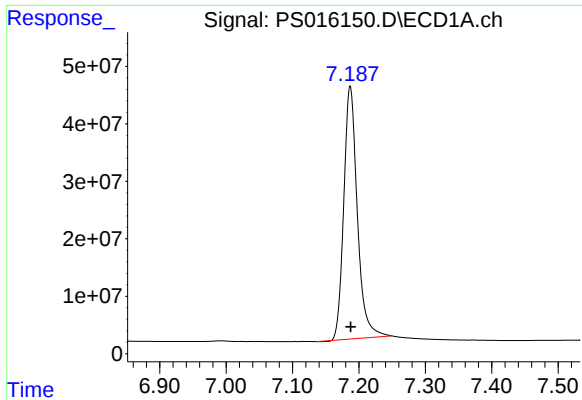

#4 2,4-DCAA


R.T.: 7.187 min
Delta R.T.: 0.000 min
Response: 622528808
Conc: 405.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

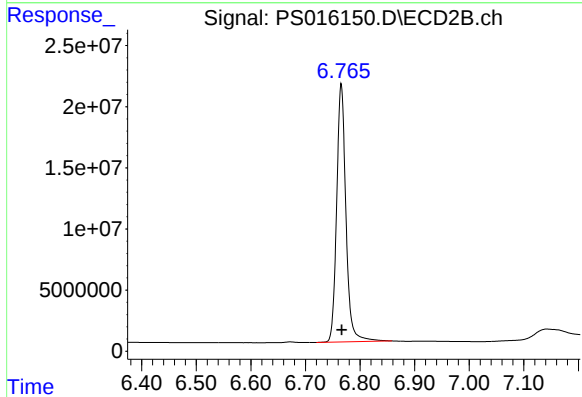


#4 2,4-DCAA

R.T.: 6.766 min
Delta R.T.: -0.001 min
Response: 249058205
Conc: 485.19 ng/ml

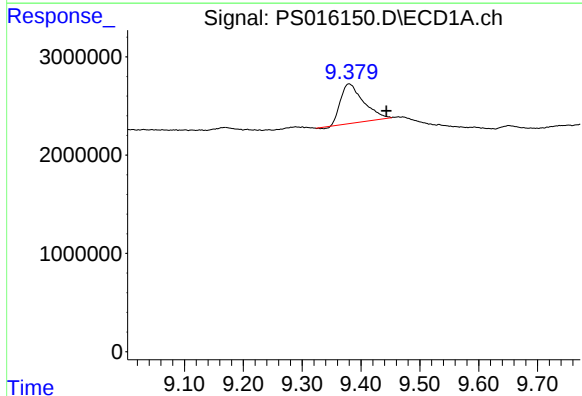


#12 2,4,5-T

R.T.: 9.380 min
Delta R.T.: -0.064 min
Response: 10828611
Conc: 1.39 ng/ml

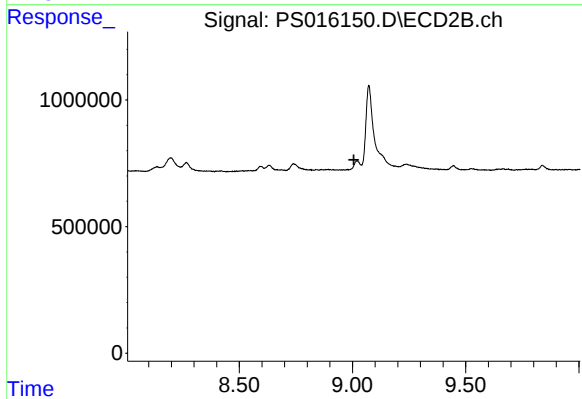

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.006 min
Response: 0
Conc: N.D.

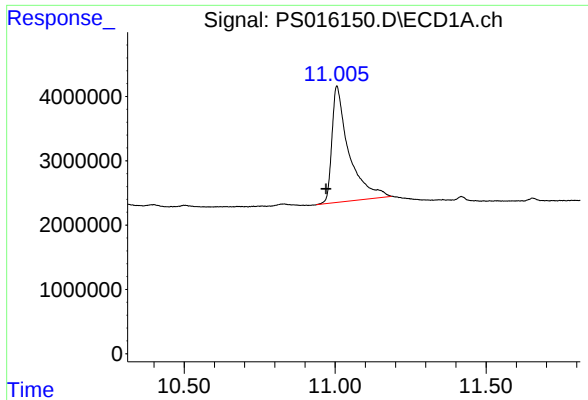

#15 Picloram


R.T.: 11.006 min
Delta R.T.: 0.036 min
Response: 70603639
Conc: 6.42 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

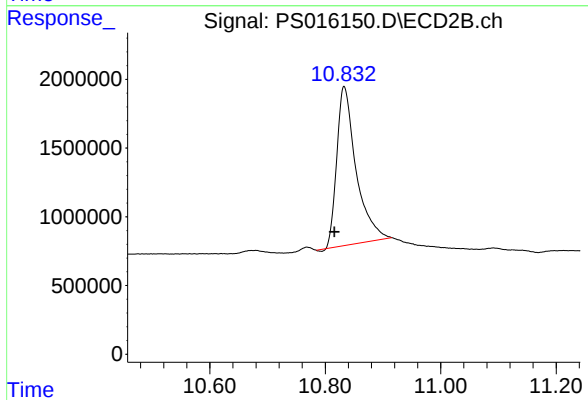


#15 Picloram

R.T.: 10.833 min
Delta R.T.: 0.016 min
Response: 26844319
Conc: 6.45 ng/ml

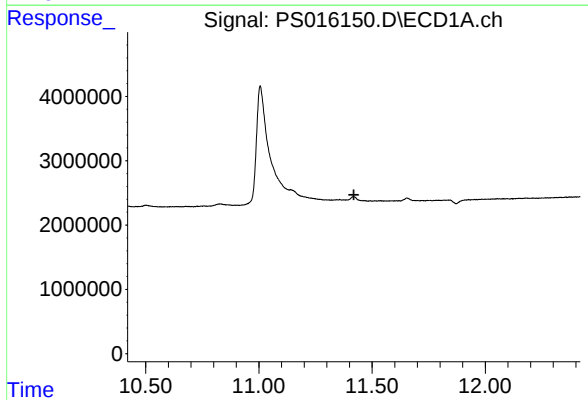

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.420 min
Response: 0
Conc: N.D.

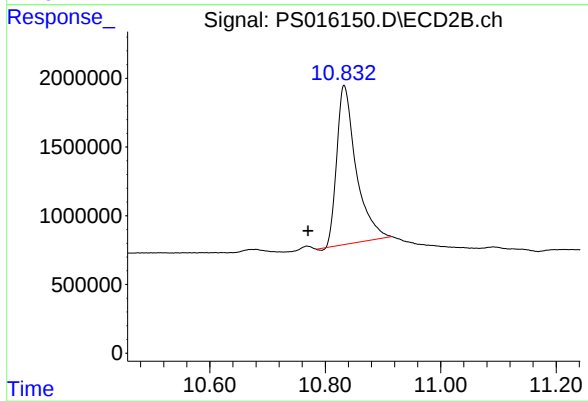

#16 DCPA

R.T.: 10.833 min
Delta R.T.: 0.063 min
Response: 26844319
Conc: 6.24 ng/ml