

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072023\
 Data File : PS023771.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jul 2023 14:31
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 21 05:40:49 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072023.M
 Quant Title : 8080.M
 QLast Update : Thu Jul 20 19:21:53 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.363	0.000	1704209	0	<MDL	N.D. #
Target Compounds							
1) T	Dalapon	2.520	2.588	4310364	4138813	2.012	3.737 #
2) T	3,5-DICHL...	5.736	0.000	263725	0	<MDL	N.D. #
3) T	4-Nitroph...	6.209	6.351f	11559258	678446	9.298	1.602 #
5) T	DICAMBA	6.507	7.004	811537	611390	<MDL	<MDL #
8) T	DICHLORPROP	7.123	7.602	278982	2949643	<MDL	3.904 #
9) T	2,4-D	0.000	7.818f	0	223562	N.D.	<MDL
10) T	Pentachlo...	7.581f	0.000	396497	0	<MDL	N.D. #
11) T	2,4,5-TP ...	8.049	8.658	1855194	626843	<MDL	<MDL #
12) T	2,4,5-T	8.313	9.037	2695321	351438	<MDL	<MDL #
14) T	DINOSEB	9.872	0.000	557534	0	<MDL	N.D. #
15) T	Picloram	9.700	10.824	31529265	11218043	2.057	1.850
16) T	DCPA	10.134	10.824	909407	11218043	<MDL	2.359 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072023\
Data File : PS023771.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jul 2023 14:31
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 21 05:40:49 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072023.M
Quant Title : 8080.M
QLast Update : Thu Jul 20 19:21:53 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

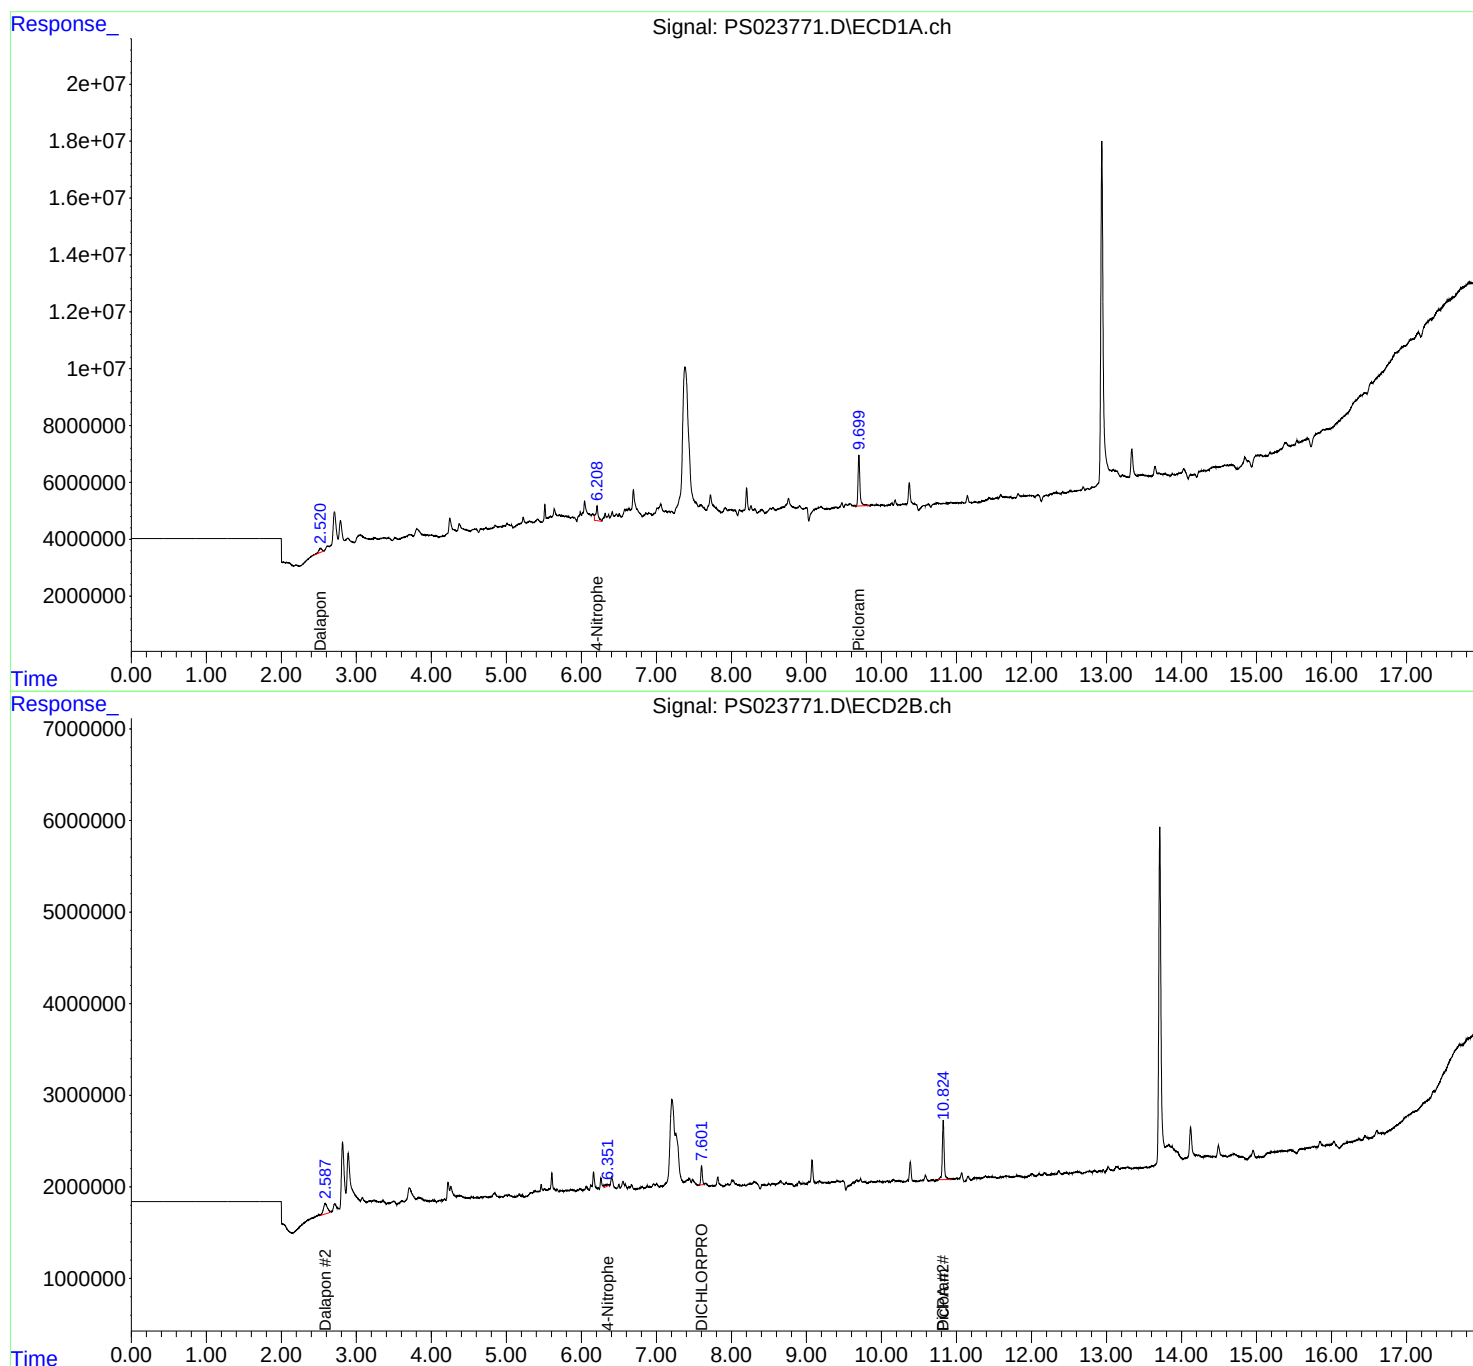


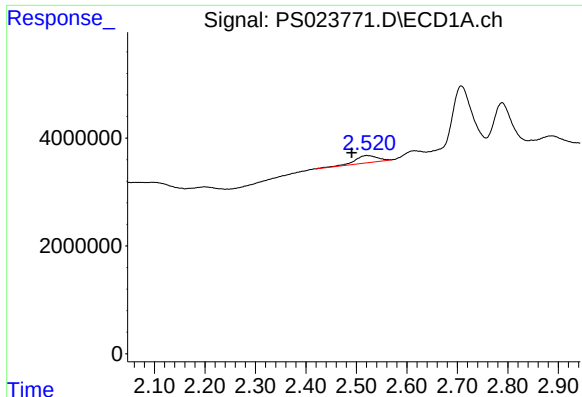

#1 Dalapon


R.T.: 2.520 min
Delta R.T.: 0.029 min
Response: 4310364
Conc: 2.01 ng/ml

Instrument :
ECD_S
ClientSampleId :

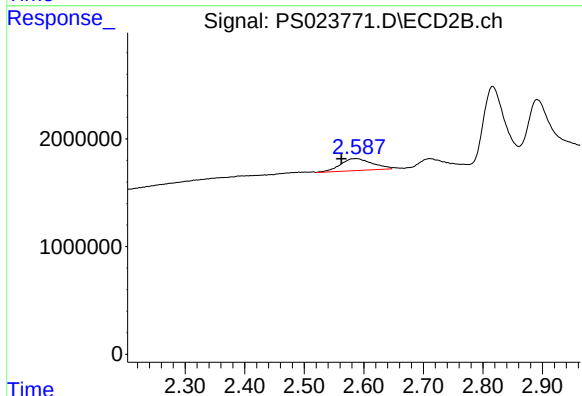


#1 Dalapon

R.T.: 2.588 min
Delta R.T.: 0.025 min
Response: 4138813
Conc: 3.74 ng/ml

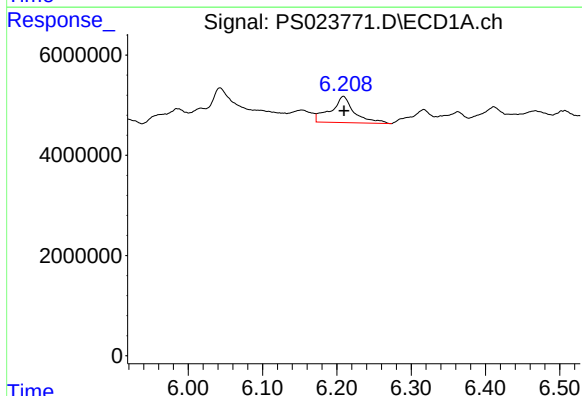


#3 4-Nitrophenol

R.T.: 6.209 min
Delta R.T.: 0.000 min
Response: 11559258
Conc: 9.30 ng/ml

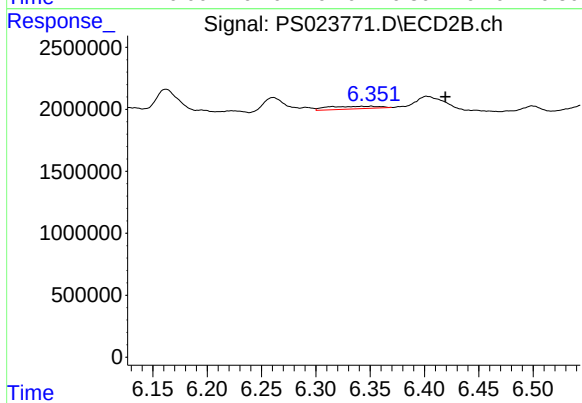

#3 4-Nitrophenol


R.T.: 6.351 min
Delta R.T.: -0.069 min
Response: 678446
Conc: 1.60 ng/ml

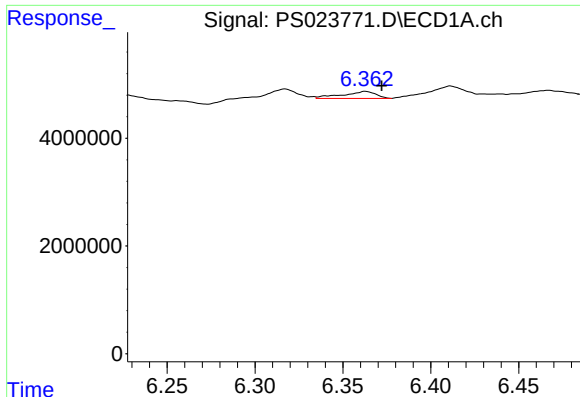

#4 2,4-DCAA


R.T.: 6.363 min
Delta R.T.: -0.009 min
Response: 1704209
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

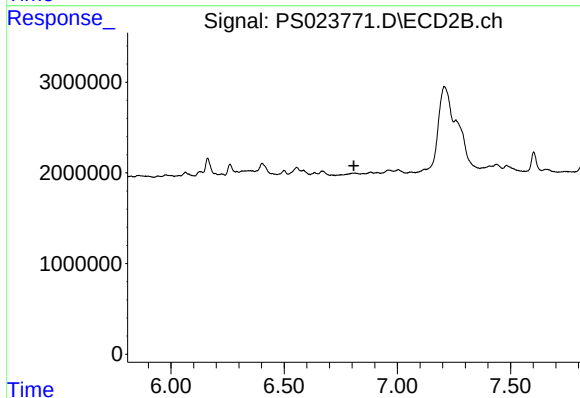


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.808 min
Response: 0
Conc: N.D.

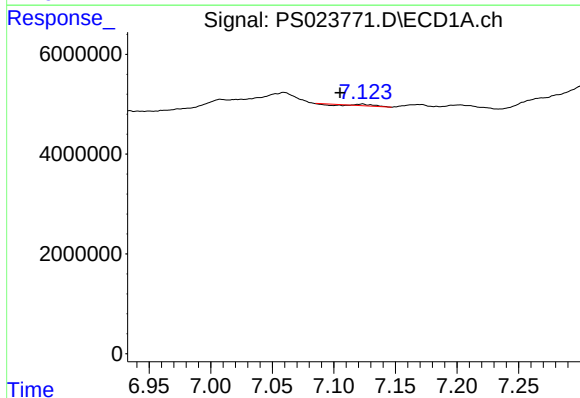


#8 DICHLORPROP

R.T.: 7.123 min
Delta R.T.: 0.018 min
Response: 278982
Conc: N.D.

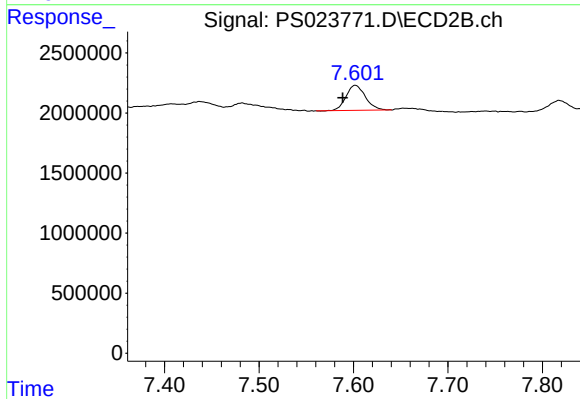

#8 DICHLORPROP


R.T.: 7.602 min
Delta R.T.: 0.013 min
Response: 2949643
Conc: 3.90 ng/ml

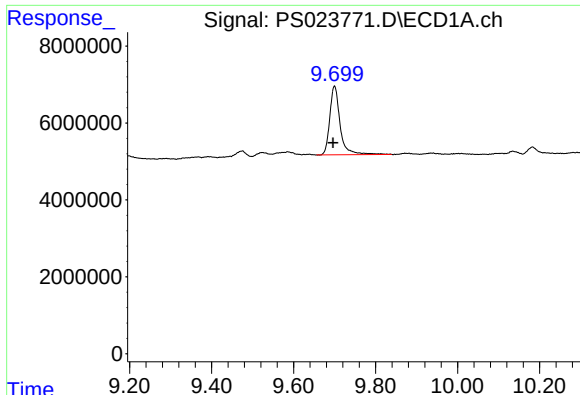

#15 Picloram


R.T.: 9.700 min
Delta R.T.: 0.003 min
Response: 31529265
Conc: 2.06 ng/ml

Instrument :
ECD_S
ClientSampleId :

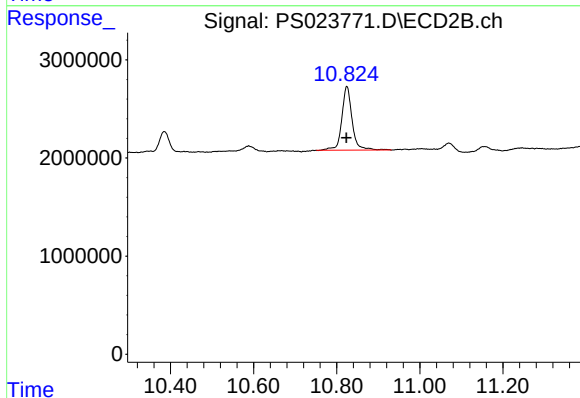


#15 Picloram

R.T.: 10.824 min
Delta R.T.: 0.001 min
Response: 11218043
Conc: 1.85 ng/ml

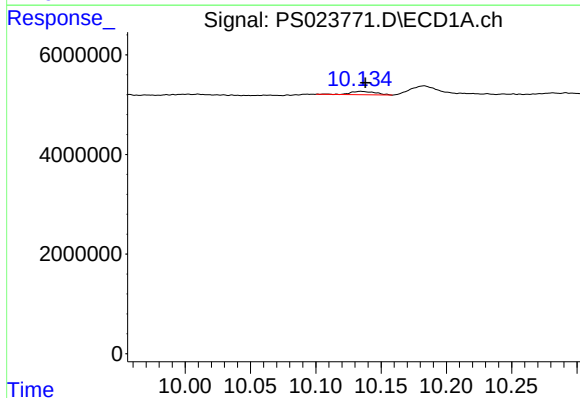

#16 DCPA

R.T.: 10.134 min
Delta R.T.: -0.004 min
Response: 909407
Conc: N.D.

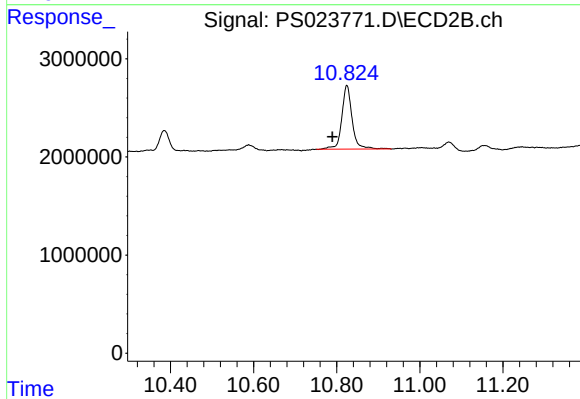

#16 DCPA

R.T.: 10.824 min
Delta R.T.: 0.035 min
Response: 11218043
Conc: 2.36 ng/ml