

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072118\
 Data File : PS001181.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2018 02:44
 Operator : UA
 Sample : PB111335BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 21 06:19:43 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072118.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 21 01:18:58 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.640	11.059	98935028	87653548	533.199	481.944
Target Compounds							
3) T	4-Nitroph...	0.000	10.215	0	6494403	N.D.	63.709 #
5) T	DICAMBA	0.000	11.303	0	6943989	N.D.	10.132 #
6) T	MCP	12.332	0.000	10261221	0	20.416	N.D. #
7) T	MCPA	12.472	0.000	5631715	0	7.141	N.D. #
10) T	Pentachlo...	0.000	13.421	0	2779916	N.D.	1.010 #
12) T	2,4,5-T	0.000	14.682	0	3744229	N.D.	4.053 #
13) T	2,4-DB	0.000	15.277	0	4774809	N.D.	35.857 #
14) T	DINOSEB	0.000	15.755	0	12901324	N.D.	18.150 #
15) T	Picloram	17.174	0.000	7097165	0	4.490	N.D. #
16) T	DCPA	0.000	16.999	0	29580064	N.D.	20.481 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072118\
Data File : PS001181.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jul 2018 02:44
Operator : UA
Sample : PB111335BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 21 06:19:43 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072118.M
Quant Title : 8080.M
QLast Update : Sat Jul 21 01:18:58 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

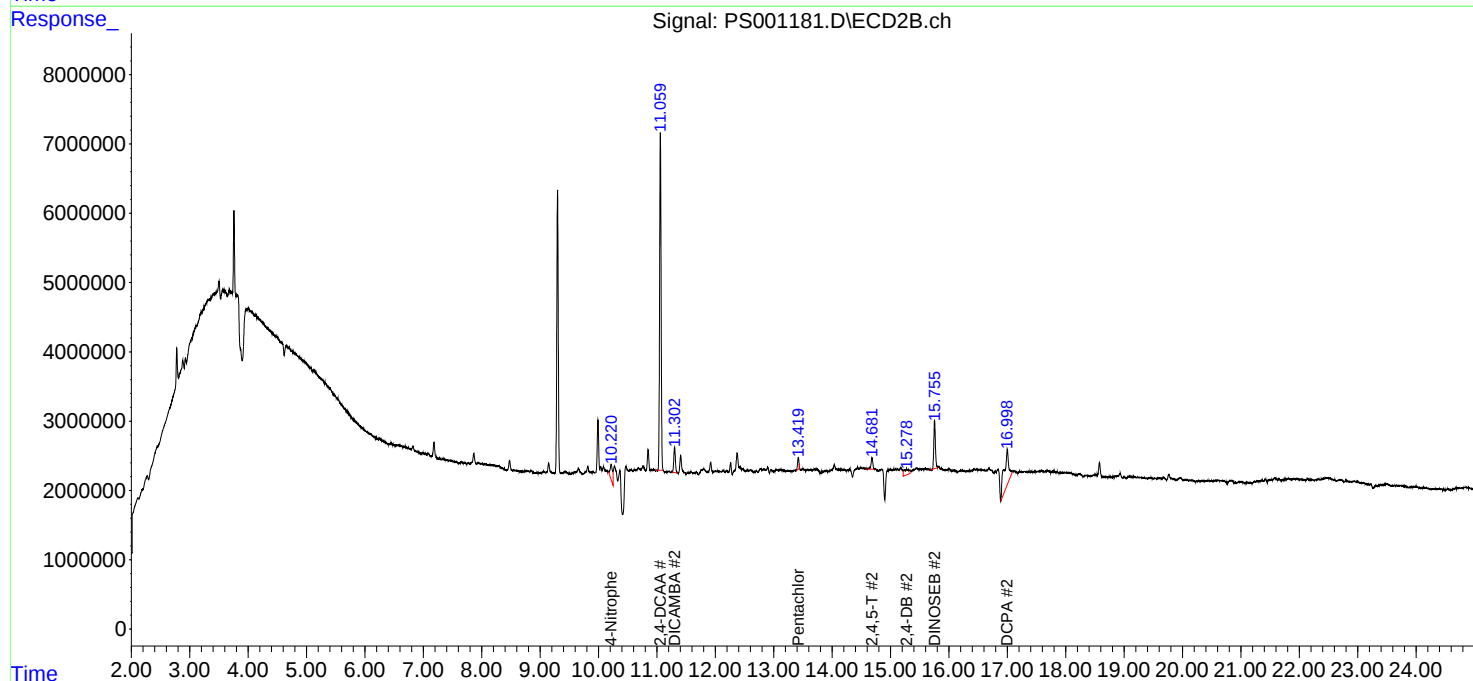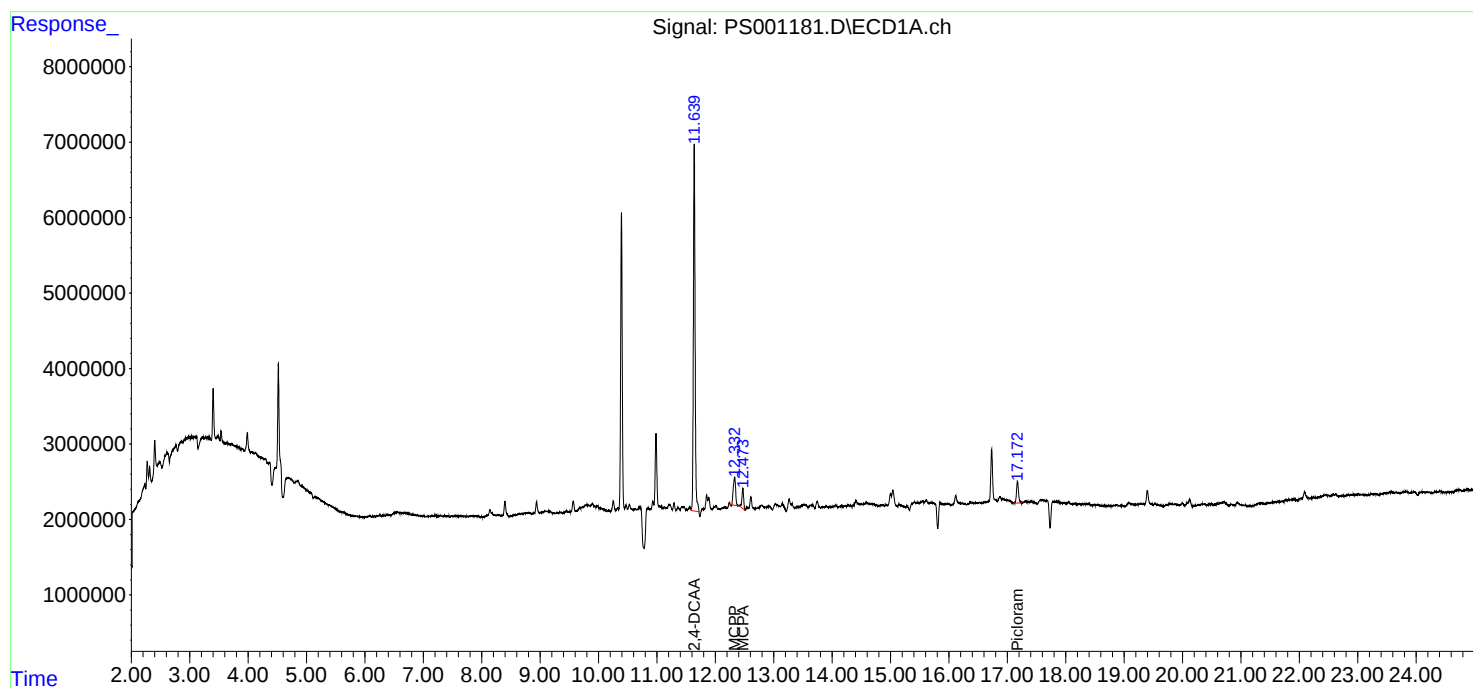


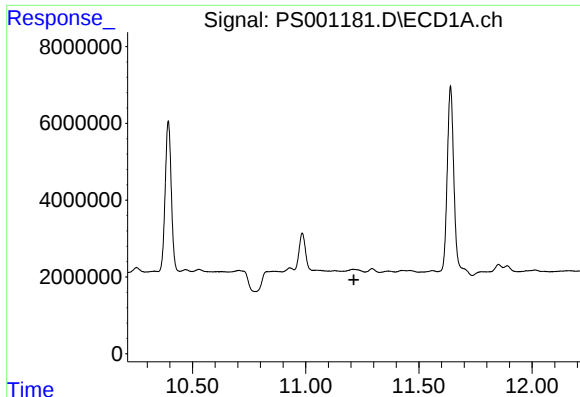

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 11.213 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

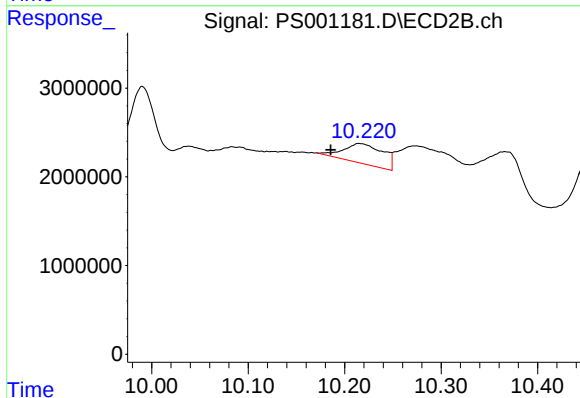


#3 4-Nitrophenol

R.T.: 10.215 min
Delta R.T.: 0.029 min
Response: 6494403
Conc: 63.71 ng/ml

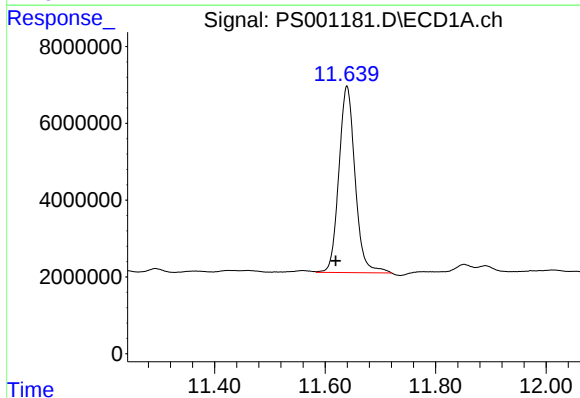


#4 2,4-DCAA

R.T.: 11.640 min
Delta R.T.: 0.020 min
Response: 98935028
Conc: 533.20 ng/ml

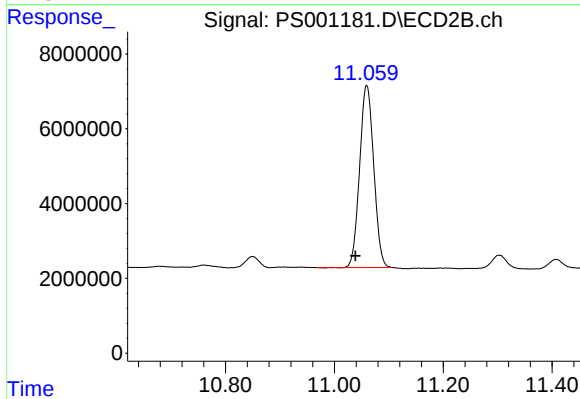

#4 2,4-DCAA


R.T.: 11.059 min
Delta R.T.: 0.021 min
Response: 87653548
Conc: 481.94 ng/ml

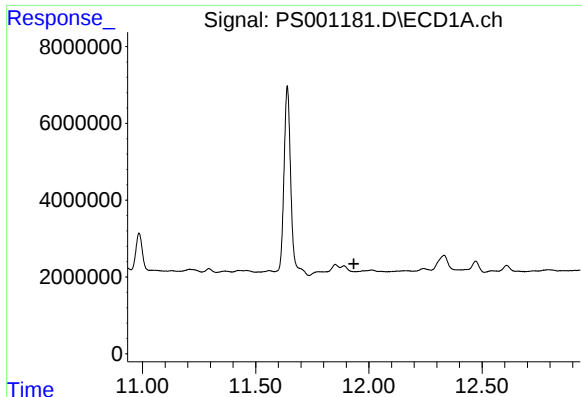

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.934 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

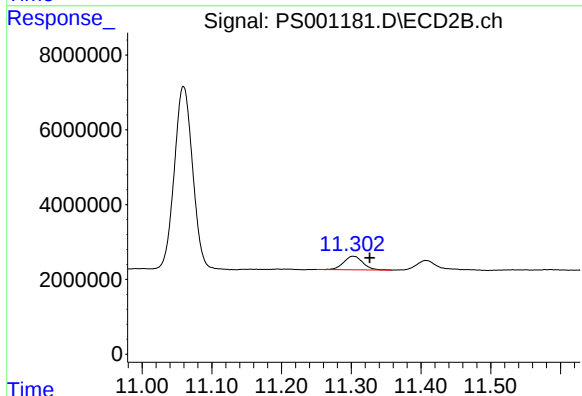


#5 DICAMBA

R.T.: 11.303 min
Delta R.T.: -0.024 min
Response: 6943989
Conc: 10.13 ng/ml

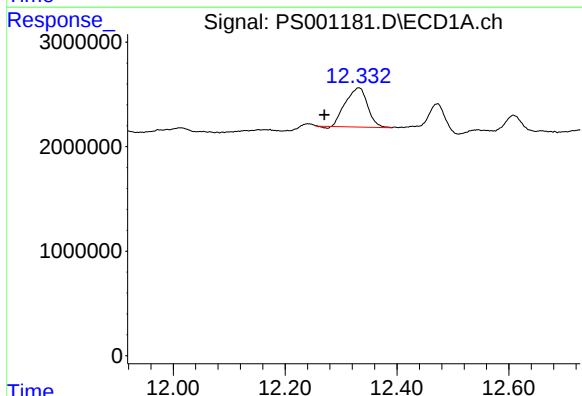


#6 MCP

R.T.: 12.332 min
Delta R.T.: 0.061 min
Response: 10261221
Conc: 20.42 ug/ml

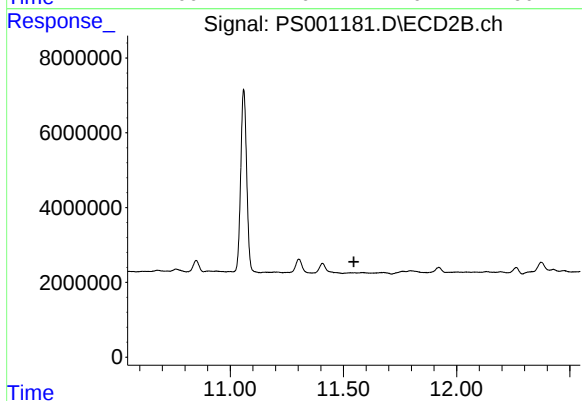

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.546 min
Response: 0
Conc: N.D.

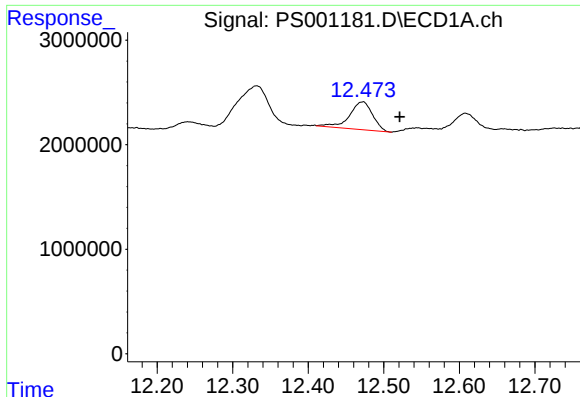

#7 MCPA


R.T.: 12.472 min
Delta R.T.: -0.050 min
Response: 5631715
Conc: 7.14 ug/ml

Instrument :
ECD_S
ClientSampleId :

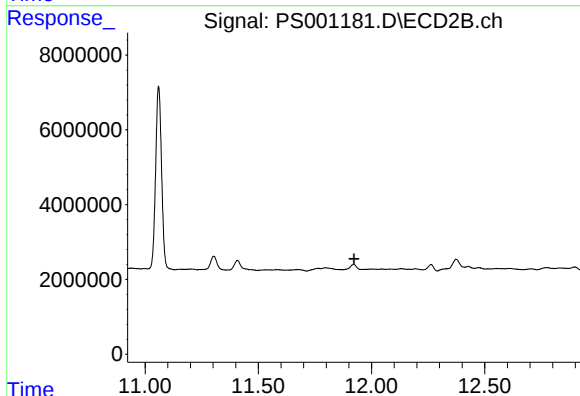


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 11.922 min
Response: 0
Conc: N.D.

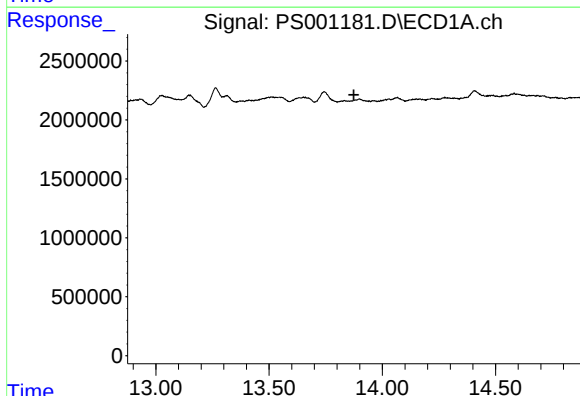


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 13.874 min
Response: 0
Conc: N.D.

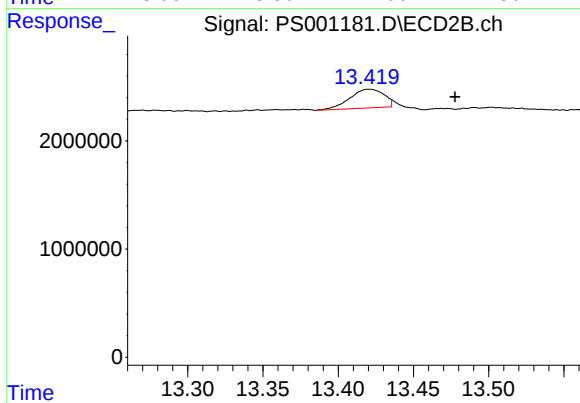

#10 Pentachlorophenol


R.T.: 13.421 min
Delta R.T.: -0.057 min
Response: 2779916
Conc: 1.01 ng/ml

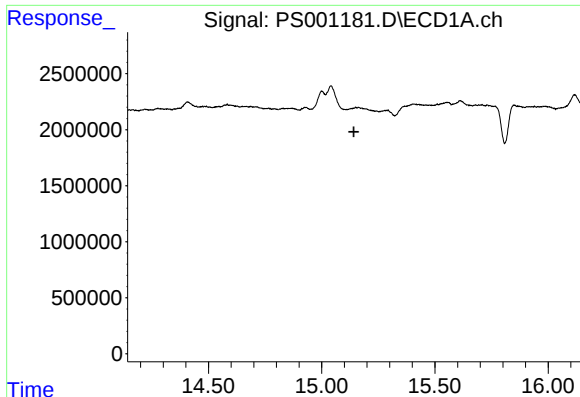

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 15.142 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

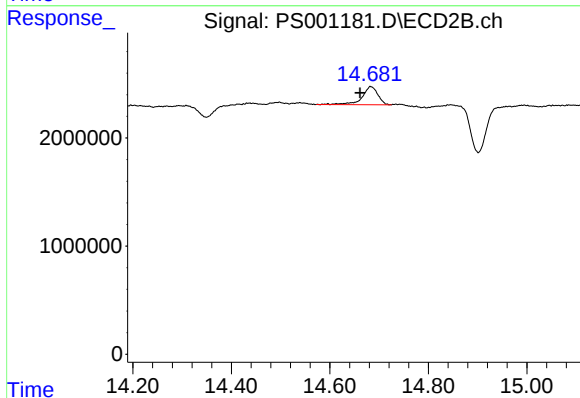


#12 2,4,5-T

R.T.: 14.682 min
Delta R.T.: 0.021 min
Response: 3744229
Conc: 4.05 ng/ml

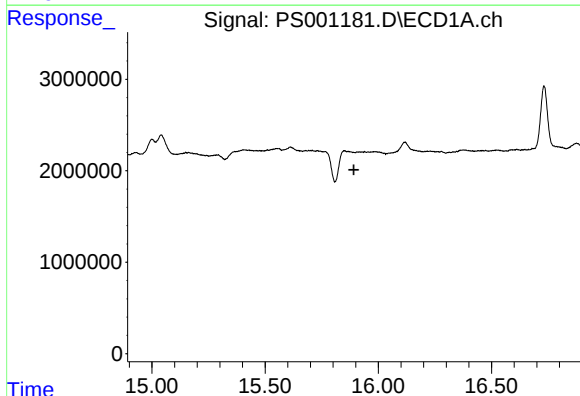


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 15.892 min
Response: 0
Conc: N.D.

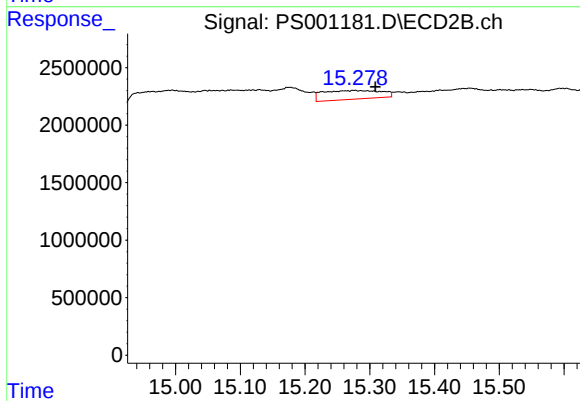

#13 2,4-DB


R.T.: 15.277 min
Delta R.T.: -0.031 min
Response: 4774809
Conc: 35.86 ng/ml

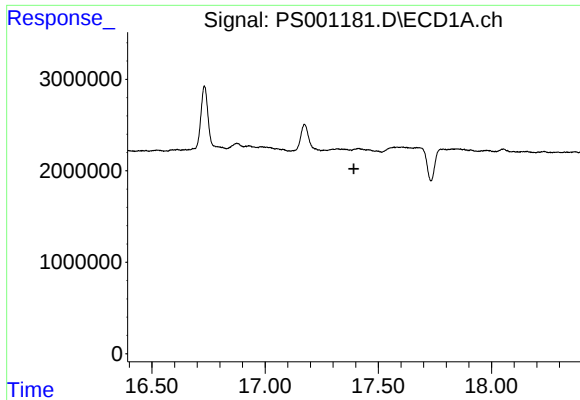

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 17.392 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

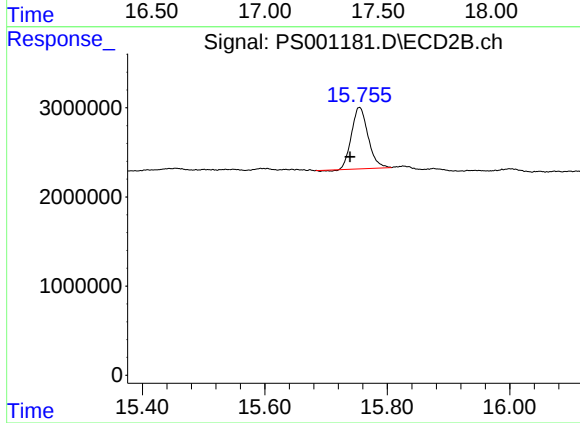


#14 DINOSEB

R.T.: 15.755 min
Delta R.T.: 0.015 min
Response: 12901324
Conc: 18.15 ng/ml

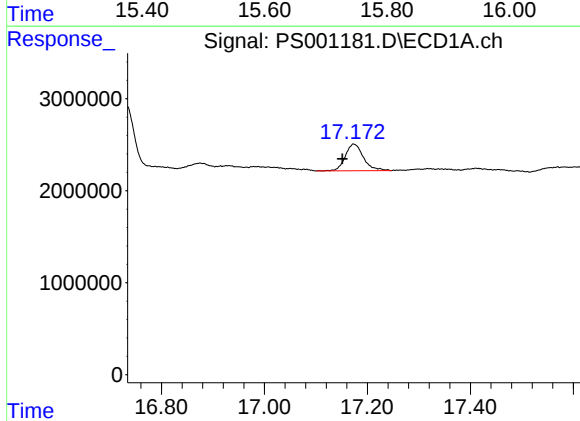


#15 Picloram

R.T.: 17.174 min
Delta R.T.: 0.022 min
Response: 7097165
Conc: 4.49 ng/ml

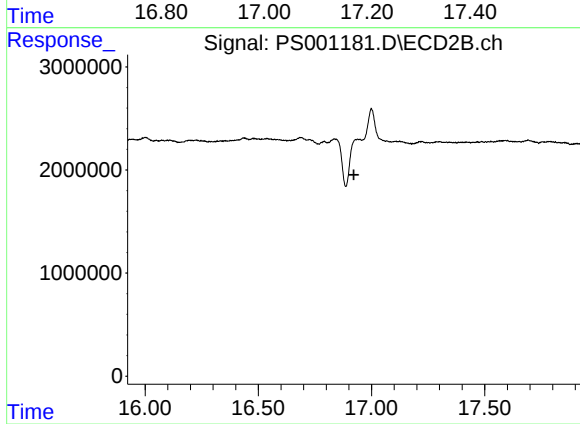

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 16.922 min
Response: 0
Conc: N.D.

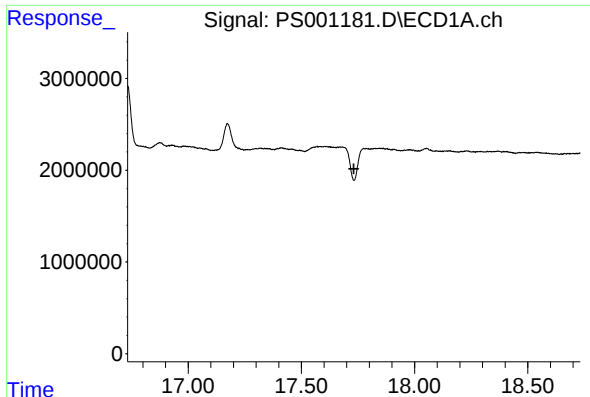

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.732 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

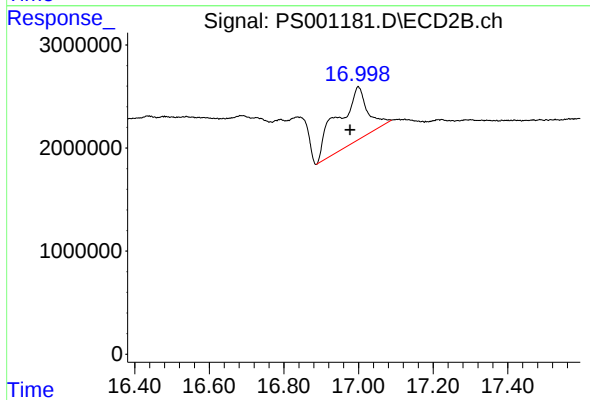

#16 DCPA

R.T.: 16.999 min
Delta R.T.: 0.021 min
Response: 29580064
Conc: 20.48 ng/ml