

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072118\
 Data File : PS001185.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2018 04:47
 Operator : UA
 Sample : J3827-04
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 21 06:21:17 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072118.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 21 01:18:58 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.617	11.037	86734781	75828342	467.447	416.926
Target Compounds							
3) T	4-Nitroph...	11.270	10.193	1764871	5678417	15.335	55.704 #
5) T	DICAMBA	0.000	11.282	0	8096453	N.D.	11.813 #
6) T	MCP	12.307	0.000	12531339	0	24.933	N.D. #
8) T	DICHLORPROP	0.000	12.403	0	1549921	N.D.	8.749 #
15) T	Picloram	0.000	16.930	0	587370	N.D.	0.426 #
16) T	DCPA	0.000	16.930	0	587370	N.D.	0.407 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072118\
Data File : PS001185.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jul 2018 04:47
Operator : UA
Sample : J3827-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 21 06:21:17 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072118.M
Quant Title : 8080.M
QLast Update : Sat Jul 21 01:18:58 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

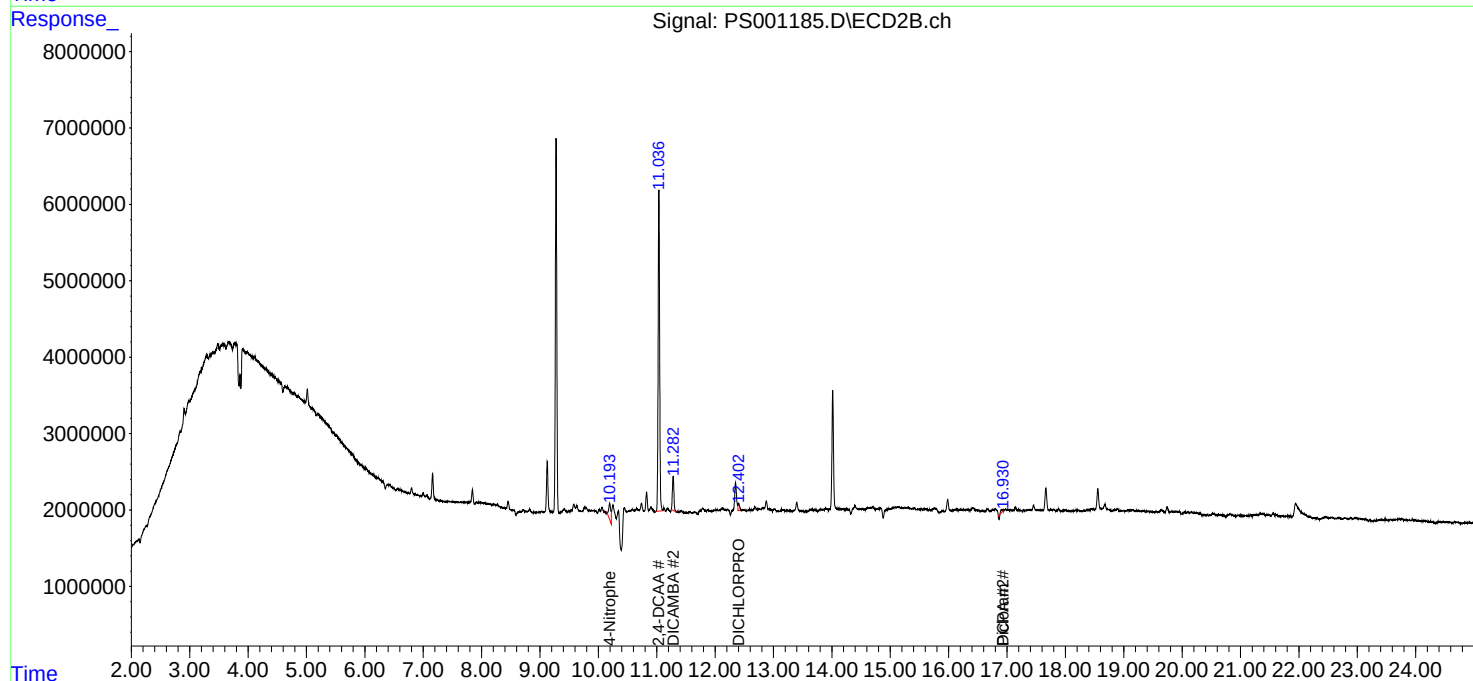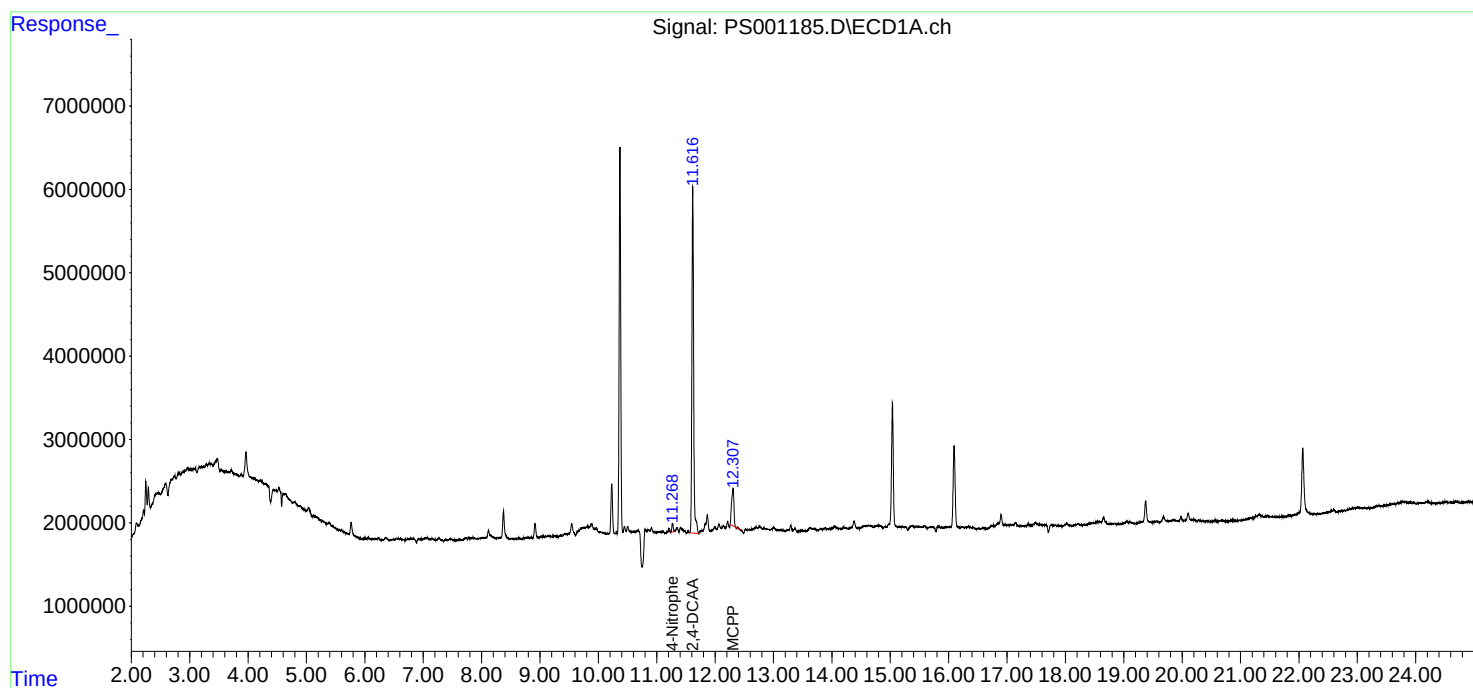


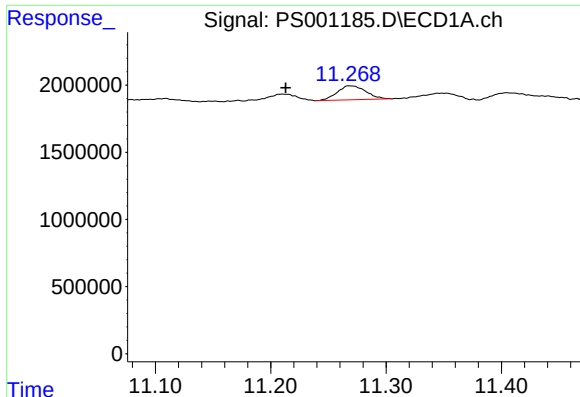

#3 4-Nitrophenol


R.T.: 11.270 min
Delta R.T.: 0.057 min
Response: 1764871
Conc: 15.33 ng/ml

Instrument :
ECD_S
ClientSampleId :

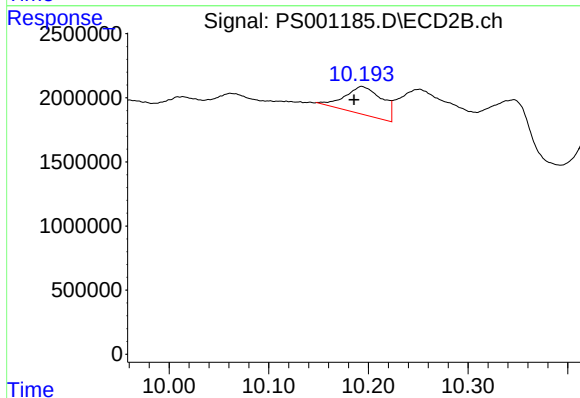


#3 4-Nitrophenol

R.T.: 10.193 min
Delta R.T.: 0.008 min
Response: 5678417
Conc: 55.70 ng/ml

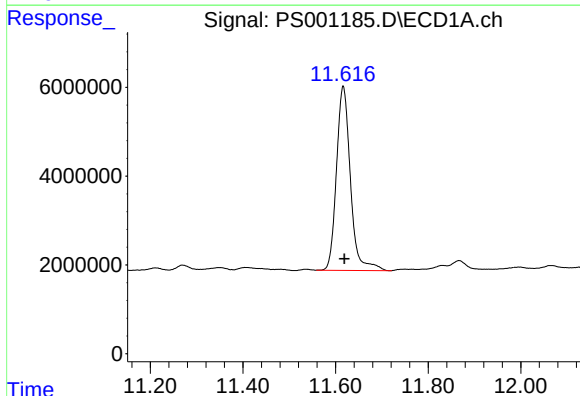


#4 2,4-DCAA

R.T.: 11.617 min
Delta R.T.: -0.003 min
Response: 86734781
Conc: 467.45 ng/ml

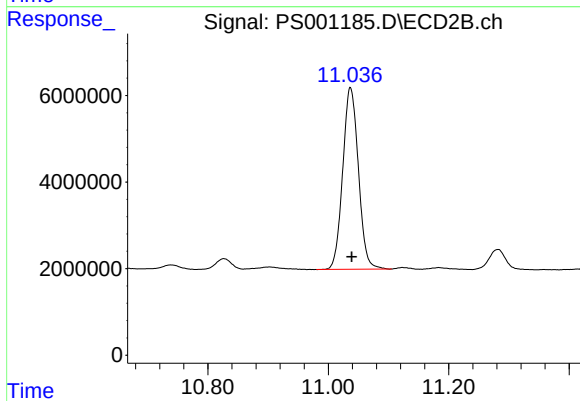

#4 2,4-DCAA


R.T.: 11.037 min
Delta R.T.: -0.002 min
Response: 75828342
Conc: 416.93 ng/ml

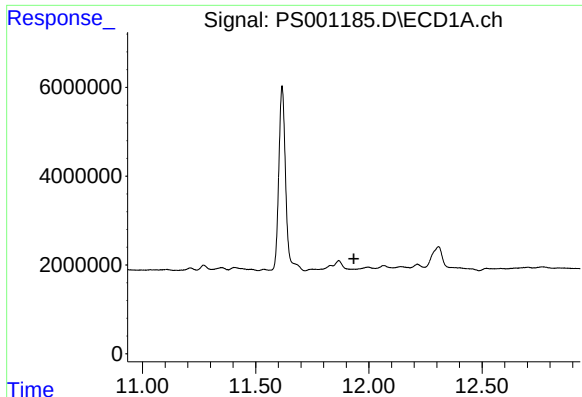

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.934 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

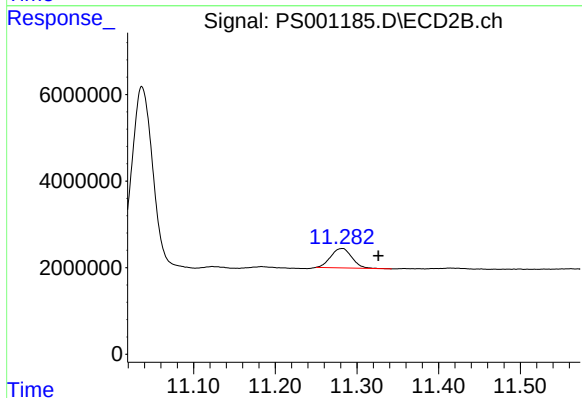


#5 DICAMBA

R.T.: 11.282 min
Delta R.T.: -0.044 min
Response: 8096453
Conc: 11.81 ng/ml

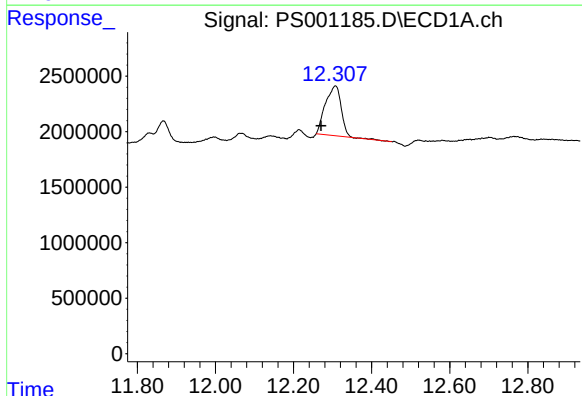


#6 MCP

R.T.: 12.307 min
Delta R.T.: 0.037 min
Response: 12531339
Conc: 24.93 ug/ml

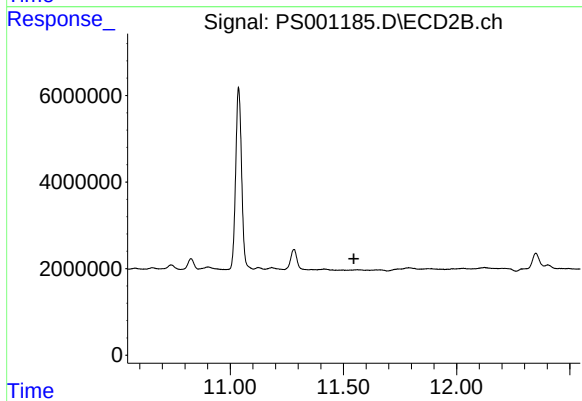

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.546 min
Response: 0
Conc: N.D.

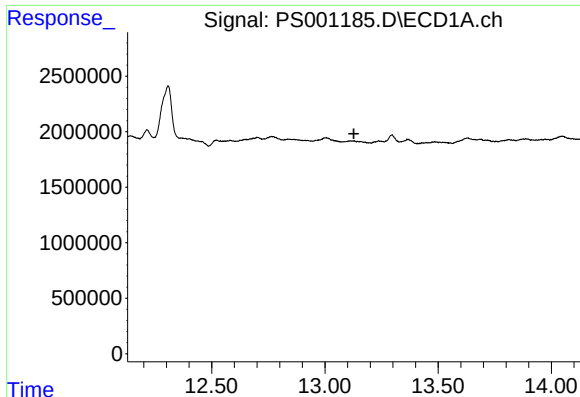

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 13.128 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

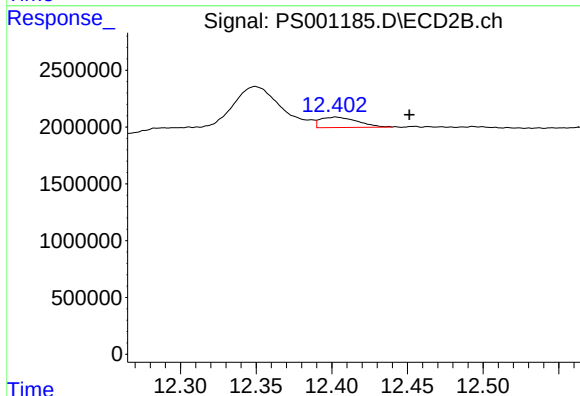


#8 DICHLORPROP

R.T.: 12.403 min
Delta R.T.: -0.048 min
Response: 1549921
Conc: 8.75 ng/ml

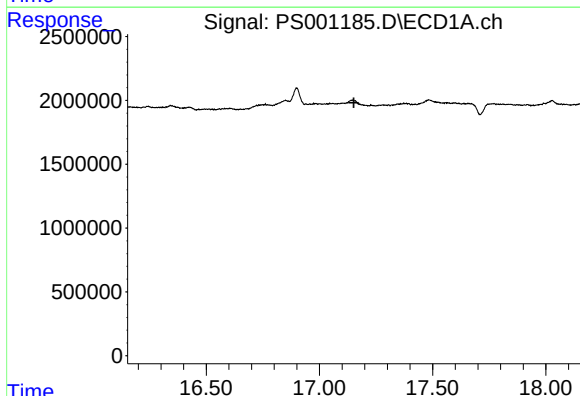


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 17.152 min
Response: 0
Conc: N.D.

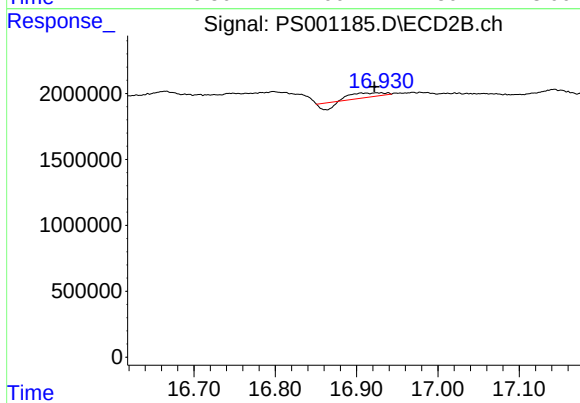

#15 Picloram


R.T.: 16.930 min
Delta R.T.: 0.008 min
Response: 587370
Conc: 0.43 ng/ml

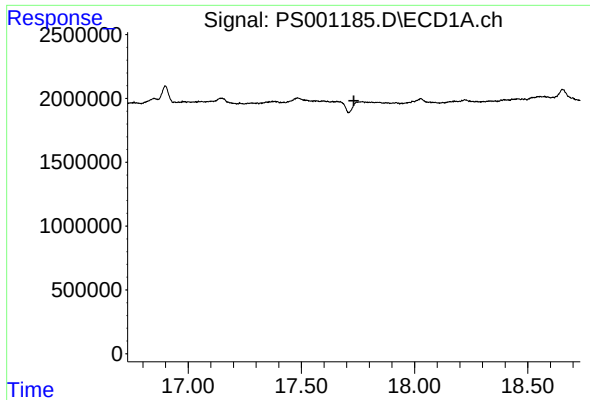

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.732 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

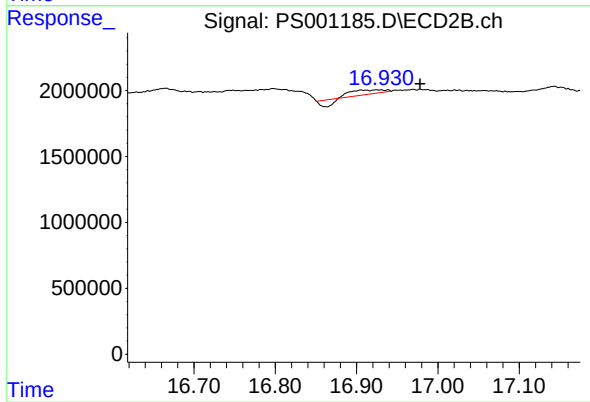

#16 DCPA

R.T.: 16.930 min
Delta R.T.: -0.047 min
Response: 587370
Conc: 0.41 ng/ml