

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072118\
 Data File : PS001188.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2018 06:20
 Operator : UA
 Sample : J4062-18
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 00:44:12 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072118.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 21 01:18:58 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.641	11.061	92396986	80662487	497.963	443.505
Target Compounds							
2) T	3,5-DICHL...	0.000	9.148	0	4028805	N.D.	15.815 #
5) T	DICAMBA	0.000	11.305	0	7034665	N.D.	10.264 #
6) T	MCP	12.331	0.000	10351835	0	20.596	N.D. #
11) T	2,4,5-TP ...	0.000	14.039	0	1156436	N.D.	1.058 #
16) T	DCPA	0.000	16.999	0	4195079	N.D.	2.905 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072118\
Data File : PS001188.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jul 2018 06:20
Operator : UA
Sample : J4062-18
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 23 00:44:12 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072118.M
Quant Title : 8080.M
QLast Update : Sat Jul 21 01:18:58 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

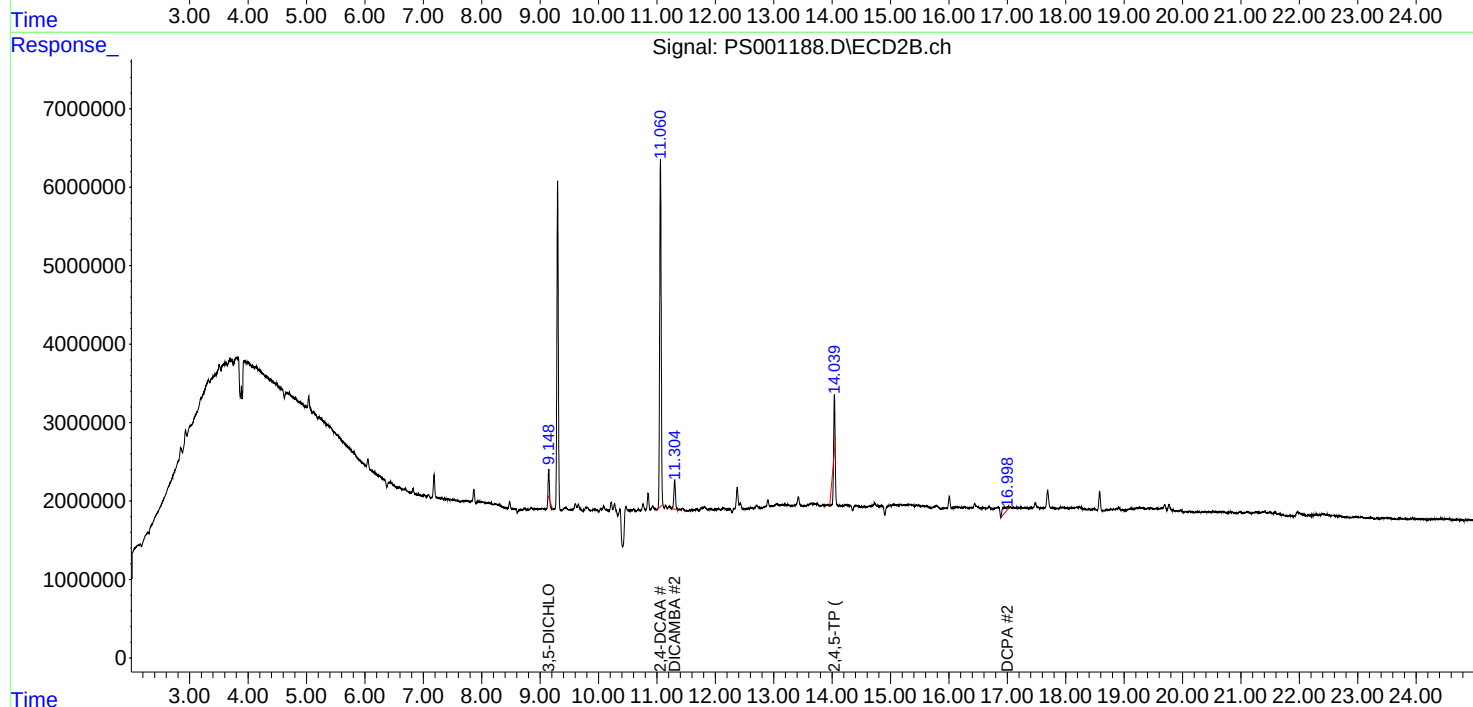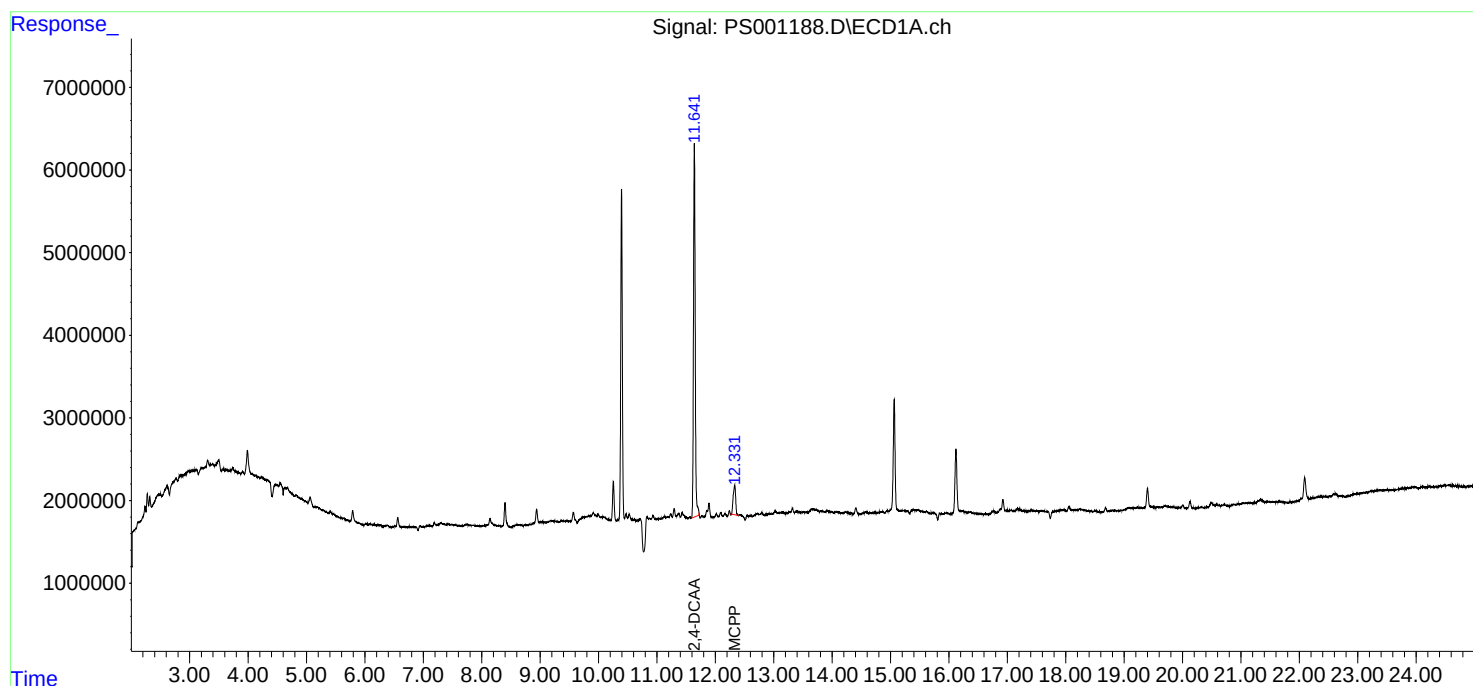


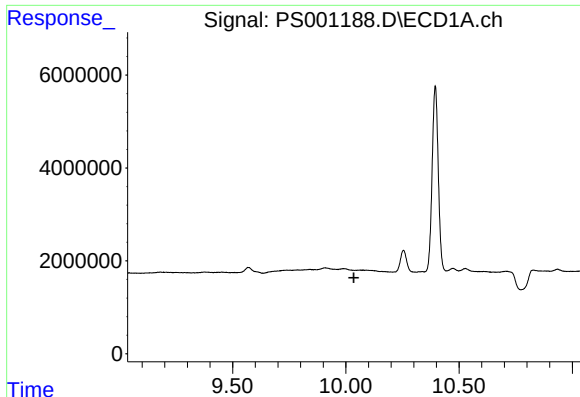

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 10.035 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

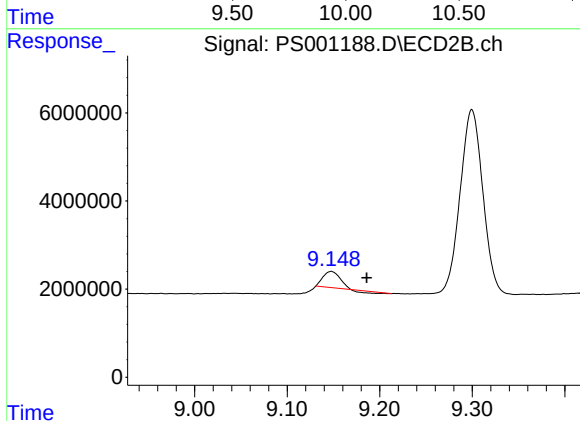


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.148 min
Delta R.T.: -0.038 min
Response: 4028805
Conc: 15.81 ng/ml

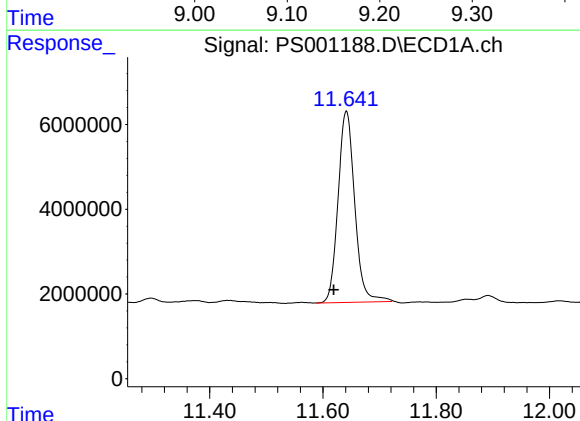


#4 2,4-DCAA

R.T.: 11.641 min
Delta R.T.: 0.022 min
Response: 92396986
Conc: 497.96 ng/ml

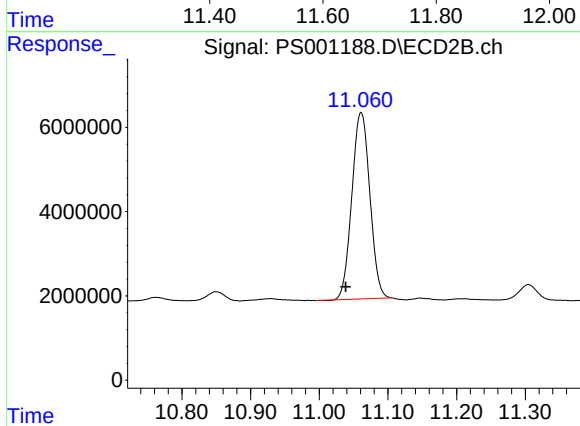

#4 2,4-DCAA


R.T.: 11.061 min
Delta R.T.: 0.022 min
Response: 80662487
Conc: 443.51 ng/ml

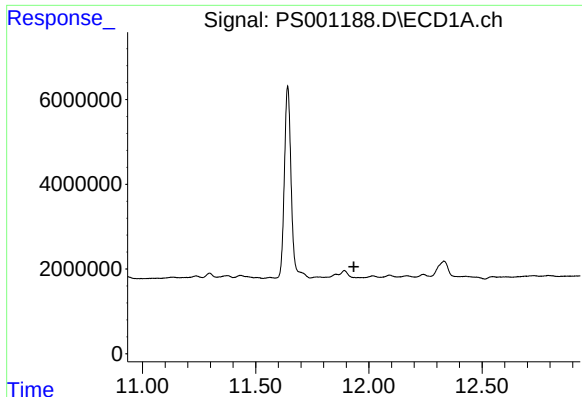

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.934 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

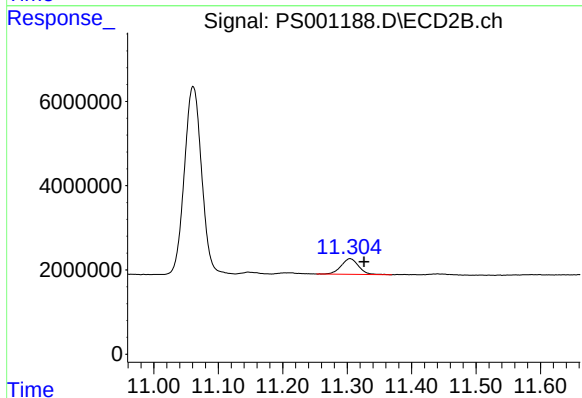


#5 DICAMBA

R.T.: 11.305 min
Delta R.T.: -0.022 min
Response: 7034665
Conc: 10.26 ng/ml

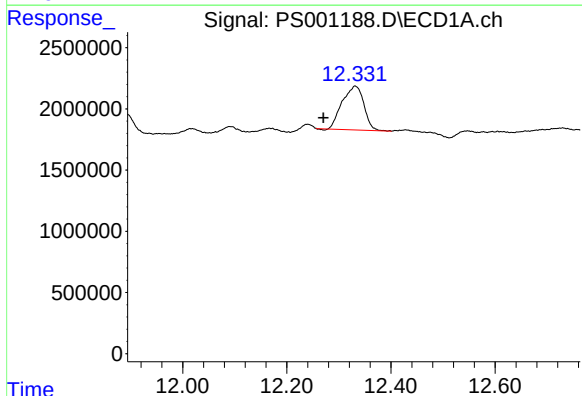


#6 MCP

R.T.: 12.331 min
Delta R.T.: 0.061 min
Response: 10351835
Conc: 20.60 ug/ml

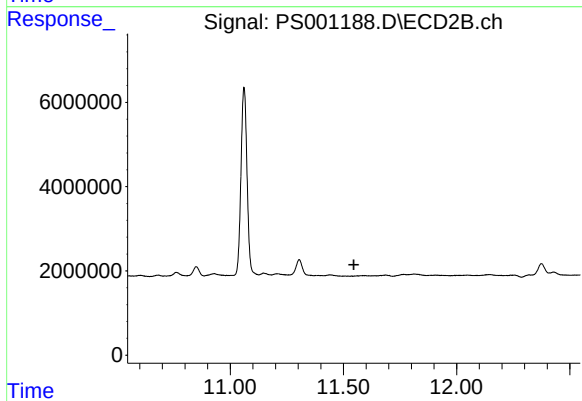

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.546 min
Response: 0
Conc: N.D.

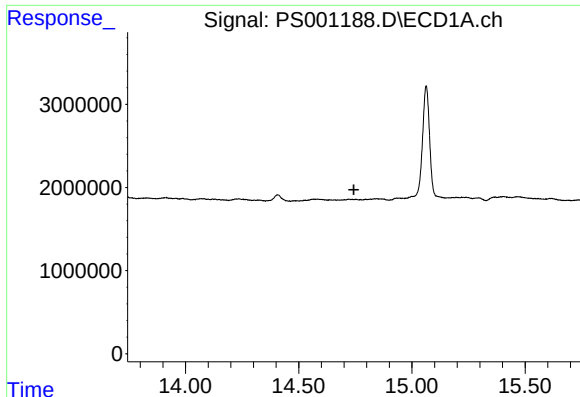

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T. : 14.743 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

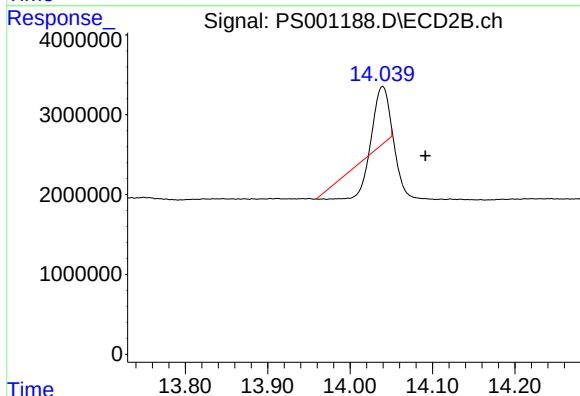


#11 2,4,5-TP (SILVEX)

R.T.: 14.039 min
Delta R.T.: -0.052 min
Response: 1156436
Conc: 1.06 ng/ml

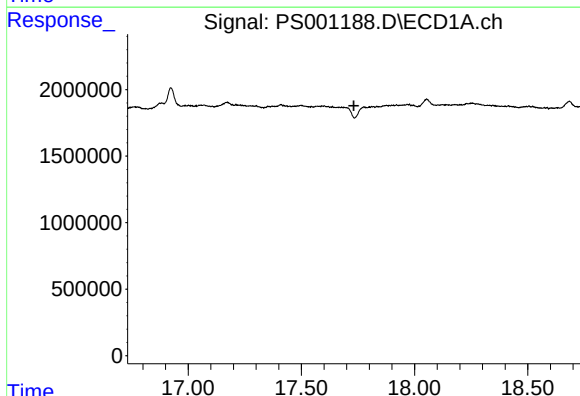

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.732 min
Response: 0
Conc: N.D.

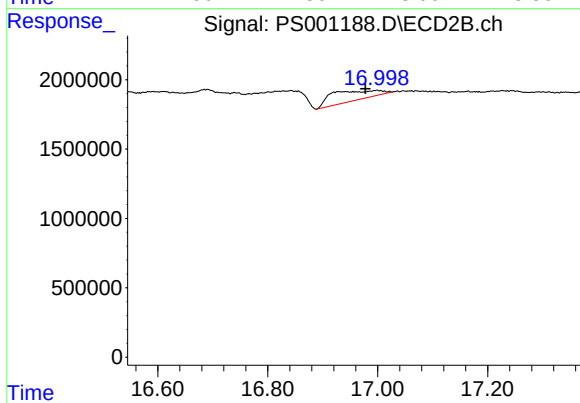

#16 DCPA

R.T.: 16.999 min
Delta R.T.: 0.021 min
Response: 4195079
Conc: 2.90 ng/ml