

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072118\
 Data File : PS001191.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2018 07:53
 Operator : UA
 Sample : J4062-24
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 00:45:37 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072118.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 21 01:18:58 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.660	11.079	85327361	63349608	459.862	348.314
Target Compounds							
2) T	3,5-DICHL...	0.000	9.166	0	10489342	N.D.	41.175 #
3) T	4-Nitroph...	0.000	10.236	0	5095534	N.D.	49.986 #
5) T	DICAMBA	0.000	11.323	0	8026679	N.D.	11.711 #
8) T	DICHLORPROP	0.000	12.448	0	1424801	N.D.	8.043 #
9) T	2,4-D	0.000	12.919	0	1841333	N.D.	7.760 #
12) T	2,4,5-T	15.081	0.000	32436227	0	29.150	N.D. #
15) T	Picloram	17.194	0.000	4073771	0	2.577	N.D. #
16) T	DCPA	0.000	17.018	0	5027995	N.D.	3.481 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072118\
Data File : PS001191.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jul 2018 07:53
Operator : UA
Sample : J4062-24
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 23 00:45:37 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072118.M
Quant Title : 8080.M
QLast Update : Sat Jul 21 01:18:58 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

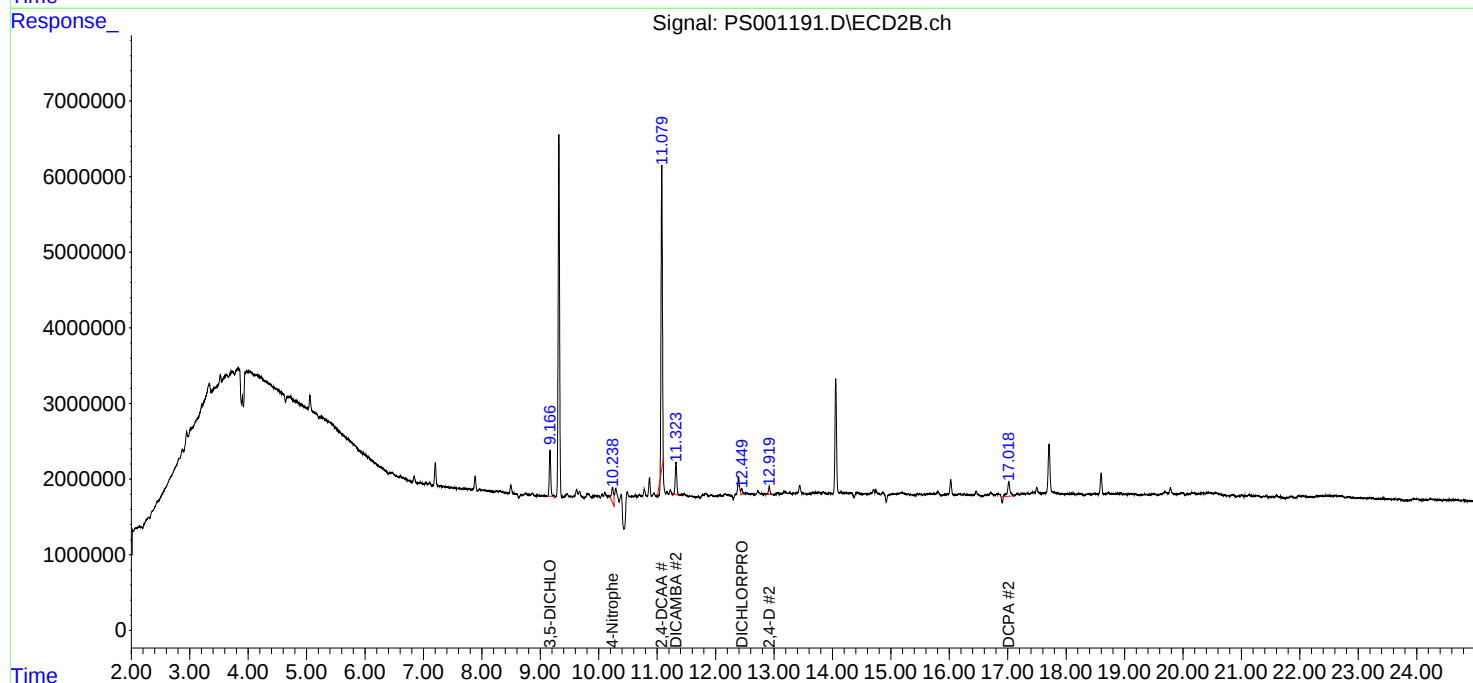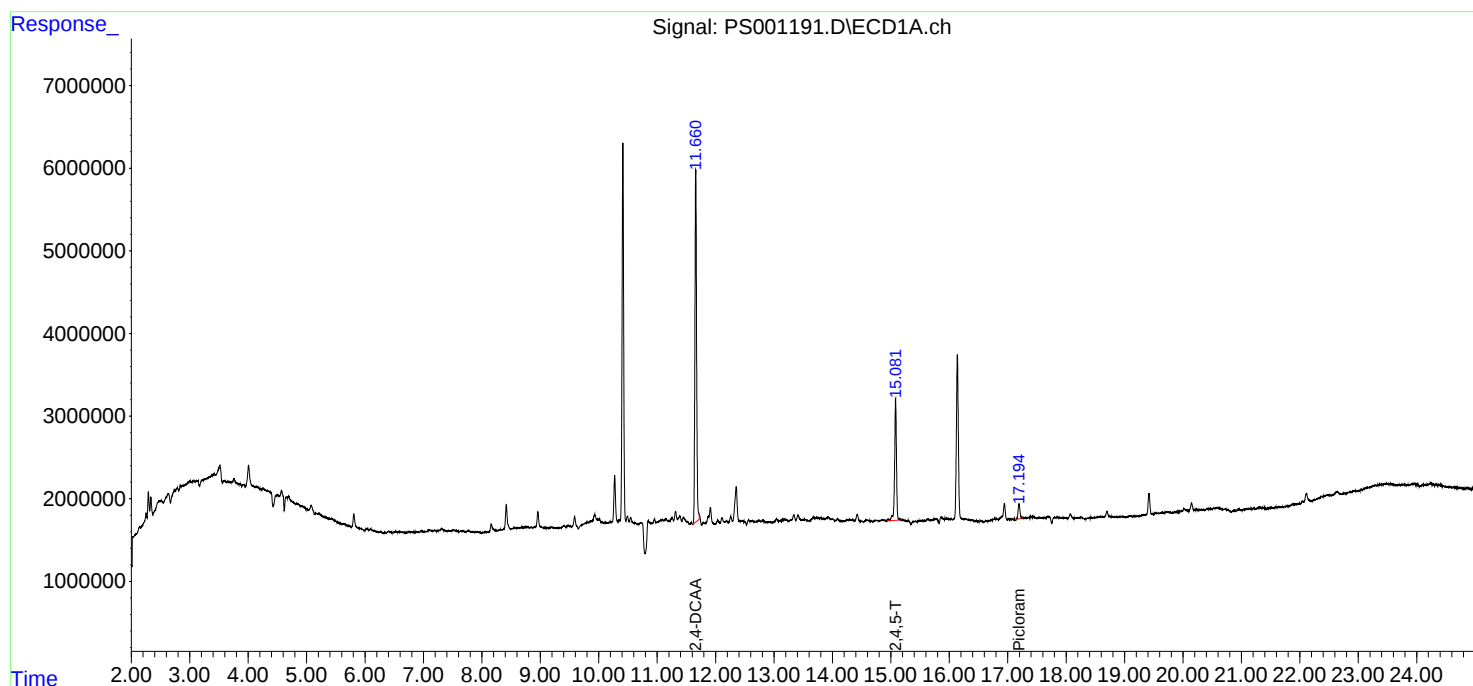


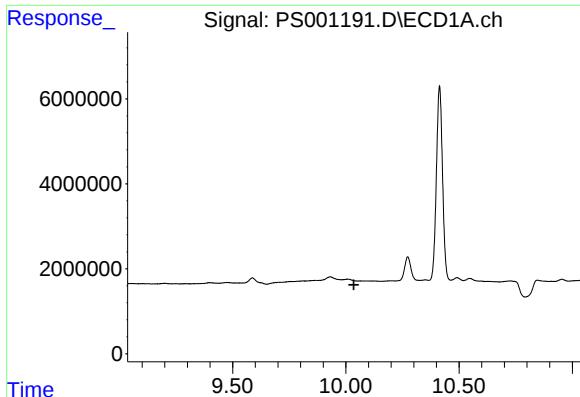

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 10.035 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

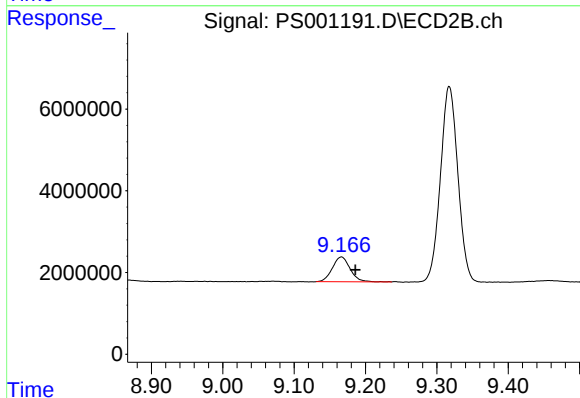


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.166 min
Delta R.T.: -0.020 min
Response: 10489342
Conc: 41.18 ng/ml

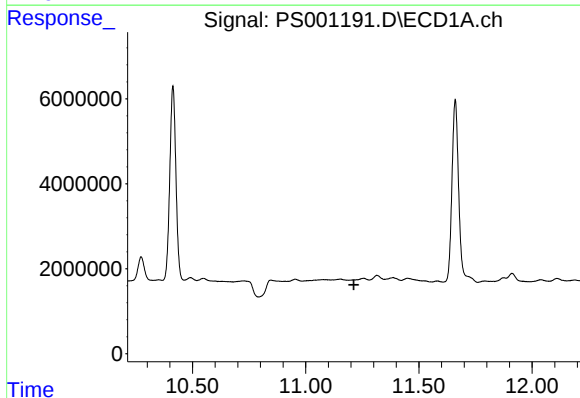


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 11.213 min
Response: 0
Conc: N.D.

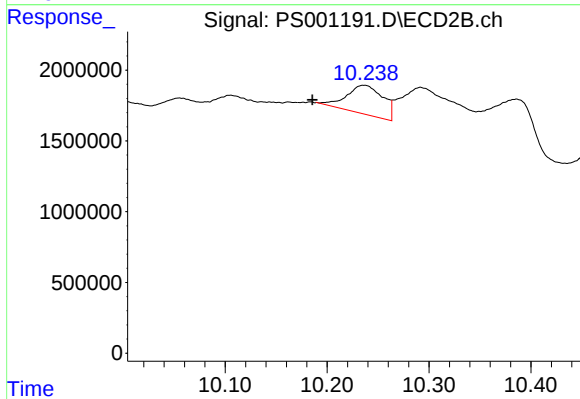

#3 4-Nitrophenol


R.T.: 10.236 min
Delta R.T.: 0.051 min
Response: 5095534
Conc: 49.99 ng/ml

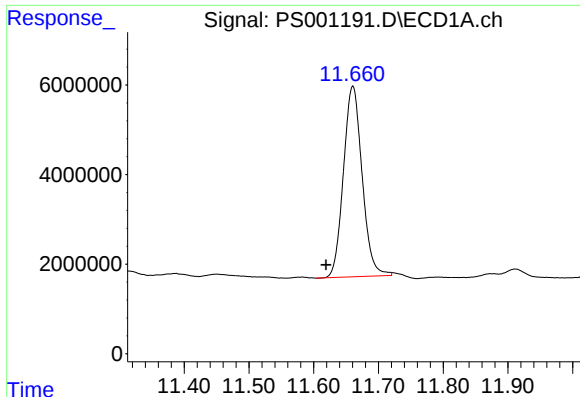

#4 2,4-DCAA


R.T.: 11.660 min
Delta R.T.: 0.041 min
Response: 85327361
Conc: 459.86 ng/ml

Instrument :
ECD_S
ClientSampleId :

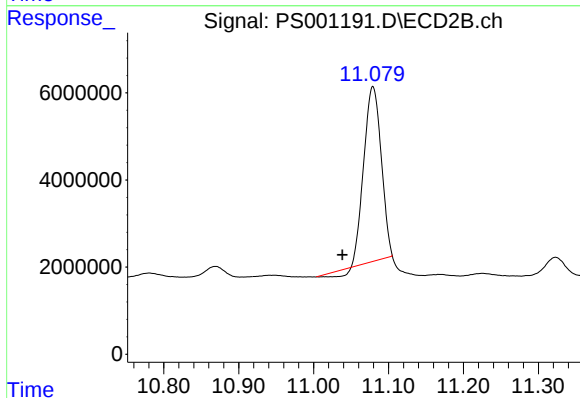


#4 2,4-DCAA

R.T.: 11.079 min
Delta R.T.: 0.040 min
Response: 63349608
Conc: 348.31 ng/ml

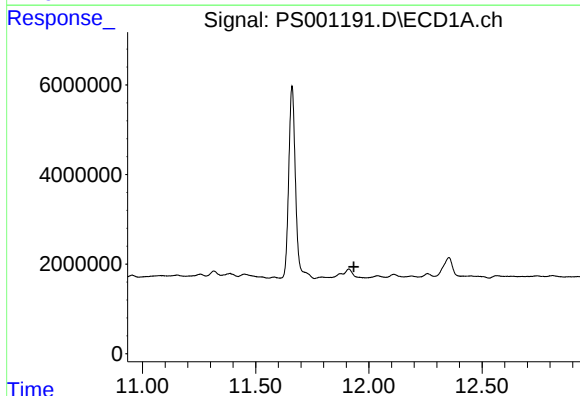


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.934 min
Response: 0
Conc: N.D.

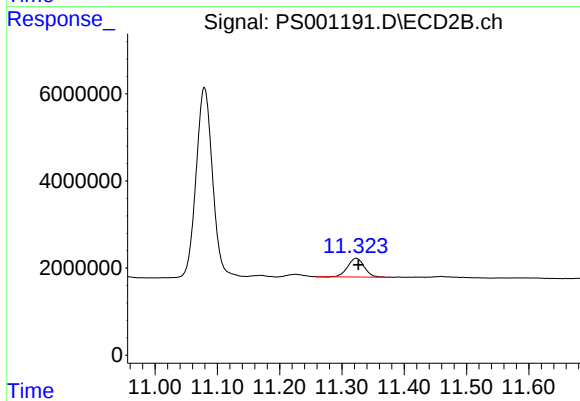

#5 DICAMBA


R.T.: 11.323 min
Delta R.T.: -0.003 min
Response: 8026679
Conc: 11.71 ng/ml

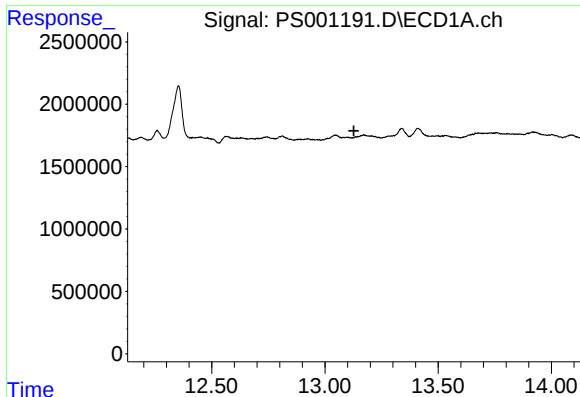

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 13.128 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

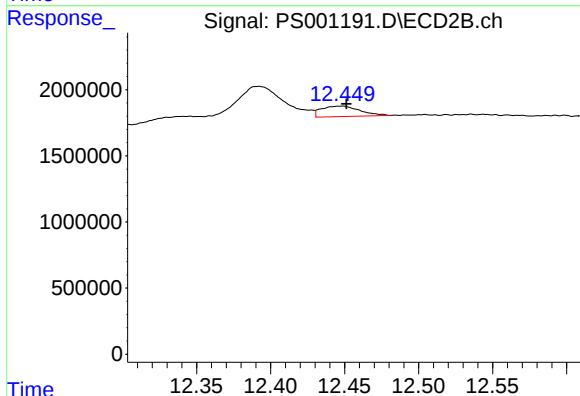


#8 DICHLORPROP

R.T.: 12.448 min
Delta R.T.: -0.003 min
Response: 1424801
Conc: 8.04 ng/ml

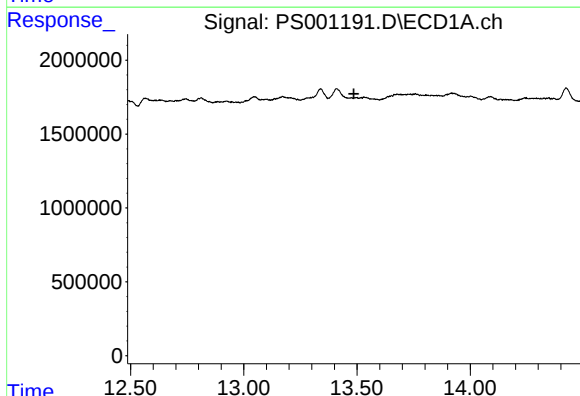


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 13.486 min
Response: 0
Conc: N.D.

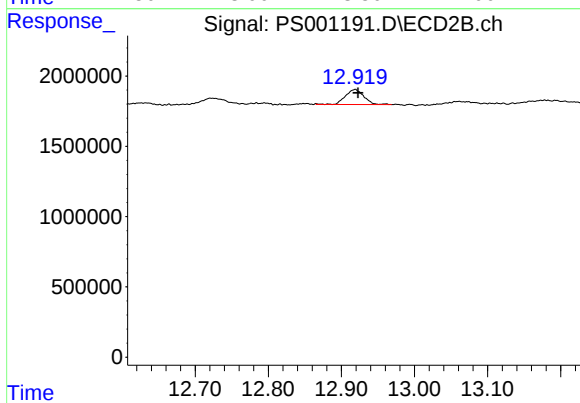

#9 2,4-D


R.T.: 12.919 min
Delta R.T.: -0.004 min
Response: 1841333
Conc: 7.76 ng/ml

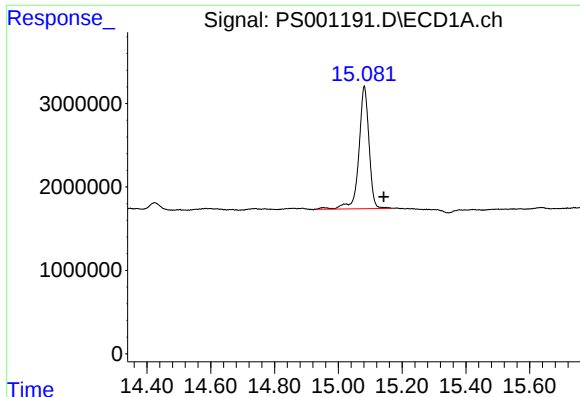

#12 2,4,5-T


R.T.: 15.081 min
Delta R.T.: -0.060 min
Response: 32436227
Conc: 29.15 ng/ml

Instrument :
ECD_S
ClientSampleId :

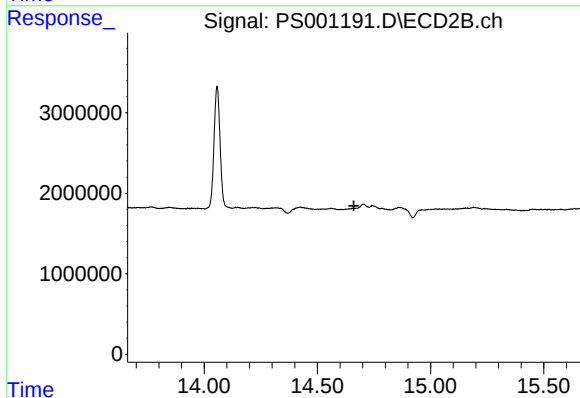


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 14.662 min
Response: 0
Conc: N.D.

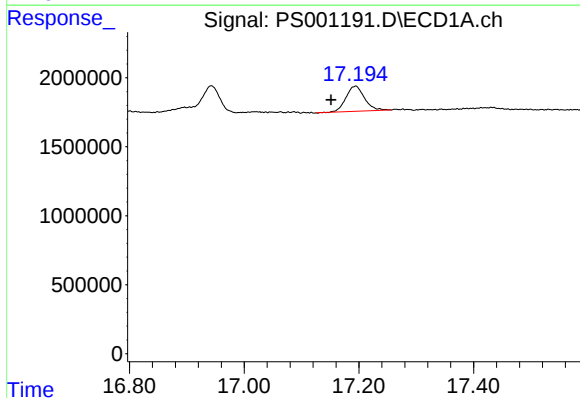


#15 Picloram

R.T.: 17.194 min
Delta R.T.: 0.042 min
Response: 4073771
Conc: 2.58 ng/ml

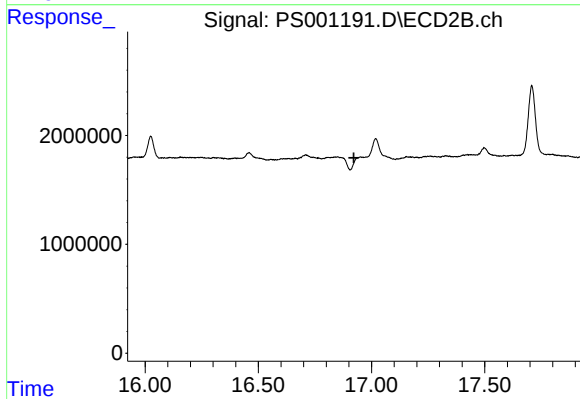

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 16.922 min
Response: 0
Conc: N.D.

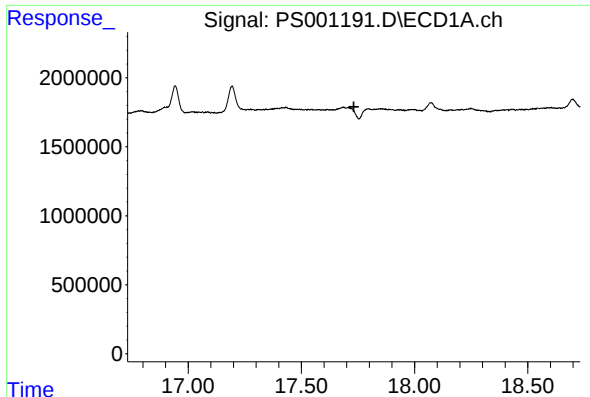

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.732 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

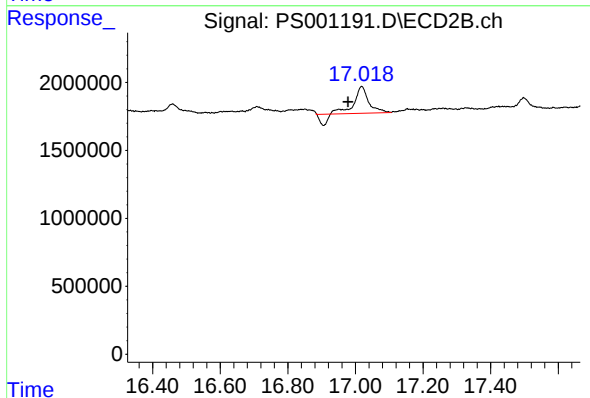

#16 DCPA

R.T.: 17.018 min
Delta R.T.: 0.040 min
Response: 5027995
Conc: 3.48 ng/ml