

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072118\
 Data File : PS001193.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2018 08:55
 Operator : UA
 Sample : J4062-36
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 00:46:20 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072118.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 21 01:18:58 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.654	11.075	88364356	78080149	476.230	429.307
Target Compounds							
2) T	3,5-DICHL...	0.000	9.162	0	9007612	N.D.	35.359 #
3) T	4-Nitroph...	0.000	10.232	0	6423439	N.D.	63.013 #
5) T	DICAMBA	0.000	11.319	0	7412373	N.D.	10.815 #
8) T	DICHLORPROP	0.000	12.443	0	1417607	N.D.	8.002 #
12) T	2,4,5-T	15.077	0.000	29748742	0	26.735	N.D. #
15) T	Picloram	0.000	16.963	0	150729	N.D.	0.109 #
16) T	DCPA	0.000	16.963	0	150729	N.D.	0.104 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072118\
Data File : PS001193.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jul 2018 08:55
Operator : UA
Sample : J4062-36
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 23 00:46:20 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072118.M
Quant Title : 8080.M
QLast Update : Sat Jul 21 01:18:58 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

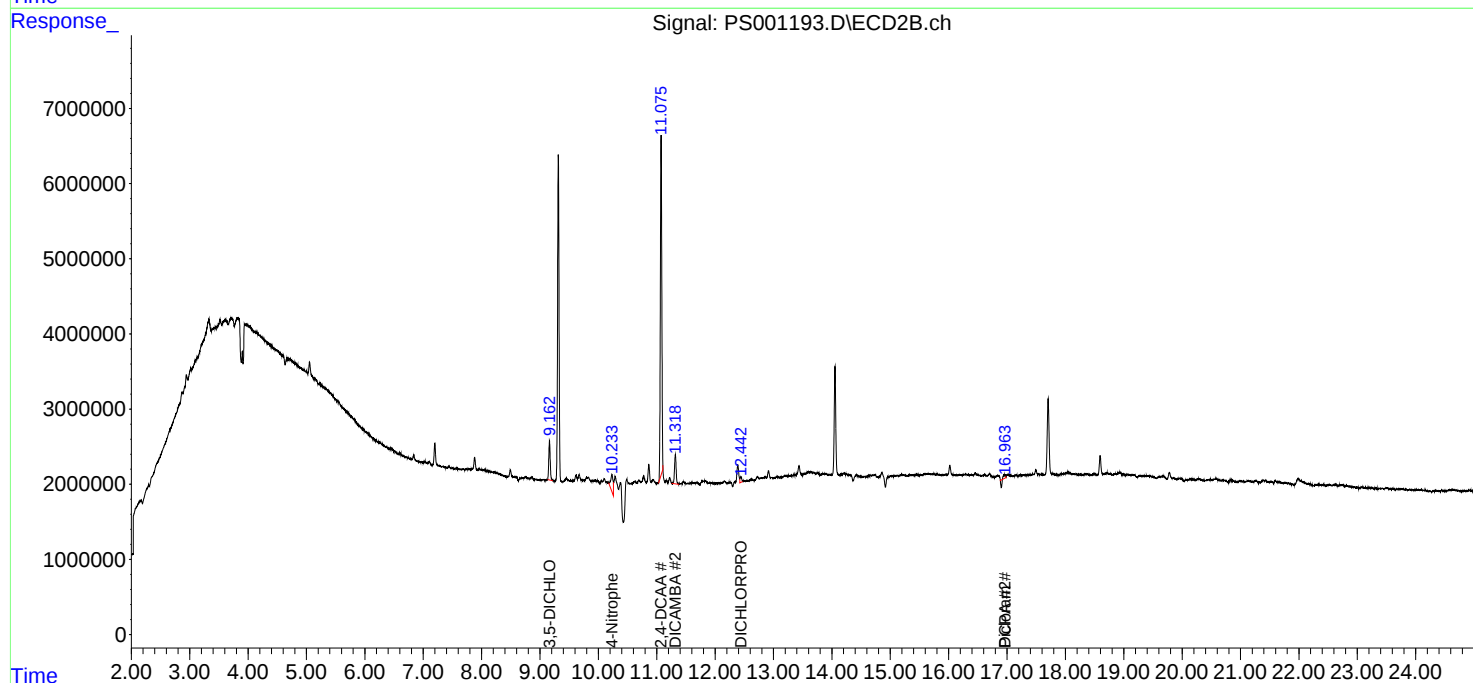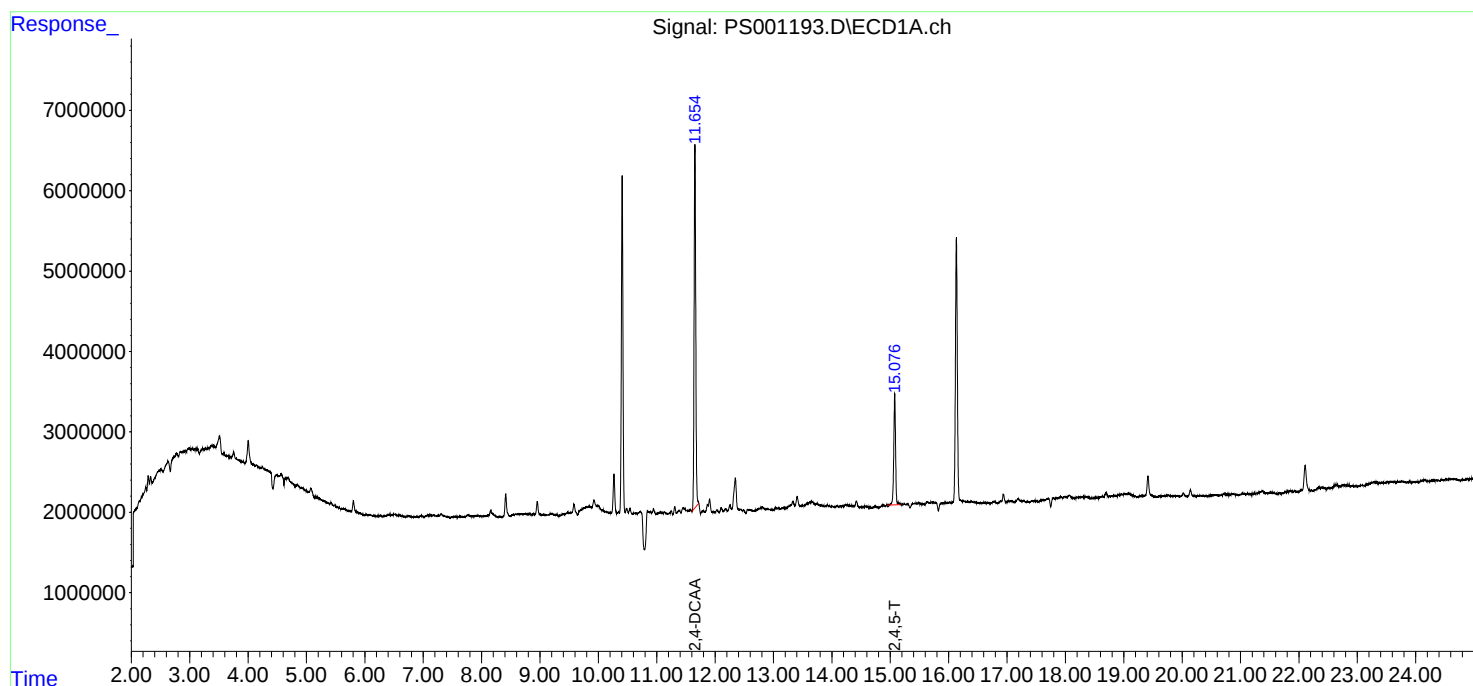


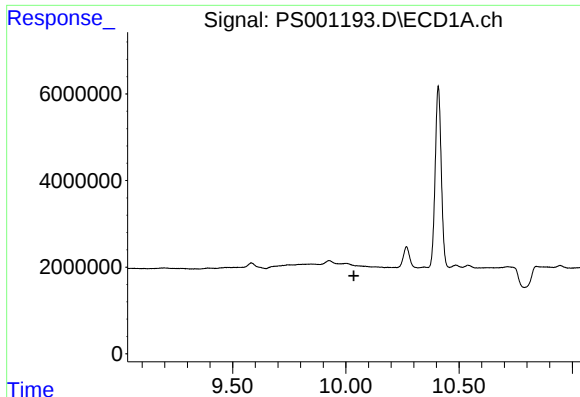

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 10.035 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

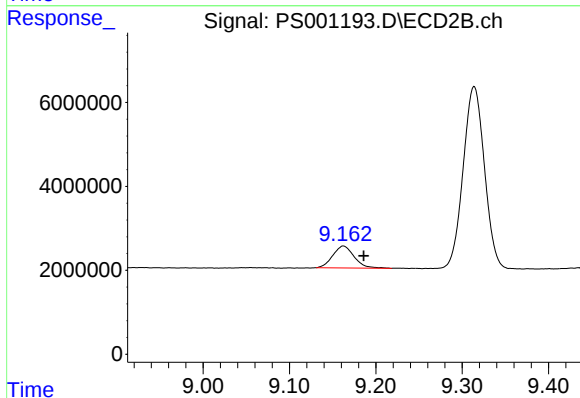


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.162 min
Delta R.T.: -0.024 min
Response: 9007612
Conc: 35.36 ng/ml

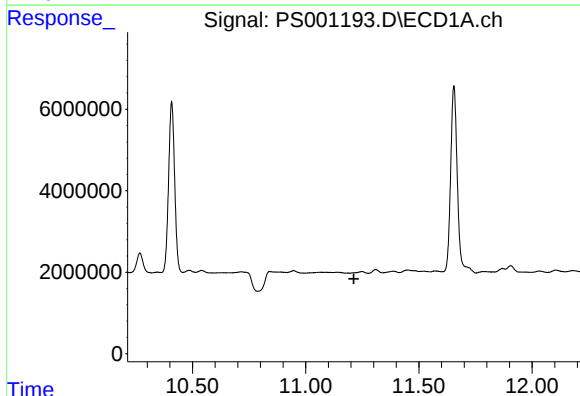


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 11.213 min
Response: 0
Conc: N.D.

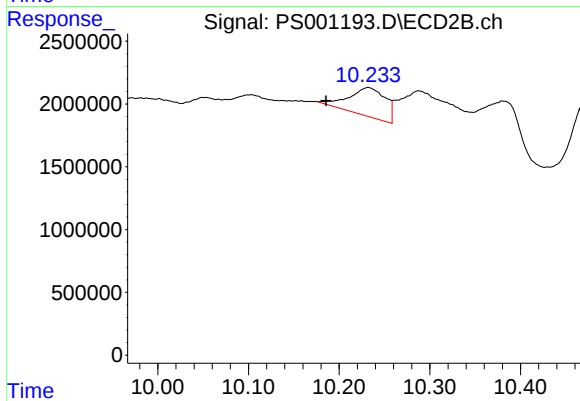

#3 4-Nitrophenol


R.T.: 10.232 min
Delta R.T.: 0.047 min
Response: 6423439
Conc: 63.01 ng/ml

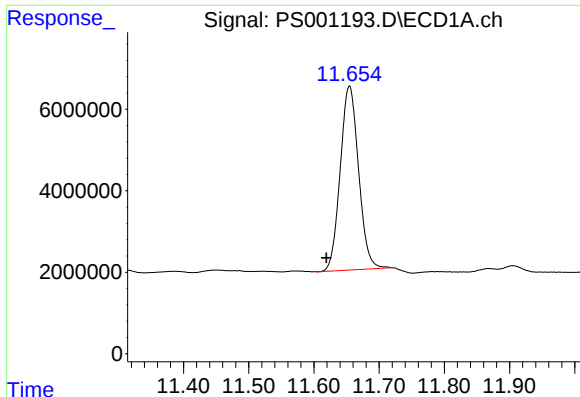

#4 2,4-DCAA


R.T.: 11.654 min
Delta R.T.: 0.035 min
Response: 88364356
Conc: 476.23 ng/ml

Instrument :
ECD_S
ClientSampleId :

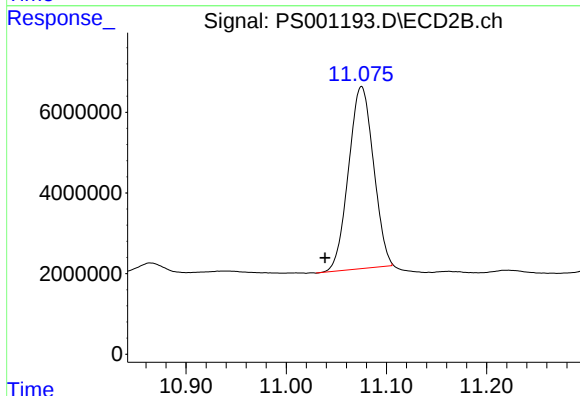


#4 2,4-DCAA

R.T.: 11.075 min
Delta R.T.: 0.036 min
Response: 78080149
Conc: 429.31 ng/ml

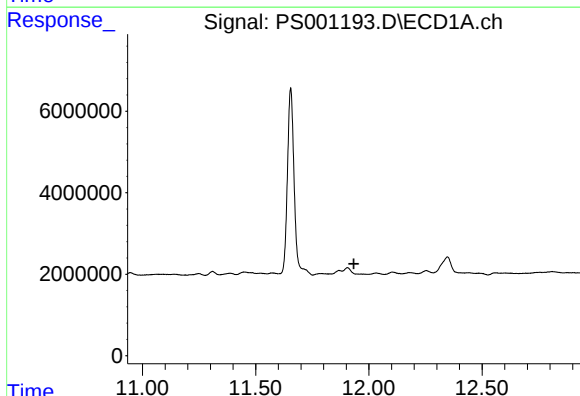


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.934 min
Response: 0
Conc: N.D.

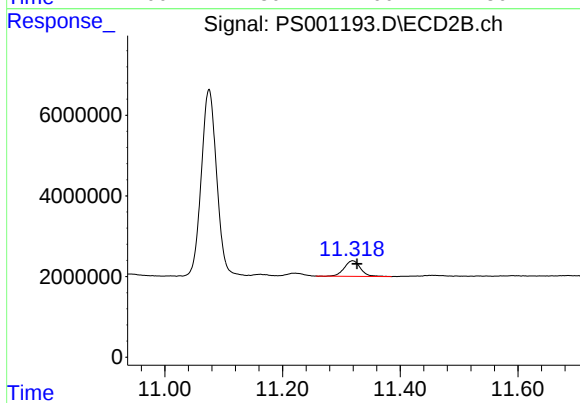

#5 DICAMBA


R.T.: 11.319 min
Delta R.T.: -0.007 min
Response: 7412373
Conc: 10.81 ng/ml

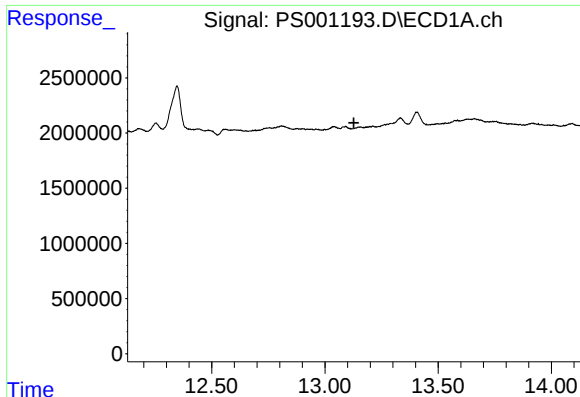

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 13.128 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

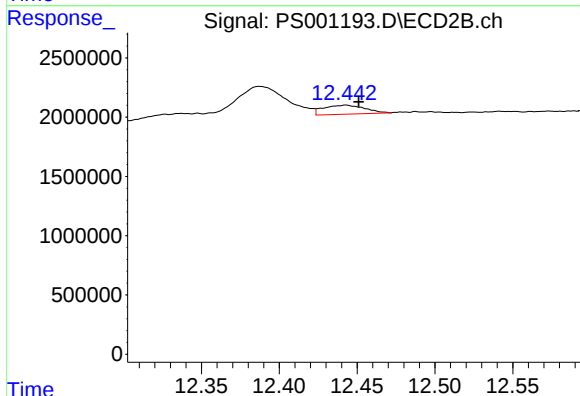


#8 DICHLORPROP

R.T.: 12.443 min
Delta R.T.: -0.008 min
Response: 1417607
Conc: 8.00 ng/ml

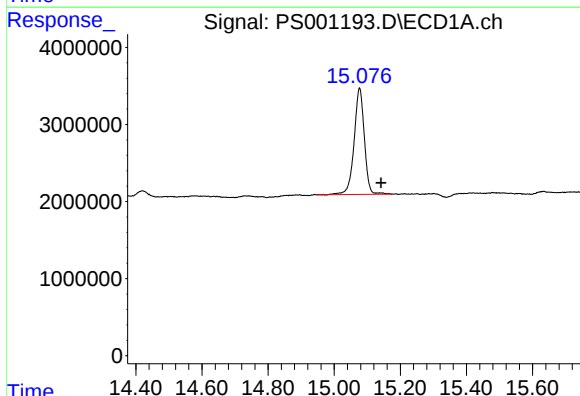


#12 2,4,5-T

R.T.: 15.077 min
Delta R.T.: -0.065 min
Response: 29748742
Conc: 26.73 ng/ml

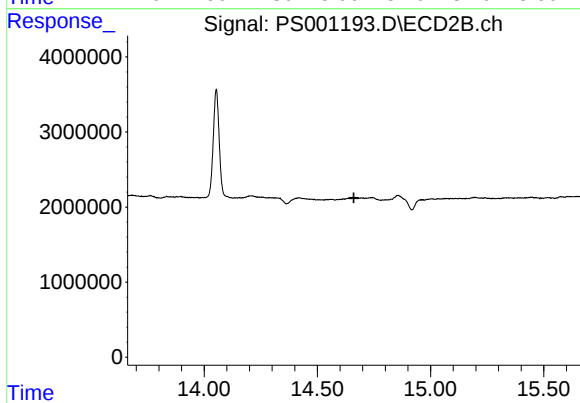

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 14.662 min
Response: 0
Conc: N.D.

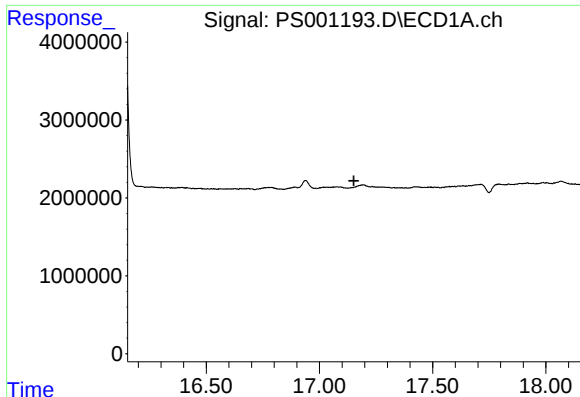

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 17.152 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

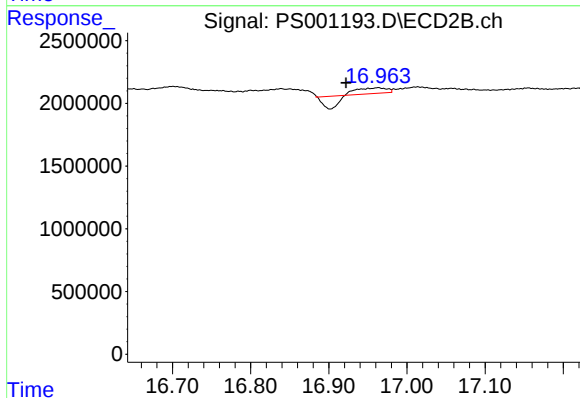


#15 Picloram

R.T.: 16.963 min
Delta R.T.: 0.041 min
Response: 150729
Conc: 0.11 ng/ml

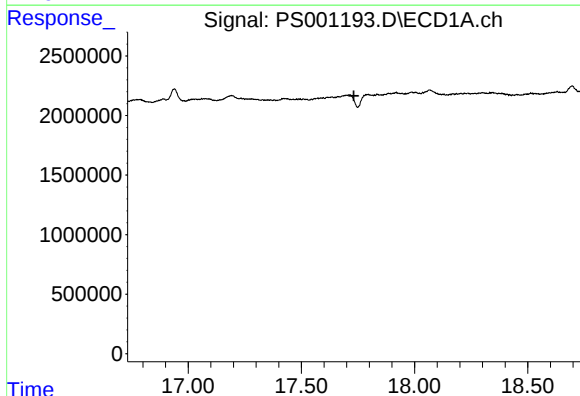

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.732 min
Response: 0
Conc: N.D.

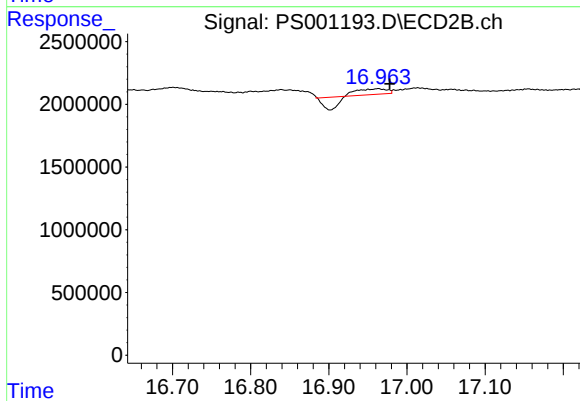

#16 DCPA

R.T.: 16.963 min
Delta R.T.: -0.015 min
Response: 150729
Conc: 0.10 ng/ml