

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072118\
 Data File : PS001194.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2018 09:26
 Operator : UA
 Sample : J4062-42
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 00:46:41 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072118.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 21 01:18:58 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.656	11.076	90961619	74536040	490.227	409.820
Target Compounds							
2) T	3,5-DICHL...	0.000	9.163	0	9904611	N.D.	38.880 #
3) T	4-Nitroph...	0.000	10.233	0	4928946	N.D.	48.352 #
5) T	DICAMBA	0.000	11.319	0	8731371	N.D.	12.739 #
8) T	DICHLORPROP	0.000	12.446	0	1665188	N.D.	9.400 #
9) T	2,4-D	0.000	12.914	0	2400469	N.D.	10.116 #
12) T	2,4,5-T	15.077	0.000	34119569	0	30.663	N.D. #
15) T	Picloram	0.000	16.945	0	2788383	N.D.	2.023 #
16) T	DCPA	0.000	16.945	0	2788383	N.D.	1.931 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072118\
Data File : PS001194.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jul 2018 09:26
Operator : UA
Sample : J4062-42
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 23 00:46:41 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072118.M
Quant Title : 8080.M
QLast Update : Sat Jul 21 01:18:58 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

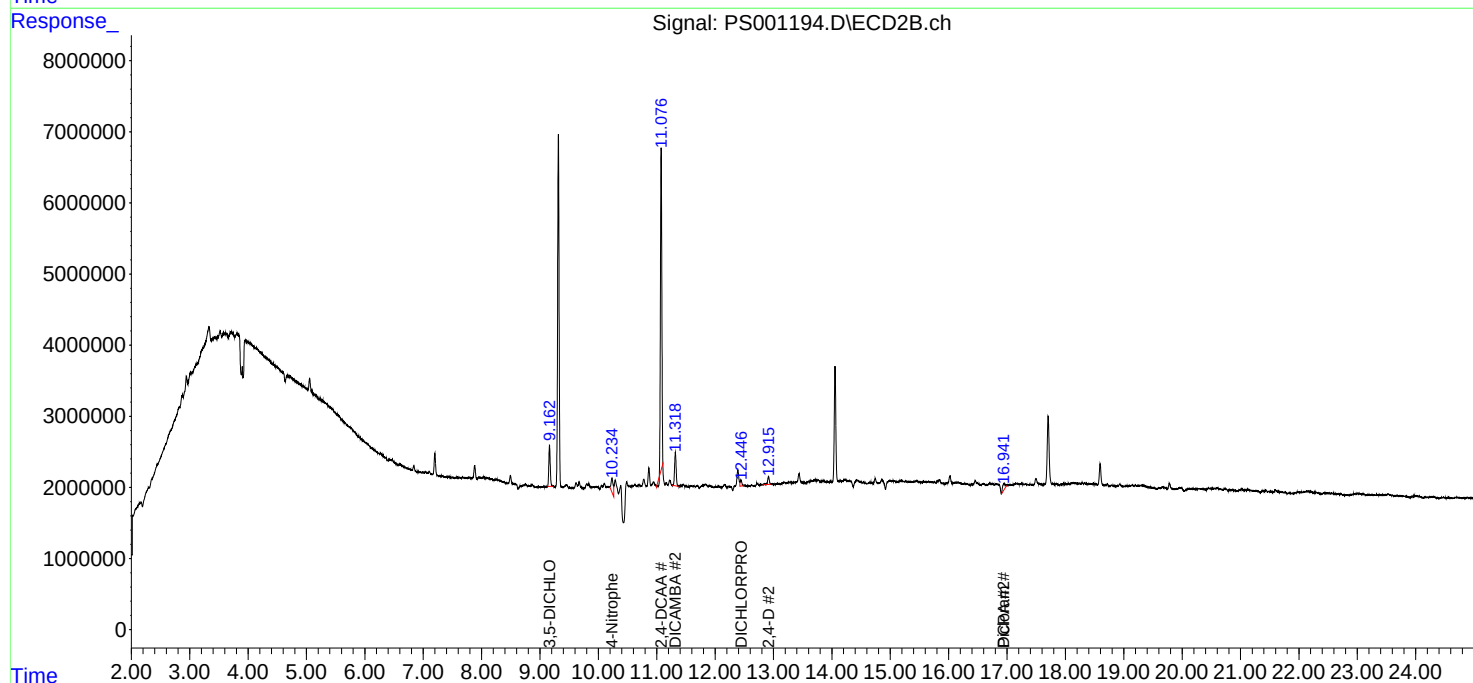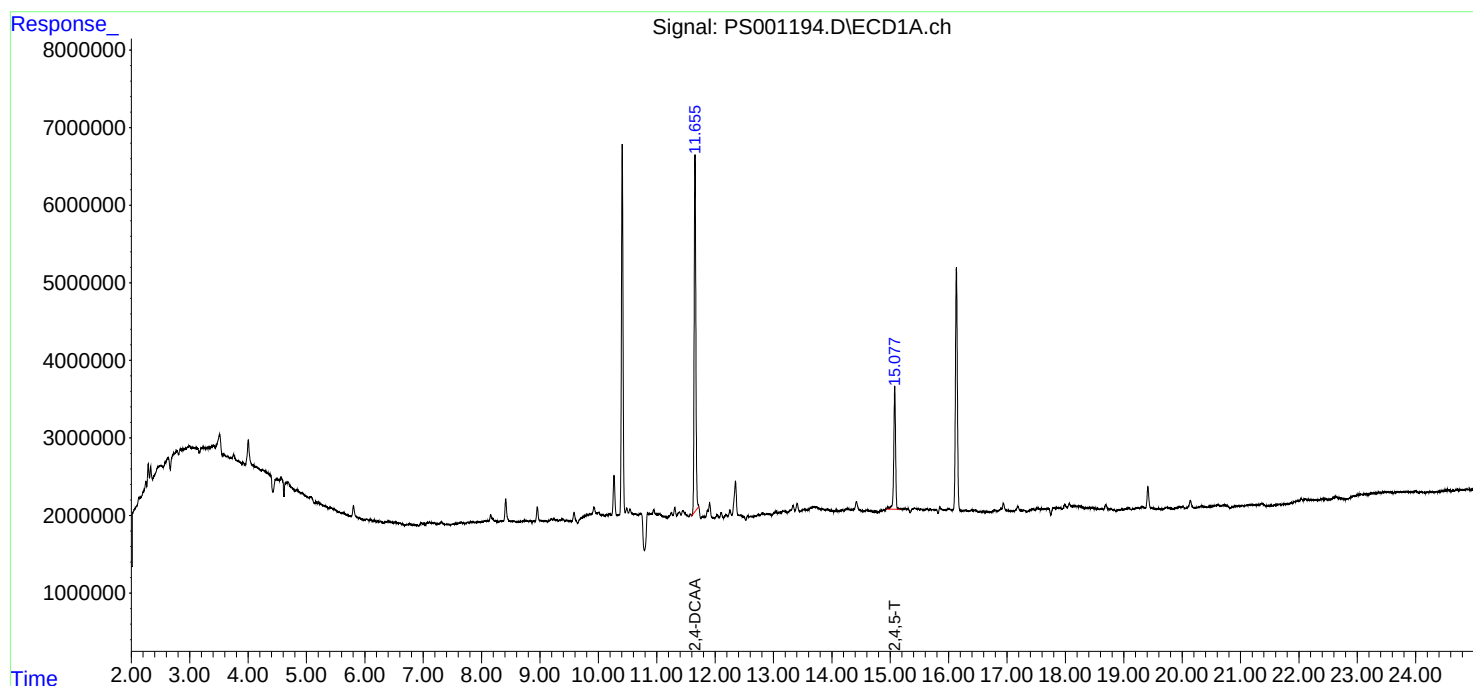


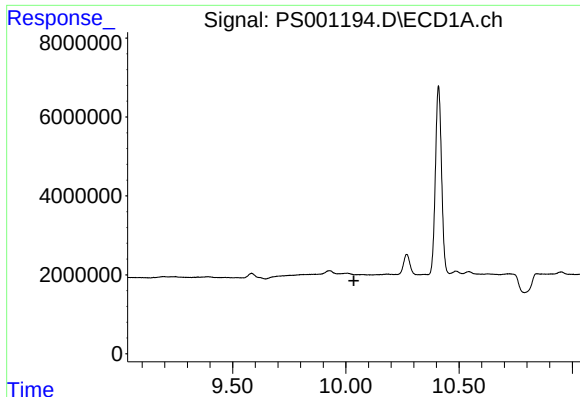

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 10.035 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

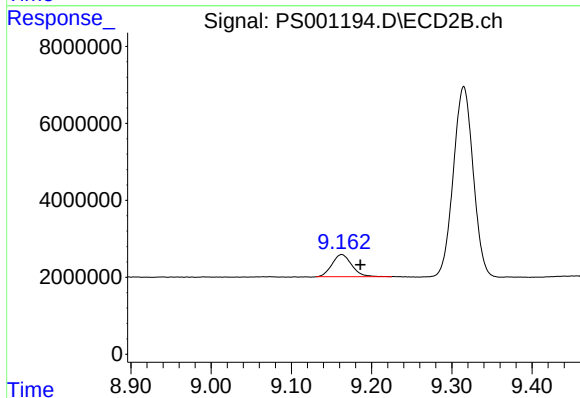


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.163 min
Delta R.T.: -0.023 min
Response: 9904611
Conc: 38.88 ng/ml

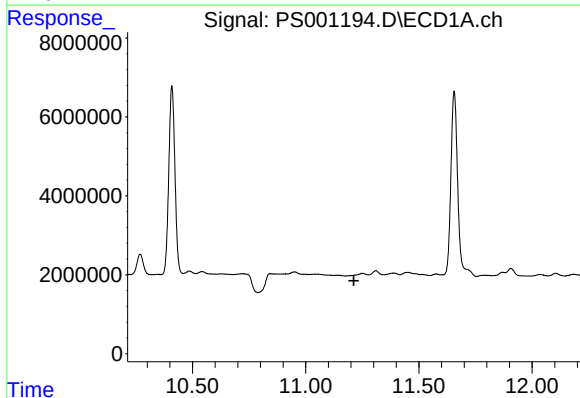


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 11.213 min
Response: 0
Conc: N.D.

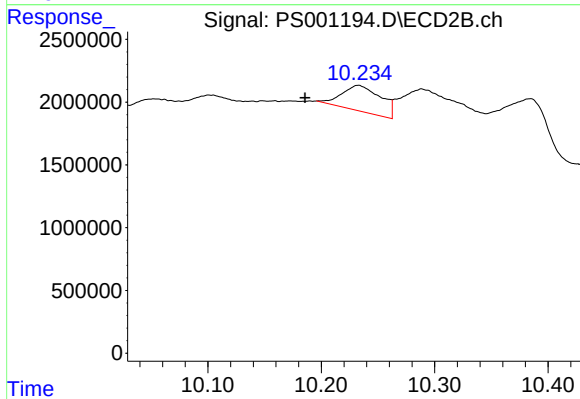

#3 4-Nitrophenol


R.T.: 10.233 min
Delta R.T.: 0.047 min
Response: 4928946
Conc: 48.35 ng/ml

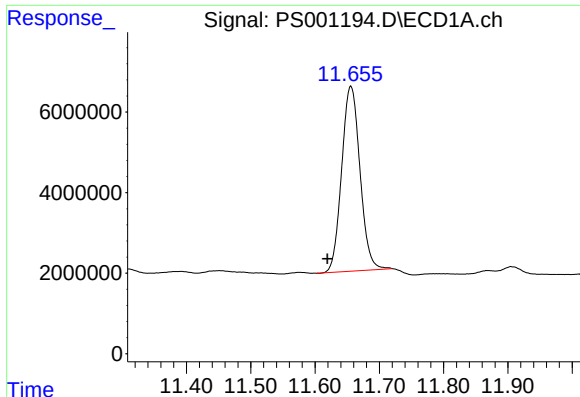

#4 2,4-DCAA


R.T.: 11.656 min
Delta R.T.: 0.036 min
Response: 90961619
Conc: 490.23 ng/ml

Instrument :
ECD_S
ClientSampleId :

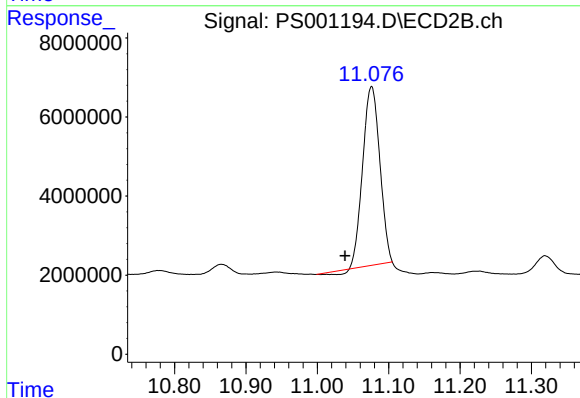


#4 2,4-DCAA

R.T.: 11.076 min
Delta R.T.: 0.037 min
Response: 74536040
Conc: 409.82 ng/ml

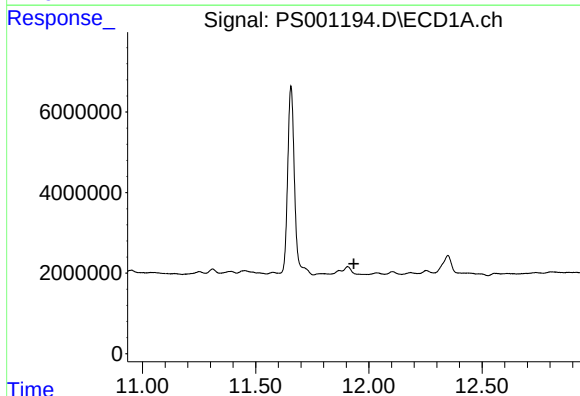


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.934 min
Response: 0
Conc: N.D.

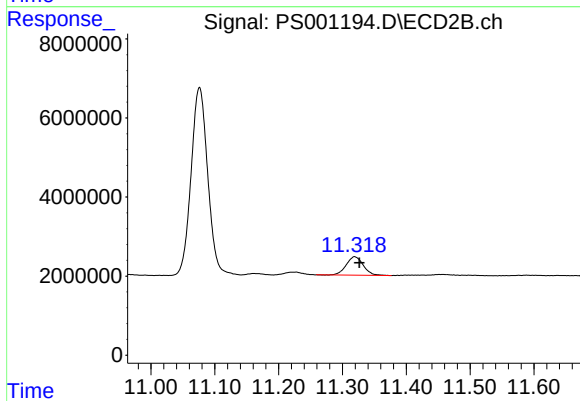

#5 DICAMBA


R.T.: 11.319 min
Delta R.T.: -0.007 min
Response: 8731371
Conc: 12.74 ng/ml

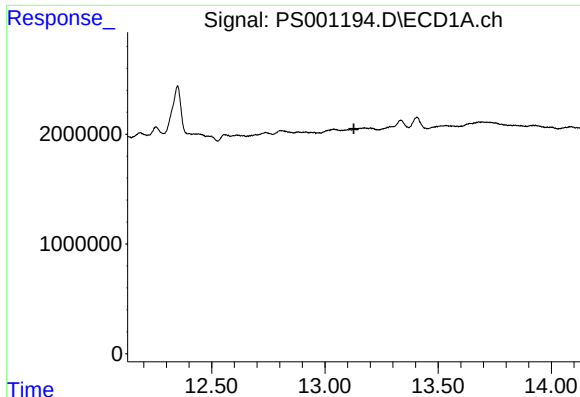

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 13.128 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

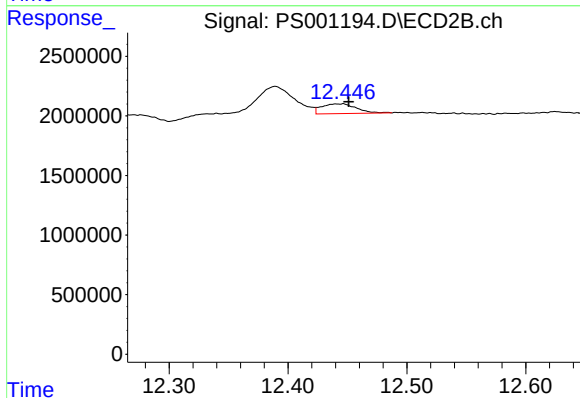


#8 DICHLORPROP

R.T.: 12.446 min
Delta R.T.: -0.005 min
Response: 1665188
Conc: 9.40 ng/ml

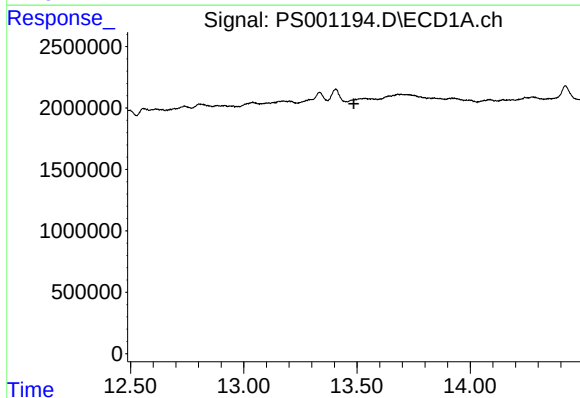


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 13.486 min
Response: 0
Conc: N.D.

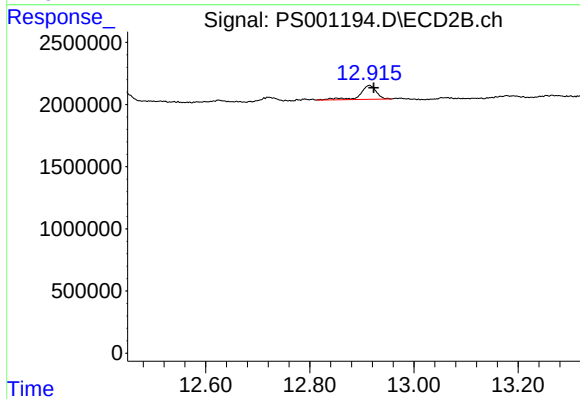

#9 2,4-D


R.T.: 12.914 min
Delta R.T.: -0.008 min
Response: 2400469
Conc: 10.12 ng/ml

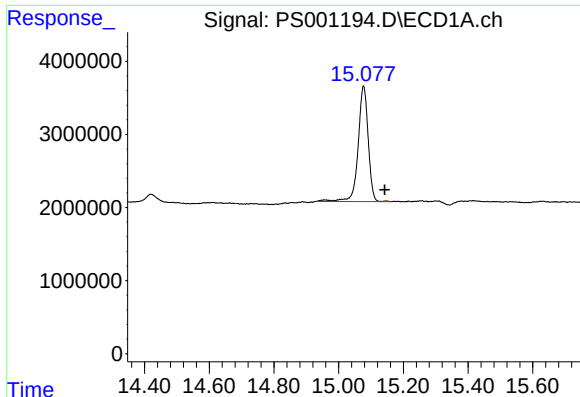

#12 2,4,5-T


R.T.: 15.077 min
Delta R.T.: -0.065 min
Response: 34119569
Conc: 30.66 ng/ml

Instrument :
ECD_S
ClientSampleId :

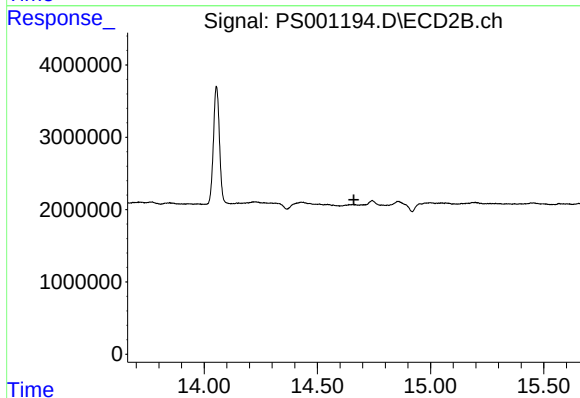


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 14.662 min
Response: 0
Conc: N.D.

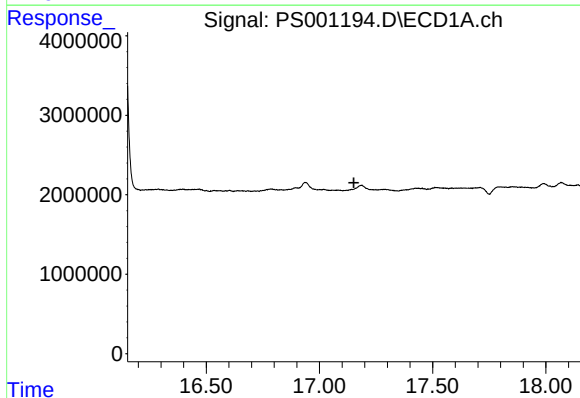


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 17.152 min
Response: 0
Conc: N.D.

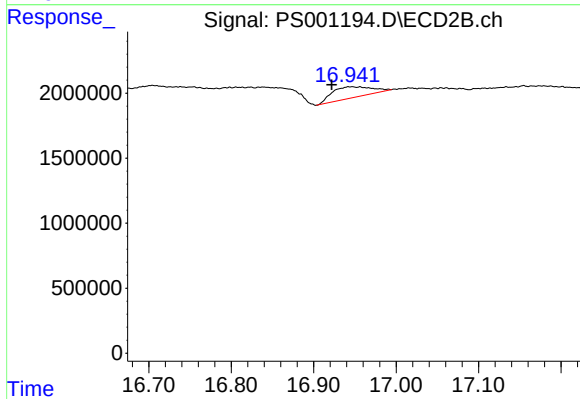

#15 Picloram


R.T.: 16.945 min
Delta R.T.: 0.023 min
Response: 2788383
Conc: 2.02 ng/ml

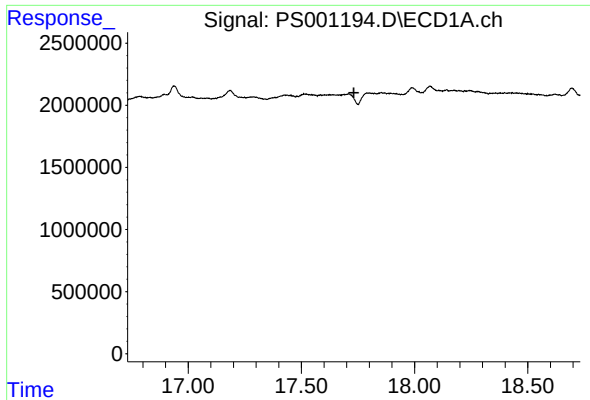

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.732 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

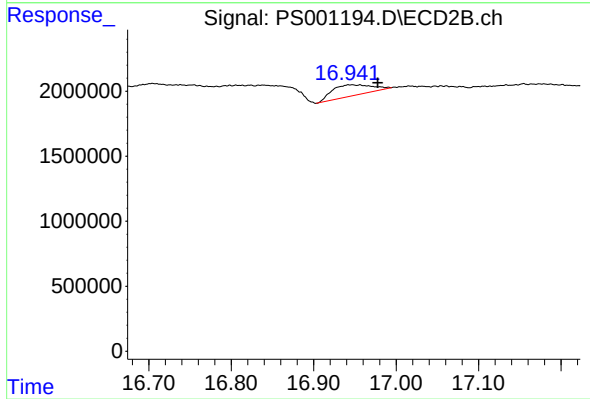

#16 DCPA

R.T.: 16.945 min
Delta R.T.: -0.033 min
Response: 2788383
Conc: 1.93 ng/ml