

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072118\
 Data File : PS001196.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2018 10:28
 Operator : UA
 Sample : J4087-53
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 00:47:21 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072118.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 21 01:18:58 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.619	11.040	99961468	87535736	538.731	481.297
Target Compounds							
3) T	4-Nitroph...	0.000	10.195	0	5916244	N.D.	58.037 #
5) T	DICAMBA	11.936	11.284	2070134	6526839	2.879	9.523 #
6) T	MCP	12.313	0.000	10043783	0	19.983	N.D. #
9) T	2,4-D	13.487	12.922	39361607	38295651	160.354	161.385
15) T	Picloram	17.152	16.978	44606083	48075524	28.220	34.875
16) T	DCPA	17.761	16.978	-631808	48075524	N.D.	33.287



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072118\
Data File : PS001196.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jul 2018 10:28
Operator : UA
Sample : J4087-53
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 23 00:47:21 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072118.M
Quant Title : 8080.M
QLast Update : Sat Jul 21 01:18:58 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

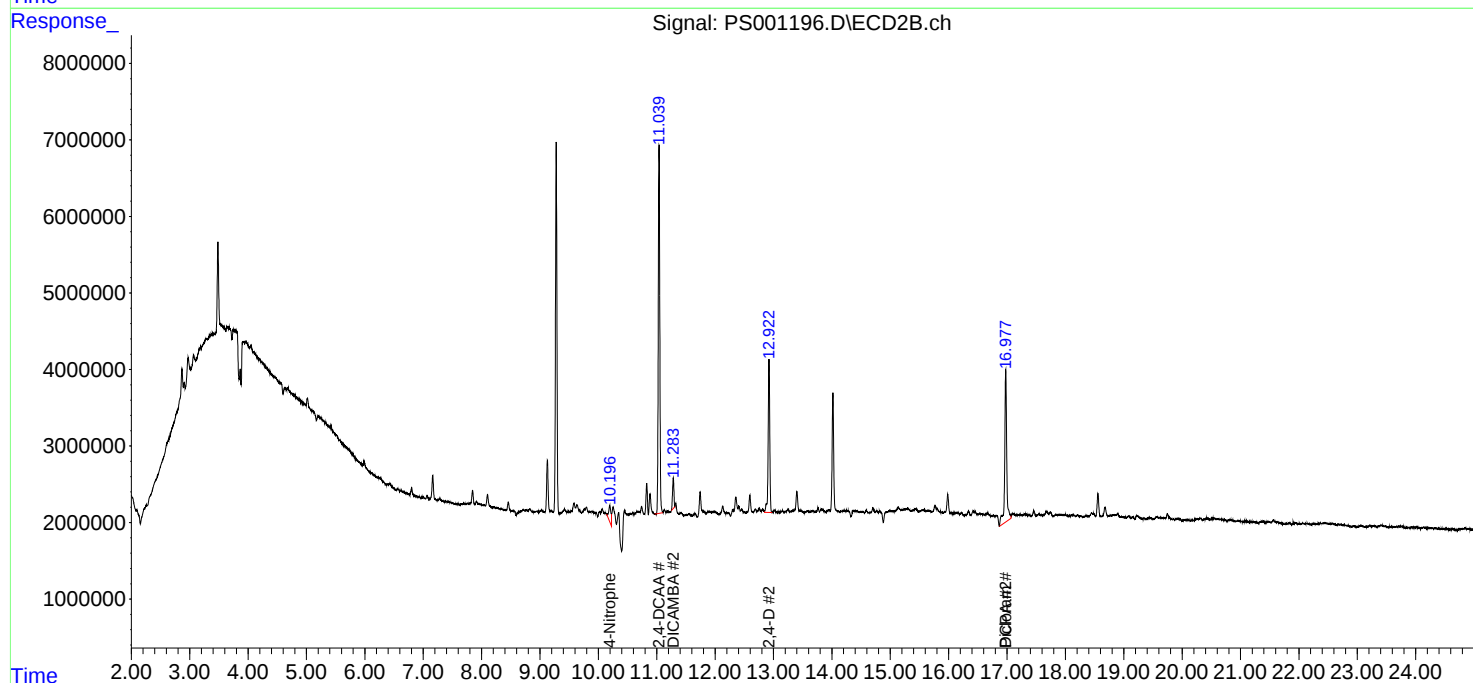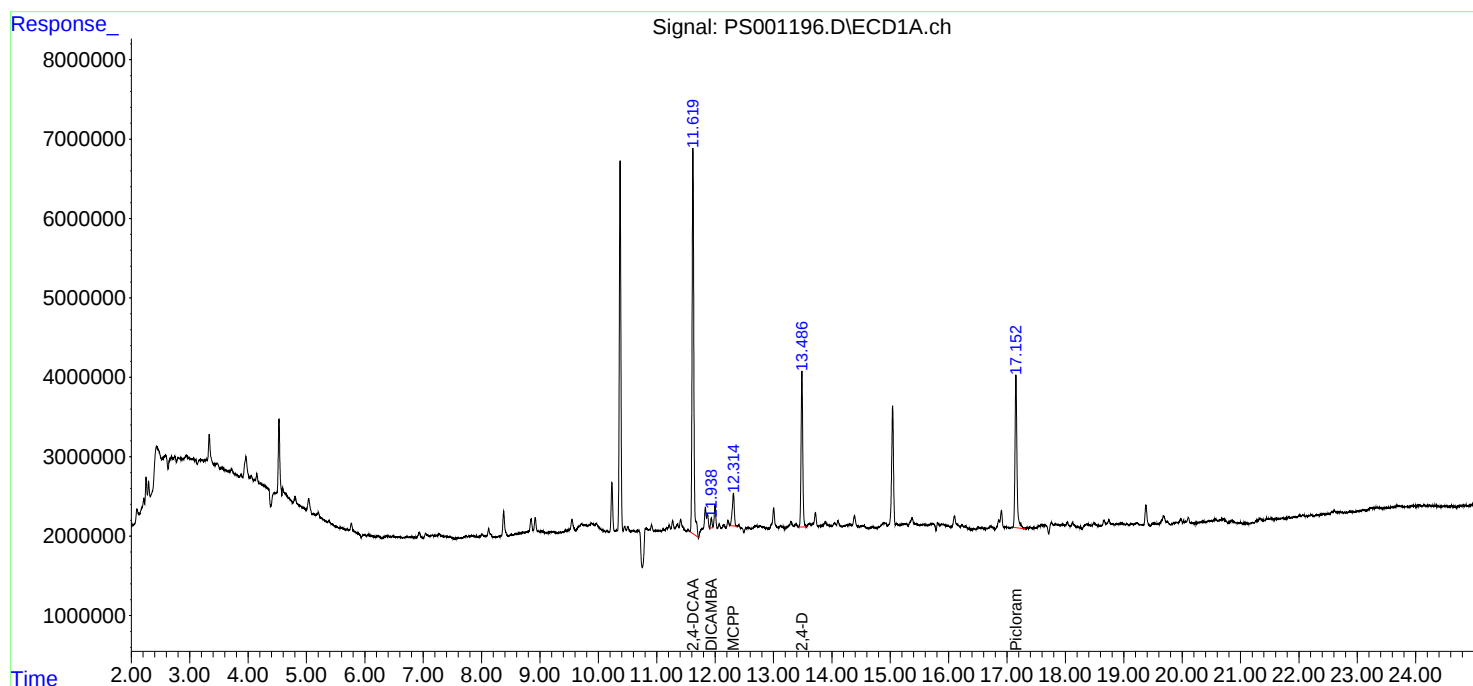


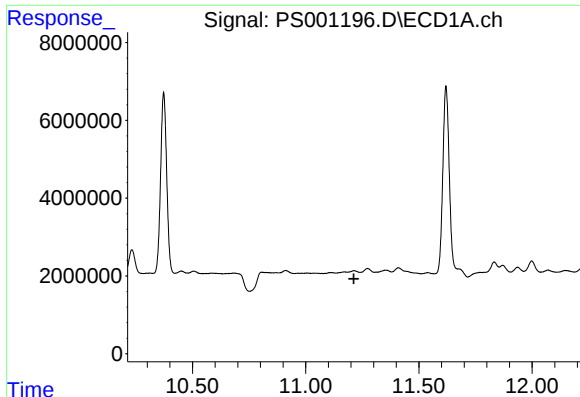

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 11.213 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

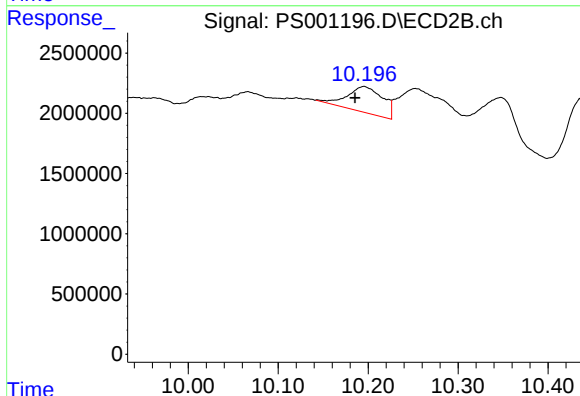


#3 4-Nitrophenol

R.T.: 10.195 min
Delta R.T.: 0.010 min
Response: 5916244
Conc: 58.04 ng/ml

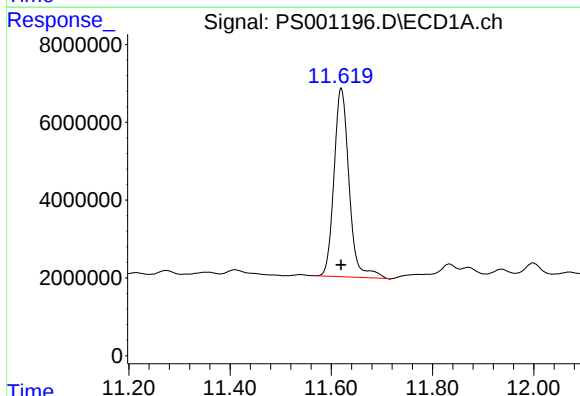


#4 2,4-DCAA

R.T.: 11.619 min
Delta R.T.: 0.000 min
Response: 99961468
Conc: 538.73 ng/ml

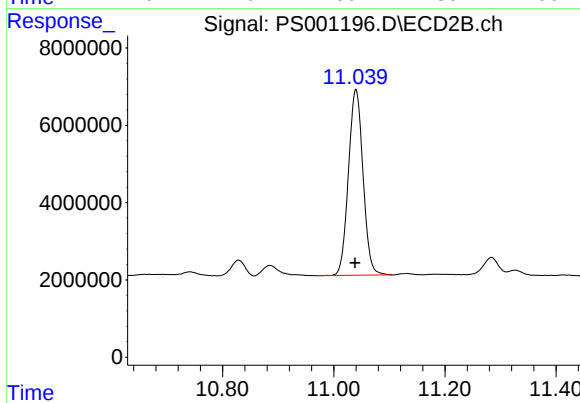

#4 2,4-DCAA


R.T.: 11.040 min
Delta R.T.: 0.001 min
Response: 87535736
Conc: 481.30 ng/ml

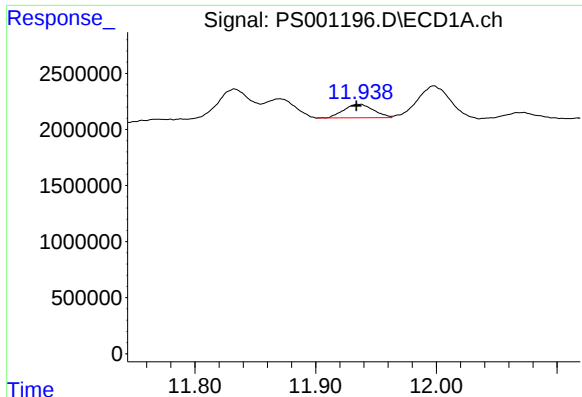

#5 DICAMBA


R.T.: 11.936 min
Delta R.T.: 0.002 min
Response: 2070134
Conc: 2.88 ng/ml

Instrument :
ECD_S
ClientSampleId :

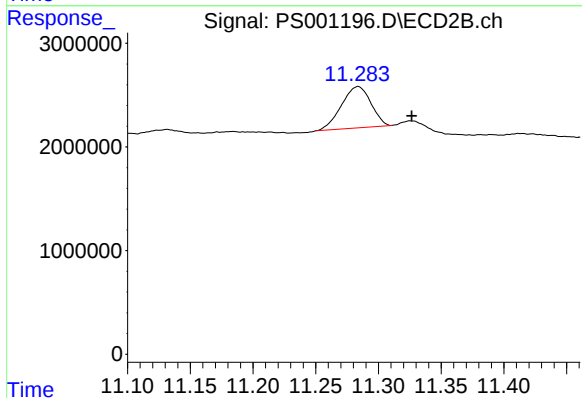


#5 DICAMBA

R.T.: 11.284 min
Delta R.T.: -0.043 min
Response: 6526839
Conc: 9.52 ng/ml

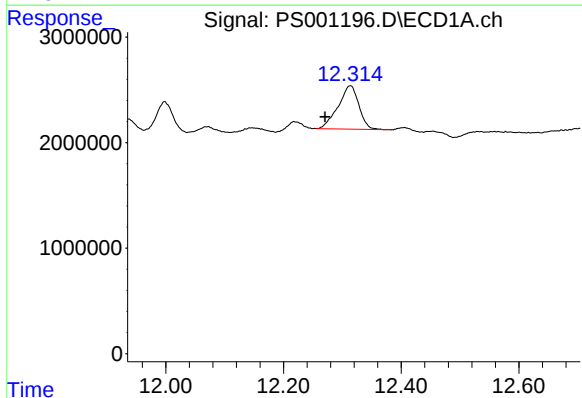


#6 MCP

R.T.: 12.313 min
Delta R.T.: 0.043 min
Response: 10043783
Conc: 19.98 ug/ml

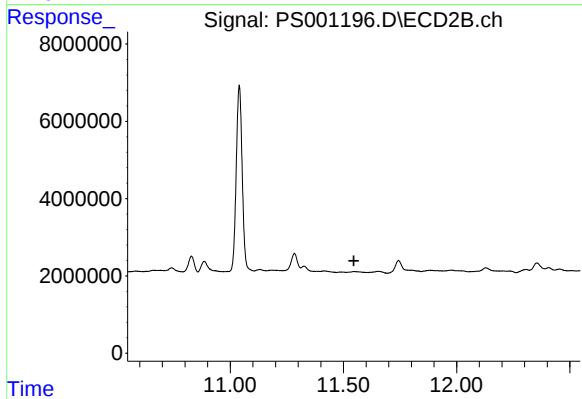

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.546 min
Response: 0
Conc: N.D.

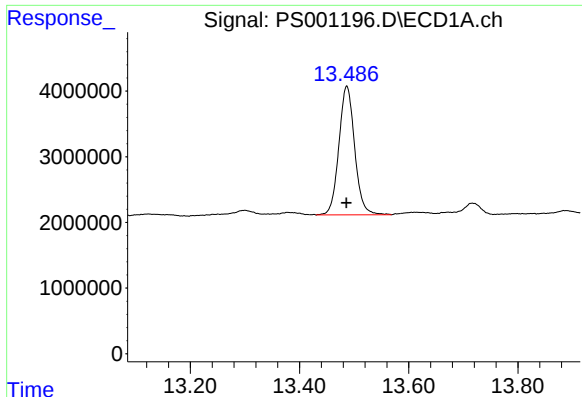

#9 2,4-D


R.T.: 13.487 min
Delta R.T.: 0.000 min
Response: 39361607
Conc: 160.35 ng/ml

Instrument :
ECD_S
ClientSampleId :

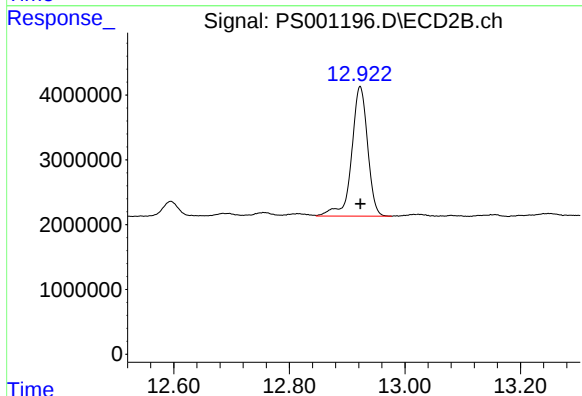


#9 2,4-D

R.T.: 12.922 min
Delta R.T.: 0.000 min
Response: 38295651
Conc: 161.39 ng/ml

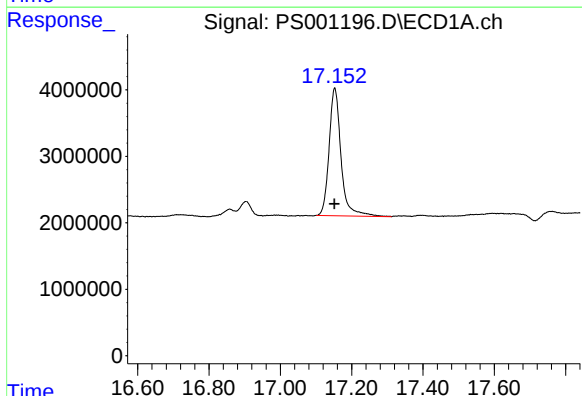


#15 Picloram

R.T.: 17.152 min
Delta R.T.: 0.000 min
Response: 44606083
Conc: 28.22 ng/ml

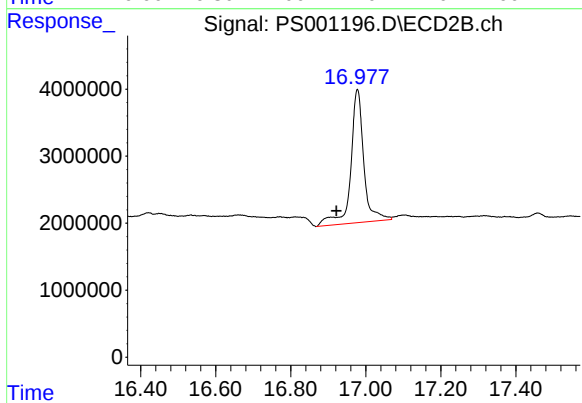

#15 Picloram


R.T.: 16.978 min
Delta R.T.: 0.056 min
Response: 48075524
Conc: 34.87 ng/ml

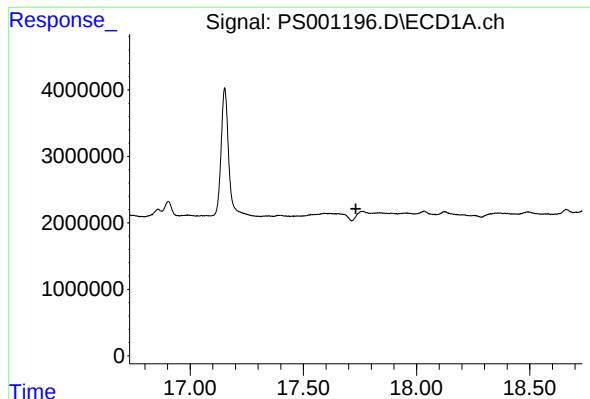

#16 DCPA

R.T.: 17.761 min
Delta R.T.: 0.030 min
Response: -631808
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

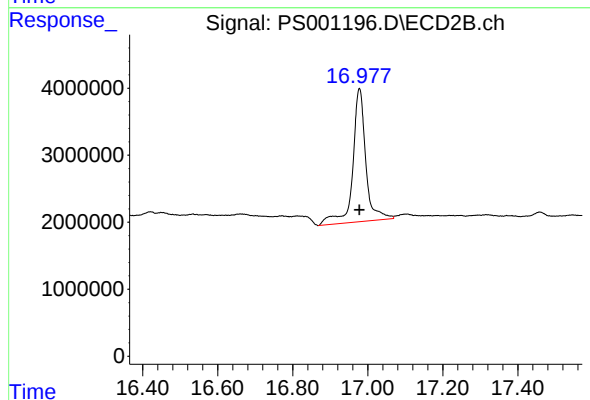

#16 DCPA

R.T.: 16.978 min
Delta R.T.: 0.000 min
Response: 48075524
Conc: 33.29 ng/ml