

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072121\
 Data File : PS016173.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2021 08:37
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 04:12:39 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS063021.M
 Quant Title : 8080.M
 QLast Update : Wed Jun 30 00:31:48 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

5) T	DICAMBA	7.379	0.000	6801959	0	1.187	N.D.	#
6) T	MCP	7.575	0.000	647120	0	<MDL	N.D.	#
7) T	MCPA	7.632f	0.000	16566671	0	2.605	N.D.	#
10) T	Pentachlo...	8.609	0.000	12594319	0	<MDL	N.D.	#
11) T	2,4,5-TP ...	9.161	0.000	9264648	0	1.249	N.D.	#
12) T	2,4,5-T	9.449	9.006	19042124	5985797	2.439	2.075	
14) T	DINOSEB	11.153	0.000	11991657	0	2.187	N.D.	#
15) T	Picloram	10.979	10.817	276.9E6	105.3E6	25.172	25.297	
16) T	DCPA	11.420	10.766	16367275	6972175	1.517	1.621	



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072121\
Data File : PS016173.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jul 2021 08:37
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 22 04:12:39 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS063021.M
Quant Title : 8080.M
QLast Update : Wed Jun 30 00:31:48 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

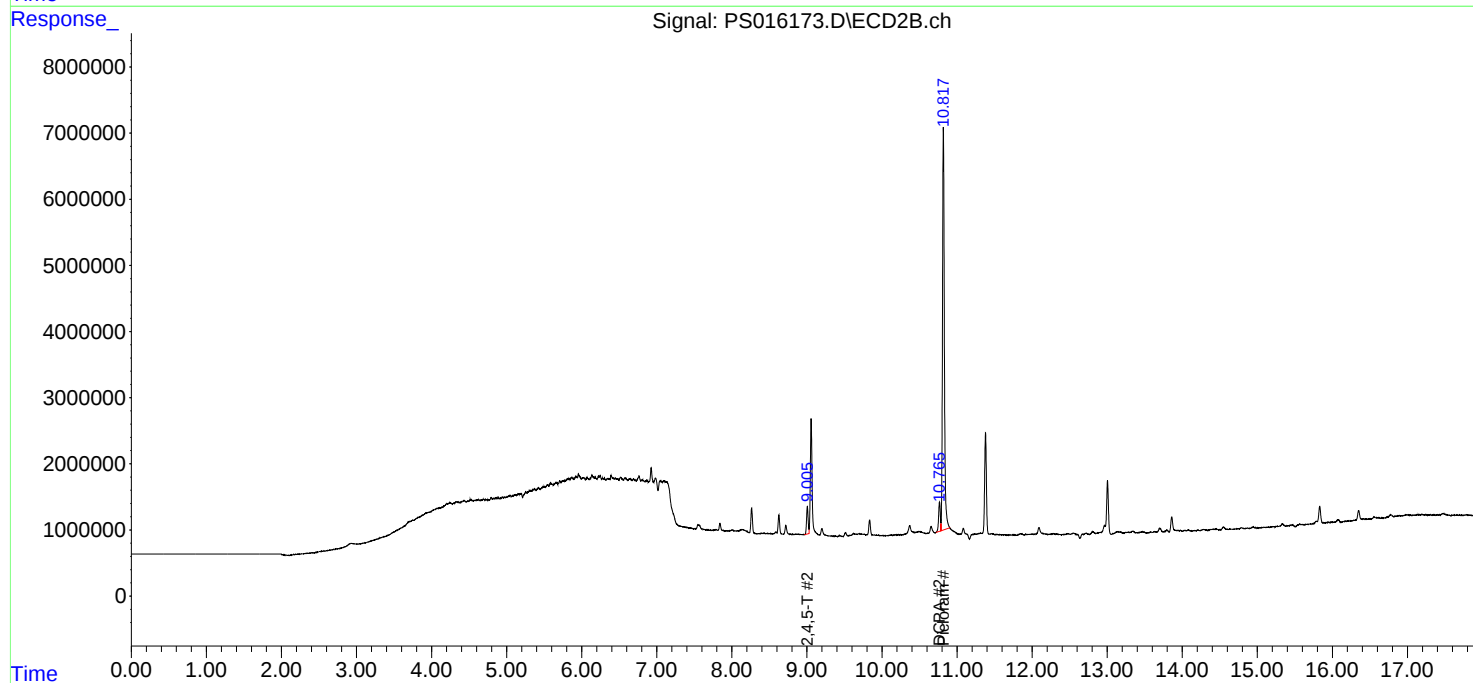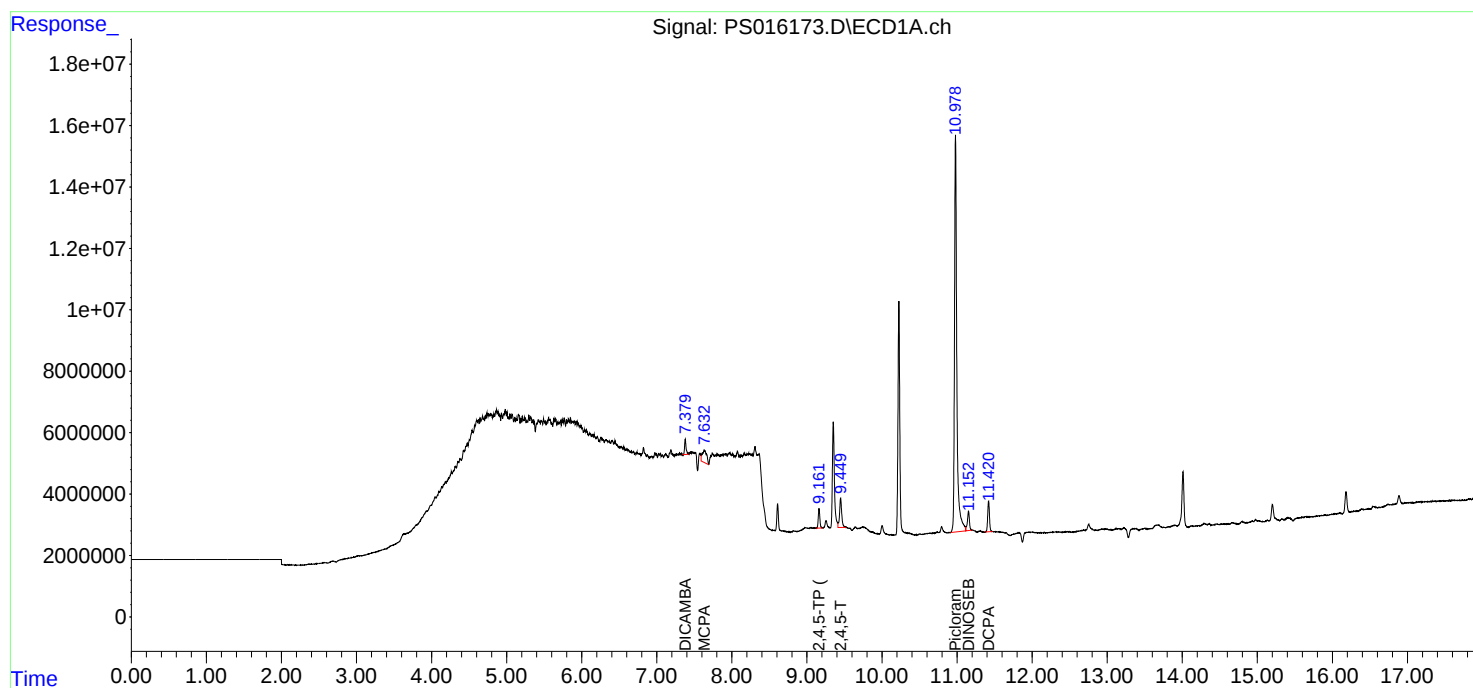


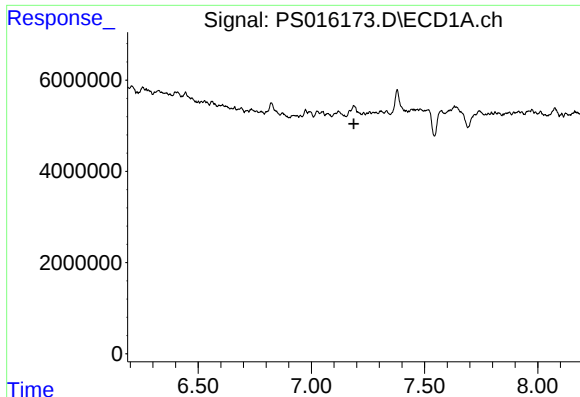

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 7.188 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

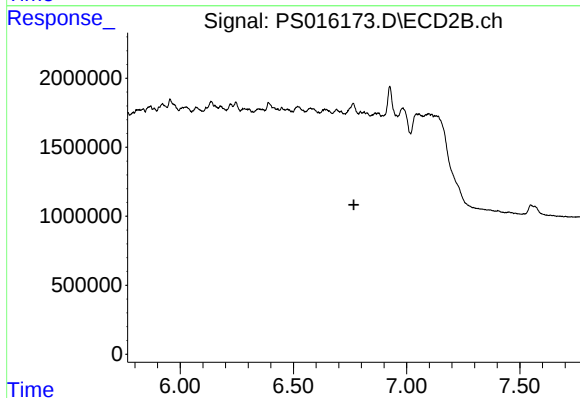


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 6.767 min
Response: 0
Conc: N.D.

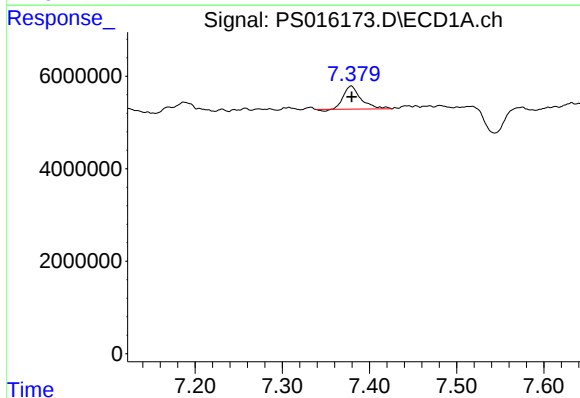


#5 DICAMBA

R.T.: 7.379 min
Delta R.T.: 0.000 min
Response: 6801959
Conc: 1.19 ng/ml

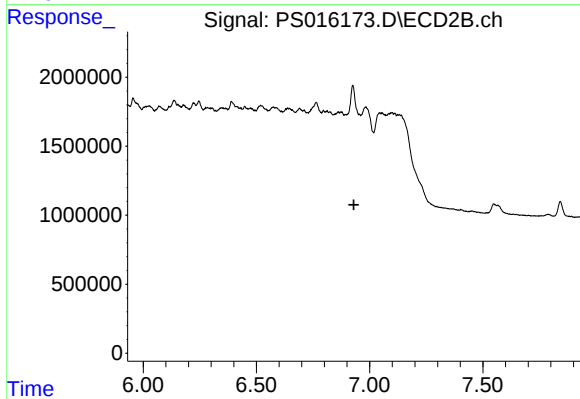

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 6.930 min
Response: 0
Conc: N.D.

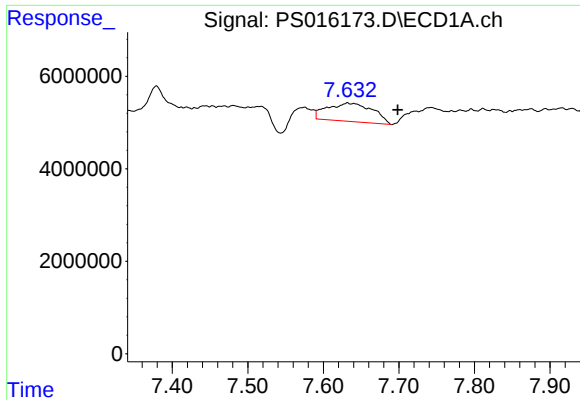

#7 MCPA


R.T.: 7.632 min
Delta R.T.: -0.067 min
Response: 16566671
Conc: 2.61 ug/ml

Instrument :
ECD_S
ClientSampleId :

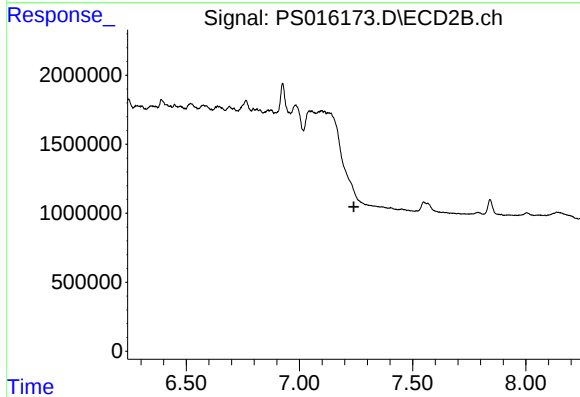


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.240 min
Response: 0
Conc: N.D.

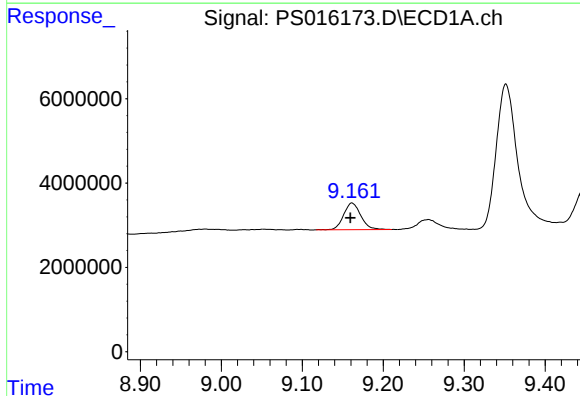


#11 2,4,5-TP (SILVEX)

R.T.: 9.161 min
Delta R.T.: 0.002 min
Response: 9264648
Conc: 1.25 ng/ml

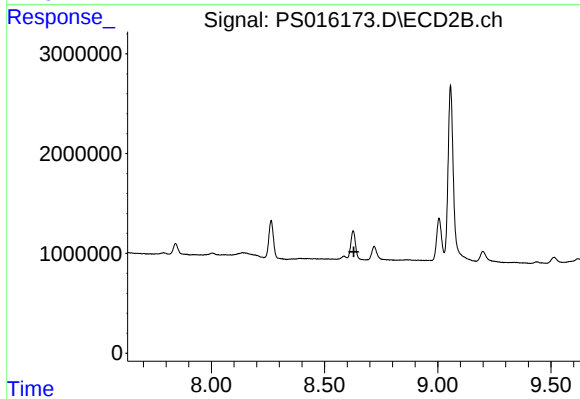

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T. : 8.630 min
Response: 0
Conc: N.D.

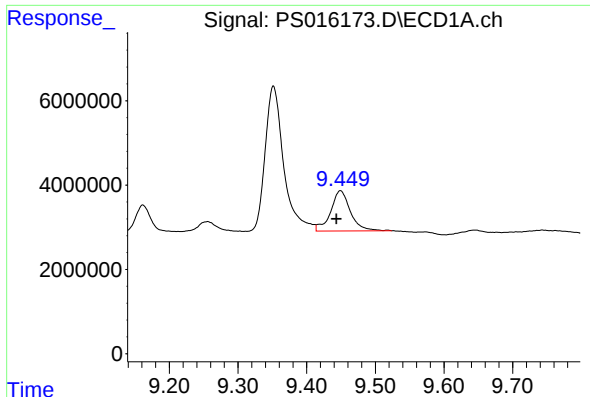

#12 2,4,5-T


R.T.: 9.449 min
Delta R.T.: 0.006 min
Response: 19042124
Conc: 2.44 ng/ml

Instrument :
ECD_S
ClientSampleId :

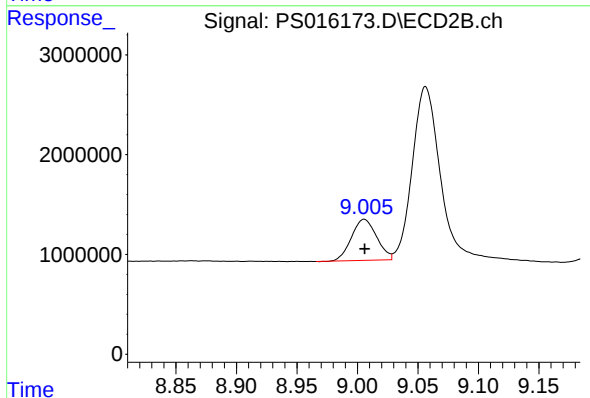


#12 2,4,5-T

R.T.: 9.006 min
Delta R.T.: 0.000 min
Response: 5985797
Conc: 2.07 ng/ml

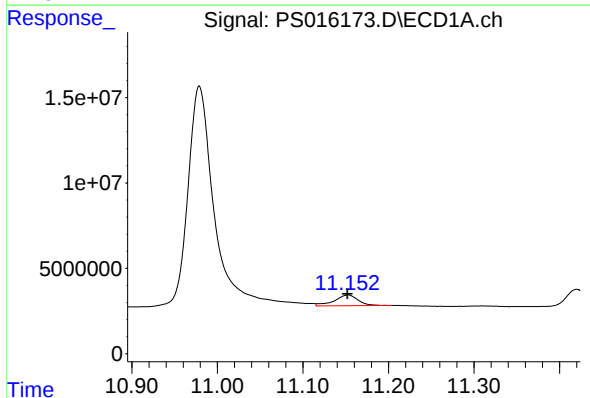


#14 DINOSEB

R.T.: 11.153 min
Delta R.T.: 0.000 min
Response: 11991657
Conc: 2.19 ng/ml

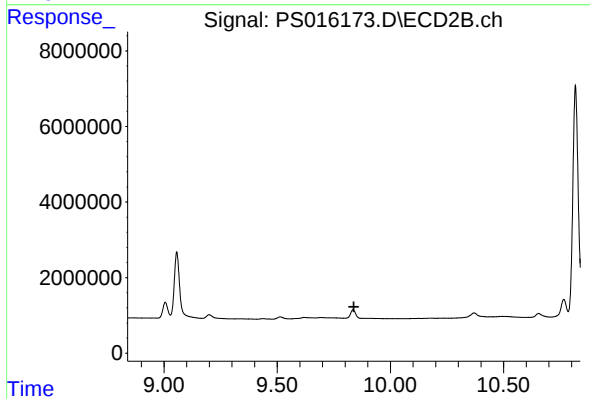

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 9.839 min
Response: 0
Conc: N.D.

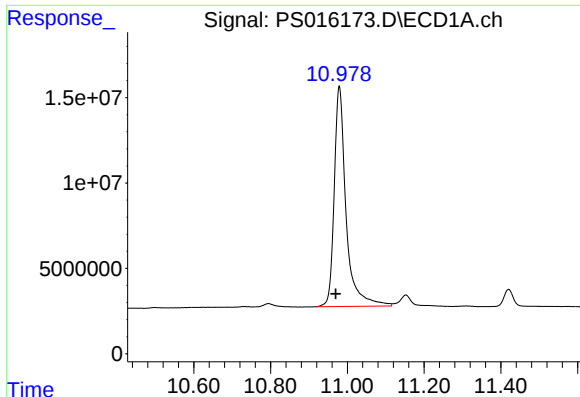

#15 Picloram


R.T.: 10.979 min
Delta R.T.: 0.009 min
Response: 276898686
Conc: 25.17 ng/ml

Instrument :
ECD_S
ClientSampleId :

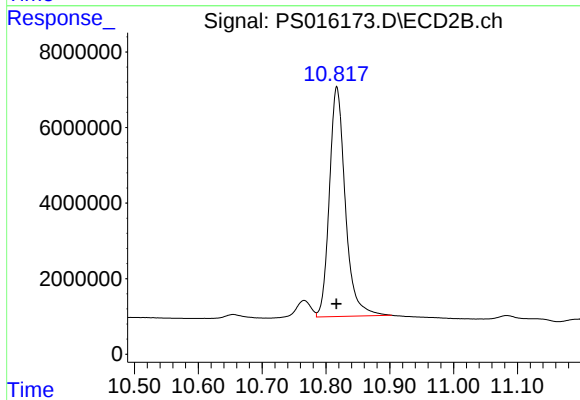


#15 Picloram

R.T.: 10.817 min
Delta R.T.: 0.000 min
Response: 105251194
Conc: 25.30 ng/ml

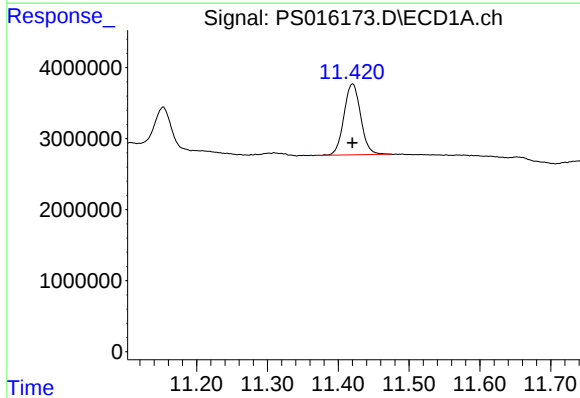

#16 DCPA

R.T.: 11.420 min
Delta R.T.: 0.000 min
Response: 16367275
Conc: 1.52 ng/ml

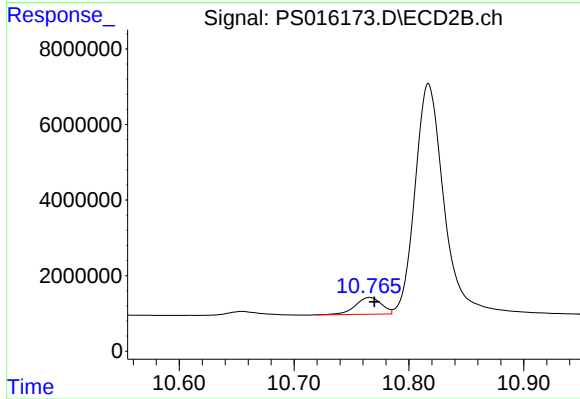

#16 DCPA

R.T.: 10.766 min
Delta R.T.: -0.004 min
Response: 6972175
Conc: 1.62 ng/ml