

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072121\
 Data File : PS016174.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2021 09:01
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 04:13:02 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS063021.M
 Quant Title : 8080.M
 QLast Update : Wed Jun 30 00:31:48 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.187	6.765	638.5E6	257.4E6	415.935	501.472
Target Compounds							
12) T	2,4,5-T	9.375f	9.070f	18325699	10534480	2.347	3.652 #
15) T	Picloram	10.999	10.828	141.1E6	50977575	12.831	12.252
16) T	DCPA	0.000	10.828f	0	50977575	N.D.	11.854



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072121\
Data File : PS016174.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jul 2021 09:01
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 22 04:13:02 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS063021.M
Quant Title : 8080.M
QLast Update : Wed Jun 30 00:31:48 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

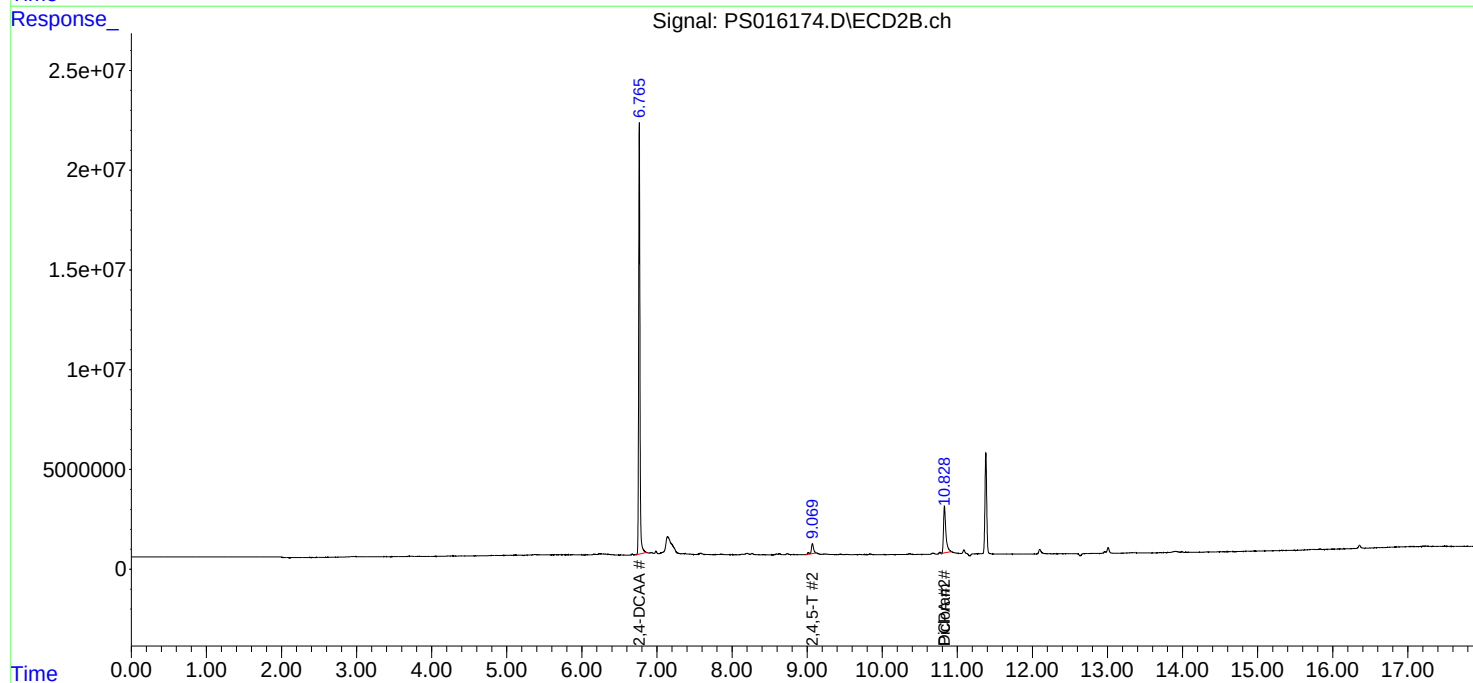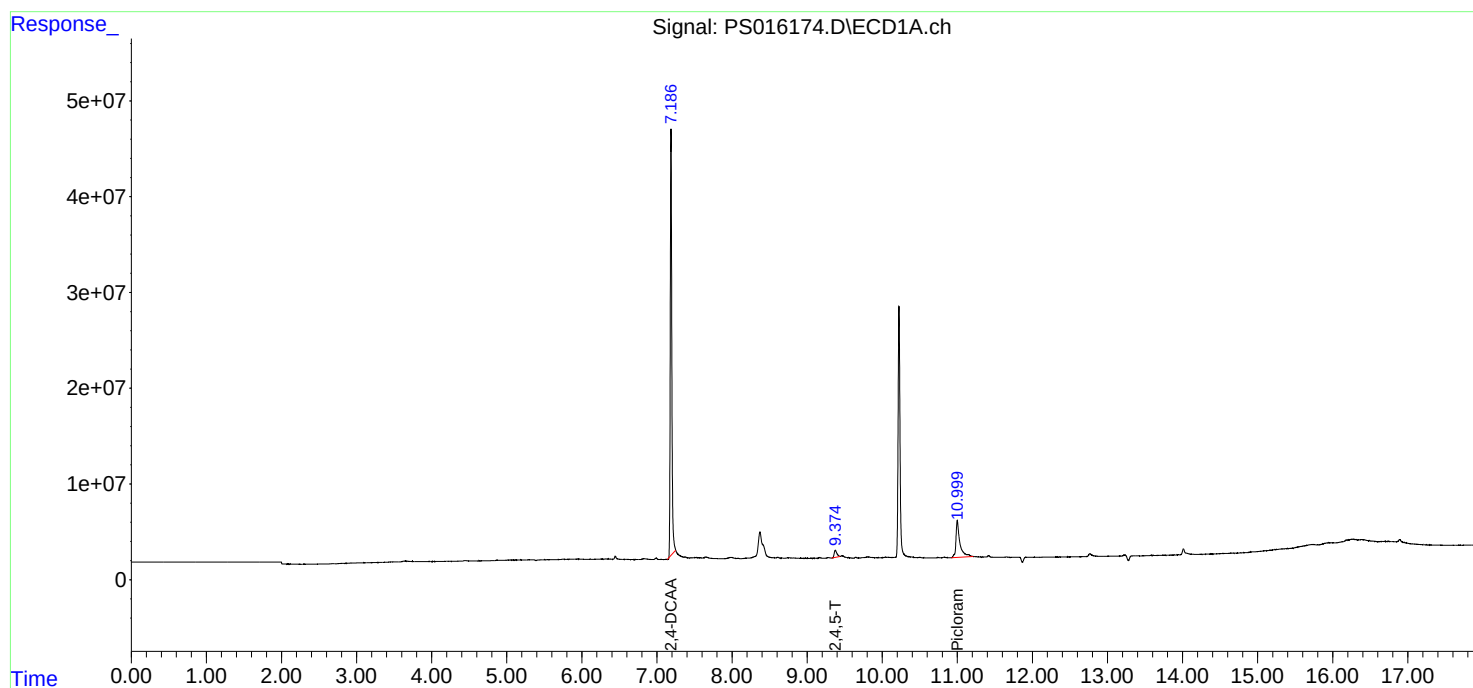


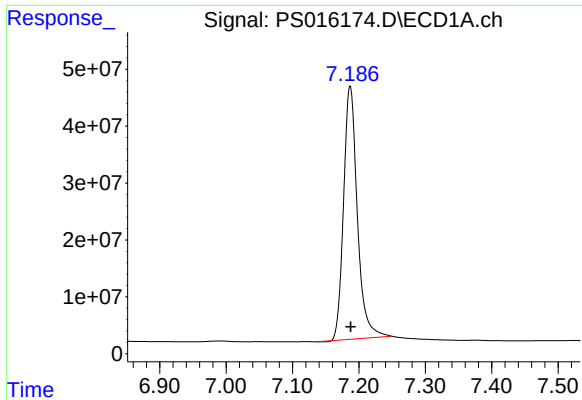

#4 2,4-DCAA


R.T.: 7.187 min
Delta R.T.: -0.001 min
Response: 638542781
Conc: 415.93 ng/ml

Instrument :
ECD_S
ClientSampleId :

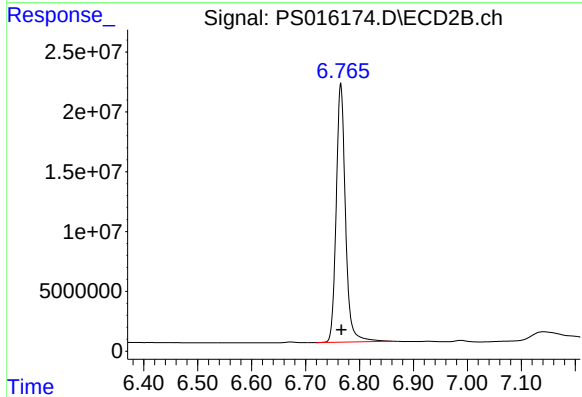


#4 2,4-DCAA

R.T.: 6.765 min
Delta R.T.: -0.001 min
Response: 257414354
Conc: 501.47 ng/ml

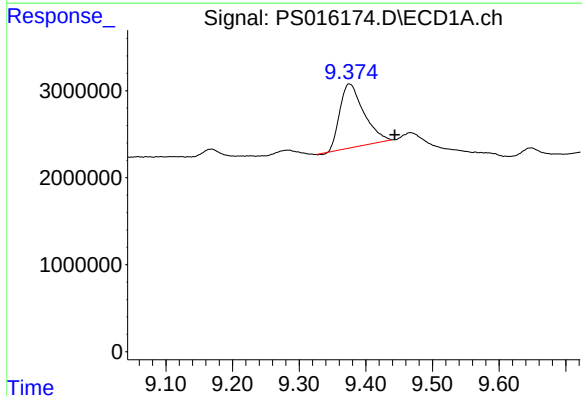


#12 2,4,5-T

R.T.: 9.375 min
Delta R.T.: -0.068 min
Response: 18325699
Conc: 2.35 ng/ml

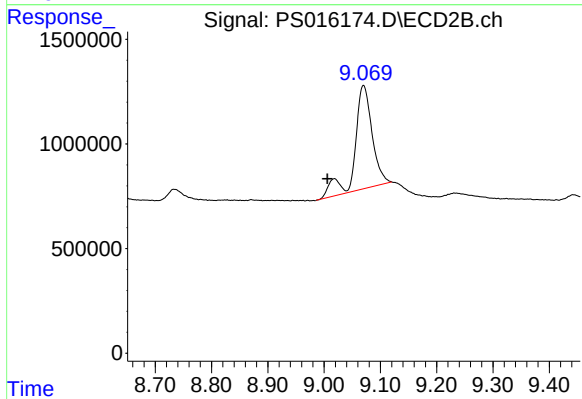

#12 2,4,5-T


R.T.: 9.070 min
Delta R.T.: 0.064 min
Response: 10534480
Conc: 3.65 ng/ml

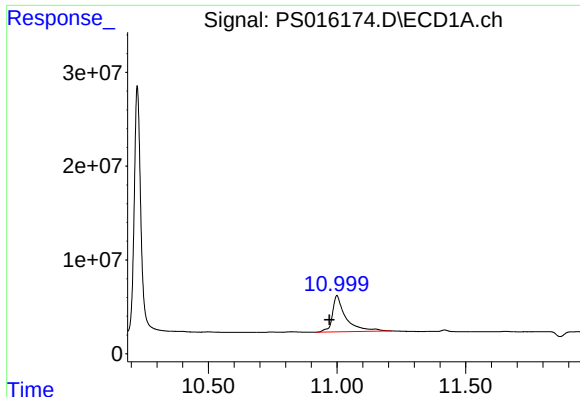

#15 Picloram


R.T.: 10.999 min
Delta R.T.: 0.029 min
Response: 141149237
Conc: 12.83 ng/ml

Instrument :
ECD_S
ClientSampleId :

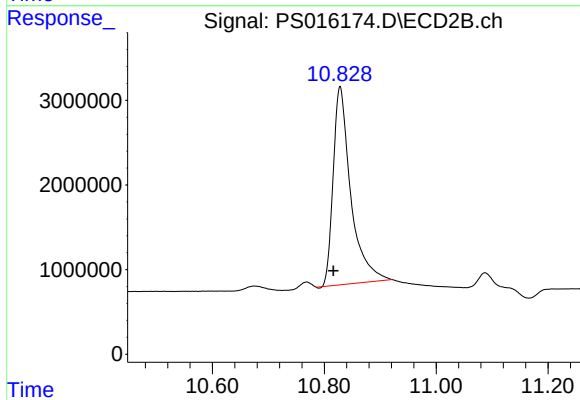


#15 Picloram

R.T.: 10.828 min
Delta R.T.: 0.012 min
Response: 50977575
Conc: 12.25 ng/ml

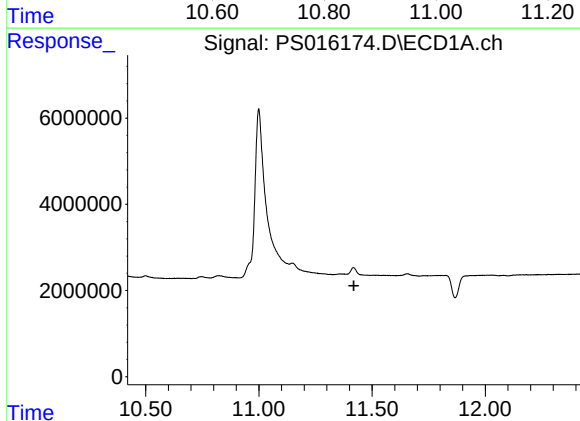

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.420 min
Response: 0
Conc: N.D.

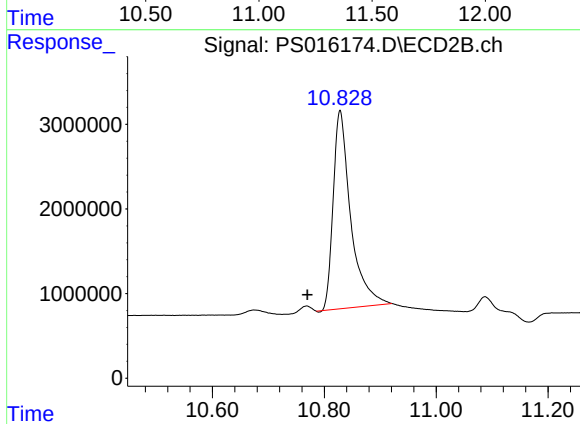

#16 DCPA

R.T.: 10.828 min
Delta R.T.: 0.058 min
Response: 50977575
Conc: 11.85 ng/ml