

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072122\
 Data File : PS020041.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2022 18:20
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 01:14:48 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072022.M
 Quant Title : 8080.M
 QLast Update : Wed Jul 20 17:52:40 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.192	6.777	1422.3E6	453.2E6	428.937	503.010
Target Compounds							
1) T	Dalapon	3.018	0.000	1075684	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.427	0.000	315751	0	<MDL	N.D. #
6) T	MCP	7.563	0.000	2311051	0	<MDL	N.D. #
7) T	MCPA	7.694	0.000	6930530	0	<MDL	N.D. #
8) T	DICHLORPROP	8.092	7.616f	235096	1884276	<MDL	1.816 #
9) T	2,4-D	0.000	7.821	0	1385456	N.D.	1.110
10) T	Pentachlo...	8.643	8.282	117679	2245884	<MDL	<MDL #
11) T	2,4,5-TP ...	9.113f	8.608	10663816	740454	<MDL	<MDL #
13) T	2,4-DB	10.015	9.462f	23671535	4735522	5.434	6.634
14) T	DINOSEB	11.117	9.843	46762209	1123073	2.602	<MDL #
15) T	Picloram	0.000	10.866f	0	11065692	N.D.	1.440
16) T	DCPA	11.423	10.772	4872	3938489	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072122\
Data File : PS020041.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jul 2022 18:20
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 22 01:14:48 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072022.M
Quant Title : 8080.M
QLast Update : Wed Jul 20 17:52:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

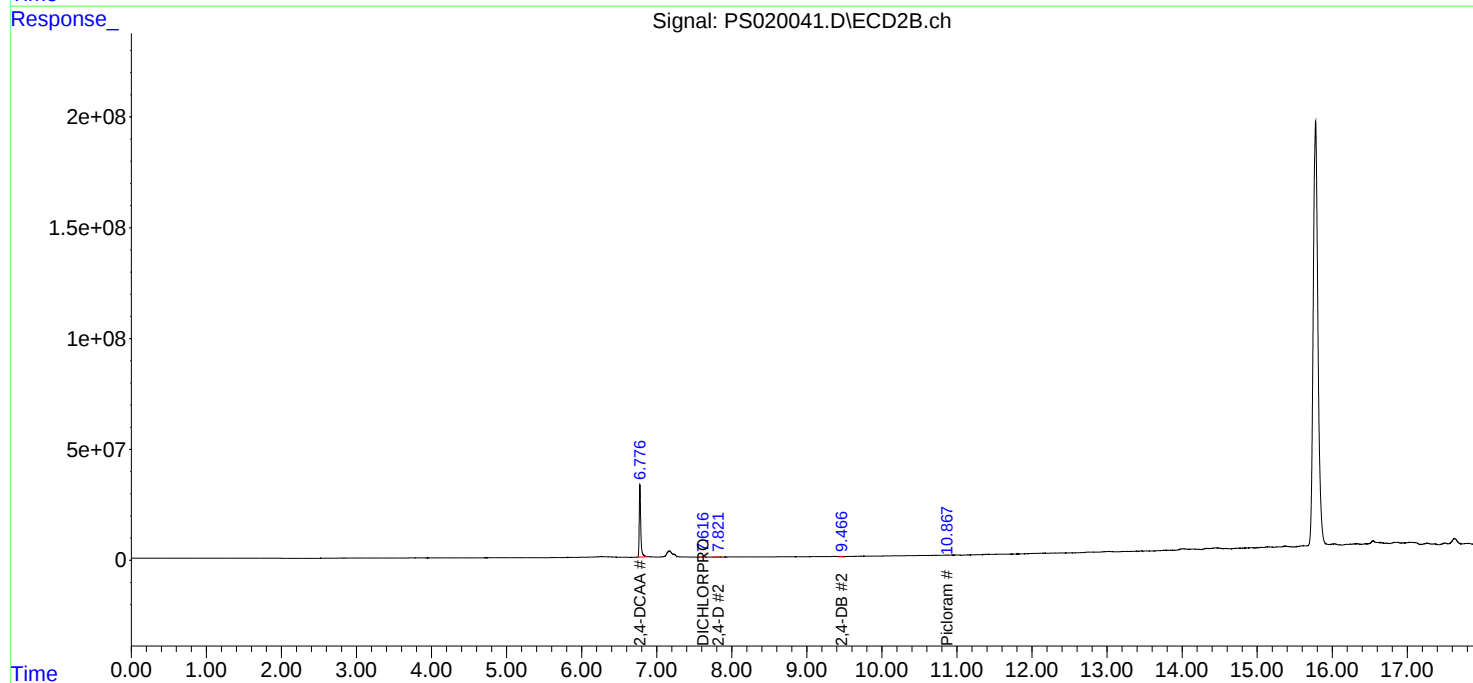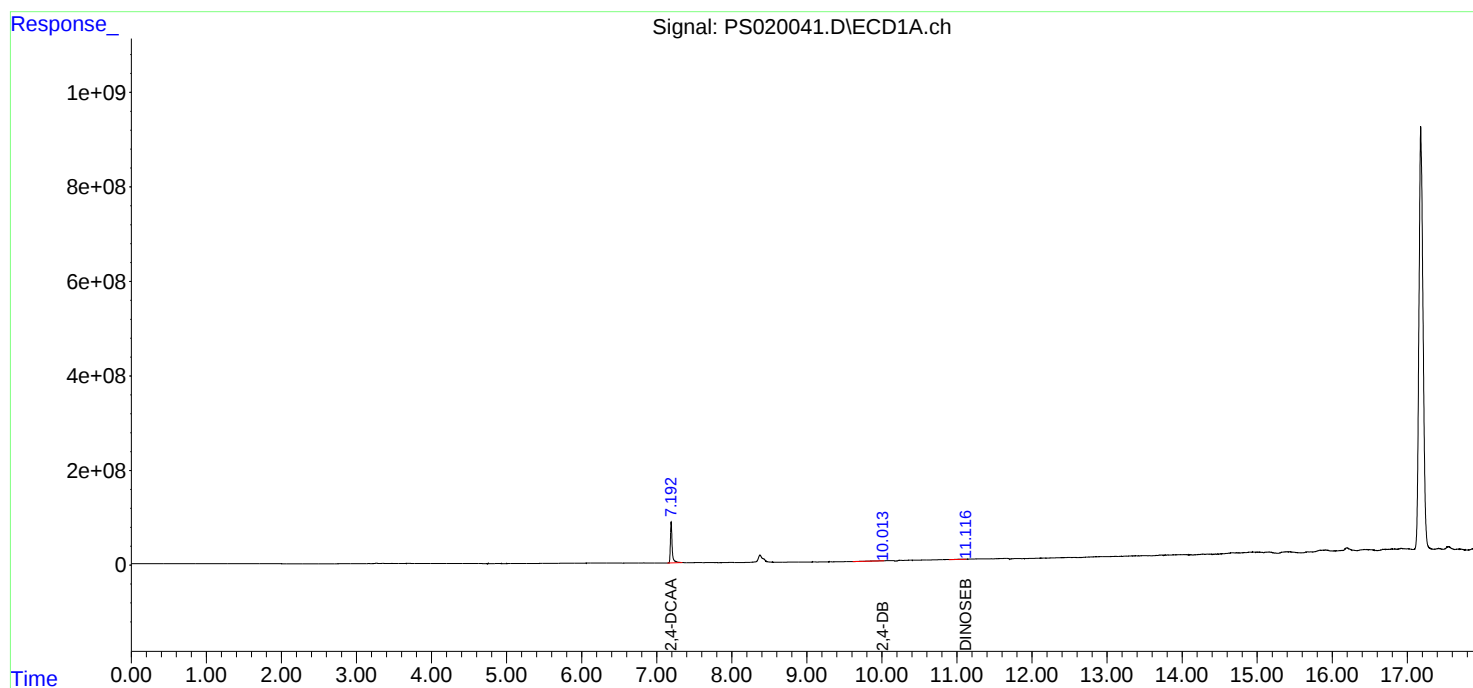


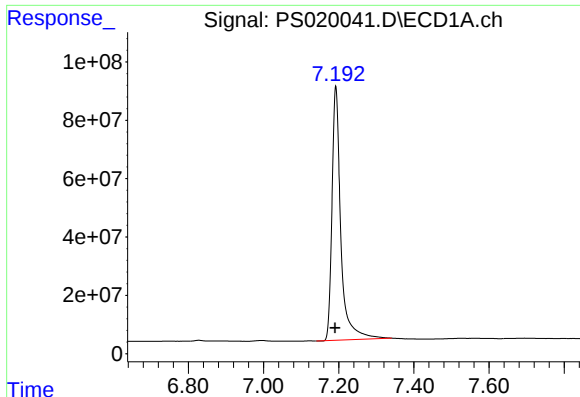

#4 2,4-DCAA


R.T.: 7.192 min
Delta R.T.: 0.002 min
Response: 1422290220
Conc: 428.94 ng/ml

Instrument :
ECD_S
ClientSampleId :

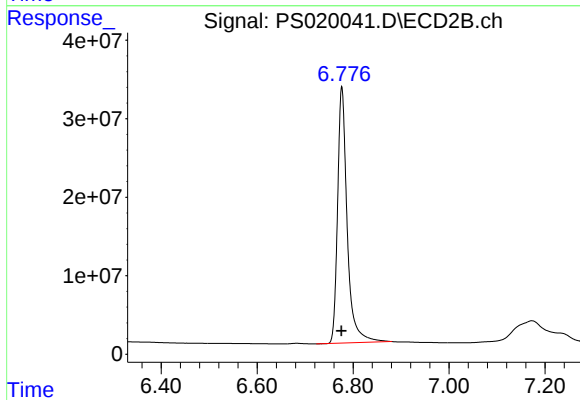


#4 2,4-DCAA

R.T.: 6.777 min
Delta R.T.: 0.000 min
Response: 453163128
Conc: 503.01 ng/ml

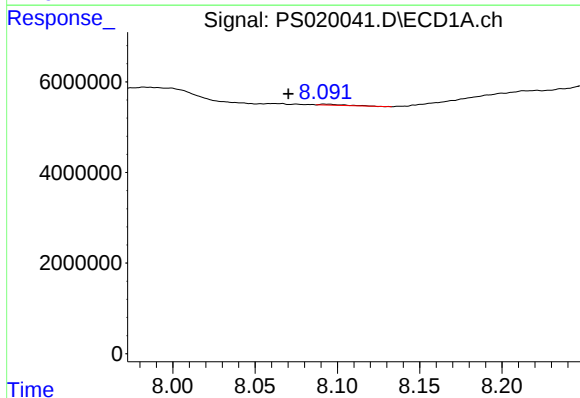


#8 DICHLORPROP

R.T.: 8.092 min
Delta R.T.: 0.022 min
Response: 235096
Conc: N.D.

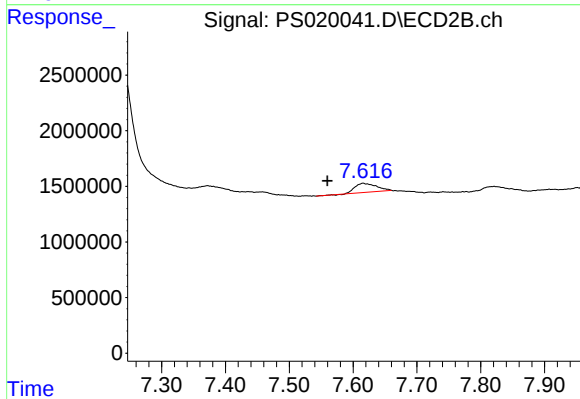

#8 DICHLORPROP


R.T.: 7.616 min
Delta R.T.: 0.056 min
Response: 1884276
Conc: 1.82 ng/ml

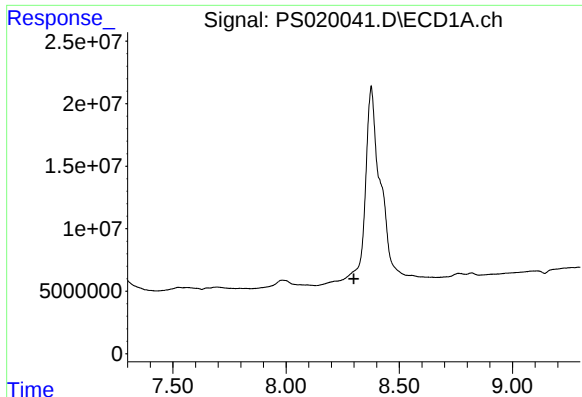

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.299 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

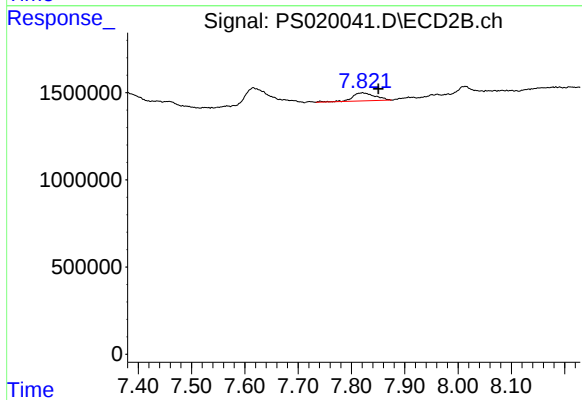


#9 2,4-D

R.T.: 7.821 min
Delta R.T.: -0.030 min
Response: 1385456
Conc: 1.11 ng/ml

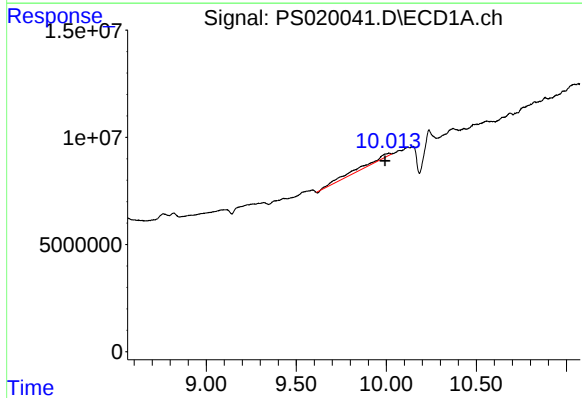


#13 2,4-DB

R.T.: 10.015 min
Delta R.T.: 0.023 min
Response: 23671535
Conc: 5.43 ng/ml

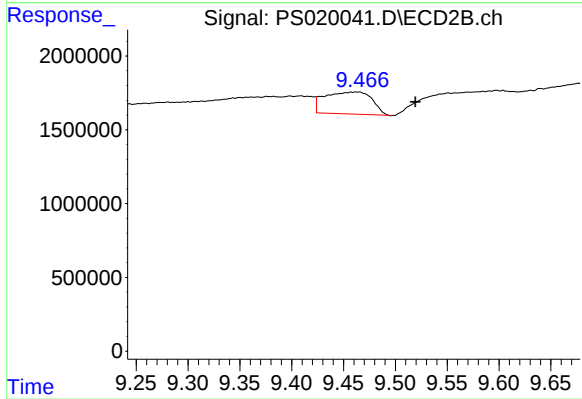

#13 2,4-DB


R.T.: 9.462 min
Delta R.T.: -0.058 min
Response: 4735522
Conc: 6.63 ng/ml

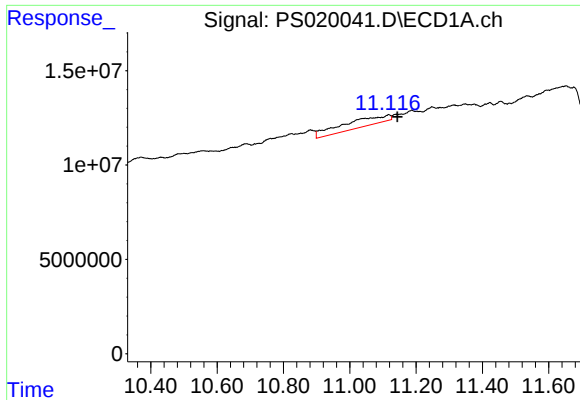

#14 DINoseb


R.T.: 11.117 min
Delta R.T.: -0.027 min
Response: 46762209
Conc: 2.60 ng/ml

Instrument :
ECD_S
ClientSampleId :

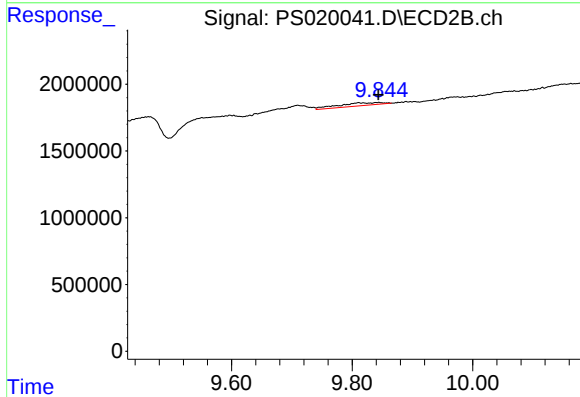


#14 DINoseb

R.T.: 9.843 min
Delta R.T.: 0.000 min
Response: 1123073
Conc: N.D.

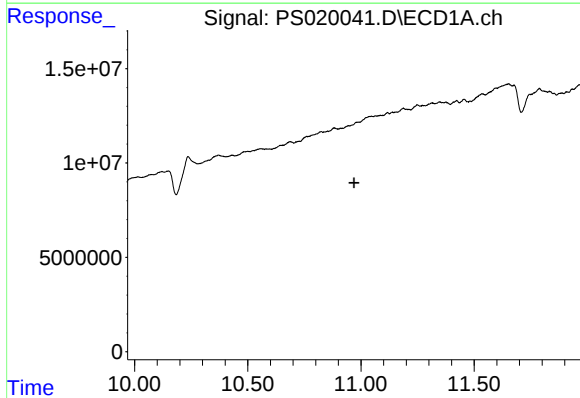

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 10.969 min
Response: 0
Conc: N.D.

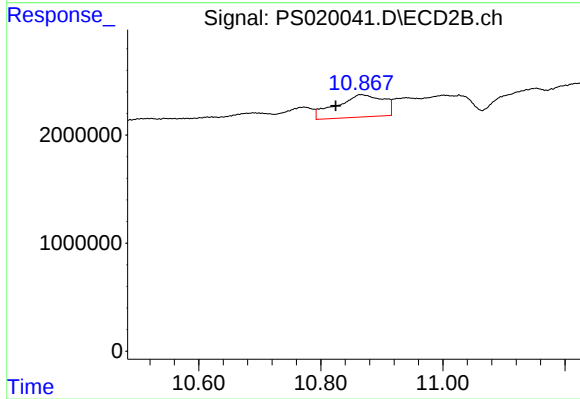

#15 Picloram

R.T.: 10.866 min
Delta R.T.: 0.042 min
Response: 11065692
Conc: 1.44 ng/ml