

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072123\
 Data File : PS023792.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2023 07:42
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 21 21:10:40 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072023.M
 Quant Title : 8080.M
 QLast Update : Thu Jul 20 19:21:53 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.372	6.801	2327082	758658	1.174	1.116
Target Compounds							
1) T	Dalapon	2.517	2.585	3211569	3041677	1.499	2.747 #
2) T	3,5-DICHL...	5.745	5.983	1271957	907580	<MDL	<MDL #
3) T	4-Nitroph...	6.212	6.370f	6465704	180703	5.201	<MDL #
5) T	DICAMBA	6.516	6.970	2697275	2001654	<MDL	<MDL #
8) T	DICHLORPROP	7.106	7.600	711998	2547962	<MDL	3.373 #
9) T	2,4-D	7.307	7.872	69587912	917534	26.974	1.076 #
10) T	Pentachlo...	7.536	8.300	9529209	2815444	<MDL	<MDL #
11) T	2,4,5-TP ...	8.061	8.658	6128024	2140960	<MDL	<MDL #
12) T	2,4,5-T	8.316	9.030	9436889	3055787	<MDL	<MDL #
13) T	2,4-DB	8.822	9.536	808782	448282	<MDL	<MDL #
14) T	DINOSEB	9.881	9.865	3202356	1273334	<MDL	<MDL #
15) T	Picloram	9.705	10.823	74196696	27763947	4.841	4.578
16) T	DCPA	10.145	10.823	5422166	27763947	<MDL	5.840 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072123\
Data File : PS023792.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jul 2023 07:42
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 21 21:10:40 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072023.M
Quant Title : 8080.M
QLast Update : Thu Jul 20 19:21:53 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

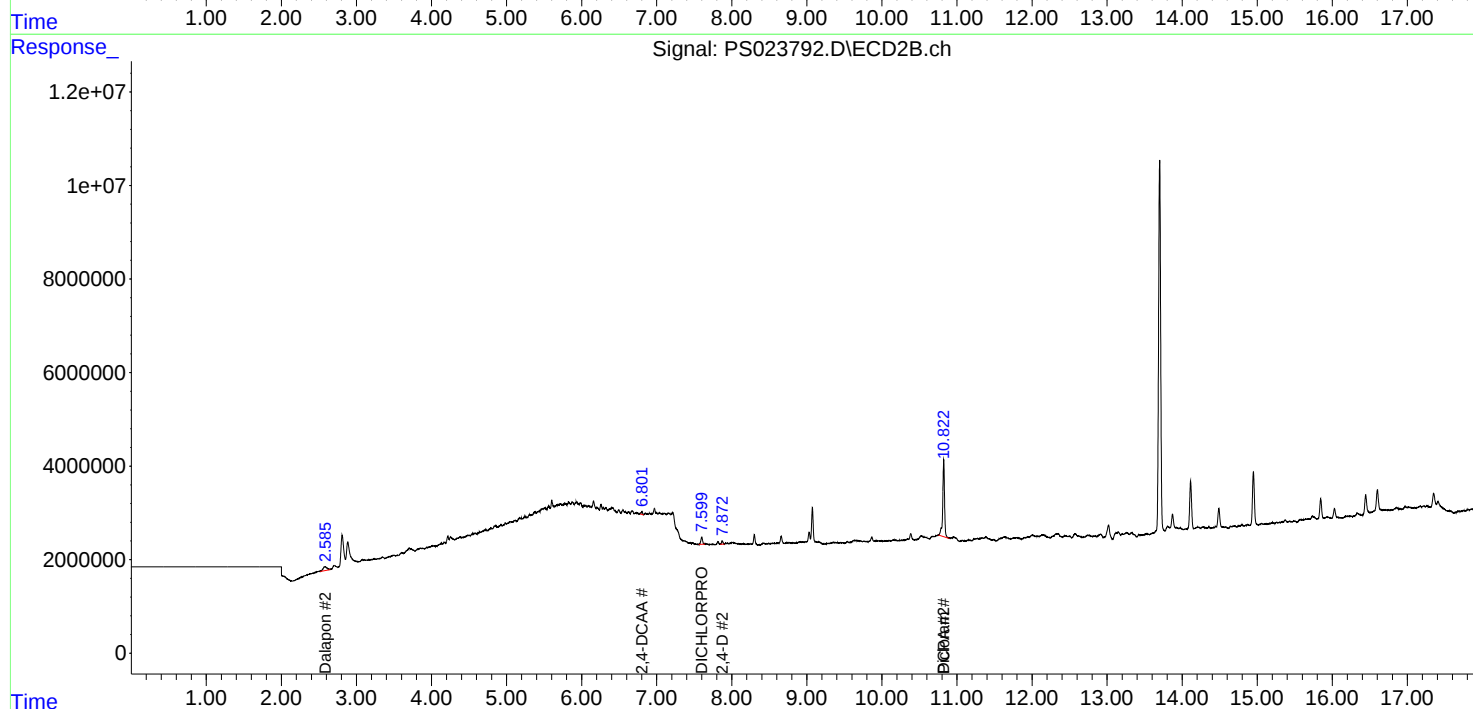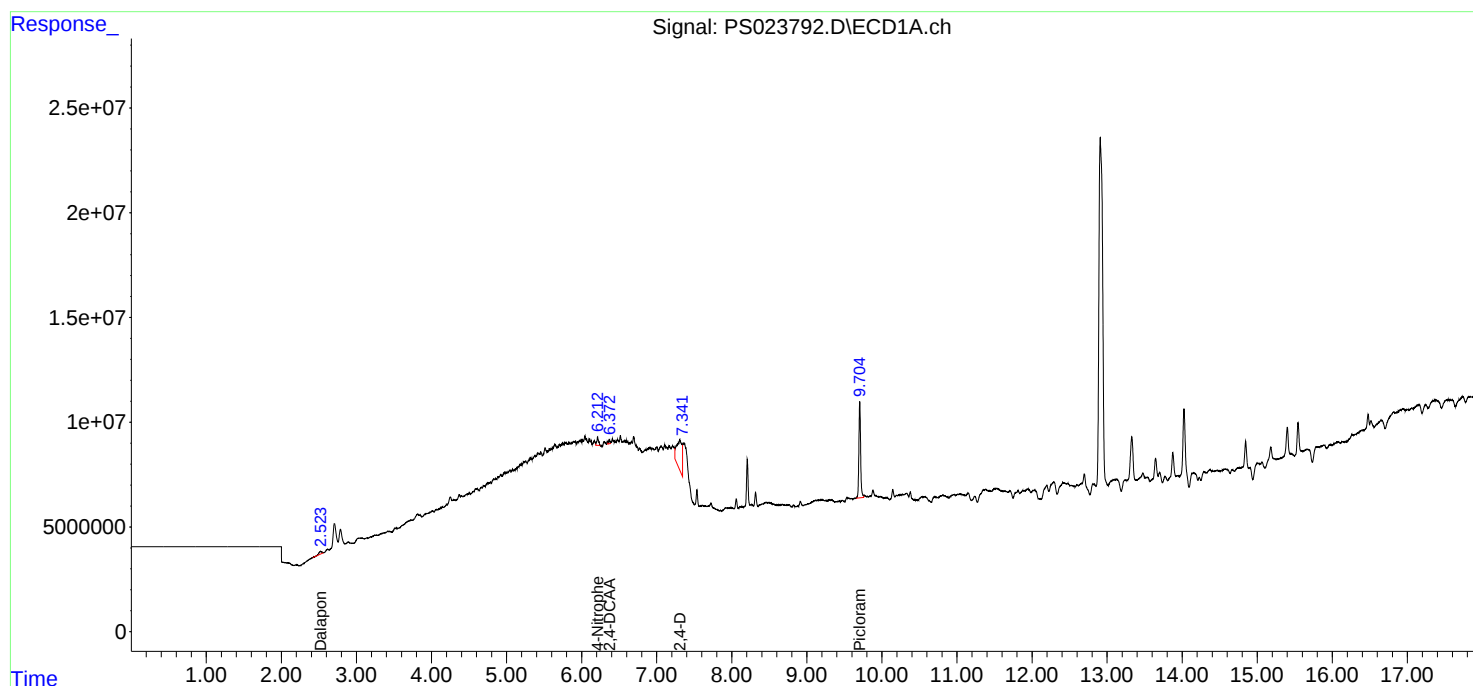


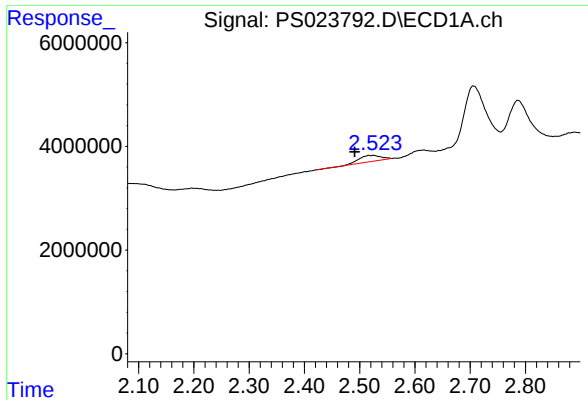

#1 Dalapon


R.T.: 2.517 min
Delta R.T.: 0.026 min
Response: 3211569
Conc: 1.50 ng/ml

Instrument :
ECD_S
ClientSampleId :

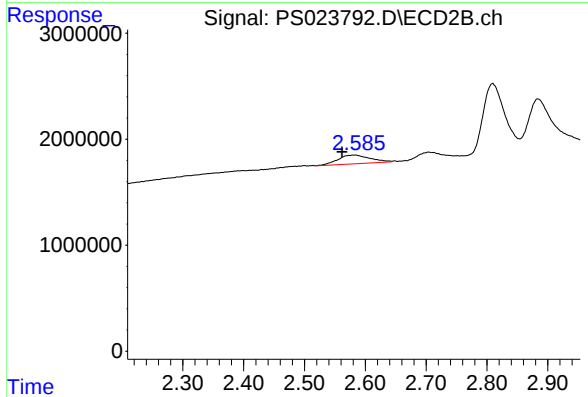


#1 Dalapon

R.T.: 2.585 min
Delta R.T.: 0.023 min
Response: 3041677
Conc: 2.75 ng/ml

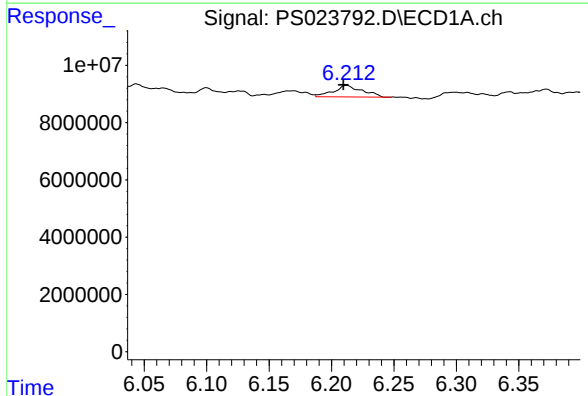


#3 4-Nitrophenol

R.T.: 6.212 min
Delta R.T.: 0.002 min
Response: 6465704
Conc: 5.20 ng/ml

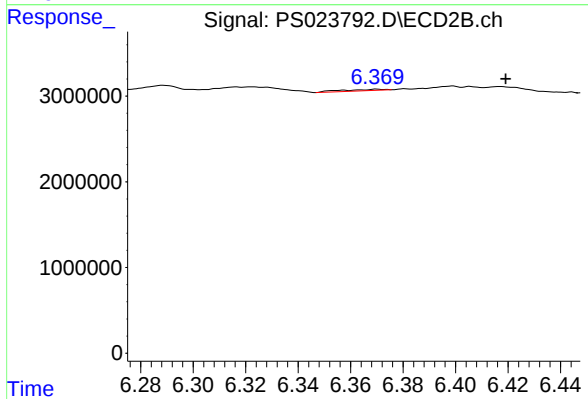

#3 4-Nitrophenol


R.T.: 6.370 min
Delta R.T.: -0.049 min
Response: 180703
Conc: N.D.

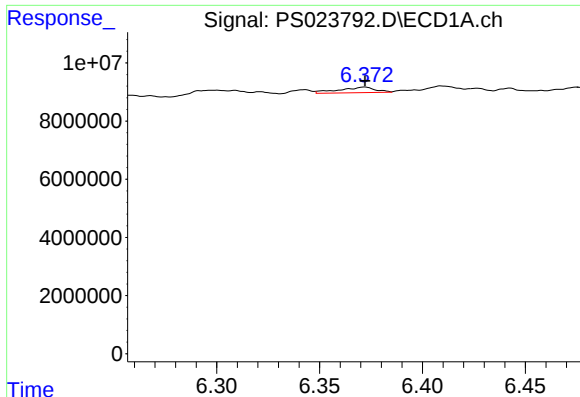

#4 2,4-DCAA


R.T.: 6.372 min
Delta R.T.: 0.000 min
Response: 2327082
Conc: 1.17 ng/ml

Instrument :
ECD_S
ClientSampleId :

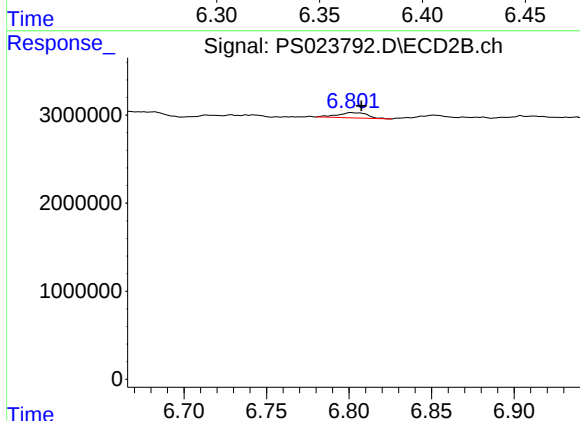


#4 2,4-DCAA

R.T.: 6.801 min
Delta R.T.: -0.006 min
Response: 758658
Conc: 1.12 ng/ml

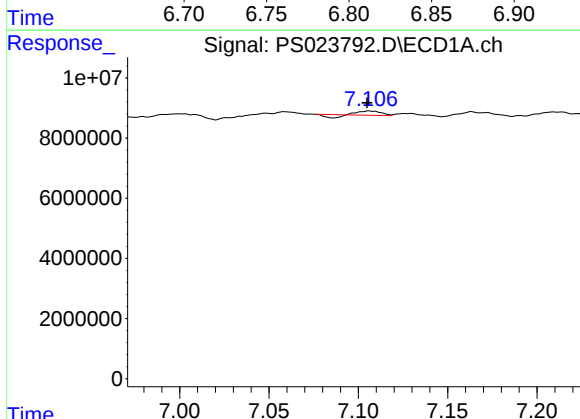


#8 DICHLORPROP

R.T.: 7.106 min
Delta R.T.: 0.001 min
Response: 711998
Conc: N.D.

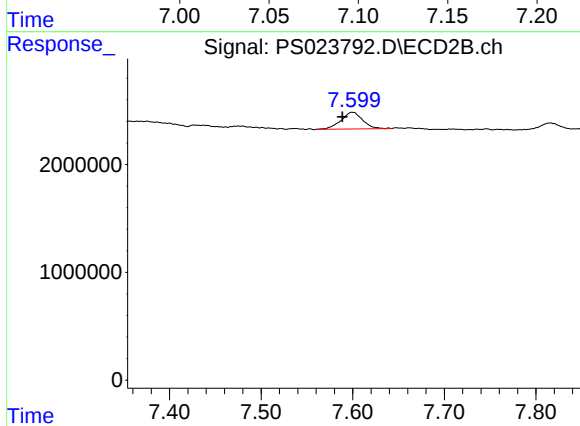

#8 DICHLORPROP


R.T.: 7.600 min
Delta R.T.: 0.011 min
Response: 2547962
Conc: 3.37 ng/ml

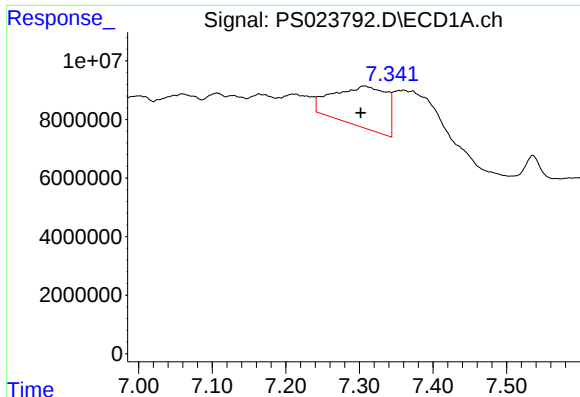

#9 2,4-D


R.T.: 7.307 min
Delta R.T.: 0.005 min
Response: 69587912
Conc: 26.97 ng/ml

Instrument :
ECD_S
ClientSampleId :

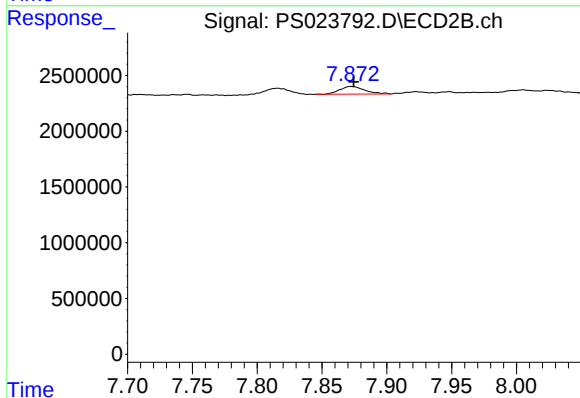


#9 2,4-D

R.T.: 7.872 min
Delta R.T.: -0.002 min
Response: 917534
Conc: 1.08 ng/ml

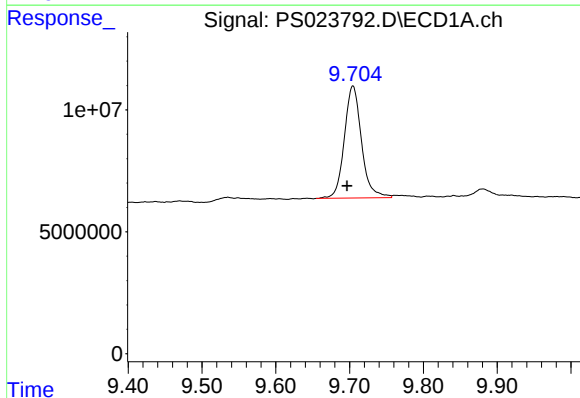


#15 Picloram

R.T.: 9.705 min
Delta R.T.: 0.008 min
Response: 74196696
Conc: 4.84 ng/ml

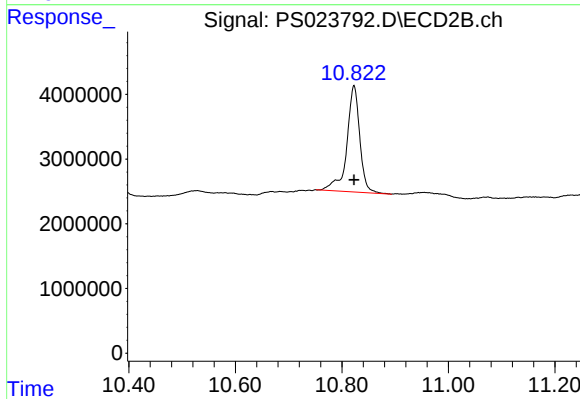

#15 Picloram


R.T.: 10.823 min
Delta R.T.: 0.000 min
Response: 27763947
Conc: 4.58 ng/ml

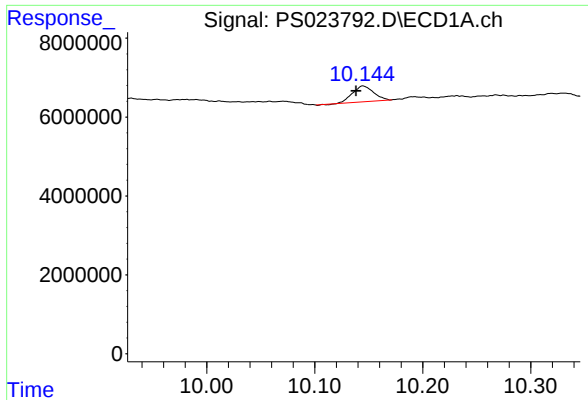

#16 DCPA

R.T.: 10.145 min
Delta R.T.: 0.007 min
Response: 5422166
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

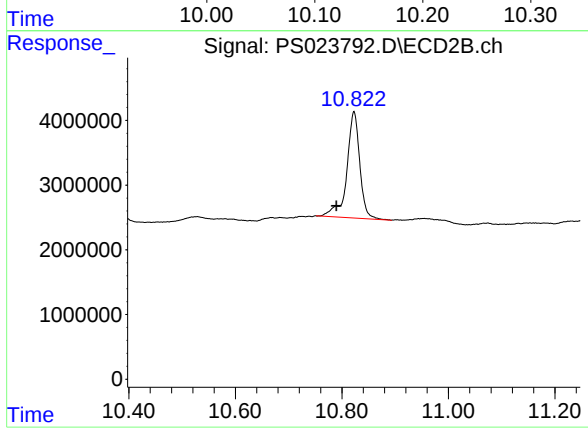

#16 DCPA

R.T.: 10.823 min
Delta R.T.: 0.033 min
Response: 27763947
Conc: 5.84 ng/ml