

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072125\
 Data File : PS031160.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2025 16:15
 Operator : AR\AJ
 Sample : HSTDICC1000
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 03:10:09 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072125.M
 Quant Title : 8080.M
 QLast Update : Tue Jul 22 02:56:38 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.325	7.767	4081.1E6	963.1E6	960.548	974.410
Target Compounds							
1) T	Dalapon	2.689	2.704	5453.5E6	2469.7E6	881.153	886.533
2) T	3,5-DICHL...	6.488	6.713	4802.5E6	1352.4E6	894.170	907.714
3) T	4-Nitroph...	7.124	7.299	1421.4E6	1607.0E6	885.429	900.562
5) T	DICAMBA	7.514	7.969	14833.0E6	5935.2E6	911.687	924.924
6) T	MCPD	7.697	8.069	988.3E6	202.3E6	96.010	94.579
7) T	MCPA	7.847	8.319	1186.7E6	292.4E6	94.362	92.559
8) T	DICHLORPROP	8.226	8.688	3335.1E6	1341.1E6	905.388	910.253
9) T	2,4-D	8.458	9.025	3339.3E6	1508.0E6	913.771	910.492
10) T	Pentachlo...	8.766	9.548	47049.8E6	36703.3E6	821.015	918.463
11) T	2,4,5-TP ...	9.343	9.929	19814.3E6	13630.7E6	915.689	918.454
12) T	2,4,5-T	9.637	10.356	18055.2E6	13055.2E6	925.505	922.208
13) T	2,4-DB	10.214	10.924	2771.7E6	1069.0E6	935.560	923.814
14) T	DINOSEB	11.428	11.308	14020.1E6	10337.9E6	909.338	919.272
15) T	Picloram	11.239	12.419	19111.4E6	23828.6E6	949.306	938.353
16) T	DCPA	11.725	12.353	25980.1E6	21487.8E6	917.296	927.856



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072125\
Data File : PS031160.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jul 2025 16:15
Operator : AR\AJ
Sample : HSTDICC1000
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 22 03:10:09 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072125.M
Quant Title : 8080.M
QLast Update : Tue Jul 22 02:56:38 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

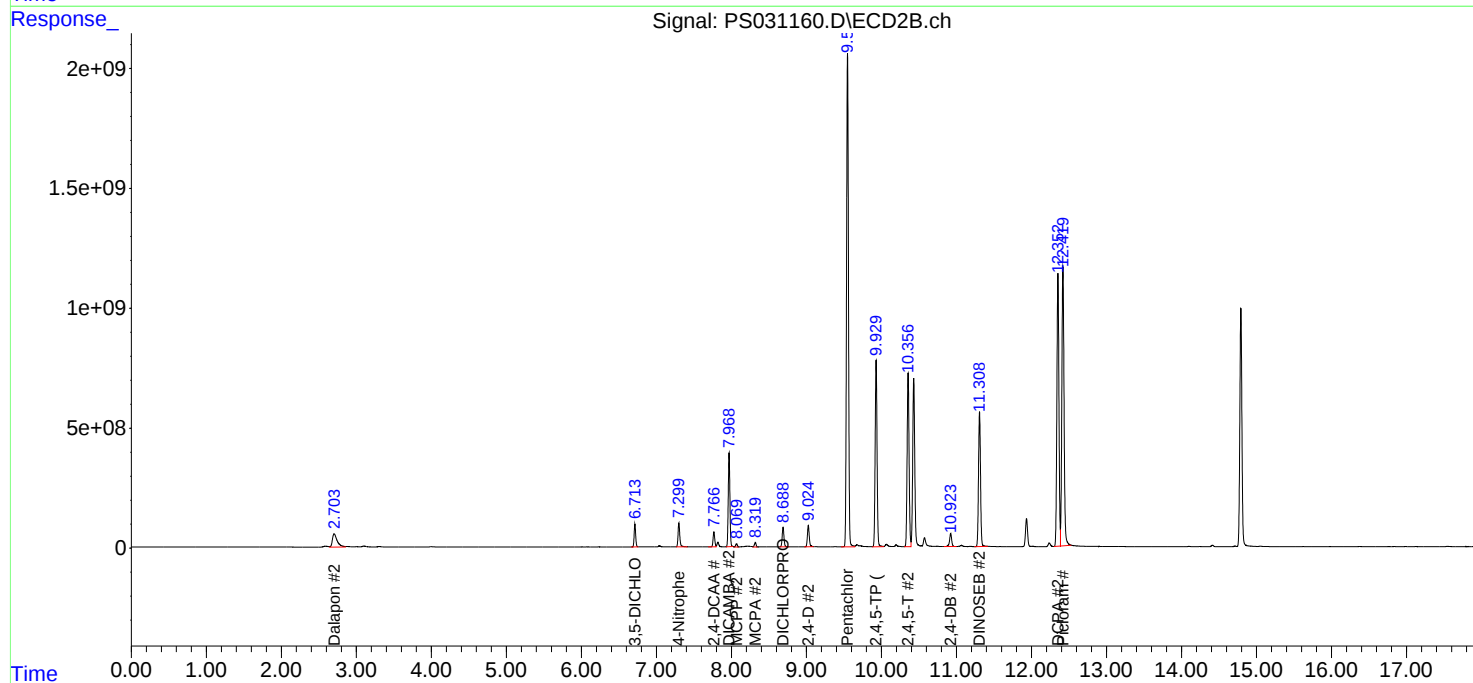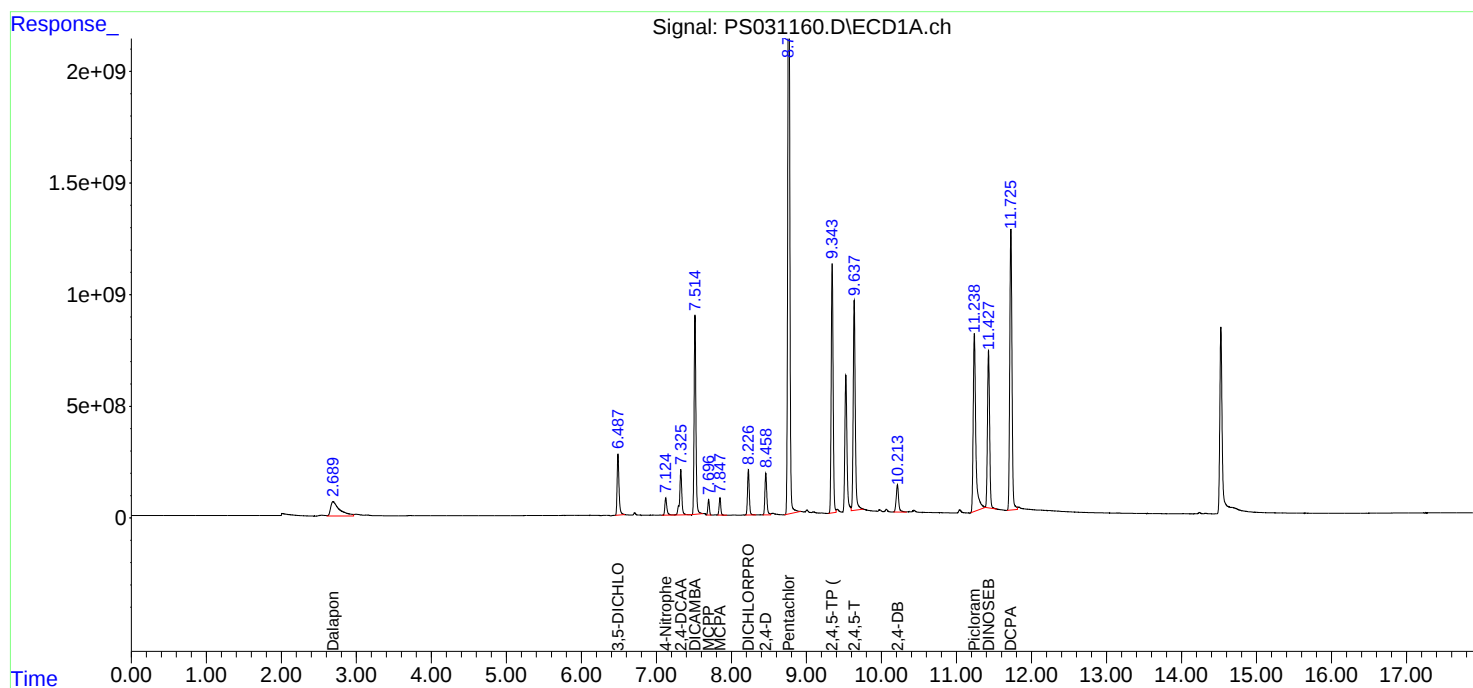


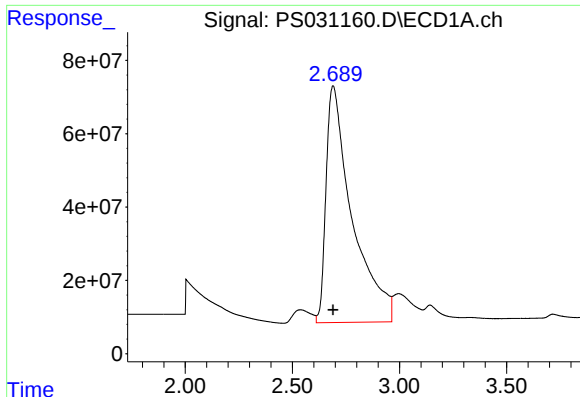

#1 Dalapon


R.T.: 2.689 min
Delta R.T.: 0.000 min
Response: 5453482387
Conc: 881.15 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC1000

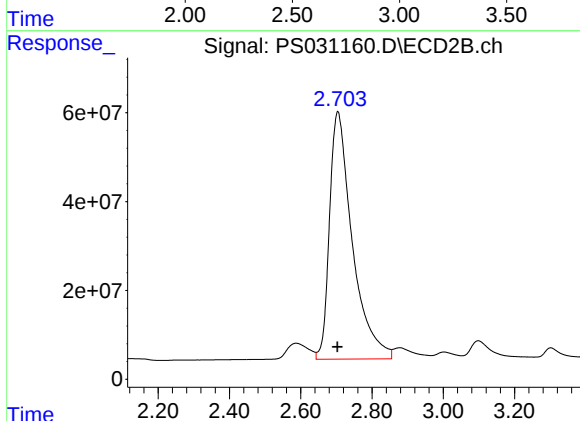


#1 Dalapon

R.T.: 2.704 min
Delta R.T.: 0.000 min
Response: 2469740297
Conc: 886.53 ng/ml

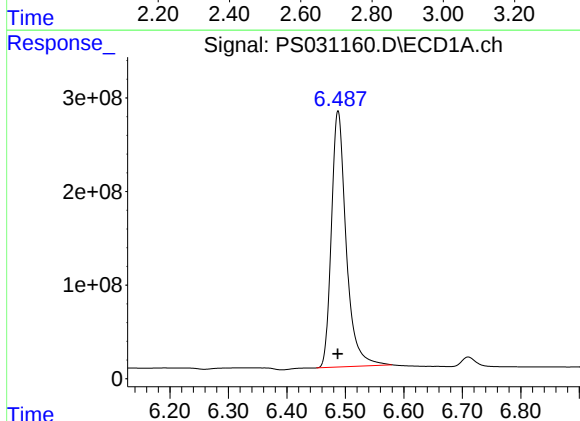


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.488 min
Delta R.T.: 0.000 min
Response: 4802454215
Conc: 894.17 ng/ml

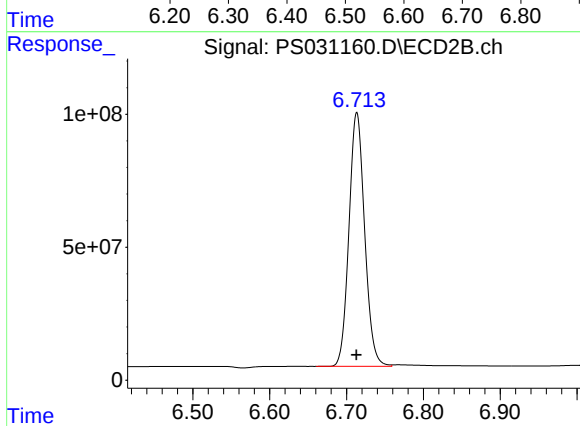

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.713 min
Delta R.T.: 0.000 min
Response: 1352413139
Conc: 907.71 ng/ml

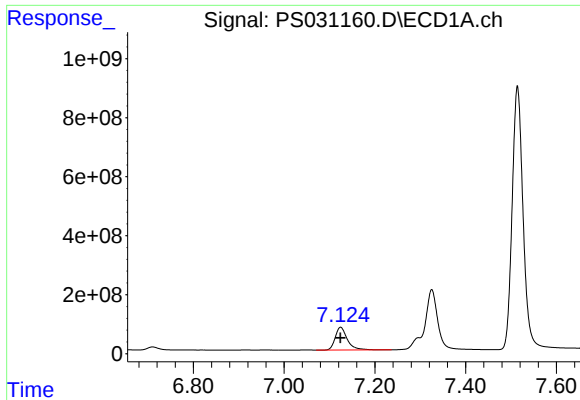

#3 4-Nitrophenol


R.T.: 7.124 min
Delta R.T.: 0.000 min
Response: 1421384436
Conc: 885.43 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC1000

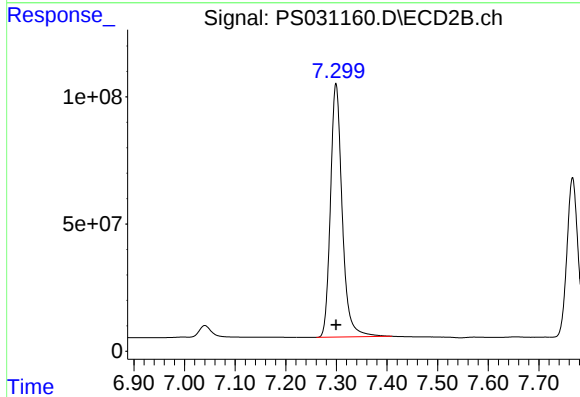


#3 4-Nitrophenol

R.T.: 7.299 min
Delta R.T.: 0.000 min
Response: 1607035149
Conc: 900.56 ng/ml

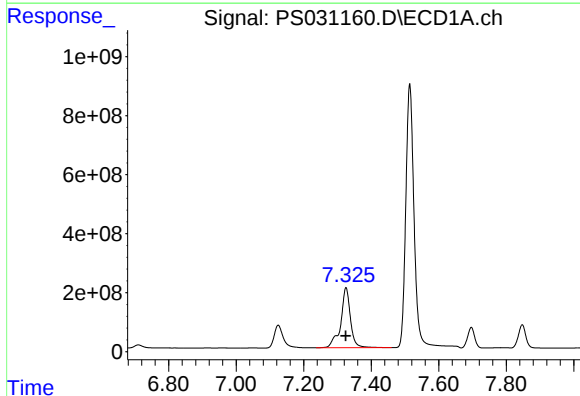


#4 2,4-DCAA

R.T.: 7.325 min
Delta R.T.: 0.000 min
Response: 4081100306
Conc: 960.55 ng/ml

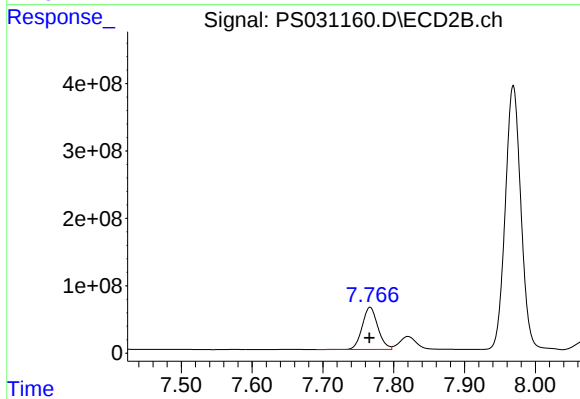

#4 2,4-DCAA


R.T.: 7.767 min
Delta R.T.: 0.000 min
Response: 963100505
Conc: 974.41 ng/ml

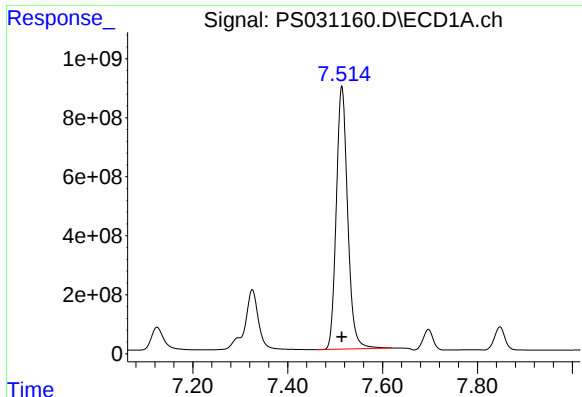

#5 DICAMBA


R.T.: 7.514 min
Delta R.T.: 0.000 min
Response: 14832958607
Conc: 911.69 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC1000

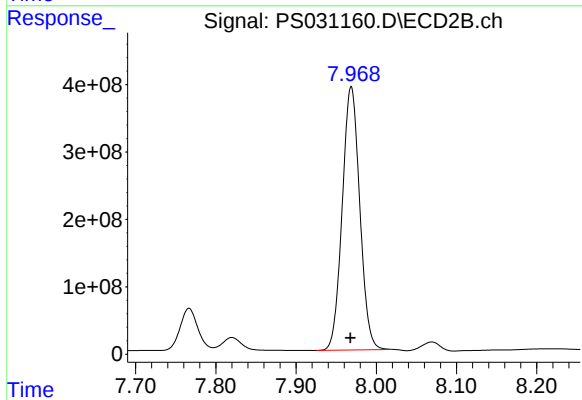


#5 DICAMBA

R.T.: 7.969 min
Delta R.T.: 0.000 min
Response: 5935186825
Conc: 924.92 ng/ml

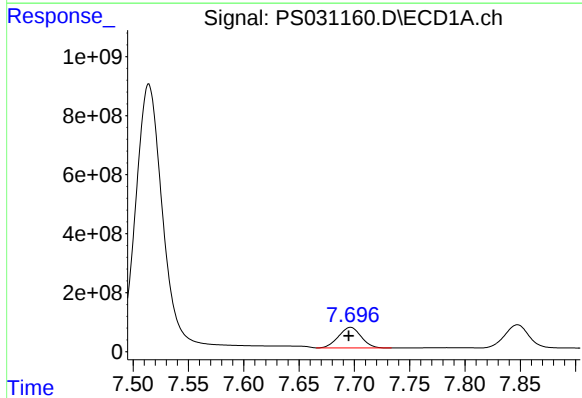


#6 MCP

R.T.: 7.697 min
Delta R.T.: 0.002 min
Response: 988309419
Conc: 96.01 ug/ml

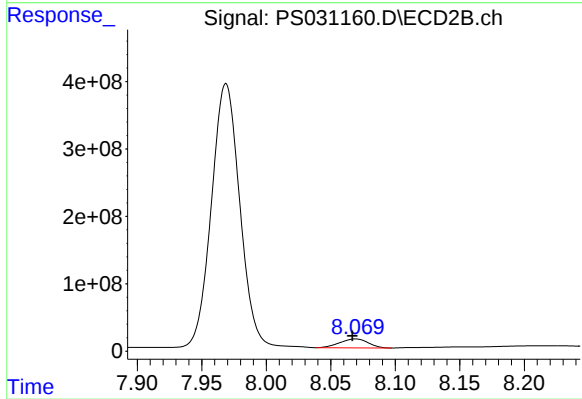

#6 MCP


R.T.: 8.069 min
Delta R.T.: 0.003 min
Response: 202250812
Conc: 94.58 ug/ml

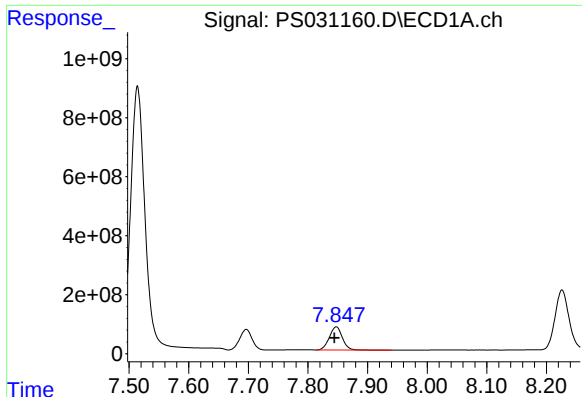

#7 MCPA


R.T.: 7.847 min
Delta R.T.: 0.003 min
Response: 1186681895
Conc: 94.36 ug/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC1000

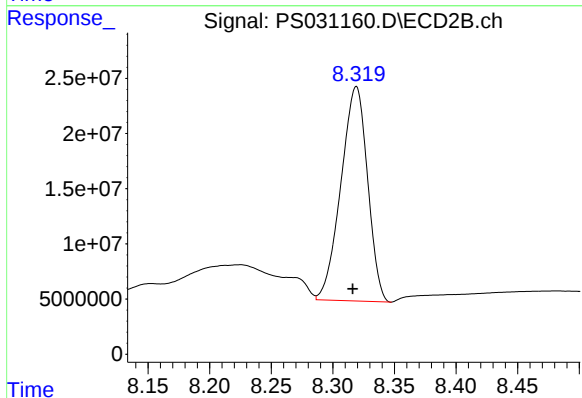


#7 MCPA

R.T.: 8.319 min
Delta R.T.: 0.003 min
Response: 292445492
Conc: 92.56 ug/ml

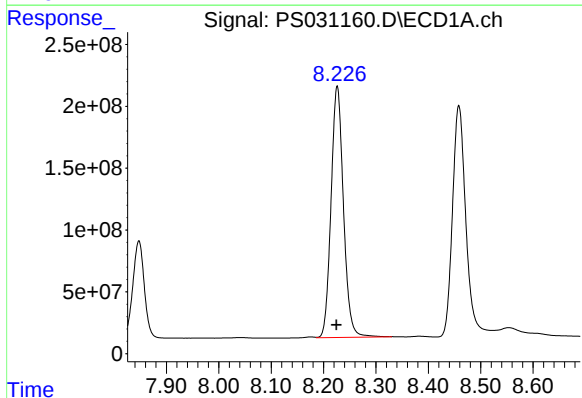


#8 DICHLORPROP

R.T.: 8.226 min
Delta R.T.: 0.002 min
Response: 3335100839
Conc: 905.39 ng/ml

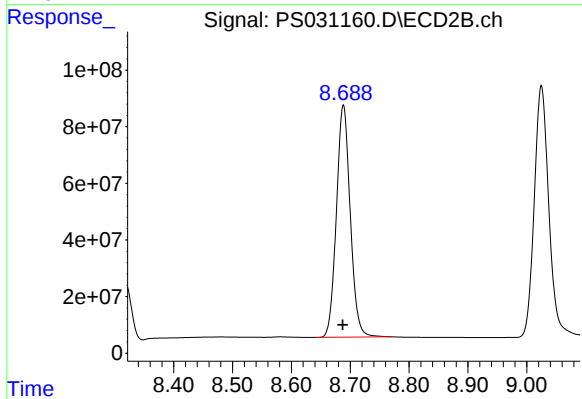

#8 DICHLORPROP


R.T.: 8.688 min
Delta R.T.: 0.000 min
Response: 1341135683
Conc: 910.25 ng/ml

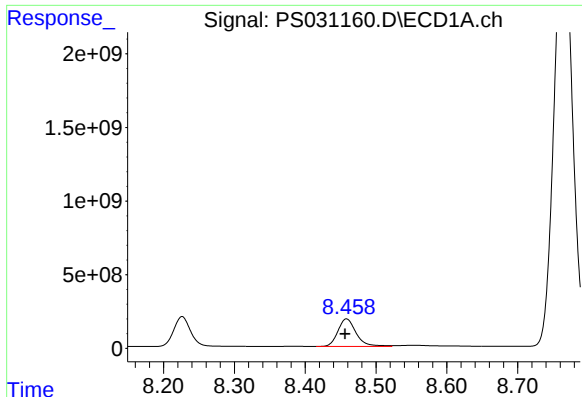

#9 2,4-D


R.T.: 8.458 min
Delta R.T.: 0.002 min
Response: 3339344621
Conc: 913.77 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC1000

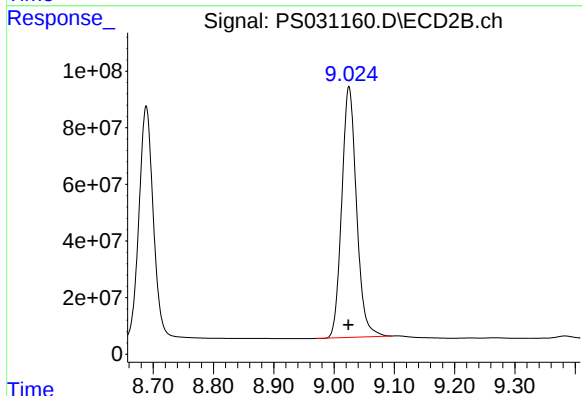


#9 2,4-D

R.T.: 9.025 min
Delta R.T.: 0.001 min
Response: 1507960462
Conc: 910.49 ng/ml

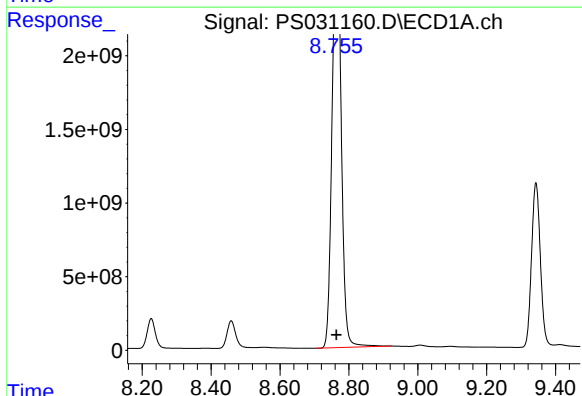


#10 Pentachlorophenol

R.T.: 8.766 min
Delta R.T.: 0.002 min
Response: 47049761792
Conc: 821.01 ng/ml

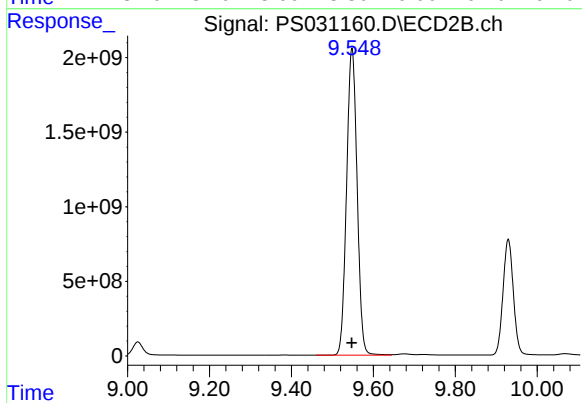

#10 Pentachlorophenol


R.T.: 9.548 min
Delta R.T.: 0.000 min
Response: 36703311197
Conc: 918.46 ng/ml

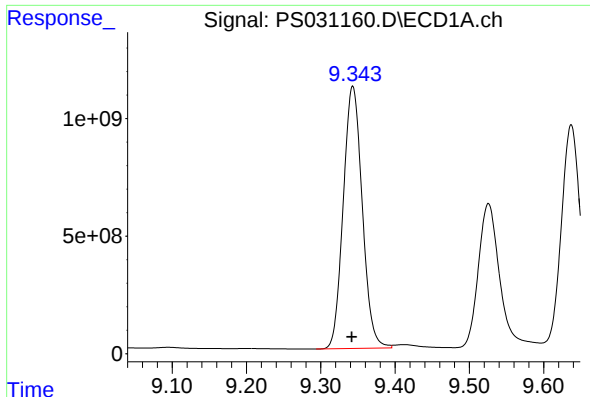

#11 2,4,5-TP (SILVEX)


R.T.: 9.343 min
Delta R.T.: 0.001 min
Response: 19814320460
Conc: 915.69 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC1000

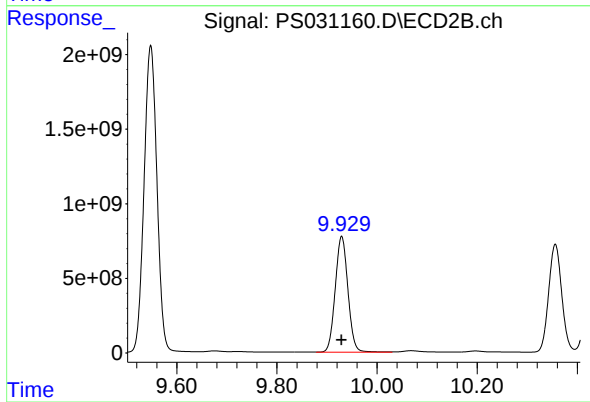


#11 2,4,5-TP (SILVEX)

R.T.: 9.929 min
Delta R.T.: 0.000 min
Response: 13630690259
Conc: 918.45 ng/ml

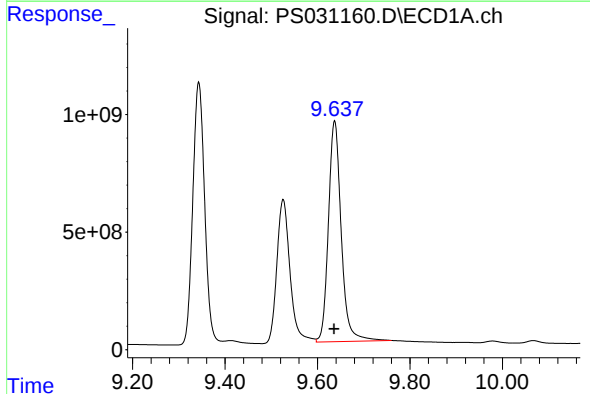


#12 2,4,5-T

R.T.: 9.637 min
Delta R.T.: 0.001 min
Response: 18055208033
Conc: 925.51 ng/ml

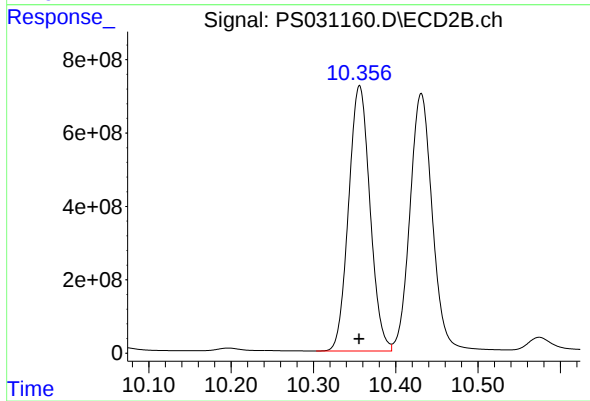

#12 2,4,5-T


R.T.: 10.356 min
Delta R.T.: 0.000 min
Response: 13055215548
Conc: 922.21 ng/ml

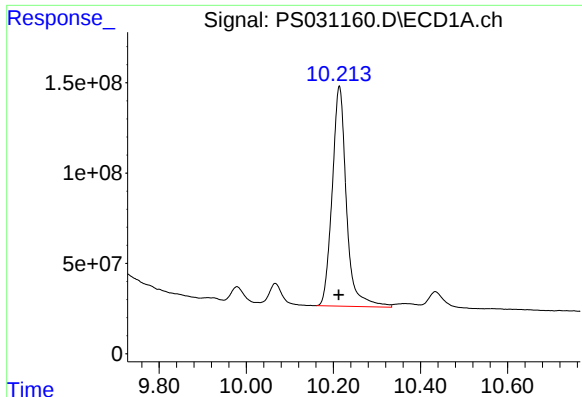

#13 2,4-DB


R.T.: 10.214 min
Delta R.T.: 0.001 min
Response: 2771712245
Conc: 935.56 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC1000

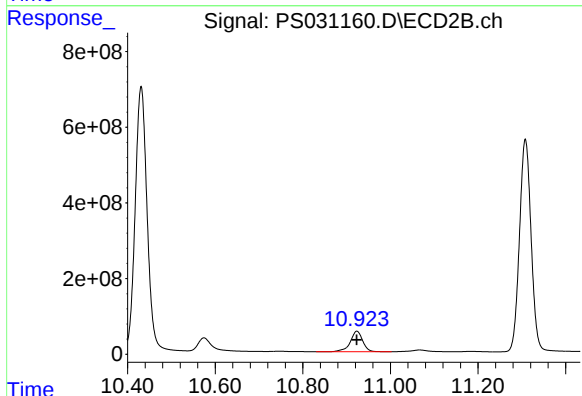


#13 2,4-DB

R.T.: 10.924 min
Delta R.T.: 0.000 min
Response: 1069032150
Conc: 923.81 ng/ml

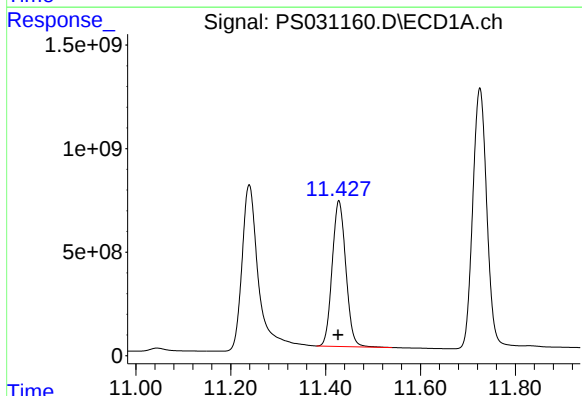


#14 DINOSEB

R.T.: 11.428 min
Delta R.T.: 0.001 min
Response: 14020122881
Conc: 909.34 ng/ml

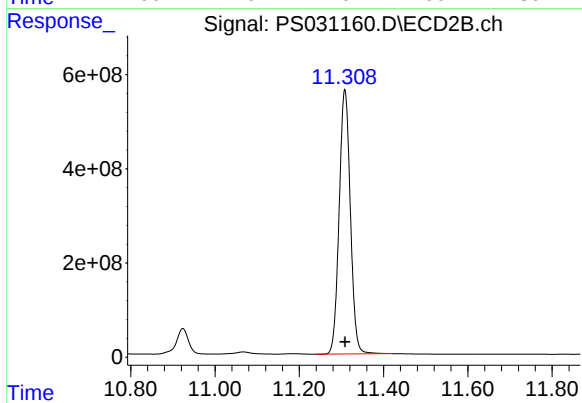

#14 DINOSEB


R.T.: 11.308 min
Delta R.T.: 0.000 min
Response: 10337937996
Conc: 919.27 ng/ml

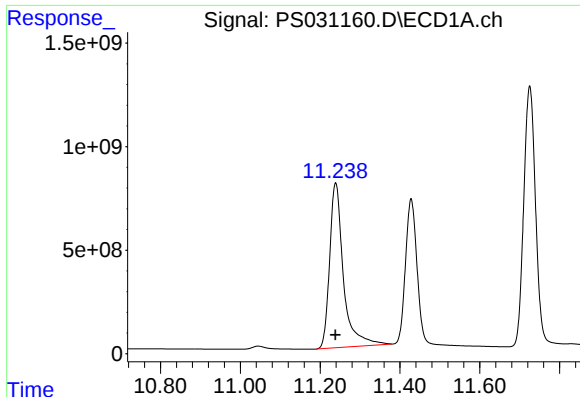

#15 Picloram


R.T.: 11.239 min
Delta R.T.: 0.000 min
Response: 19111405619
Conc: 949.31 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC1000

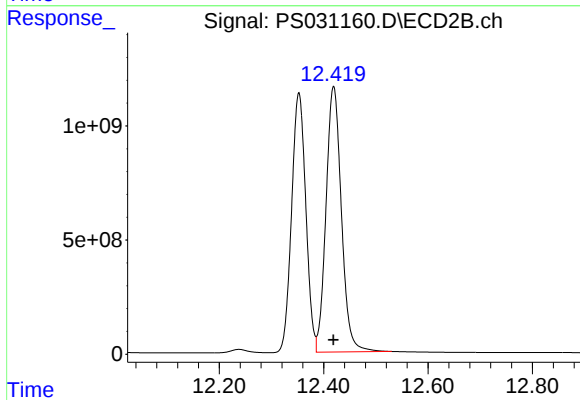


#15 Picloram

R.T.: 12.419 min
Delta R.T.: 0.000 min
Response: 23828587760
Conc: 938.35 ng/ml

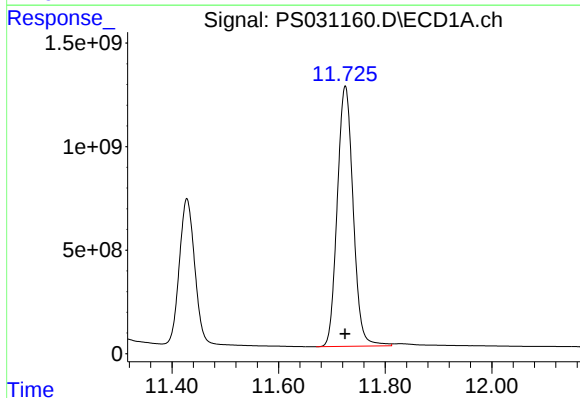

#16 DCPA

R.T.: 11.725 min
Delta R.T.: 0.000 min
Response: 25980070197
Conc: 917.30 ng/ml

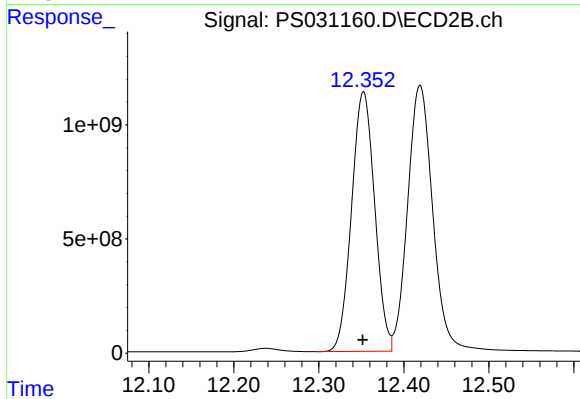

#16 DCPA

R.T.: 12.353 min
Delta R.T.: 0.000 min
Response: 21487768861
Conc: 927.86 ng/ml